

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
 Data File : PL071621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2021 02:28
 Operator : AR\AJ
 Sample : M5065-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 UV-1WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 02:52:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	11.384	0	42488	N.D.	0.039 #
Target Compounds							
7)	B delta-BHC	0.000	7.024f	0	104964	N.D.	0.069 #
9)	A Endosulfan I	0.000	8.345	0	63336	N.D.	0.053 #
10)	B gamma-Chl...	0.000	8.232	0	282720	N.D.	0.219 #
11)	B alpha-Chl...	0.000	8.327f	0	113174	N.D.	0.089 #
13)	MA Dieldrin	0.000	8.651	0	72081	N.D.	0.059 #
15)	B Endosulfa...	0.000	9.147f	0	457096	N.D.	0.453 #
16)	A 4,4'-DDD	0.000	9.033	0	107346	N.D.	0.122 #
17)	MA 4,4'-DDT	0.000	9.358	0	246732	N.D.	0.250 #
23)	Chlordane-1	0.000	6.891	0	250982	N.D.	5.460 #
24)	Chlordane-2	0.000	7.451f	0	119146	N.D.	2.526 #
25)	Chlordane-3	0.000	8.232	0	282720	N.D.	1.615 #
26)	Chlordane-4	0.000	8.327f	0	113174	N.D.	0.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
Data File : PL071621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2021 02:28
Operator : AR\AJ
Sample : M5065-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
UV-1WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 02:52:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

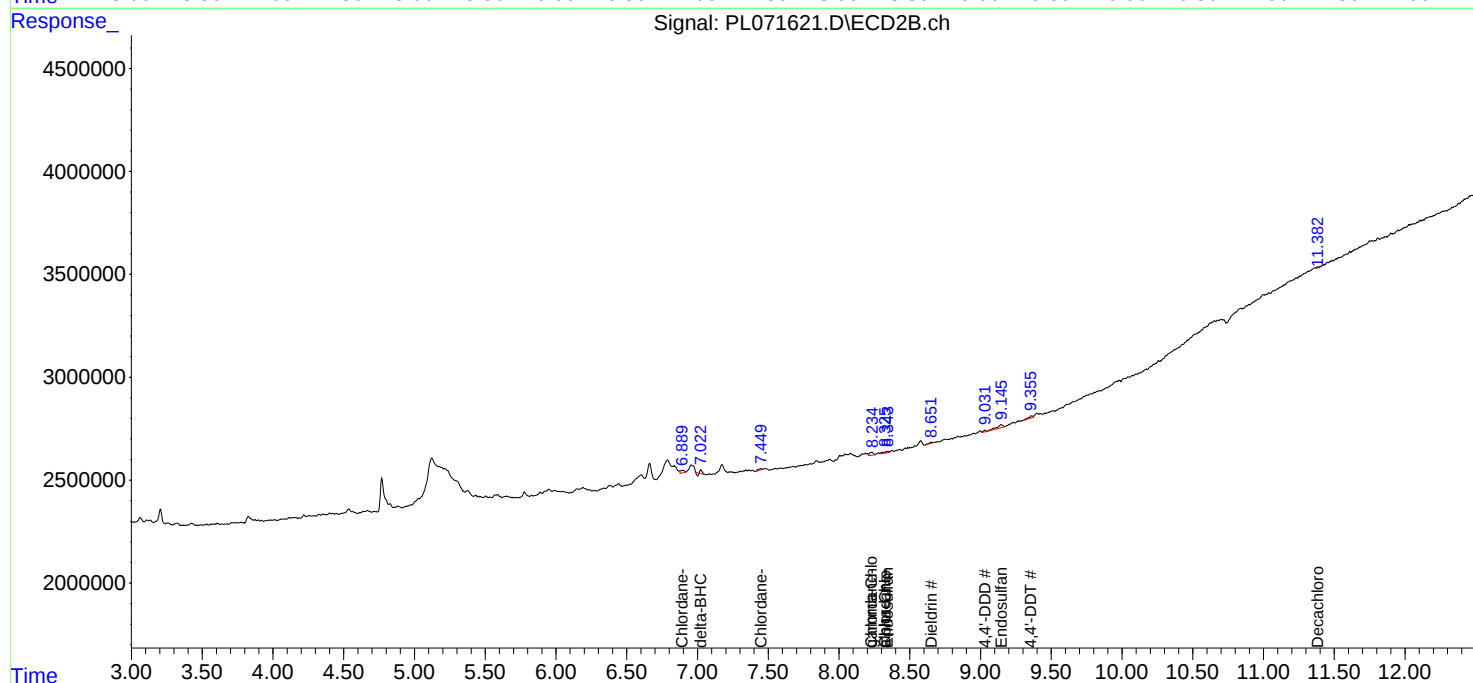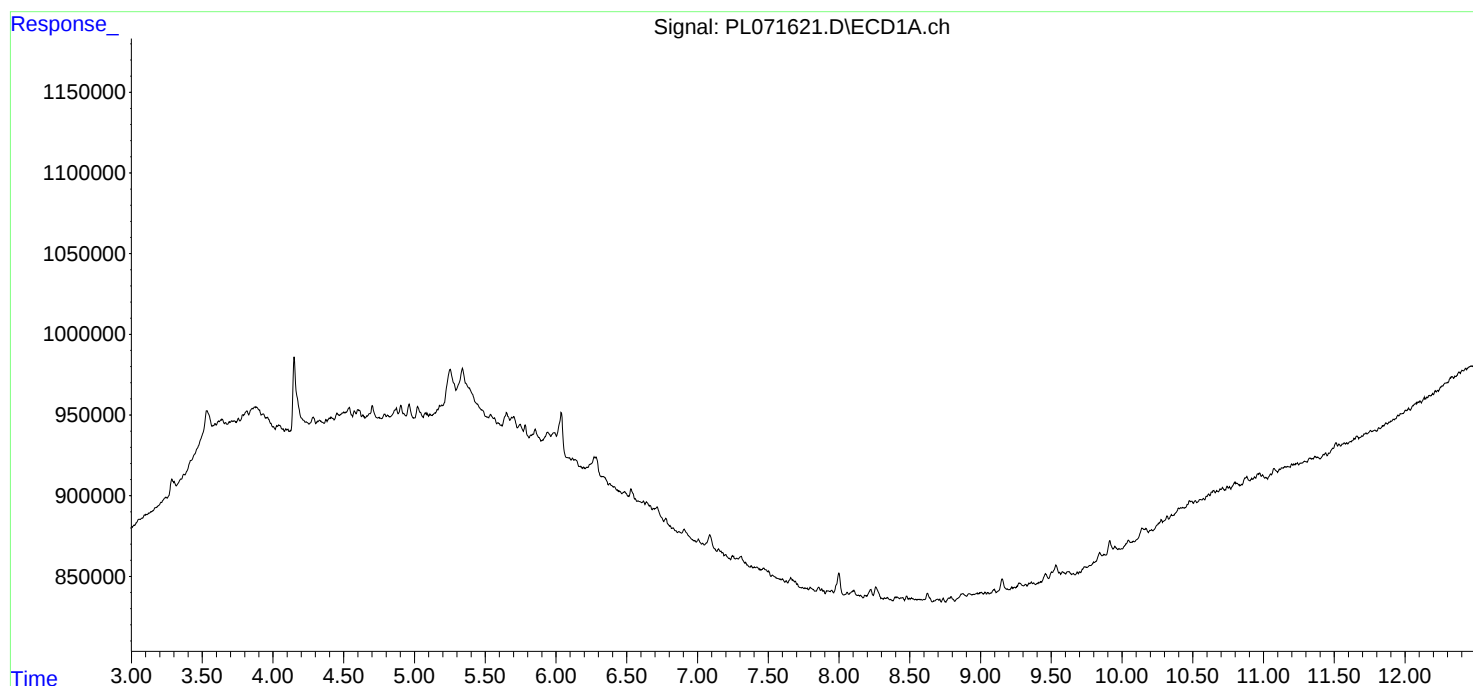


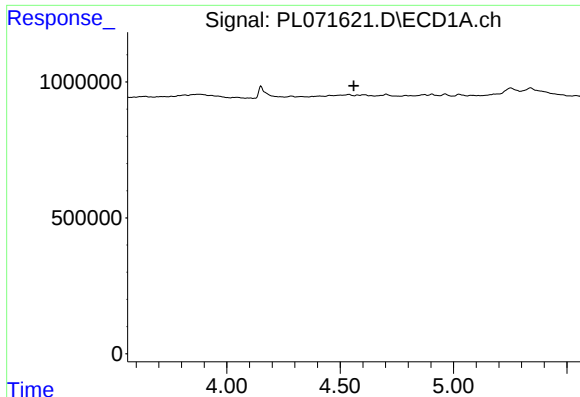

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

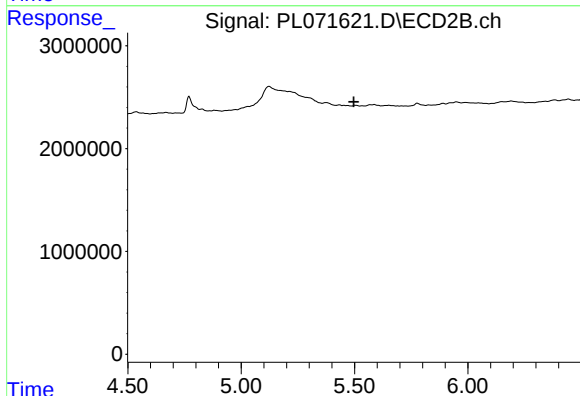


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

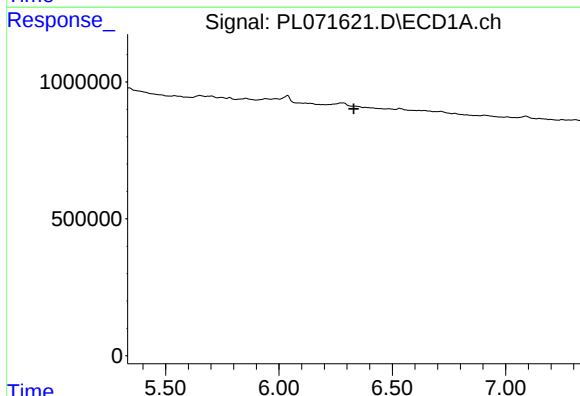


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

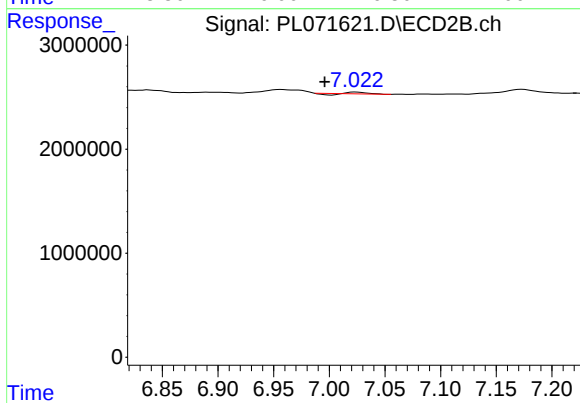

#7 delta-BHC


R.T.: 7.024 min
Delta R.T.: 0.028 min
Response: 104964
Conc: 0.07 ng/ml

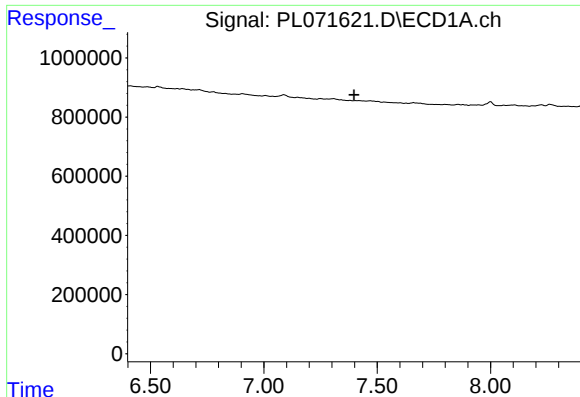

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

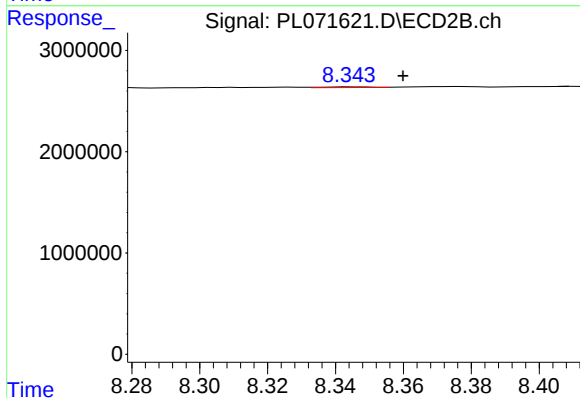


#9 Endosulfan I

R.T.: 8.345 min
Delta R.T.: -0.015 min
Response: 63336
Conc: 0.05 ng/ml

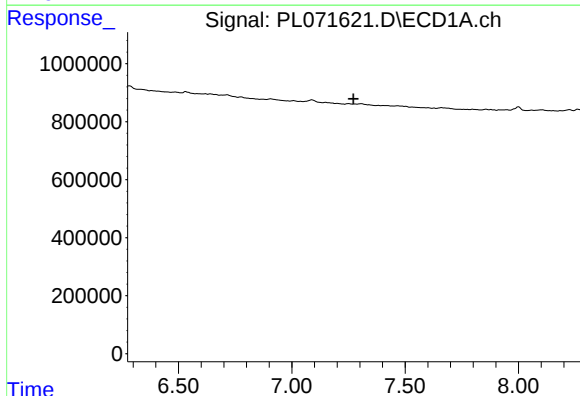


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

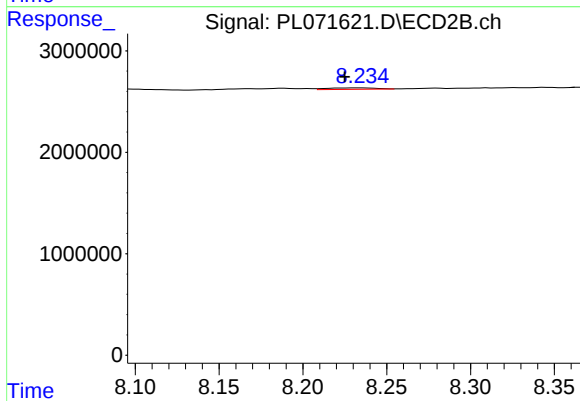

#10 gamma-Chlordane


R.T.: 8.232 min
Delta R.T.: 0.008 min
Response: 282720
Conc: 0.22 ng/ml

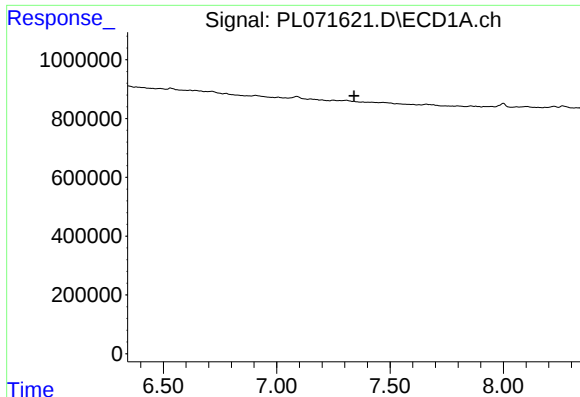

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

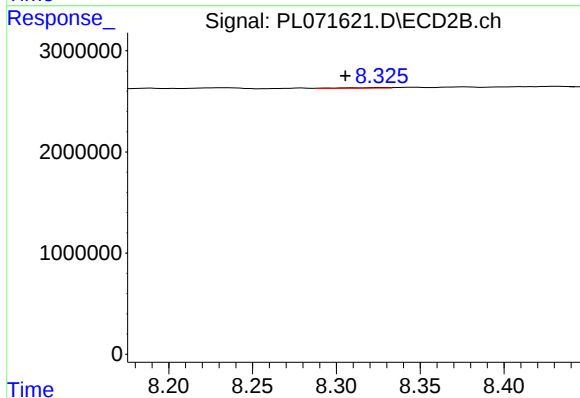


#11 alpha-Chlordane

R.T.: 8.327 min
Delta R.T.: 0.021 min
Response: 113174
Conc: 0.09 ng/ml

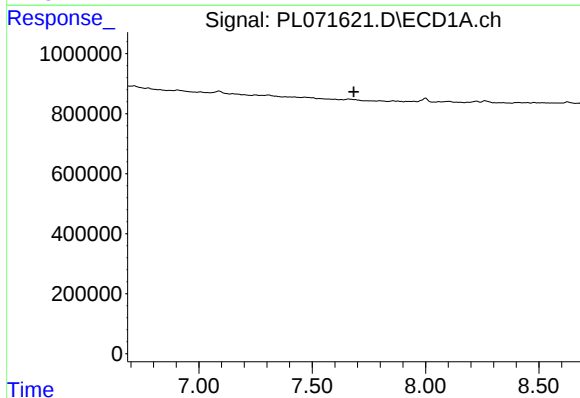


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.684 min
Response: 0
Conc: N.D.

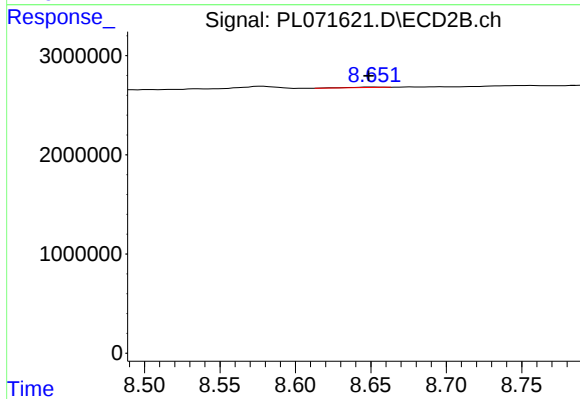

#13 Dieldrin


R.T.: 8.651 min
Delta R.T.: 0.002 min
Response: 72081
Conc: 0.06 ng/ml

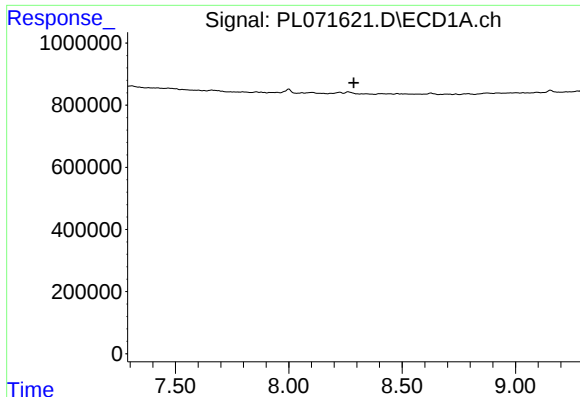

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

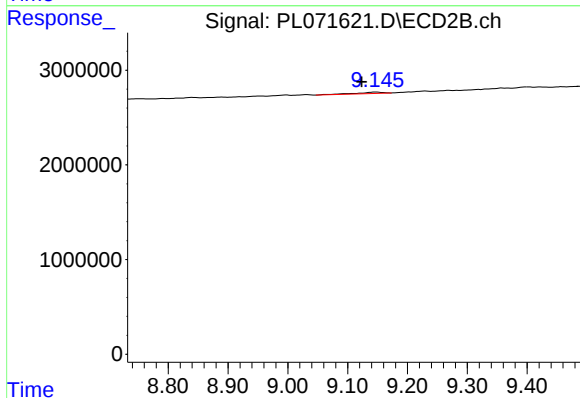


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.024 min
Response: 457096
Conc: 0.45 ng/ml

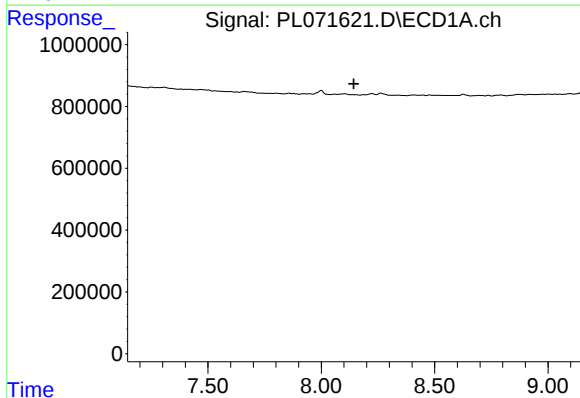


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.143 min
Response: 0
Conc: N.D.

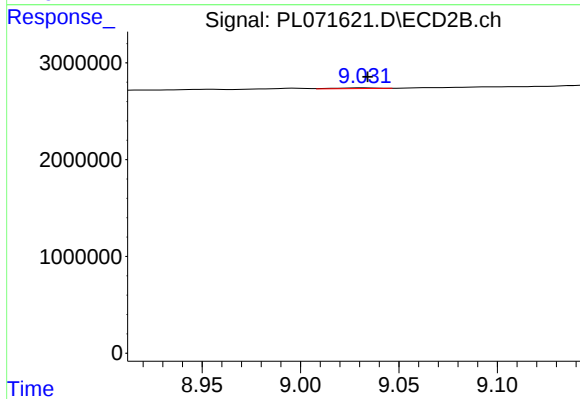

#16 4,4'-DDD


R.T.: 9.033 min
Delta R.T.: -0.002 min
Response: 107346
Conc: 0.12 ng/ml

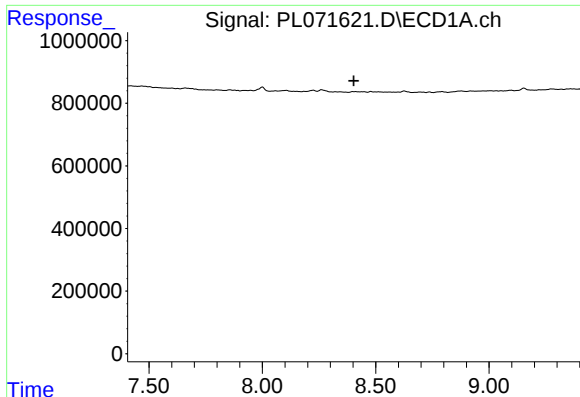

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

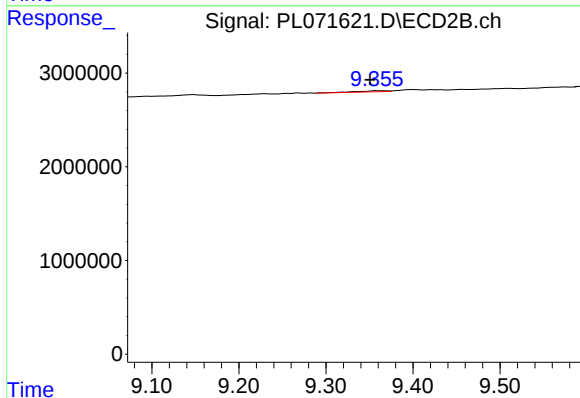


#17 4,4'-DDT

R.T.: 9.358 min
Delta R.T.: 0.007 min
Response: 246732
Conc: 0.25 ng/ml

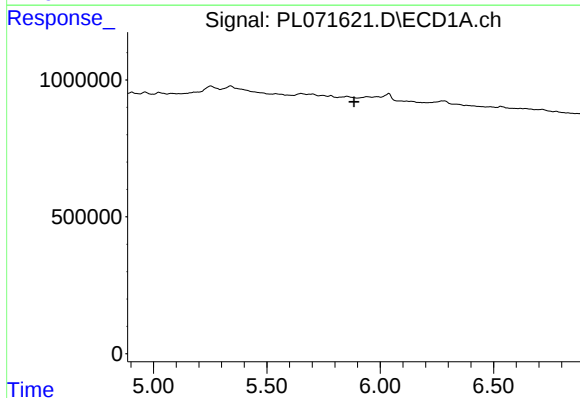


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

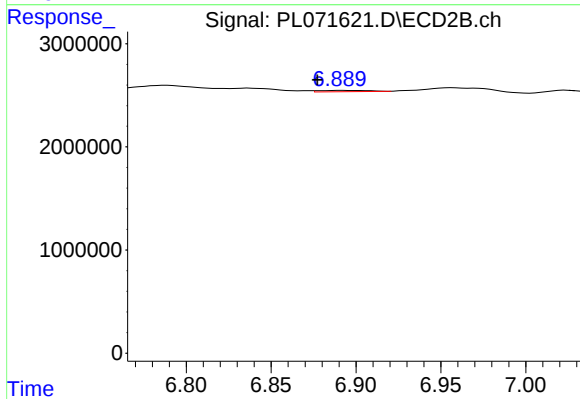

#23 Chlordane-1


R.T.: 6.891 min
Delta R.T.: 0.014 min
Response: 250982
Conc: 5.46 ng/ml

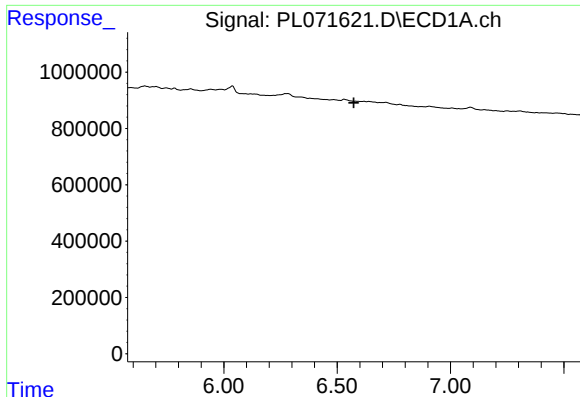

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

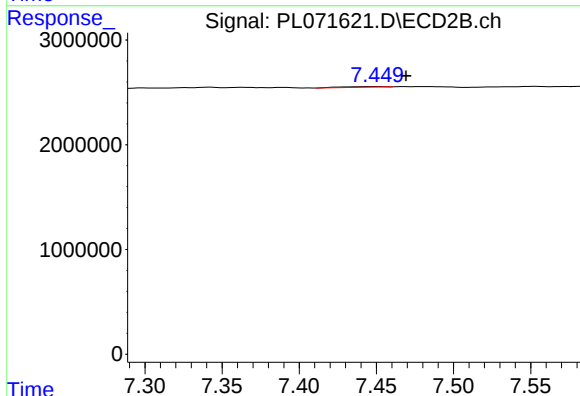


#24 Chlordane-2

R.T.: 7.451 min
Delta R.T.: -0.018 min
Response: 119146
Conc: 2.53 ng/ml

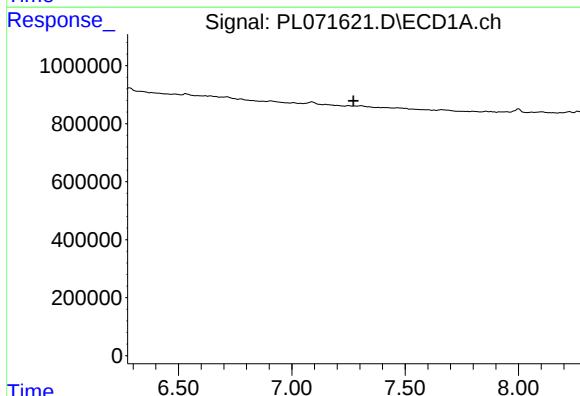


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

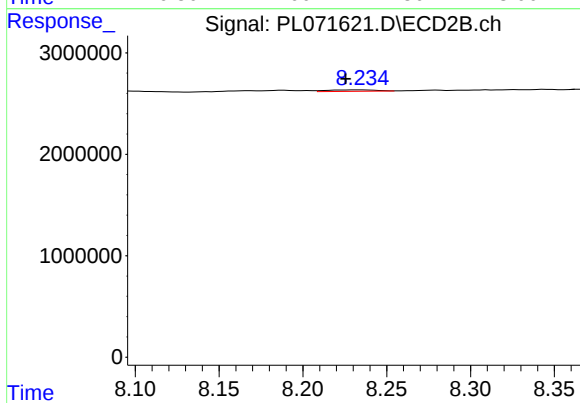

#25 Chlordane-3


R.T.: 8.232 min
Delta R.T.: 0.007 min
Response: 282720
Conc: 1.62 ng/ml

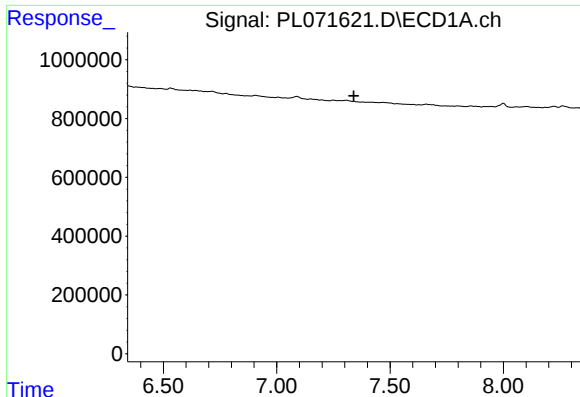

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

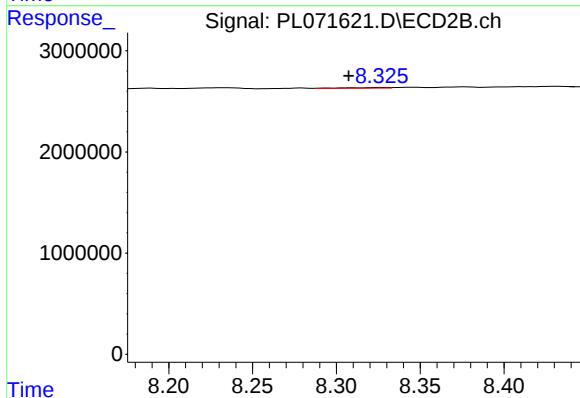


#26 Chlordane-4

R.T.: 8.327 min
Delta R.T.: 0.020 min
Response: 113174
Conc: 0.54 ng/ml

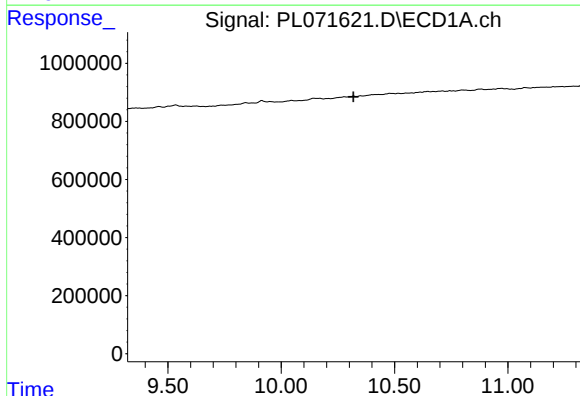

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.319 min
Response: 0
Conc: N.D.

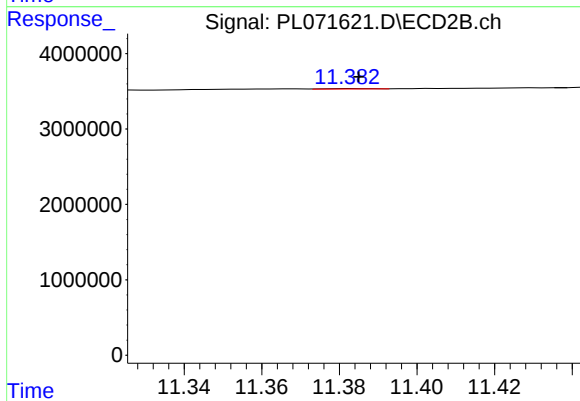

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.002 min
Response: 42488
Conc: 0.04 ng/ml