

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 16:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:14:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.563	171.0E6	245.8E6	72.186	71.446
28)	SA Decachlor...	8.771	7.632	142.5E6	163.5E6	71.429	70.854
Target Compounds							
23)	Chlordane-1	4.466	3.528	72823164	78685113	721.913	702.353
24)	Chlordane-2	4.999	4.094	77246378	83287641	705.048	698.619
25)	Chlordane-3	5.710	4.713	311.7E6	247.6E6	733.063	714.604
26)	Chlordane-4	5.788	4.774	375.0E6	263.8E6	726.395	705.138
27)	Chlordane-5	6.644	5.435	69896329	64605736	724.510	664.911



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 16:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:14:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

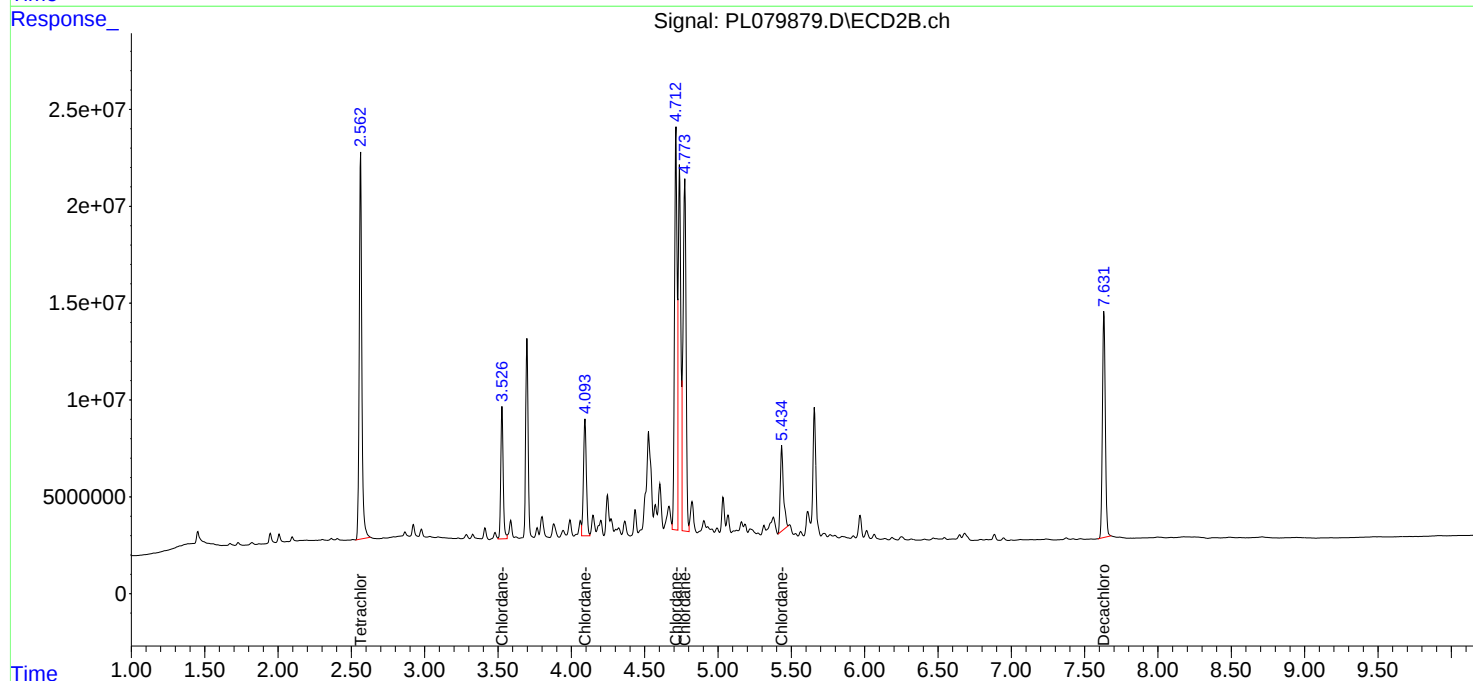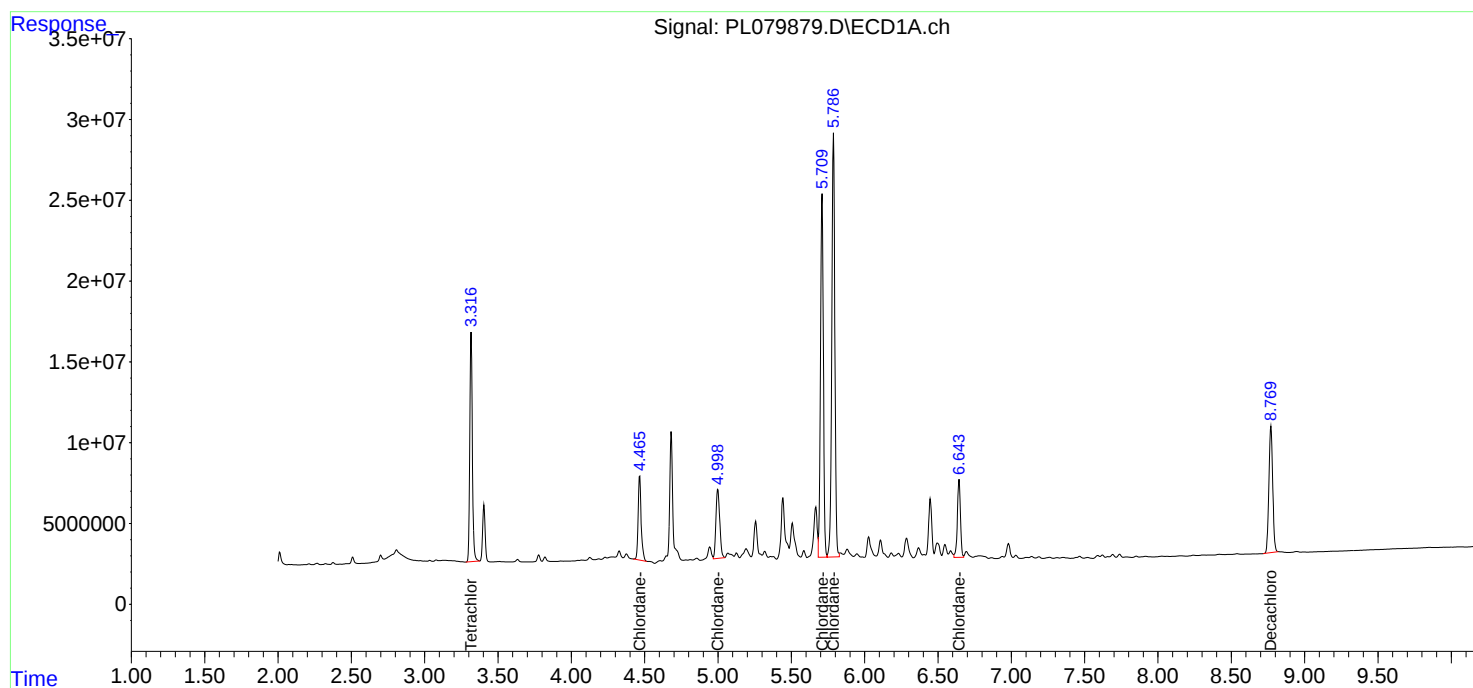


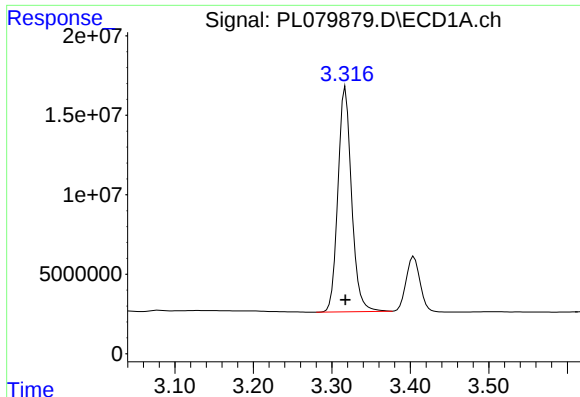

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 171042246
Conc: 72.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

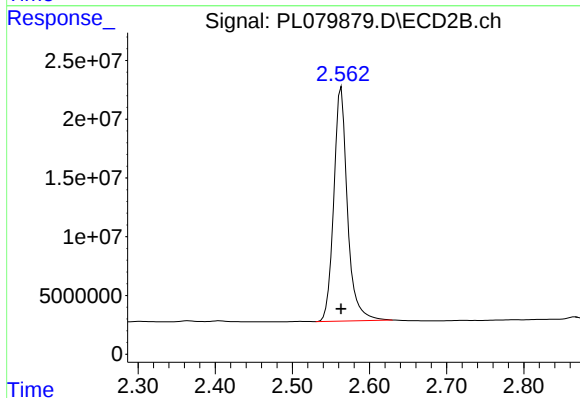


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 245849107
Conc: 71.45 ng/ml

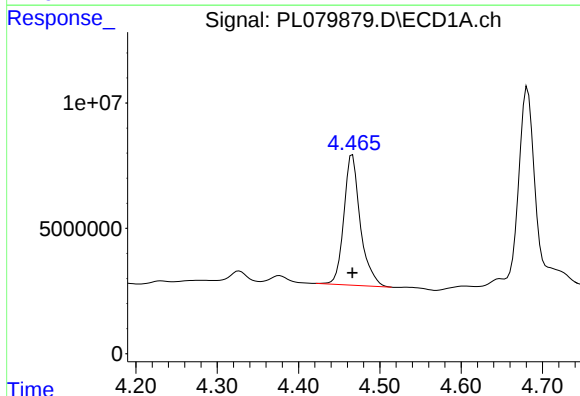


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 72823164
Conc: 721.91 ng/ml

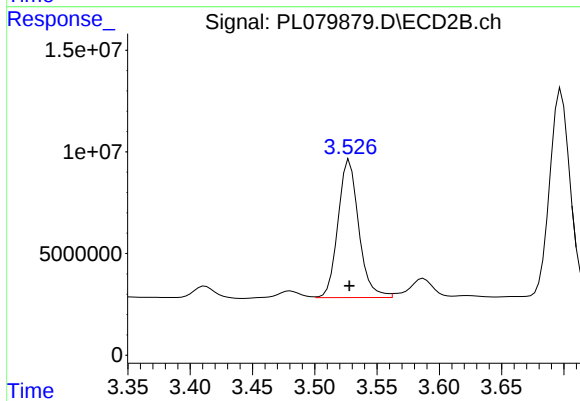

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 78685113
Conc: 702.35 ng/ml

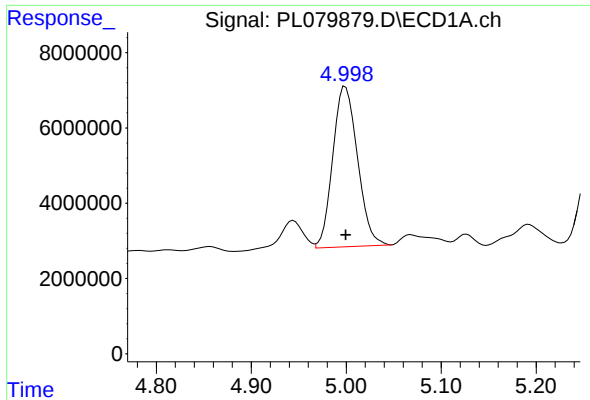

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 77246378
Conc: 705.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

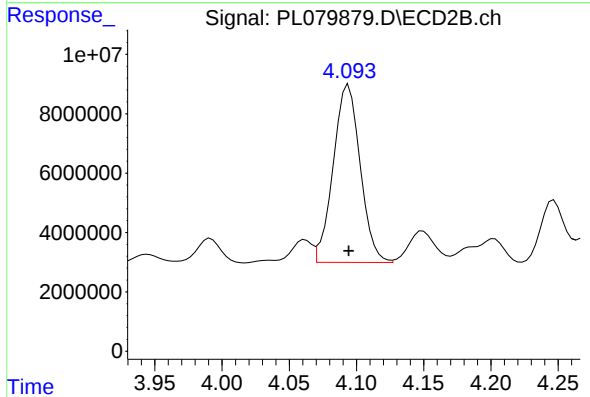


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 83287641
Conc: 698.62 ng/ml

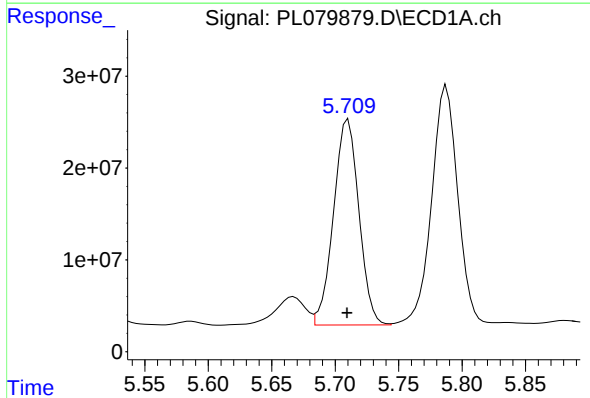


#25 Chlordane-3

R.T.: 5.710 min
Delta R.T.: 0.000 min
Response: 311738453
Conc: 733.06 ng/ml

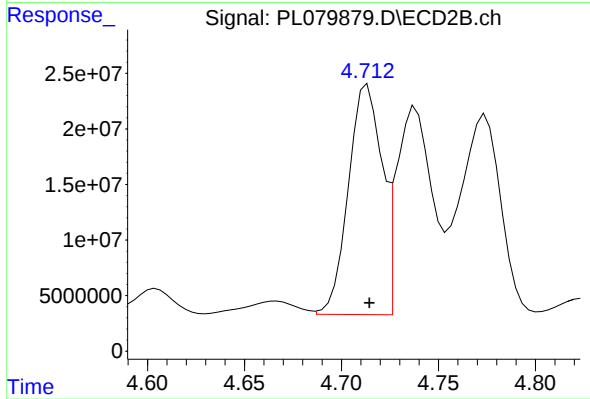

#25 Chlordane-3


R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 247581428
Conc: 714.60 ng/ml

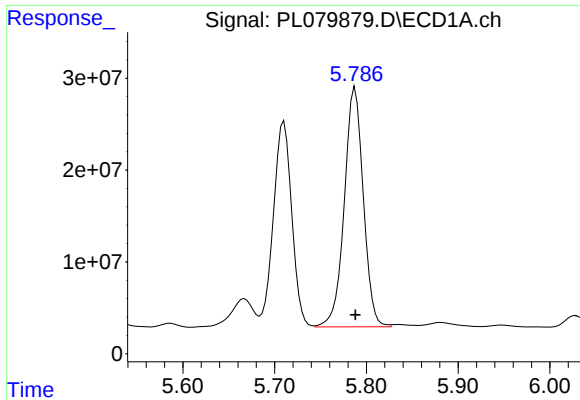

#26 Chlordane-4


R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 374967542
Conc: 726.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

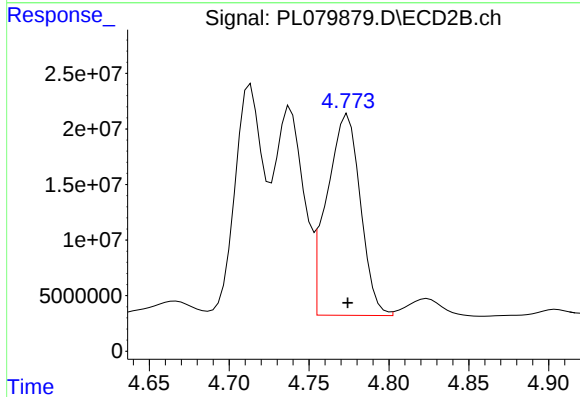


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 263791923
Conc: 705.14 ng/ml

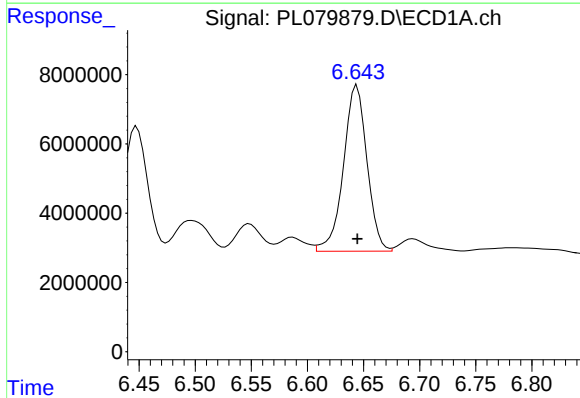


#27 Chlordane-5

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 69896329
Conc: 724.51 ng/ml

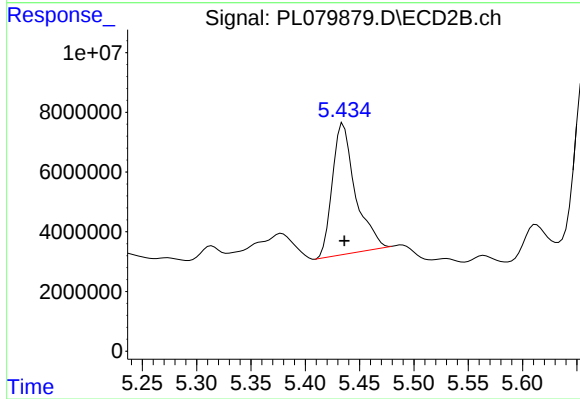

#27 Chlordane-5


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 64605736
Conc: 664.91 ng/ml

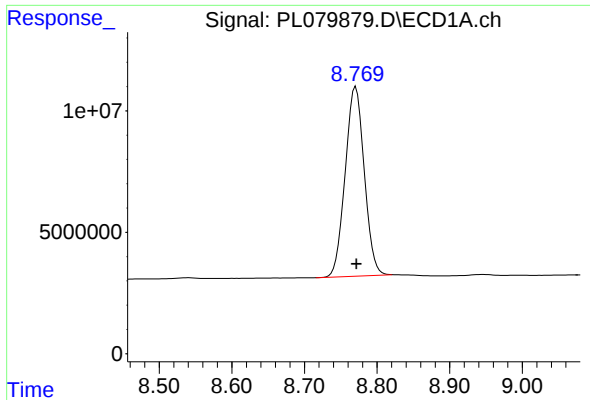

#28 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 142516901
Conc: 71.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

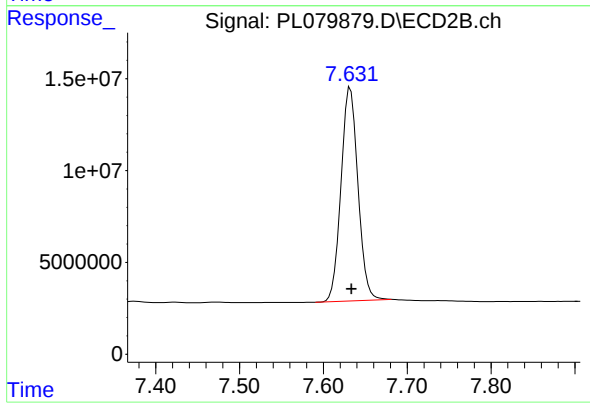

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: -0.001 min
Response: 163505824
Conc: 70.85 ng/ml