

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 17:16
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:15:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.563	10714875	16524771	4.522	4.802
28)	SA Decachlor...	8.772	7.634	10472745	12725439	5.249	5.514
Target Compounds							
23)	Chlordane-1	4.466	3.528	4322233	6729061	42.847	60.064 #
24)	Chlordane-2	4.999	4.094	6080755	6683337	55.501	56.060
25)	Chlordane-3	5.711	4.714	21237057	17302056	49.940	49.940
26)	Chlordane-4	5.788	4.774	25835285	18786164	50.049	50.217
27)	Chlordane-5	6.645	5.436	4739213	4440638	49.124	45.702



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 17:16
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:15:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

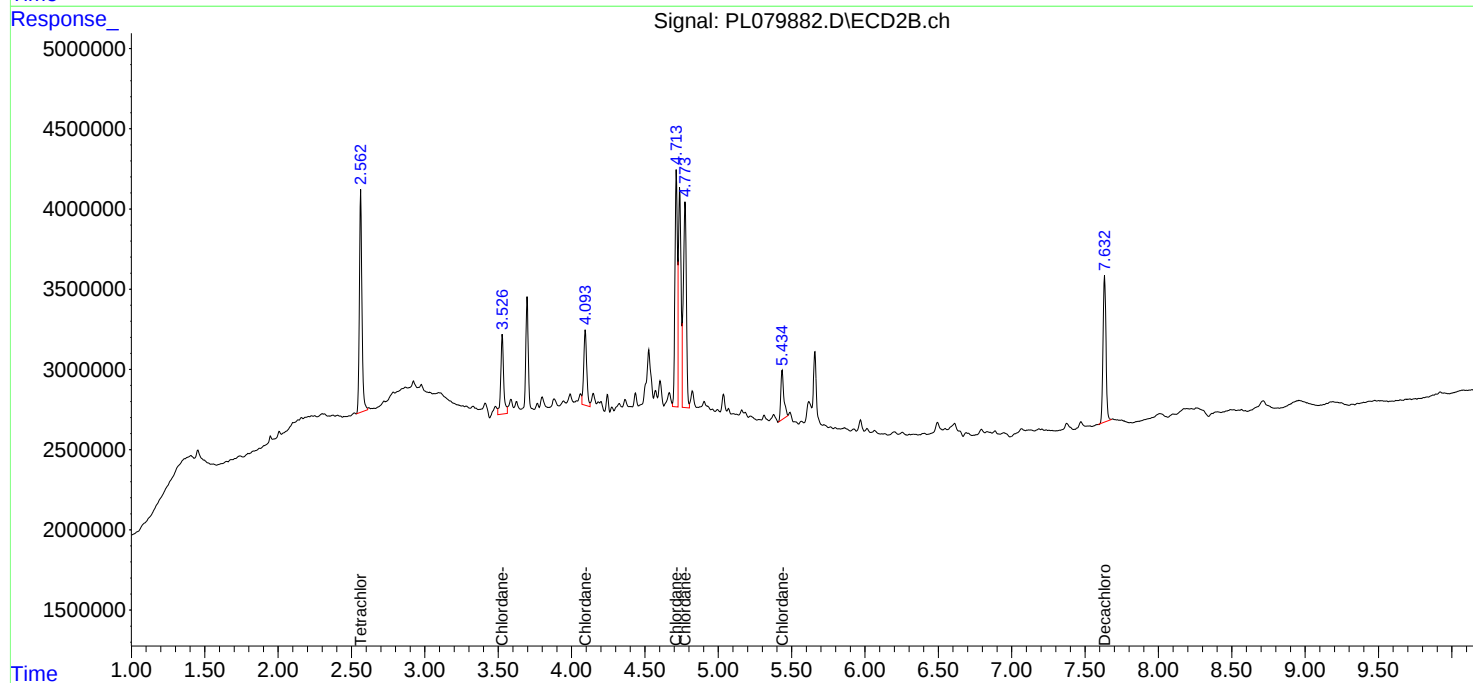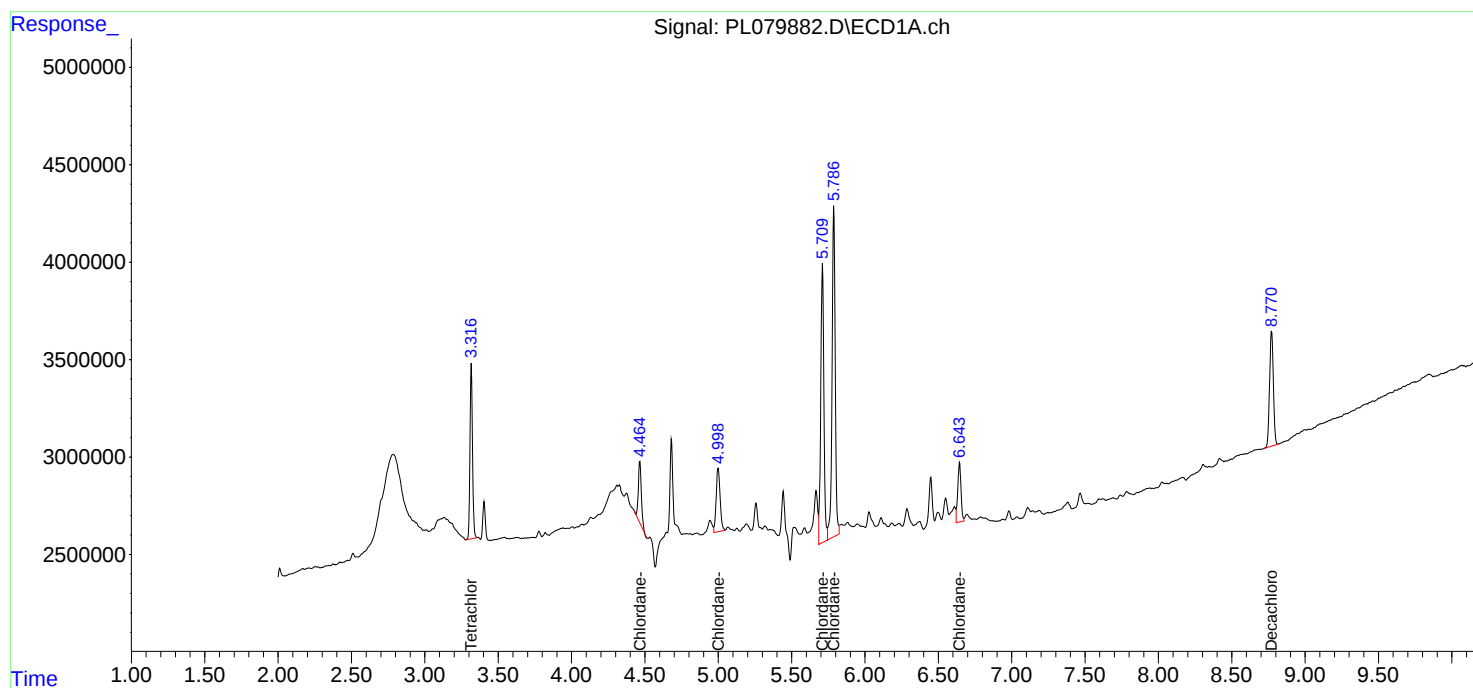


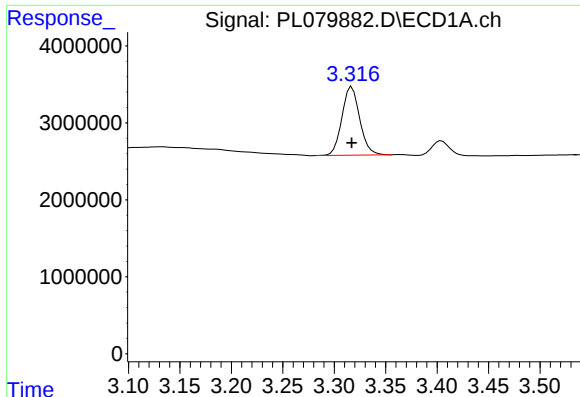

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 10714875
Conc: 4.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

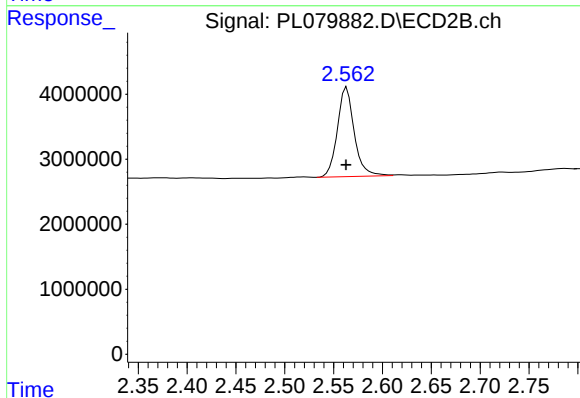


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 16524771
Conc: 4.80 ng/ml

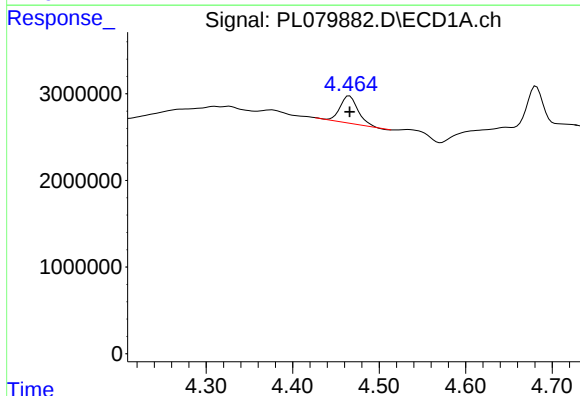


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 4322233
Conc: 42.85 ng/ml

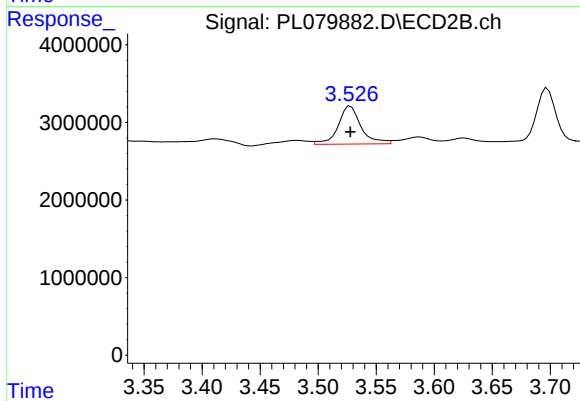

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 6729061
Conc: 60.06 ng/ml

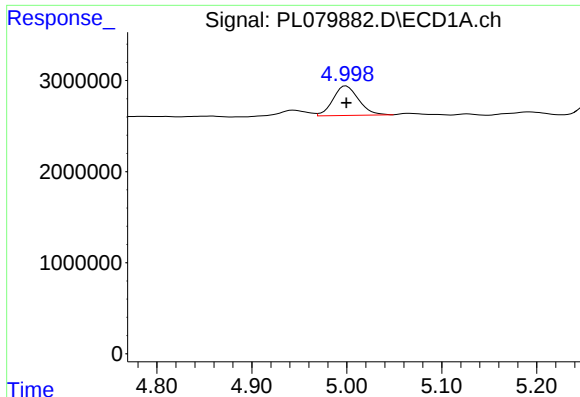

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 6080755
Conc: 55.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

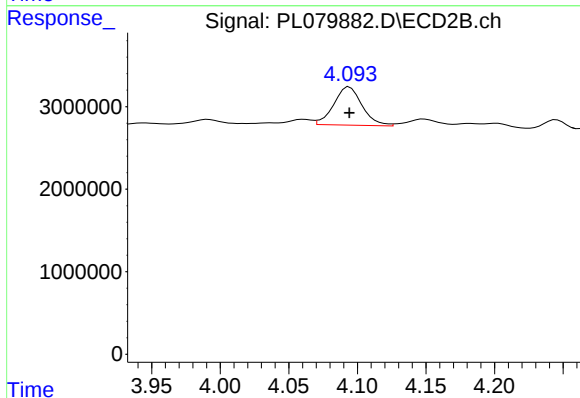


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 6683337
Conc: 56.06 ng/ml

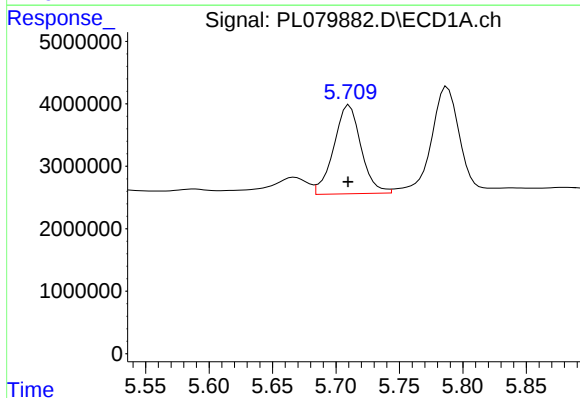


#25 Chlordane-3

R.T.: 5.711 min
Delta R.T.: 0.001 min
Response: 21237057
Conc: 49.94 ng/ml

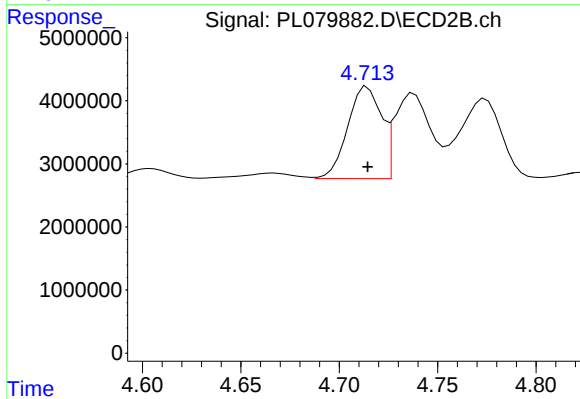

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 17302056
Conc: 49.94 ng/ml

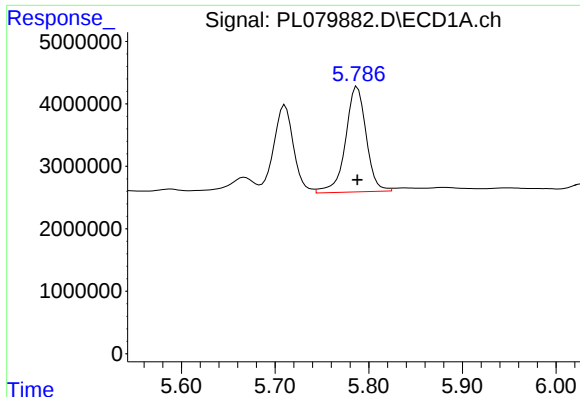

#26 Chlordane-4


R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 25835285
Conc: 50.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

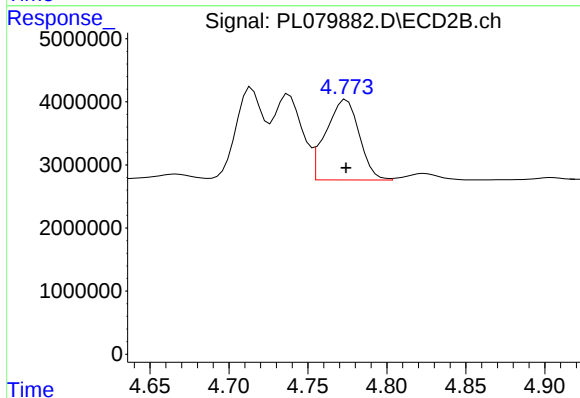


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 18786164
Conc: 50.22 ng/ml

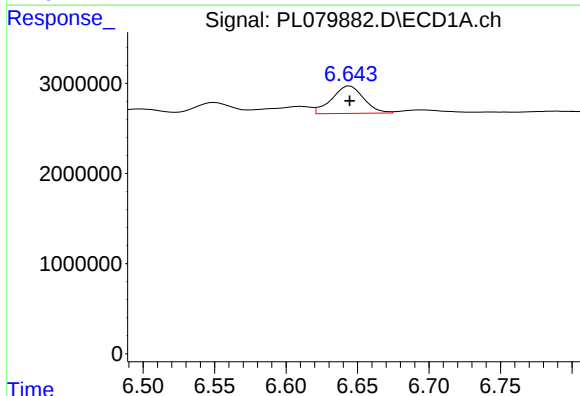


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 4739213
Conc: 49.12 ng/ml

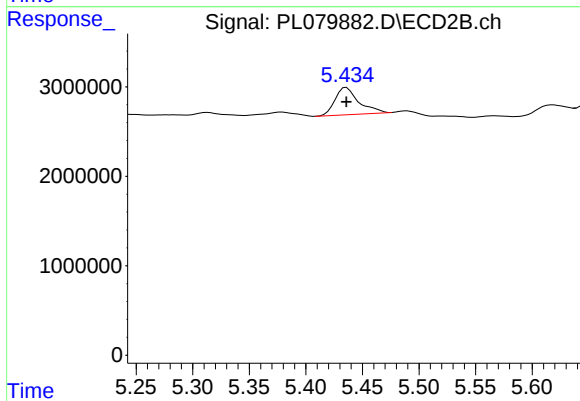

#27 Chlordane-5


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 4440638
Conc: 45.70 ng/ml

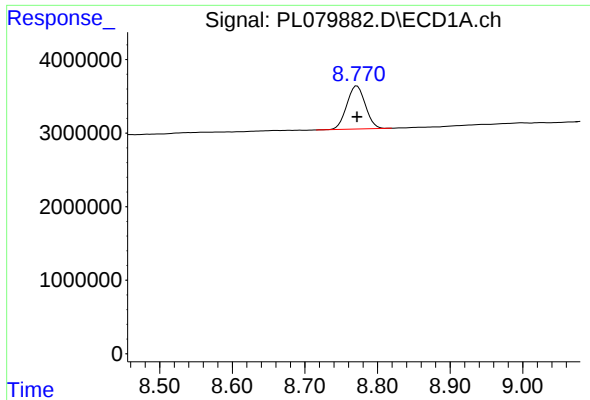

#28 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: 0.000 min
Response: 10472745
Conc: 5.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

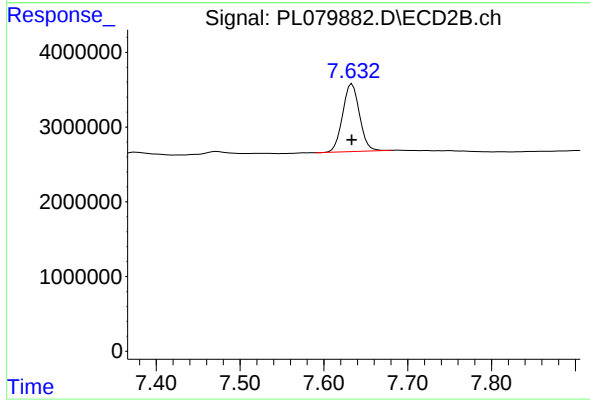

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 12725439
Conc: 5.51 ng/ml