

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 18:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL122322CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:15:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.563	119.6E6	171.4E6	50.494	49.820
28)	SA Decachlor...	8.769	7.632	101.2E6	116.0E6	50.746	50.259
Target Compounds							
23)	Chlordane-1	4.466	3.527	51607690	55795842	511.599	498.041
24)	Chlordane-2	4.999	4.094	55491212	59901206	506.483	502.453
25)	Chlordane-3	5.709	4.714	216.8E6	174.7E6	509.916	504.195
26)	Chlordane-4	5.787	4.774	262.6E6	187.3E6	508.690	500.648
27)	Chlordane-5	6.644	5.435	49057029	48778704	508.501	502.022



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 18:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL122322CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:15:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

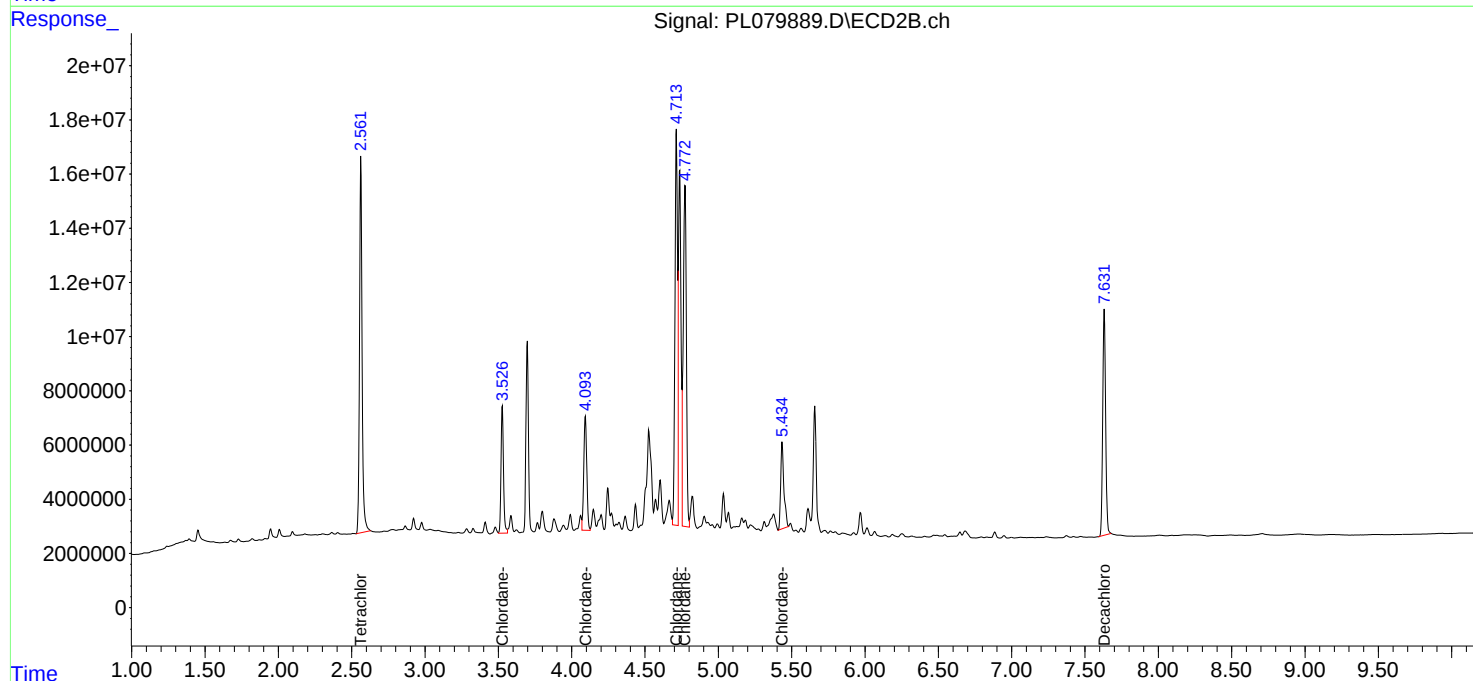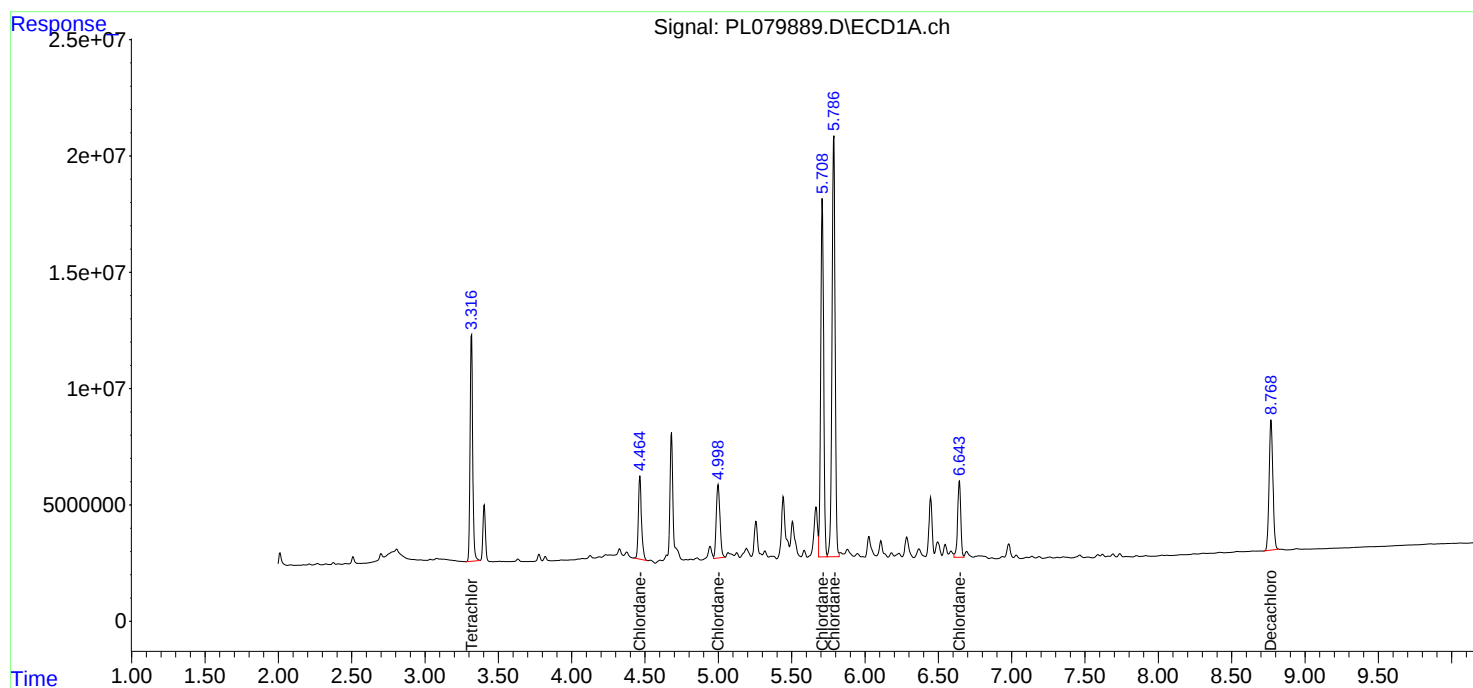


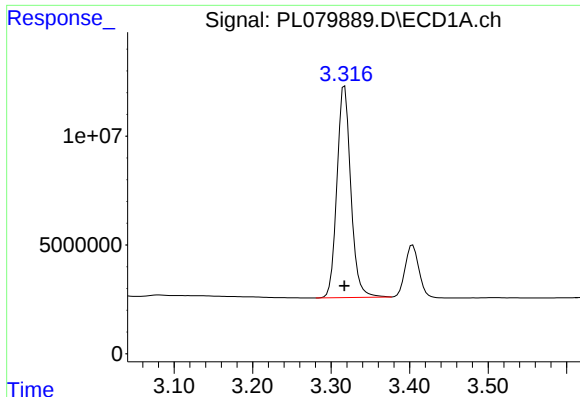

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 119644281
Conc: 50.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122322CHLOR

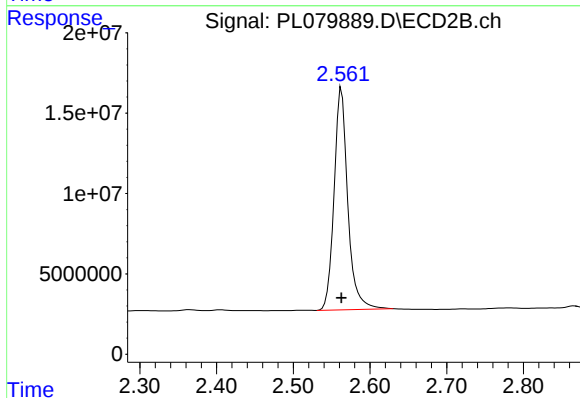


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 171434573
Conc: 49.82 ng/ml

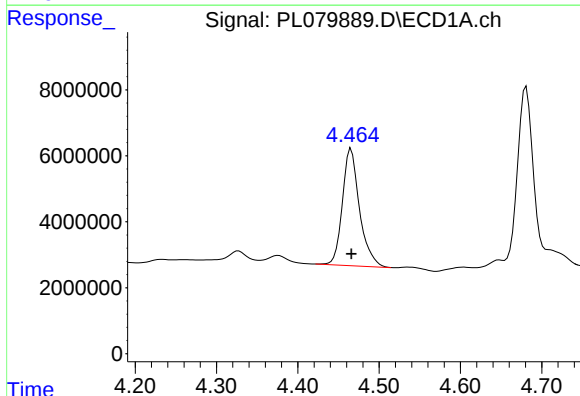


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 51607690
Conc: 511.60 ng/ml

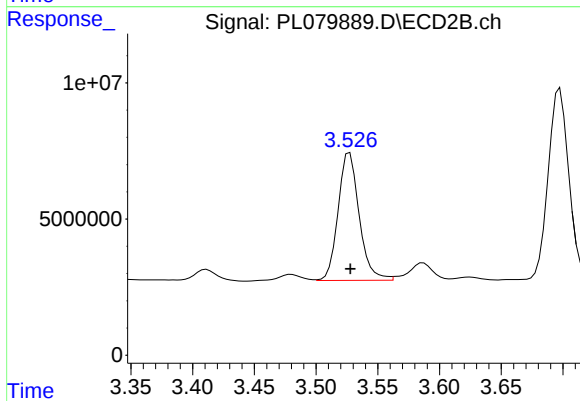

#23 Chlordane-1


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 55795842
Conc: 498.04 ng/ml

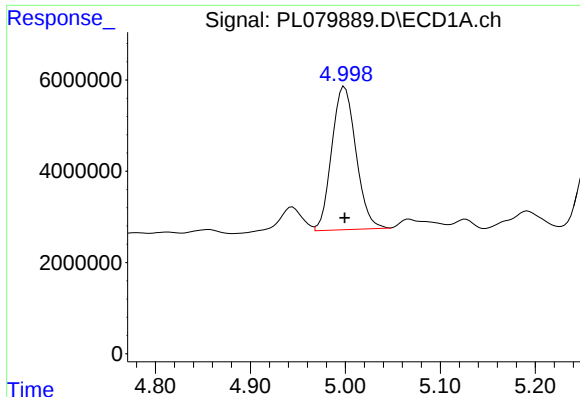

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 55491212
Conc: 506.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122322CHLOR

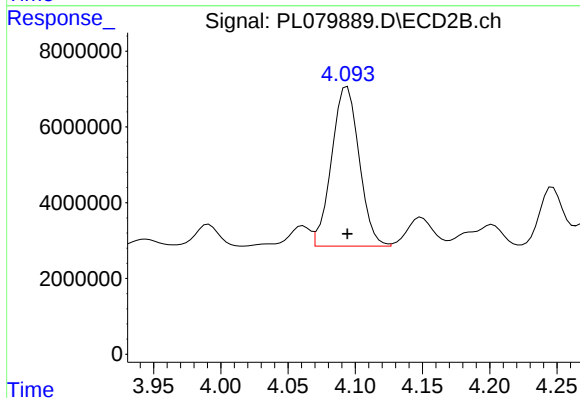


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 59901206
Conc: 502.45 ng/ml

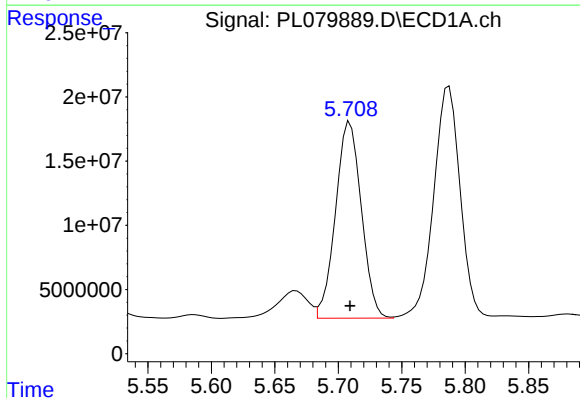


#25 Chlordane-3

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 216844132
Conc: 509.92 ng/ml

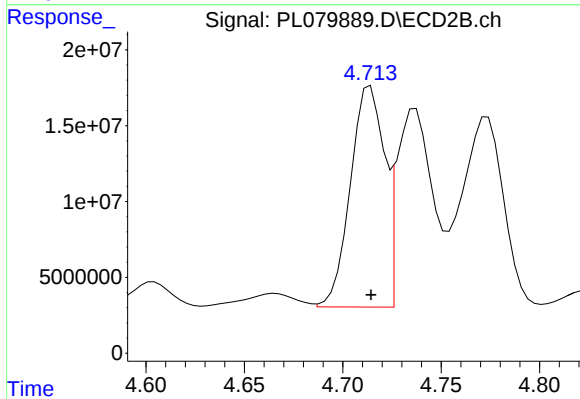

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 174683349
Conc: 504.20 ng/ml

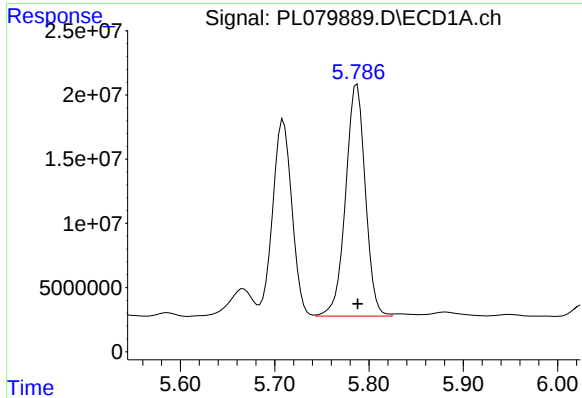

#26 Chlordane-4


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 262587212
Conc: 508.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122322CHLOR

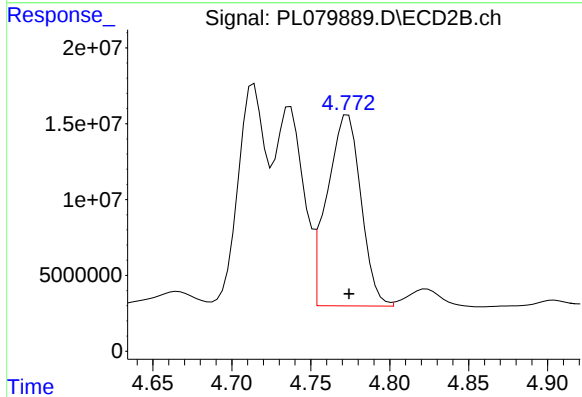


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 187292243
Conc: 500.65 ng/ml

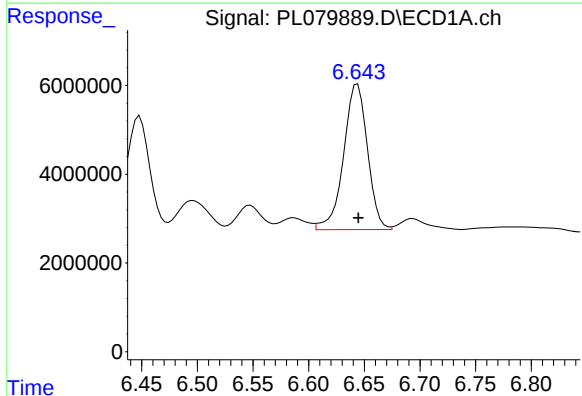


#27 Chlordane-5

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 49057029
Conc: 508.50 ng/ml

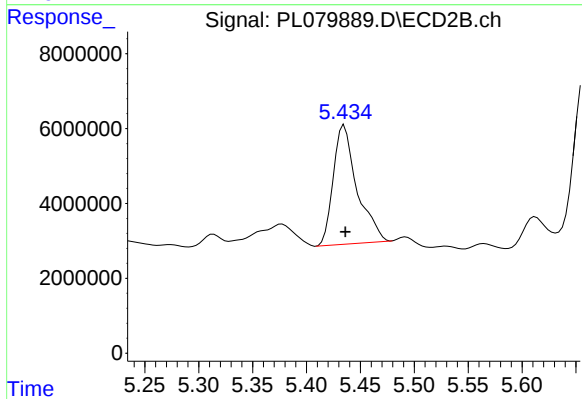

#27 Chlordane-5

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 48778704
Conc: 502.02 ng/ml

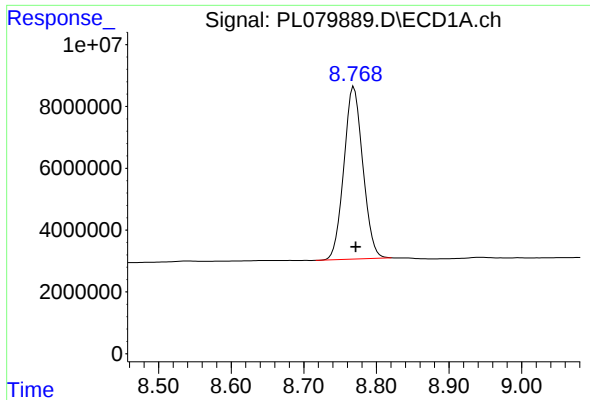

#28 Decachlorobiphenyl


R.T.: 8.769 min

Delta R.T.: -0.002 min

Response: 101249850

Conc: 50.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122322CHLOR

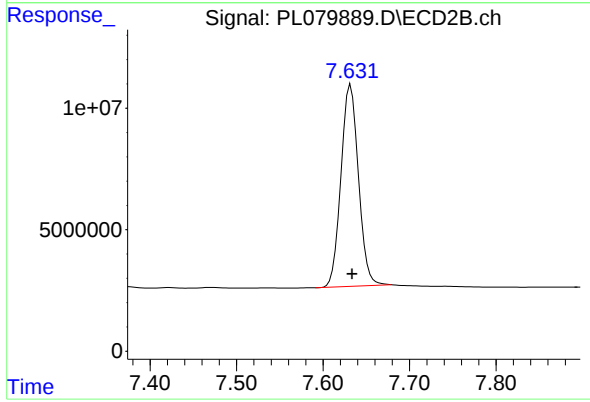

#28 Decachlorobiphenyl

R.T.: 7.632 min

Delta R.T.: -0.001 min

Response: 115979134

Conc: 50.26 ng/ml