

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 16:20
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:17:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:17:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.563	235.2E6	338.9E6	99.638	99.232
28)	SA Decachlor...	8.772	7.632	188.1E6	216.6E6	97.046	96.829
Target Compounds							
23)	Chlordane-1	4.466	3.528	99764591	107.8E6	994.464	980.687
24)	Chlordane-2	5.001	4.095	103.1E6	112.3E6	969.498	969.911
25)	Chlordane-3	5.711	4.714	428.0E6	342.8E6	1003.247	994.690
26)	Chlordane-4	5.789	4.775	512.0E6	365.0E6	995.896	987.659
27)	Chlordane-5	6.645	5.436	94382612	92157201	989.043	973.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 16:20
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:17:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:17:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

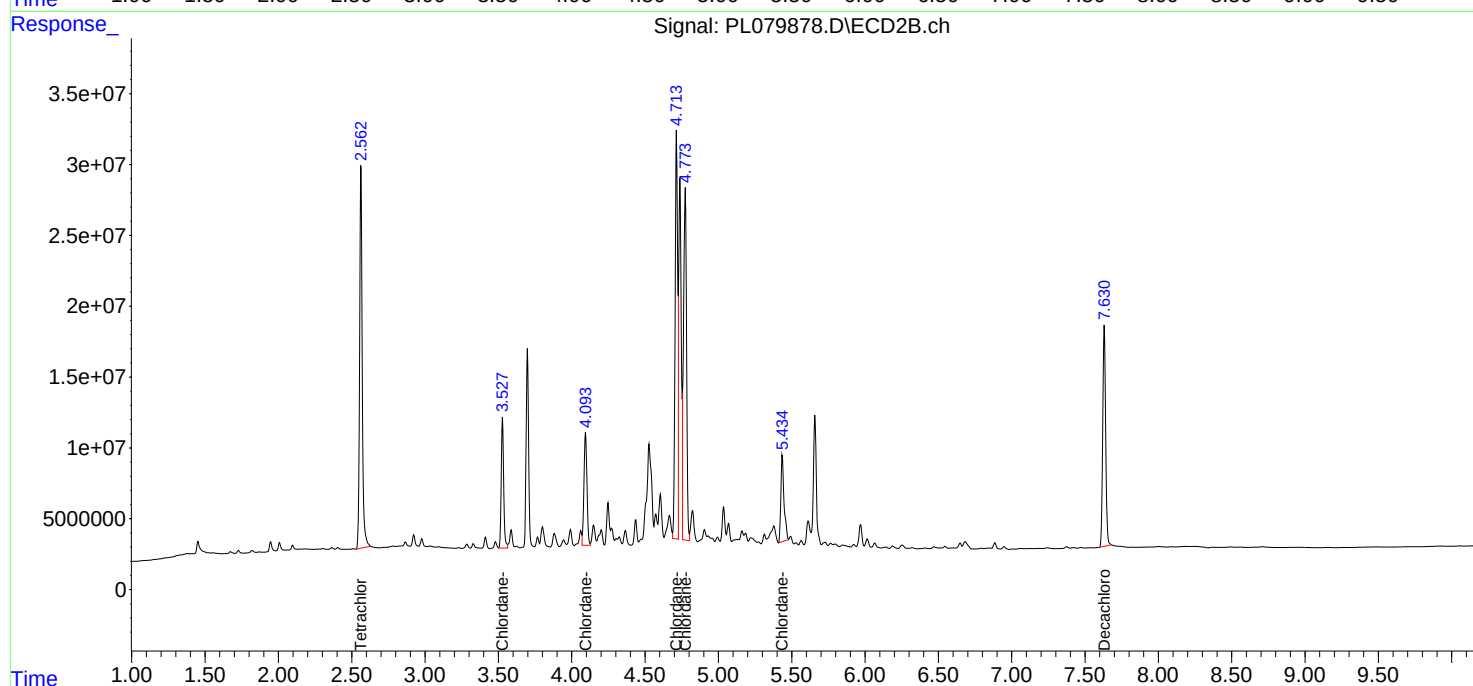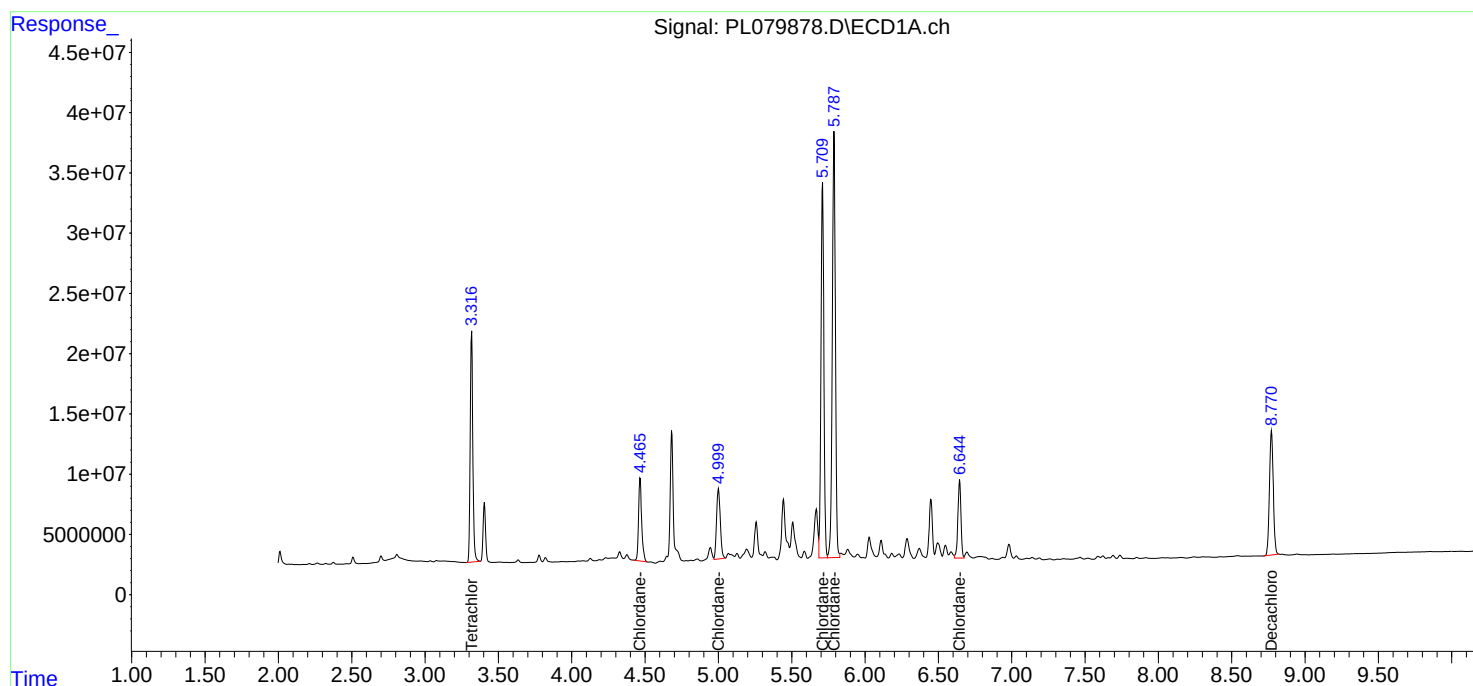


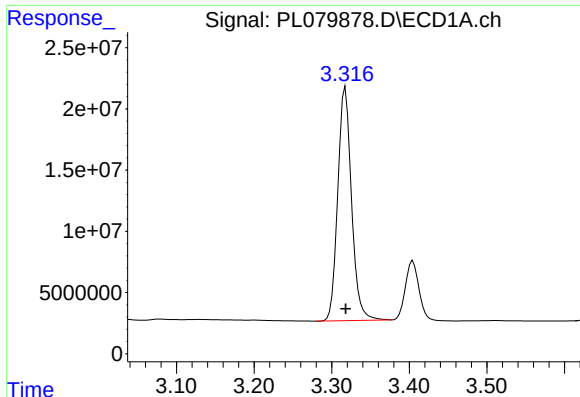

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 235238231
Conc: 99.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

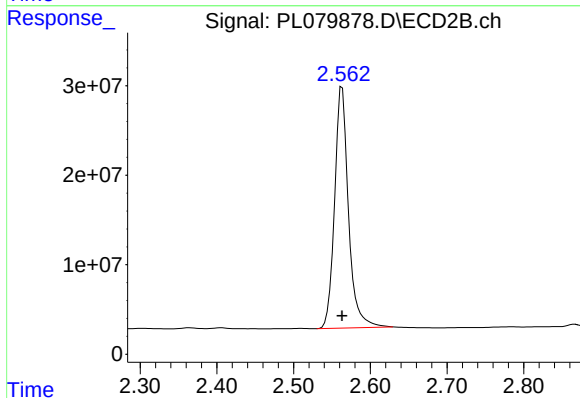


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 338862144
Conc: 99.23 ng/ml

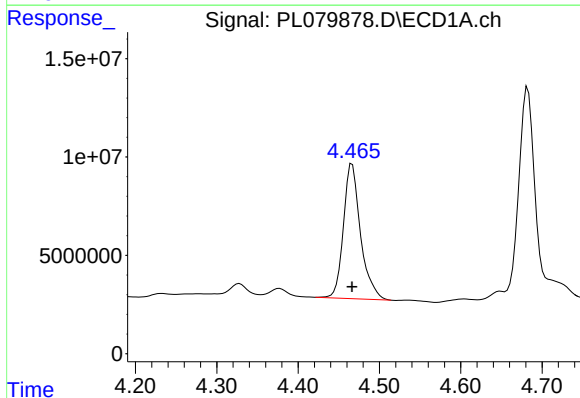


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 99764591
Conc: 994.46 ng/ml

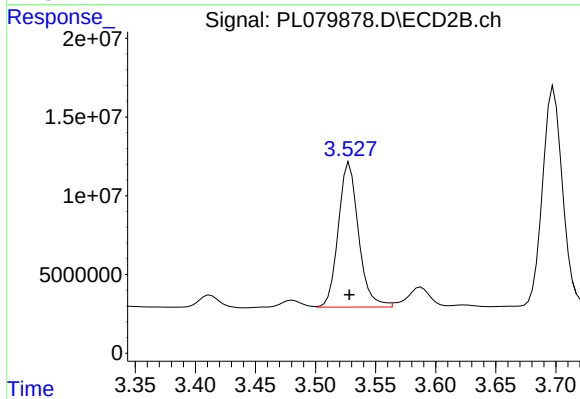

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 107785287
Conc: 980.69 ng/ml

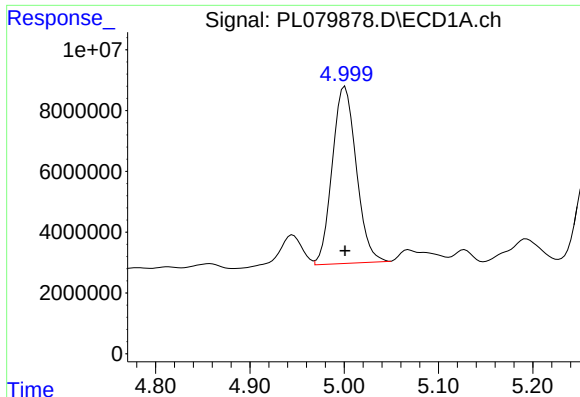

#24 Chlordane-2


R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 103076067
Conc: 969.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

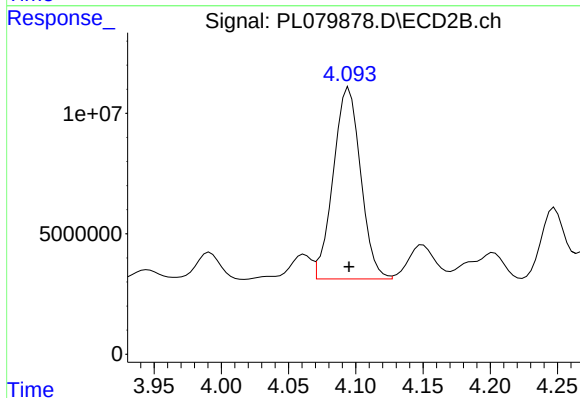


#24 Chlordane-2

R.T.: 4.095 min
Delta R.T.: 0.000 min
Response: 112252967
Conc: 969.91 ng/ml

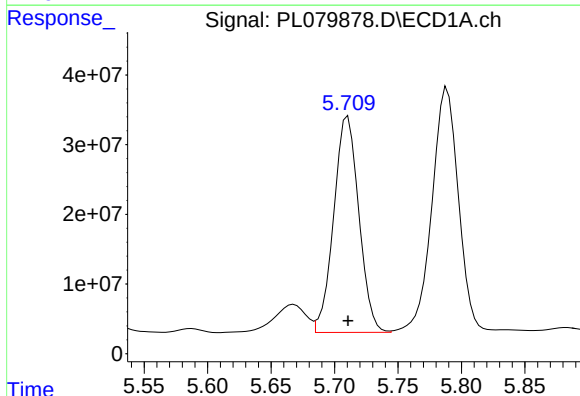


#25 Chlordane-3

R.T.: 5.711 min
Delta R.T.: 0.000 min
Response: 428024942
Conc: 1003.25 ng/ml

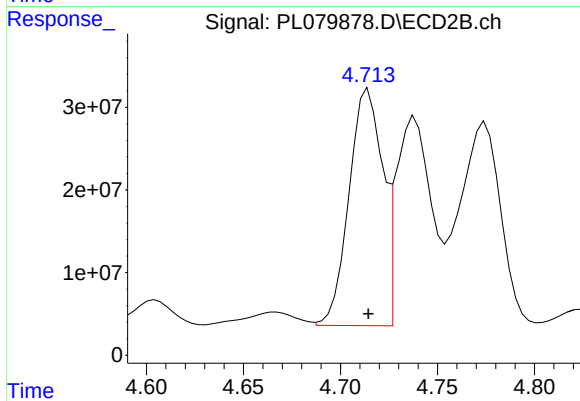

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 342799976
Conc: 994.69 ng/ml

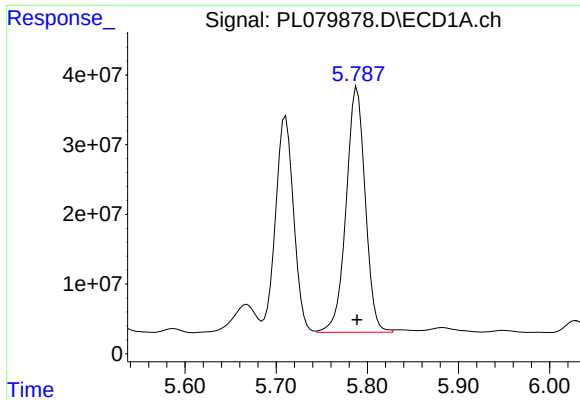

#26 Chlordane-4


R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 511983341
Conc: 995.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

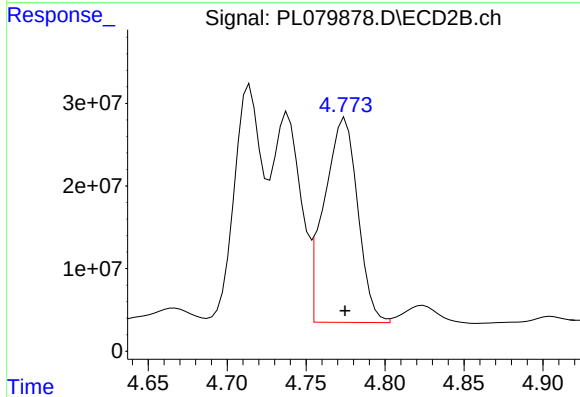


#26 Chlordane-4

R.T.: 4.775 min
Delta R.T.: 0.000 min
Response: 364978762
Conc: 987.66 ng/ml

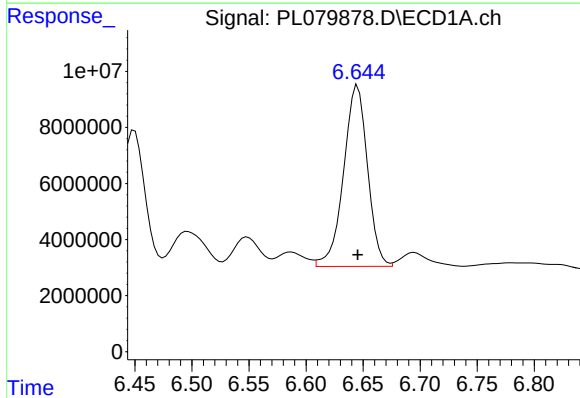


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 94382612
Conc: 989.04 ng/ml

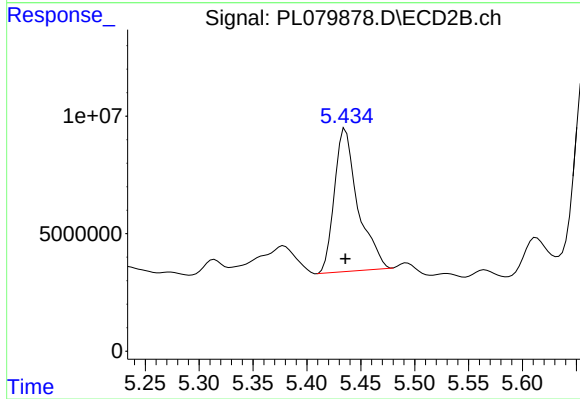

#27 Chlordane-5


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 92157201
Conc: 973.55 ng/ml

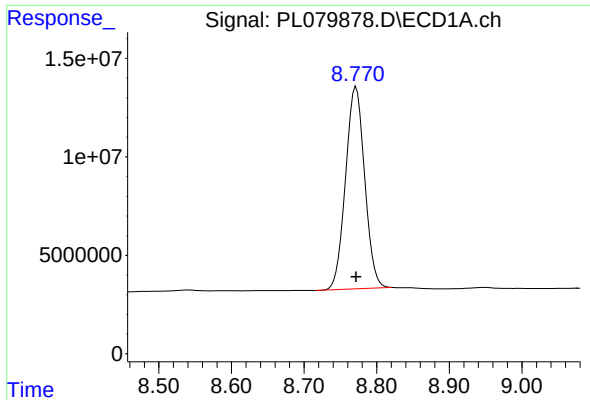

#28 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: 0.000 min
Response: 188072639
Conc: 97.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

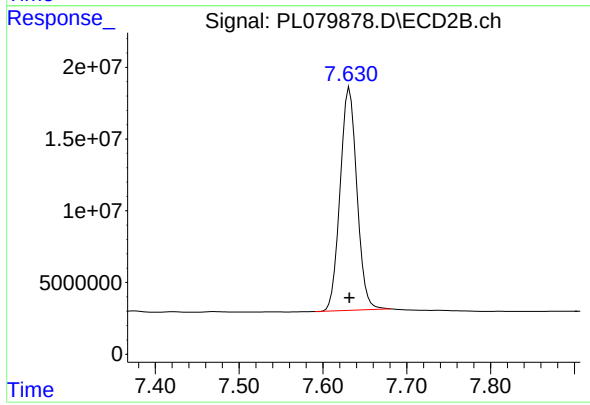

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: 0.000 min
Response: 216576424
Conc: 96.83 ng/ml