

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 16:48
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:14:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.563	118.5E6	172.1E6	50.000	50.000
28)	SA Decachlor...	8.772	7.633	99761143	115.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.466	3.528	50437627	56015350	500.000	500.000
24)	Chlordane-2	4.999	4.094	54780925	59608797	500.000	500.000
25)	Chlordane-3	5.709	4.714	212.6E6	173.2E6	500.000	500.000
26)	Chlordane-4	5.788	4.774	258.1E6	187.0E6	500.000	500.000
27)	Chlordane-5	6.645	5.436	48236950	48582228	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 16:48
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:14:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

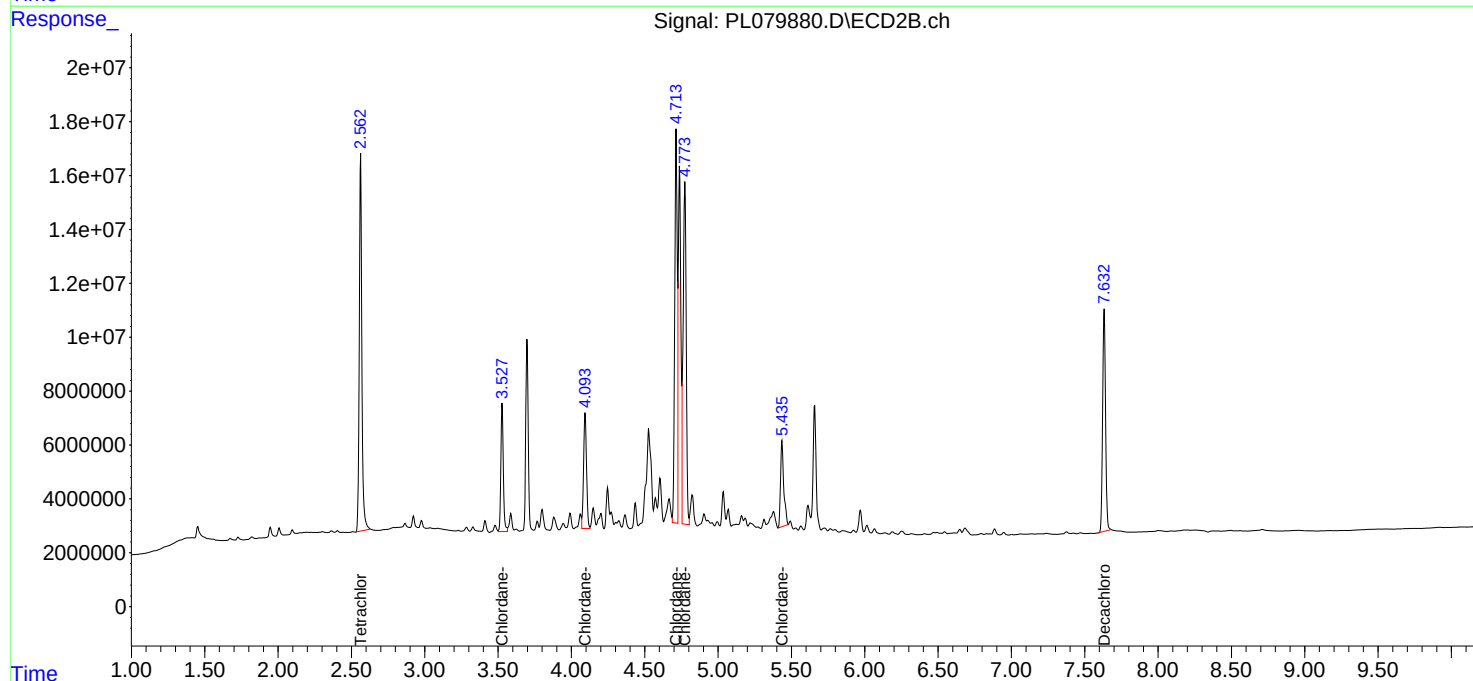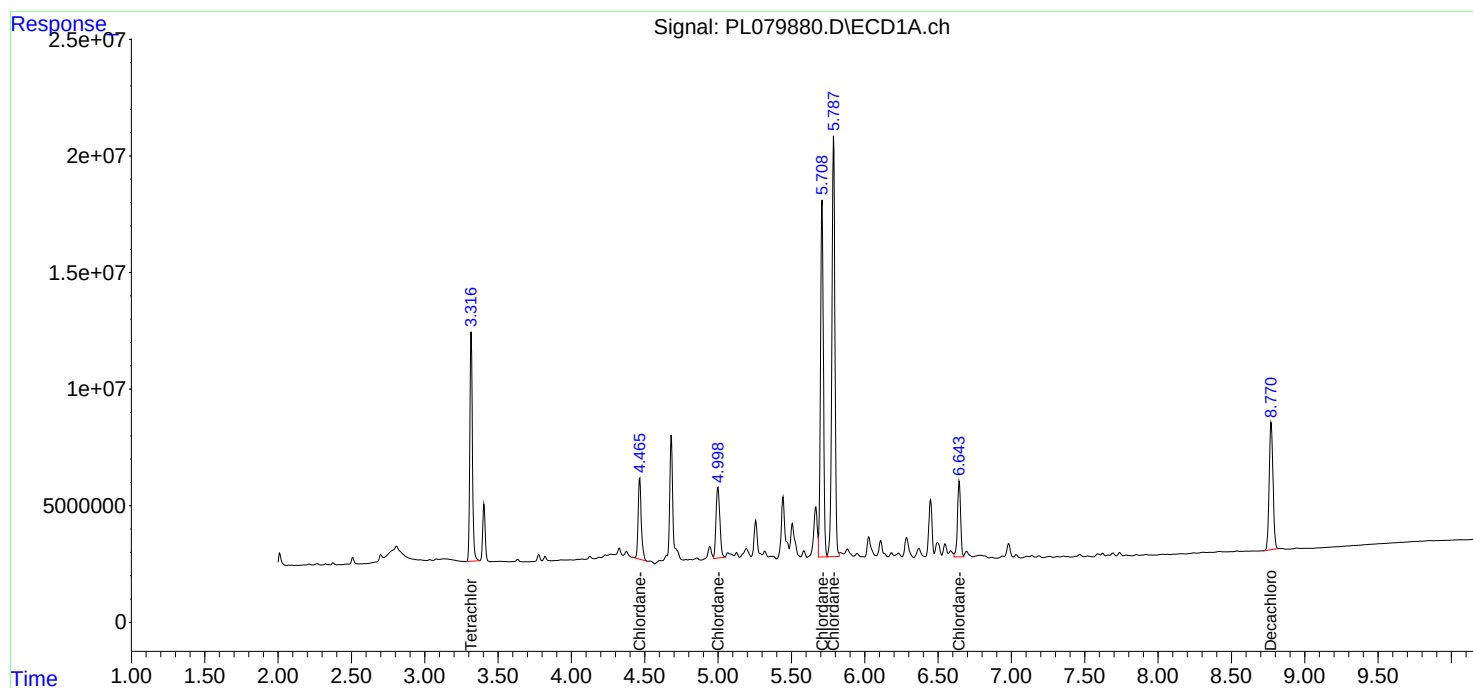


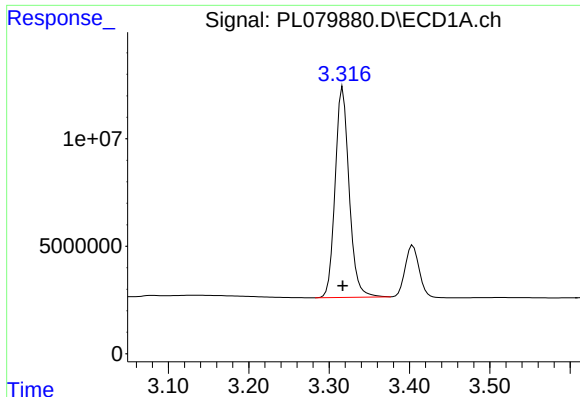

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 118473518
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

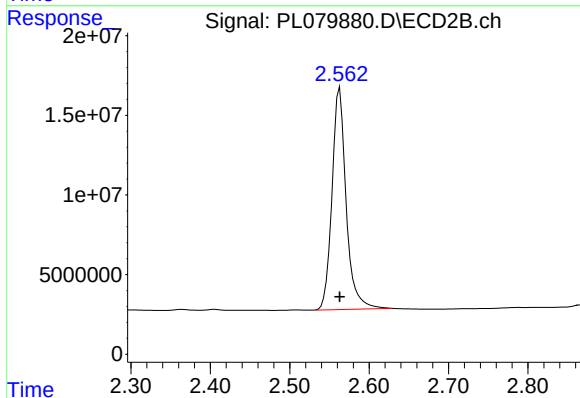


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 172053596
Conc: 50.00 ng/ml

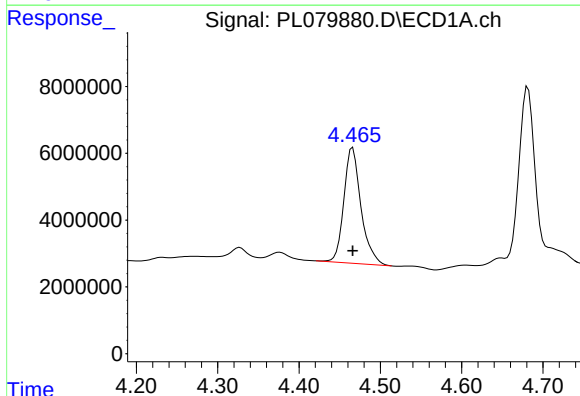


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 50437627
Conc: 500.00 ng/ml

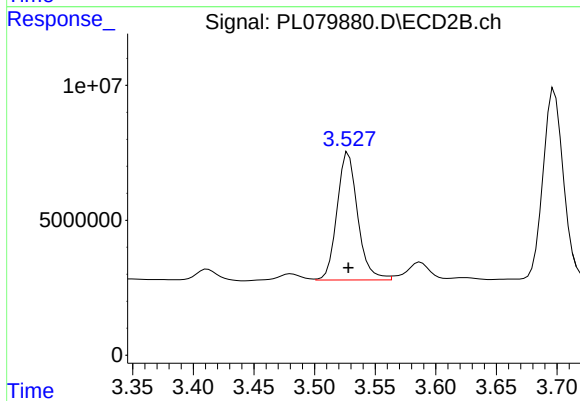

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 56015350
Conc: 500.00 ng/ml

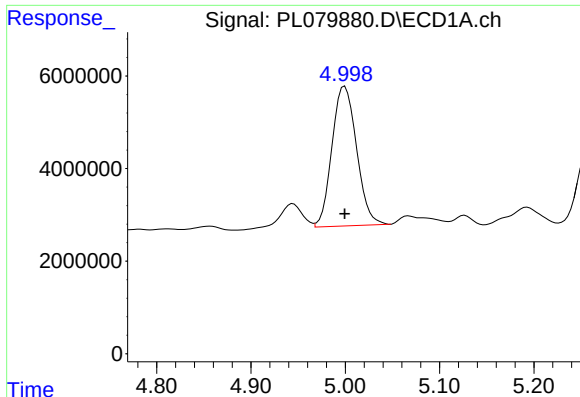

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 54780925
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

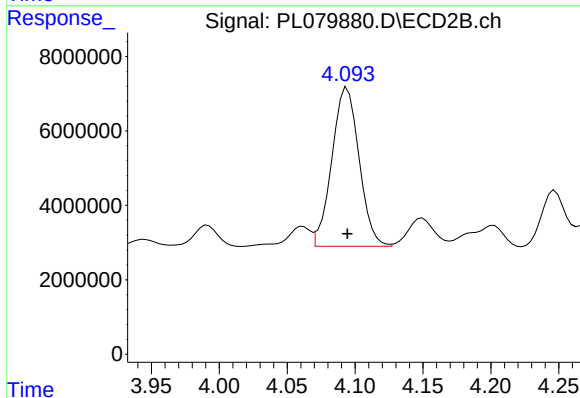


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 59608797
Conc: 500.00 ng/ml

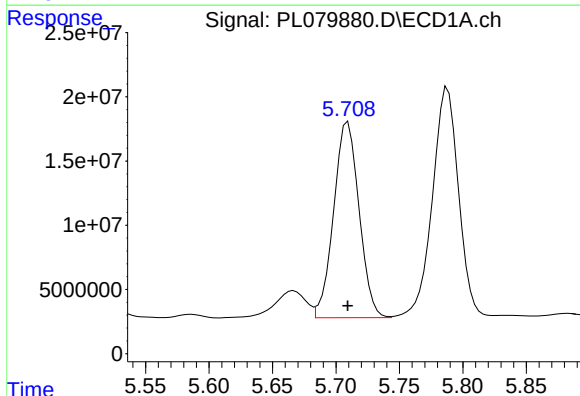


#25 Chlordane-3

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 212627184
Conc: 500.00 ng/ml

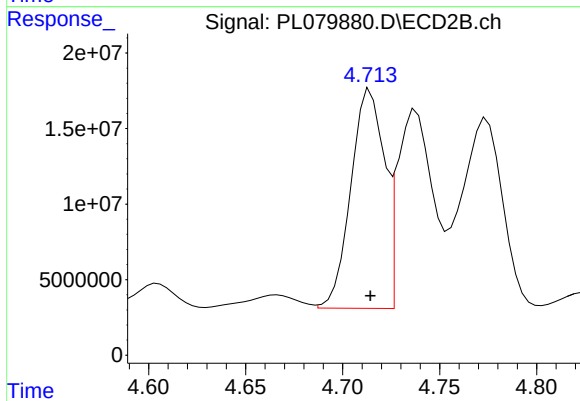

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 173229817
Conc: 500.00 ng/ml

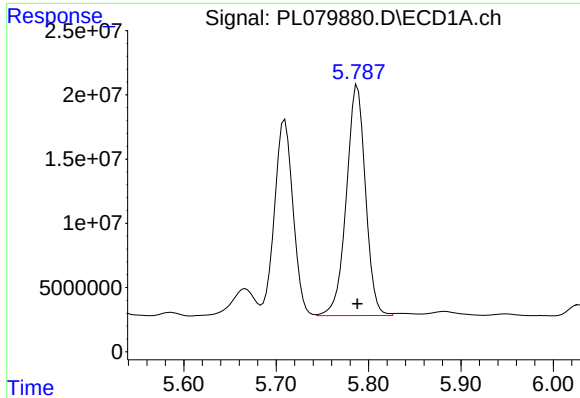

#26 Chlordane-4


R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 258101537
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

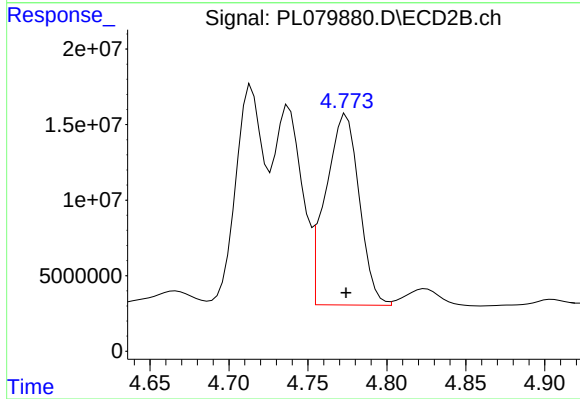


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 187049879
Conc: 500.00 ng/ml

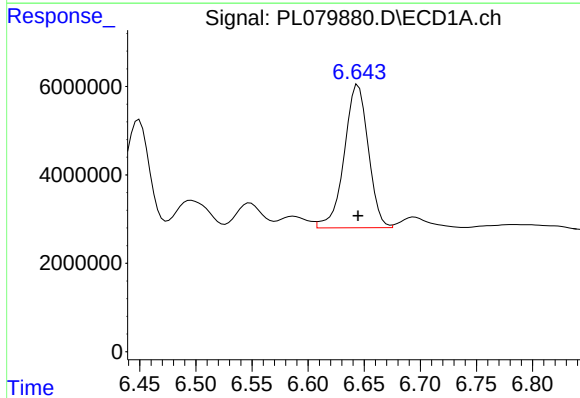


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 48236950
Conc: 500.00 ng/ml

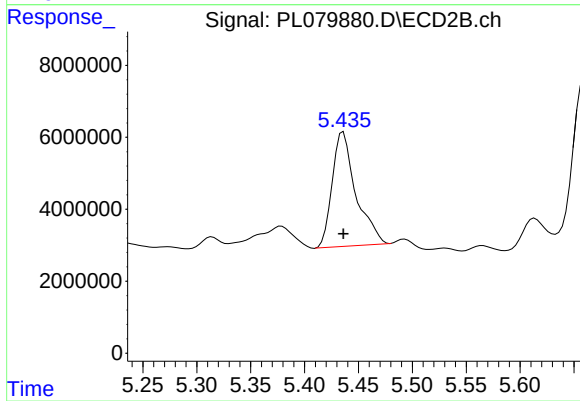

#27 Chlordane-5


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 48582228
Conc: 500.00 ng/ml

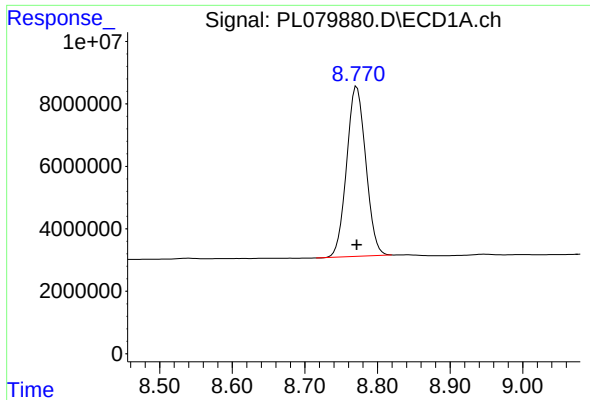

#28 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: 0.000 min
Response: 99761143
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

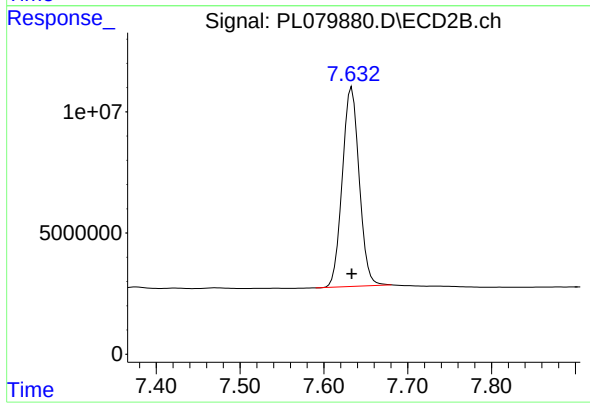

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: 0.000 min
Response: 115381777
Conc: 50.00 ng/ml