

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
 Data File : PL079881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 17:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 05:49:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 05:49:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.563	56805812	83725712	24.499	24.887
28)	SA Decachlor...	8.770	7.631	50113460	58924435	25.763	26.158
Target Compounds							
23)	Chlordane-1	4.466	3.527	23947563	27895620	243.414	255.740
24)	Chlordane-2	4.999	4.094	27694733	30485984	259.793	262.547
25)	Chlordane-3	5.709	4.714	99829296	85477821	239.363	251.169
26)	Chlordane-4	5.787	4.774	123.1E6	91502055	243.667	251.240
27)	Chlordane-5	6.644	5.435	23481524	23970205	248.496	258.200



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122322\
Data File : PL079881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 17:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 05:49:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122322.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 05:49:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

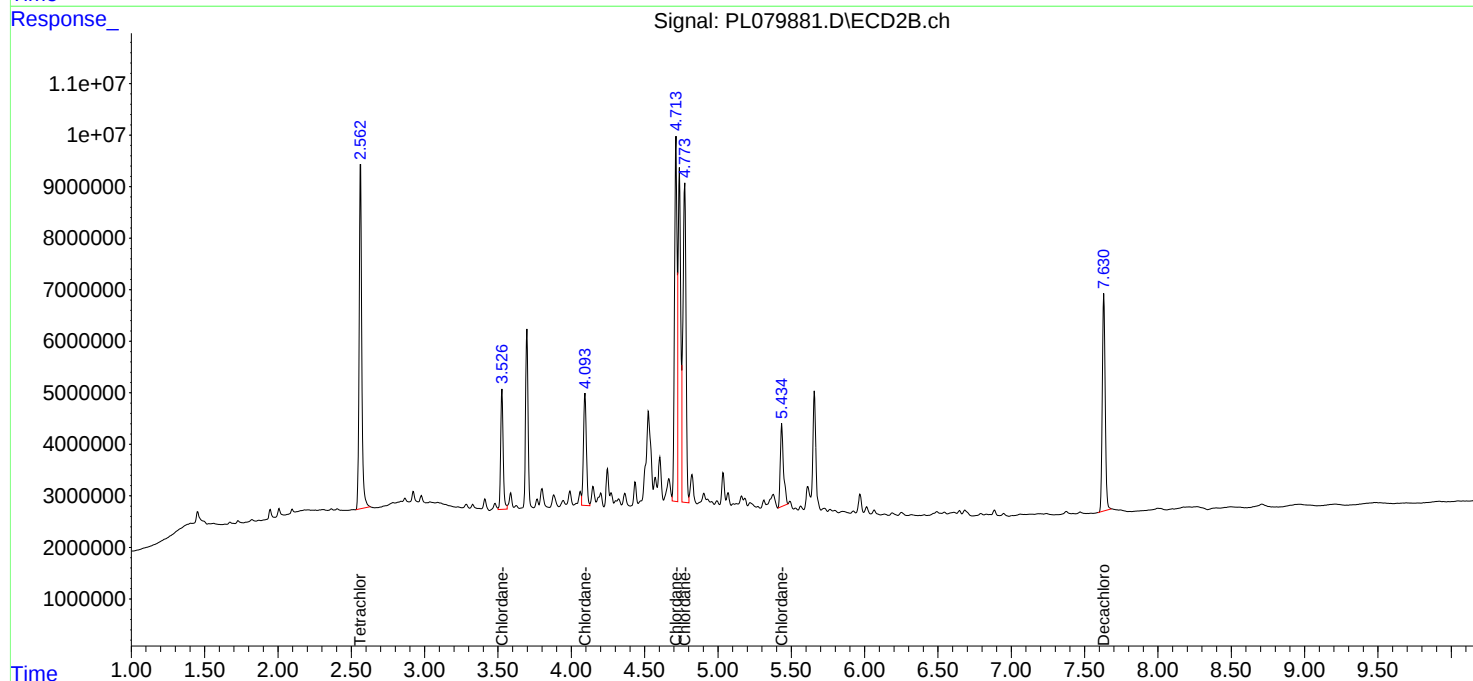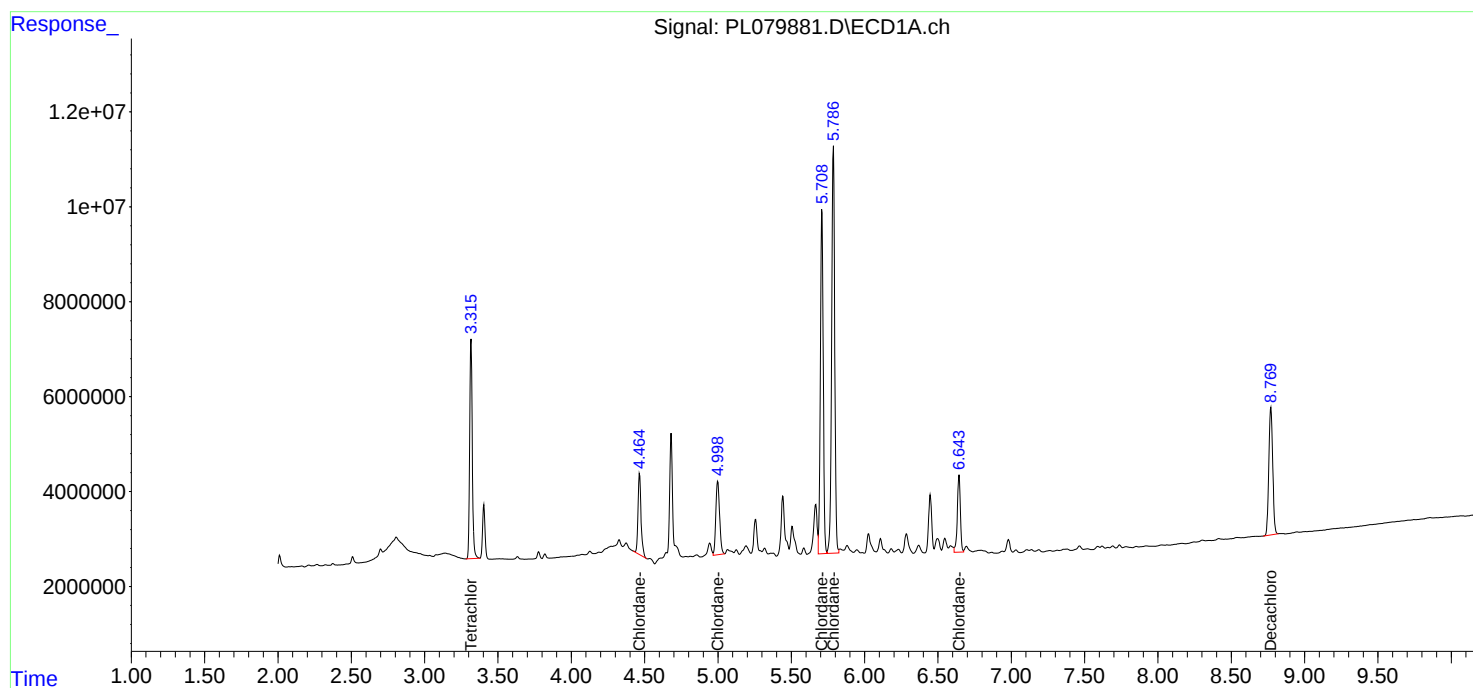


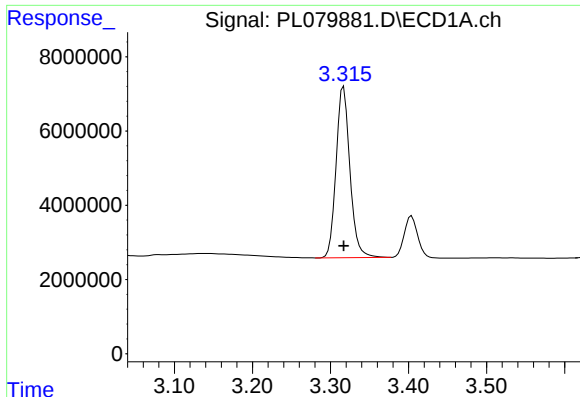

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 56805812
Conc: 24.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

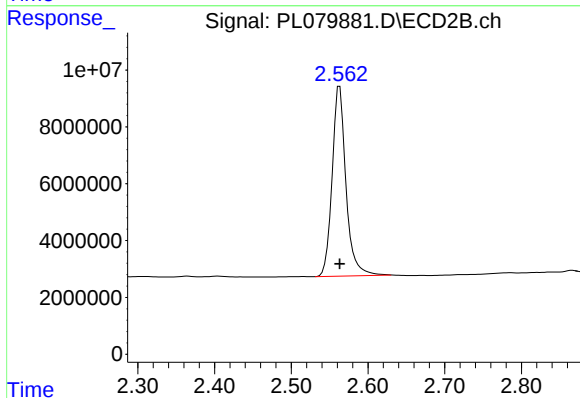


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 83725712
Conc: 24.89 ng/ml

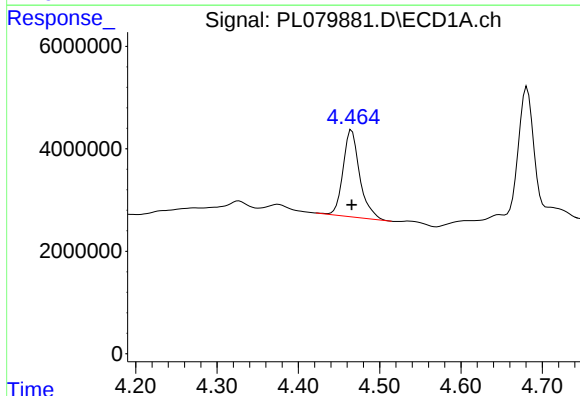


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 23947563
Conc: 243.41 ng/ml

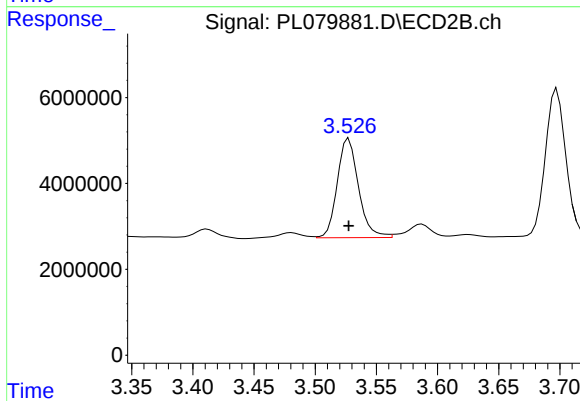

#23 Chlordane-1


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 27895620
Conc: 255.74 ng/ml

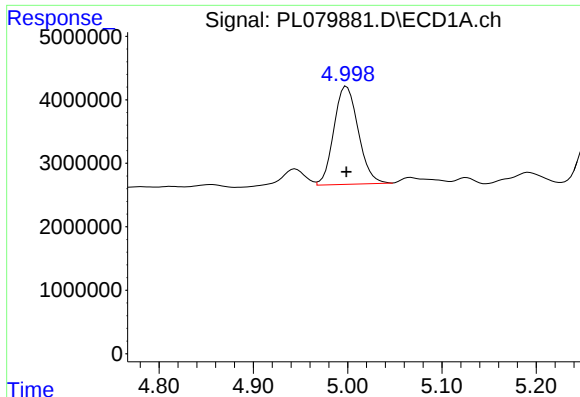

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 27694733
Conc: 259.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

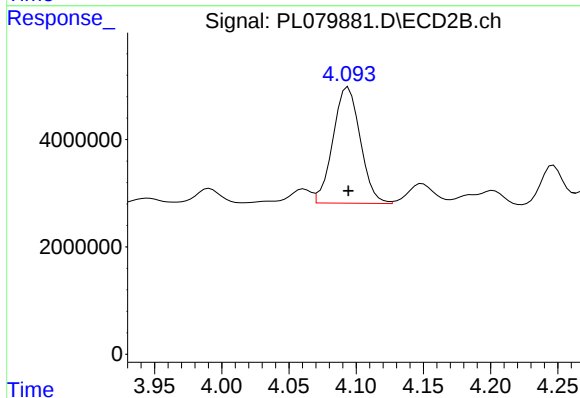


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 30485984
Conc: 262.55 ng/ml

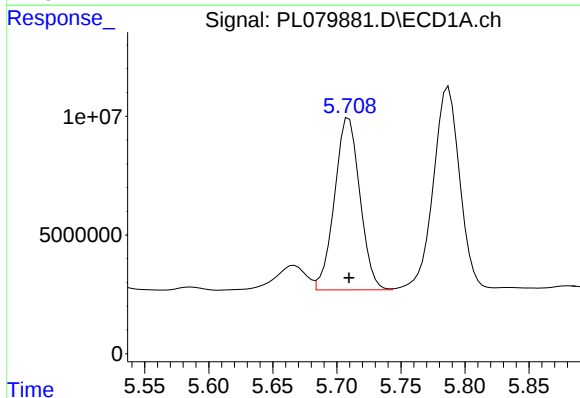


#25 Chlordane-3

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 99829296
Conc: 239.36 ng/ml

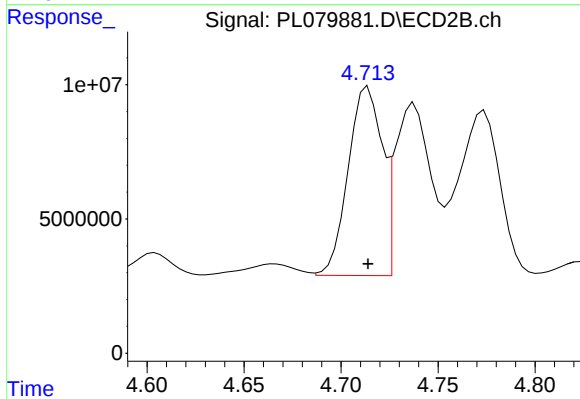

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 85477821
Conc: 251.17 ng/ml

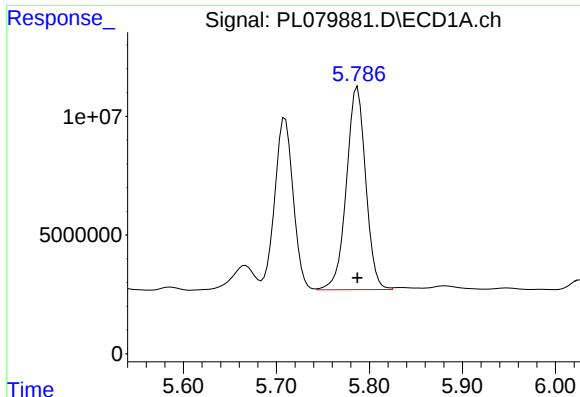

#26 Chlordane-4


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 123080023
Conc: 243.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

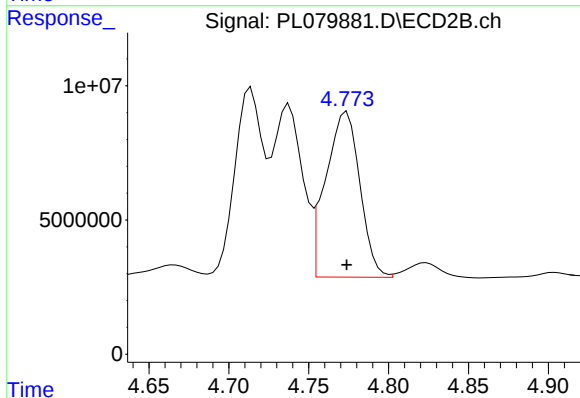


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 91502055
Conc: 251.24 ng/ml

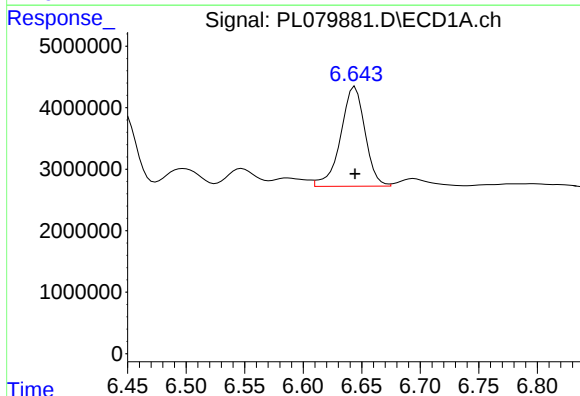


#27 Chlordane-5

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 23481524
Conc: 248.50 ng/ml

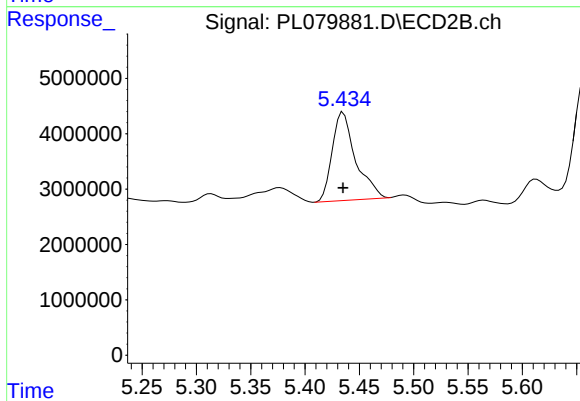

#27 Chlordane-5


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 23970205
Conc: 258.20 ng/ml

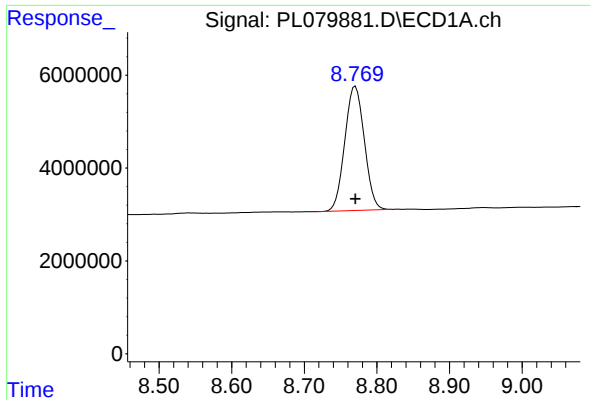

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: 0.000 min
Response: 50113460
Conc: 25.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

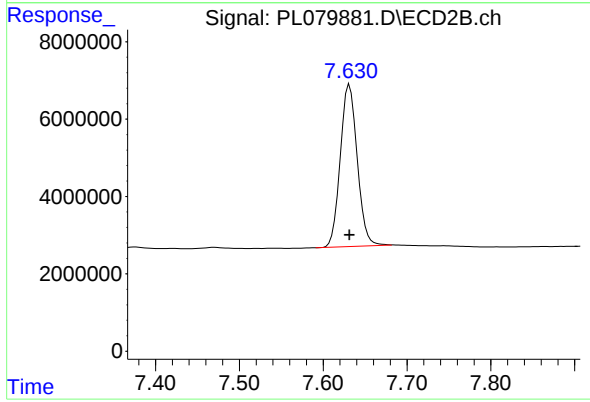

#28 Decachlorobiphenyl

R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 58924435
Conc: 26.16 ng/ml