

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
 Data File : PL093489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 14:23
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 15:22:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:21:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.776	227.5E6	354.9E6	97.716	102.603
28)	SA Decachlor...	9.055	7.912	163.0E6	291.9E6	92.809	98.435
Target Compounds							
23)	Chlordane-1	4.703	3.774	102.0E6	121.6E6	971.548	1030.274
24)	Chlordane-2	5.232	4.351	98976001	135.6E6	945.399	999.846
25)	Chlordane-3	5.942	4.980	353.9E6	435.0E6	990.724	1045.660
26)	Chlordane-4	6.024	5.043	423.1E6	416.0E6	986.171	1021.200
27)	Chlordane-5	6.873	5.938	78915832	136.9E6	952.793	1034.057



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
Data File : PL093489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 14:23
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 15:22:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:21:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

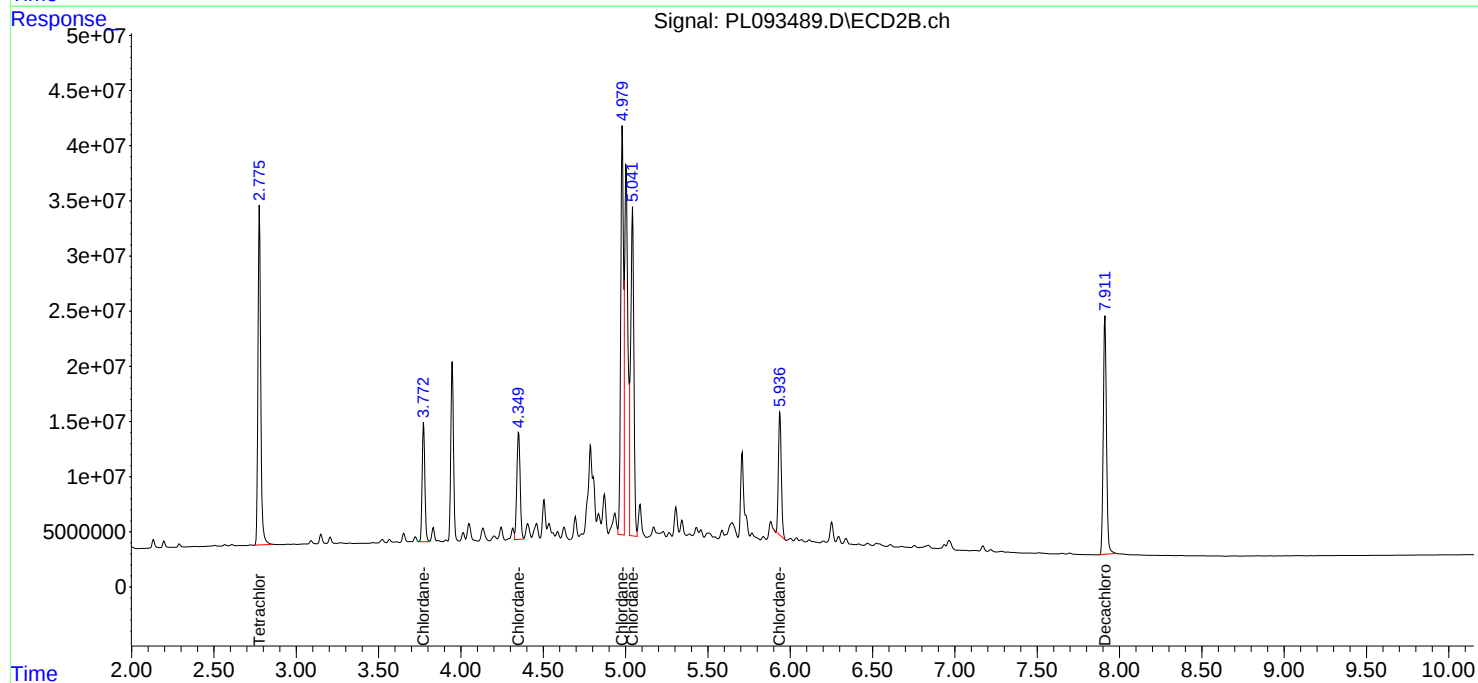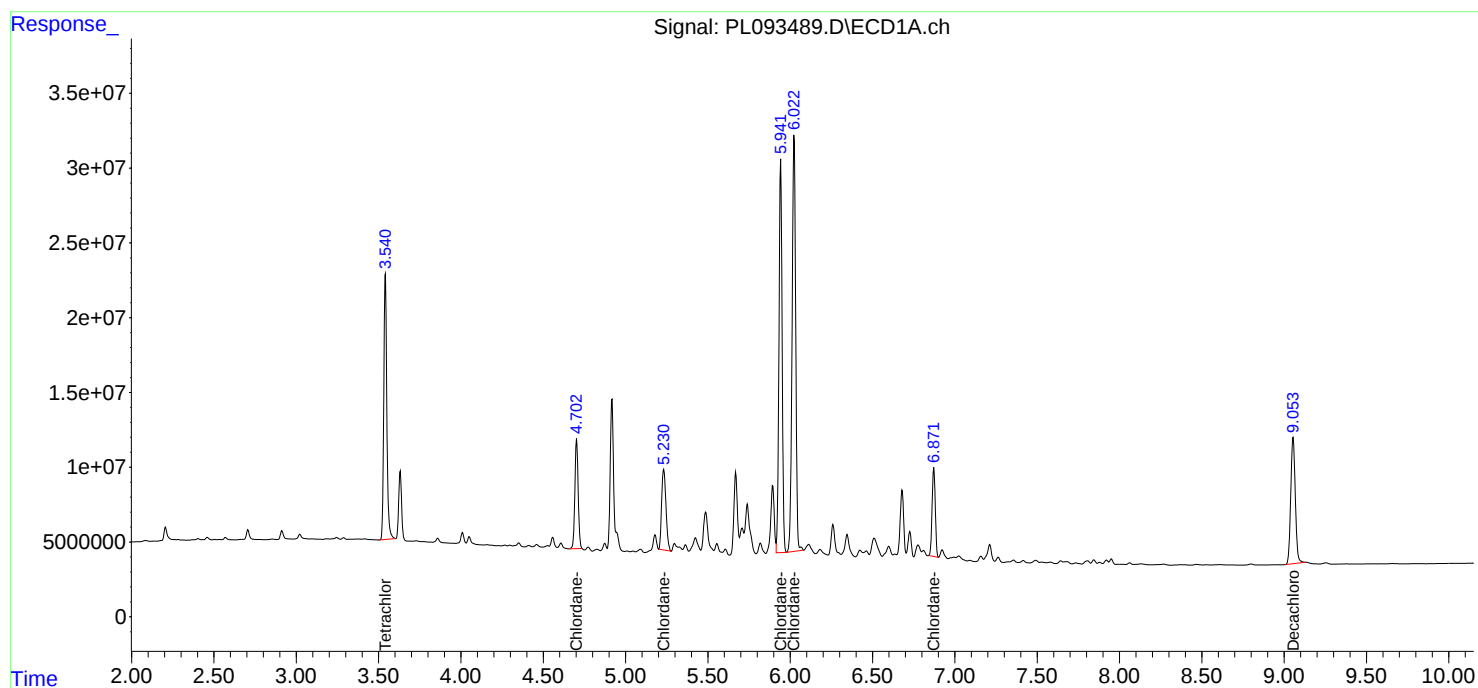


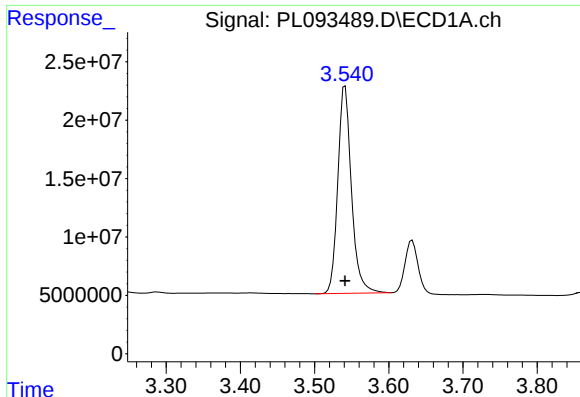

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 227499305
Conc: 97.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

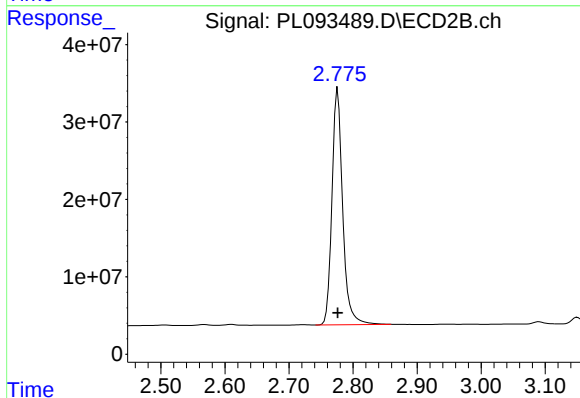


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 354859280
Conc: 102.60 ng/ml

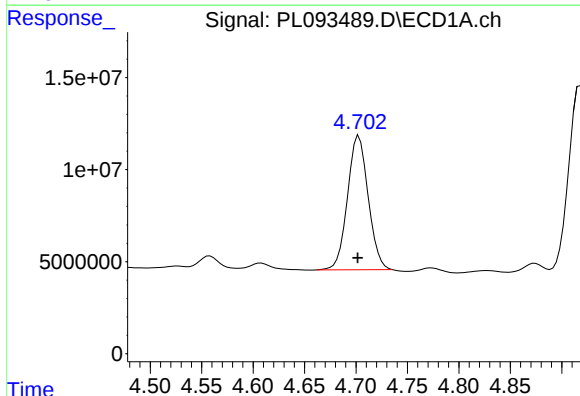


#23 Chlordane-1

R.T.: 4.703 min
Delta R.T.: 0.001 min
Response: 102022301
Conc: 971.55 ng/ml

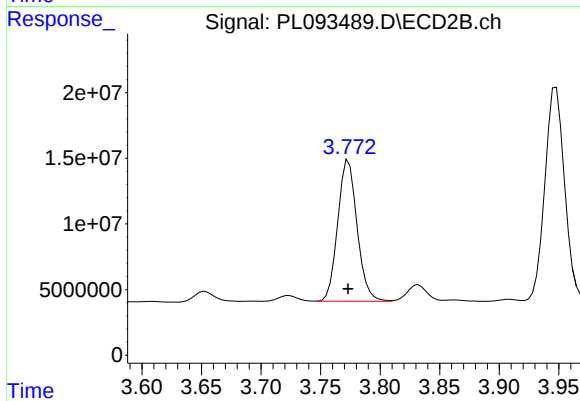

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 121553656
Conc: 1030.27 ng/ml

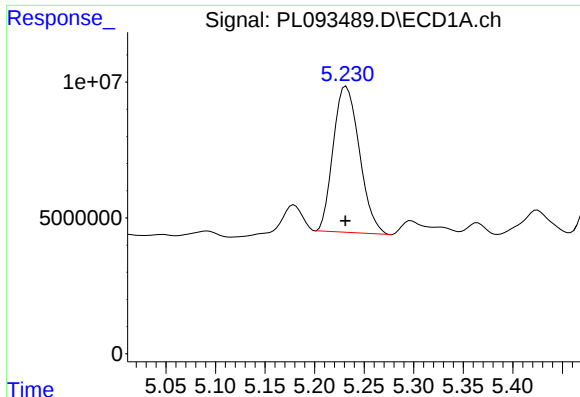

#24 Chlordane-2


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 98976001
Conc: 945.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

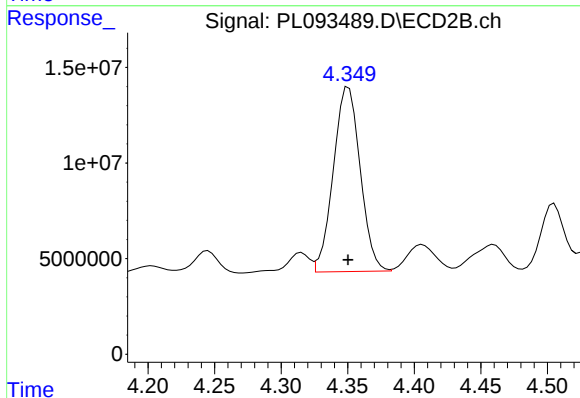


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 135605981
Conc: 999.85 ng/ml

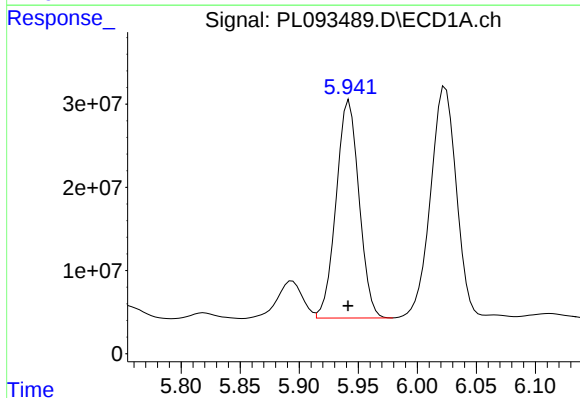


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: 0.001 min
Response: 353887167
Conc: 990.72 ng/ml

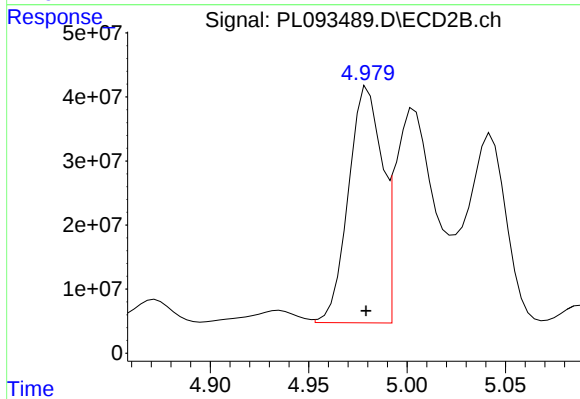

#25 Chlordane-3


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 434967203
Conc: 1045.66 ng/ml

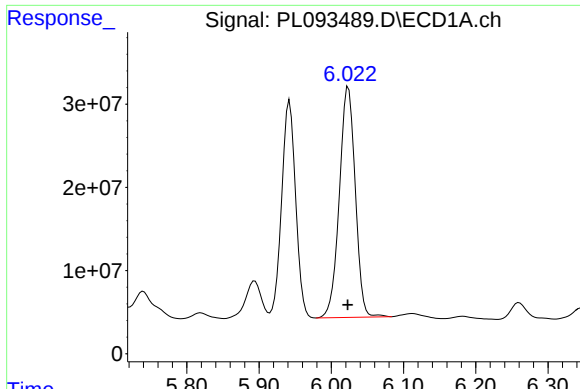

#26 Chlordane-4


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 423084816
Conc: 986.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

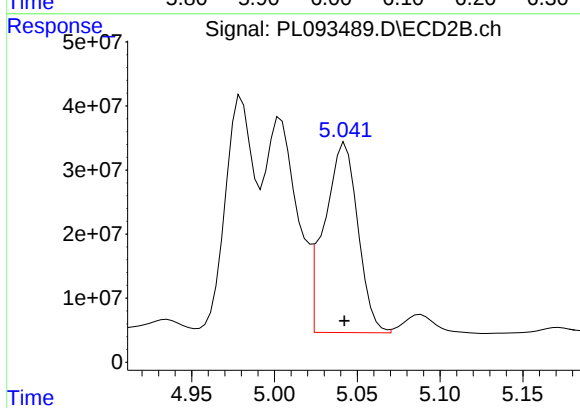


#26 Chlordane-4

R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 415996371
Conc: 1021.20 ng/ml

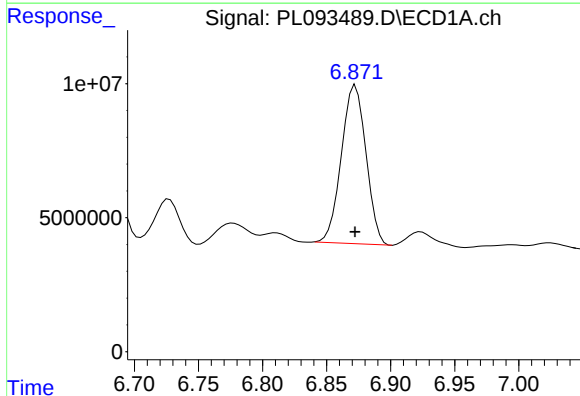


#27 Chlordane-5

R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 78915832
Conc: 952.79 ng/ml

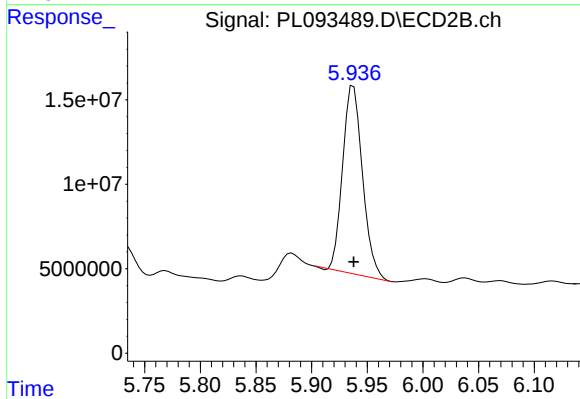

#27 Chlordane-5

R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 136907546
Conc: 1034.06 ng/ml

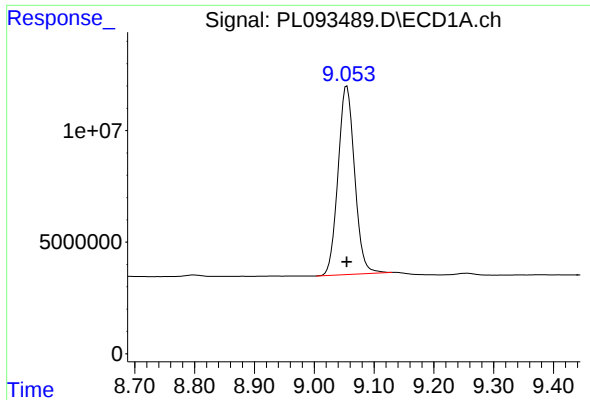

#28 Decachlorobiphenyl


R.T.: 9.055 min

Delta R.T.: 0.000 min

Response: 162993925

Conc: 92.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

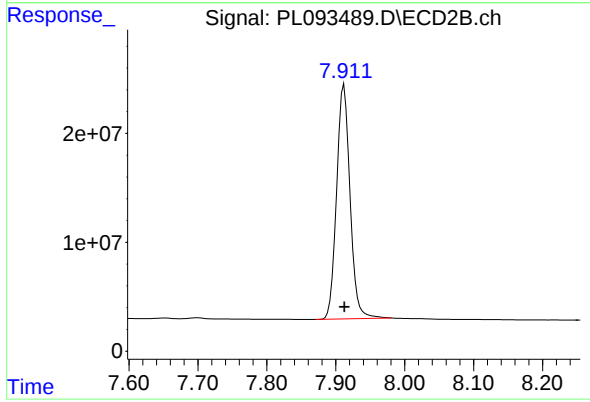

#28 Decachlorobiphenyl

R.T.: 7.912 min

Delta R.T.: 0.000 min

Response: 291893233

Conc: 98.44 ng/ml