

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
 Data File : PL093500-1.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 17:19
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 15:23:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:21:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.776	118.0E6	175.8E6	50.694	50.831
28)	SA Decachlor...	9.054	7.912	88395241	150.1E6	50.333	50.605
Target Compounds							
23)	Chlordane-1	4.701	3.773	52824653	56389200	503.044	477.948
24)	Chlordane-2	5.230	4.350	52312134	68660129	499.675	506.243
25)	Chlordane-3	5.941	4.980	177.6E6	208.3E6	497.267	500.669
26)	Chlordane-4	6.022	5.042	212.0E6	199.5E6	494.134	489.711
27)	Chlordane-5	6.871	5.937	41102903	64957816	496.257	490.624



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
Data File : PL093500-1.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 17:19
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 15:23:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:21:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

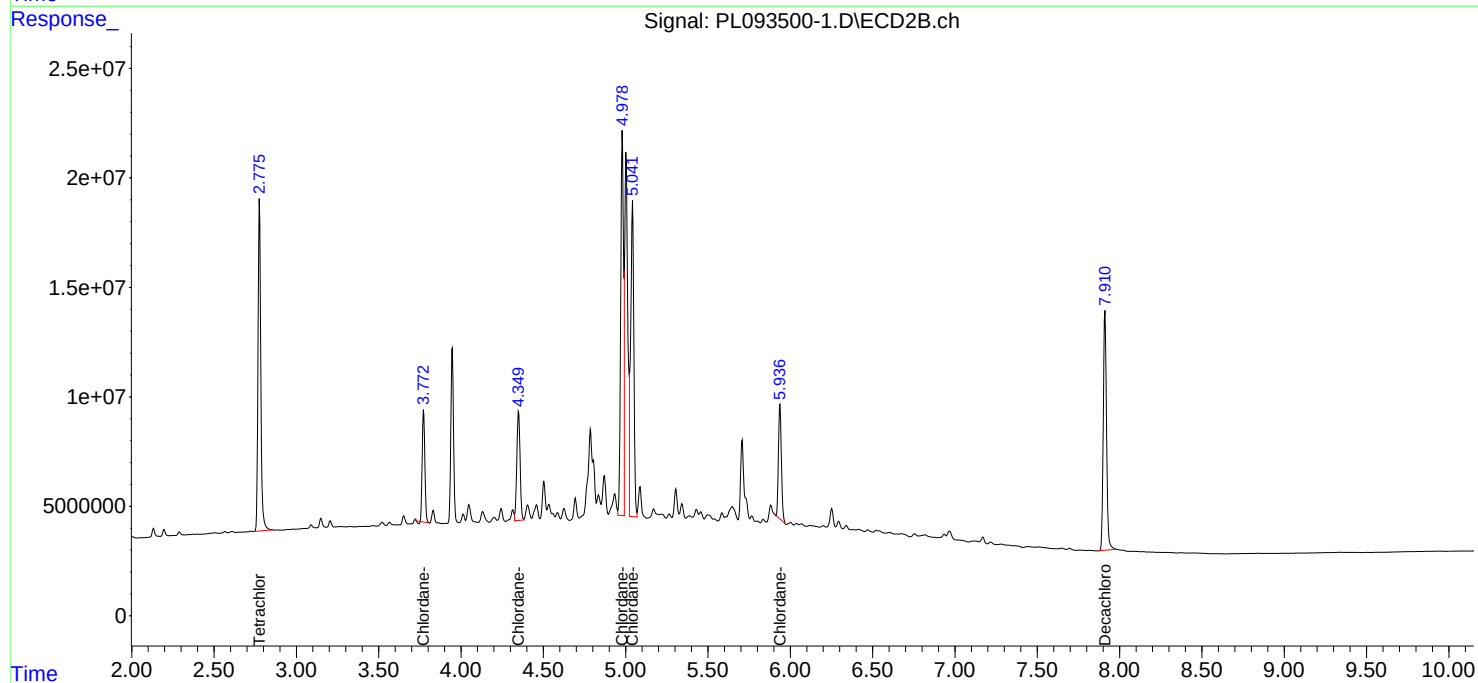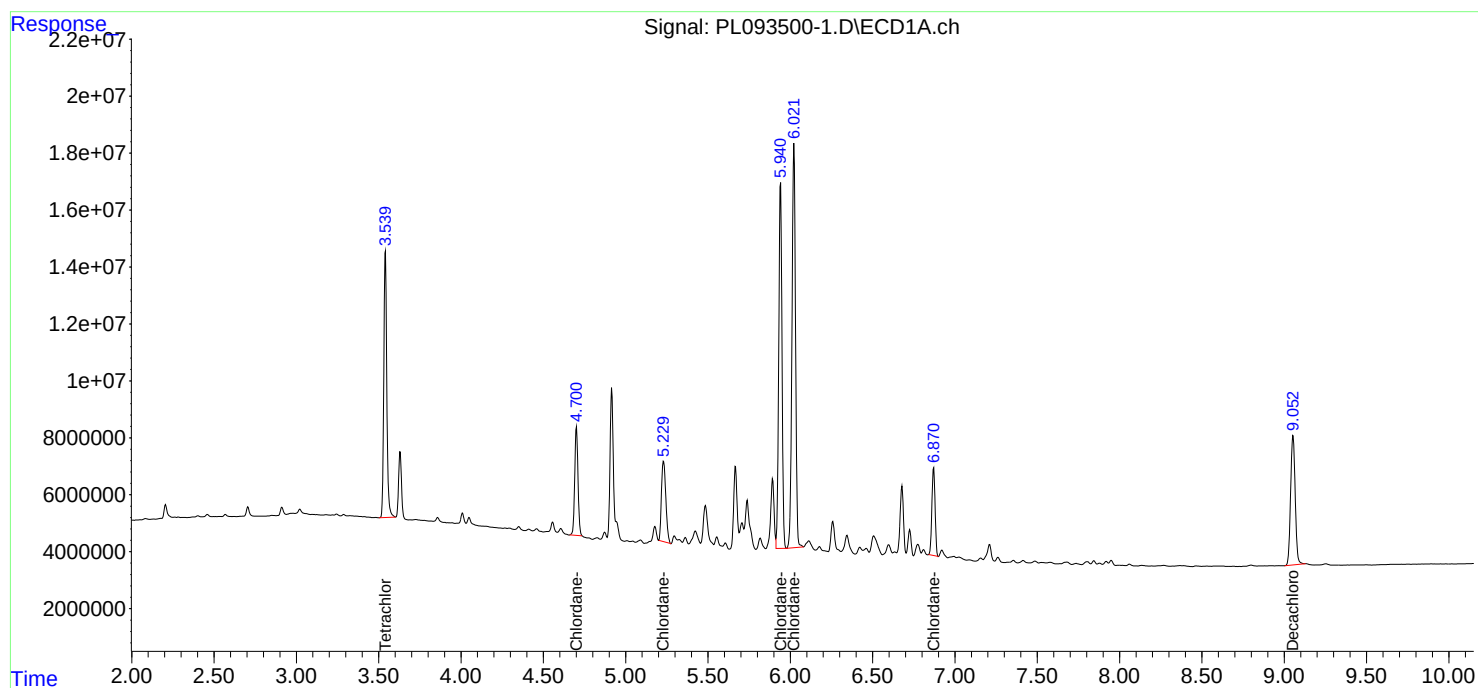


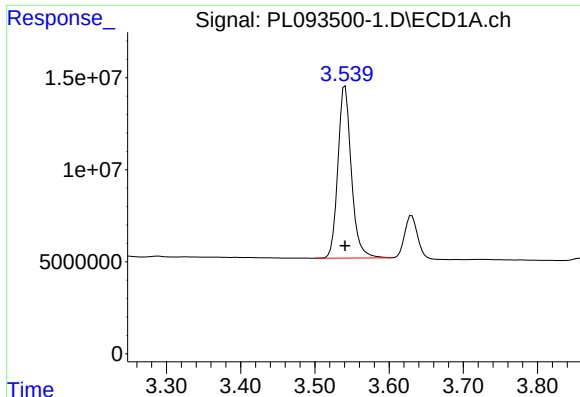

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 118025551
Conc: 50.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

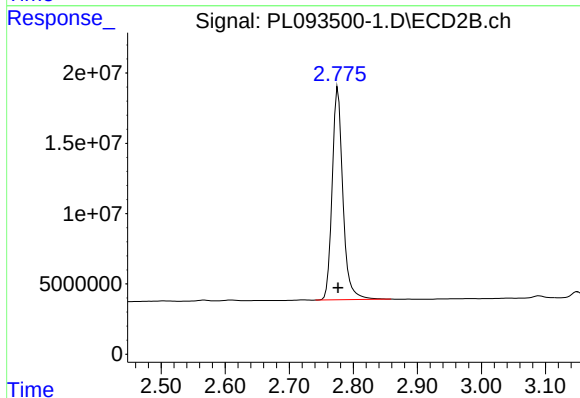


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 175801523
Conc: 50.83 ng/ml

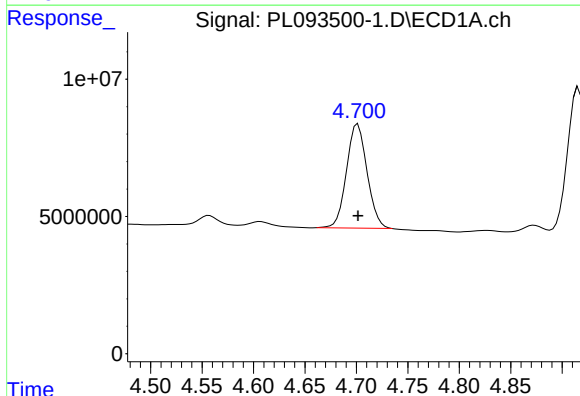


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 52824653
Conc: 503.04 ng/ml

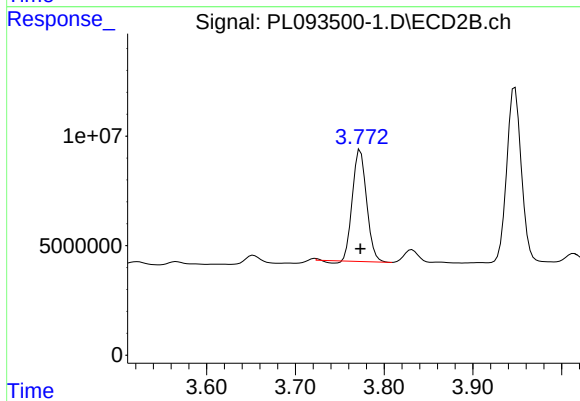

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 56389200
Conc: 477.95 ng/ml

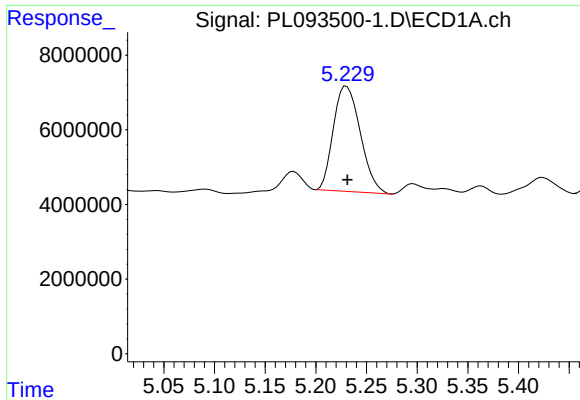

#24 Chlordane-2


R.T.: 5.230 min
Delta R.T.: 0.000 min
Response: 52312134
Conc: 499.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

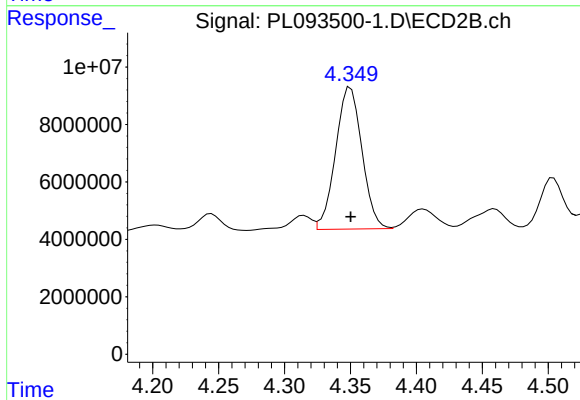


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 68660129
Conc: 506.24 ng/ml

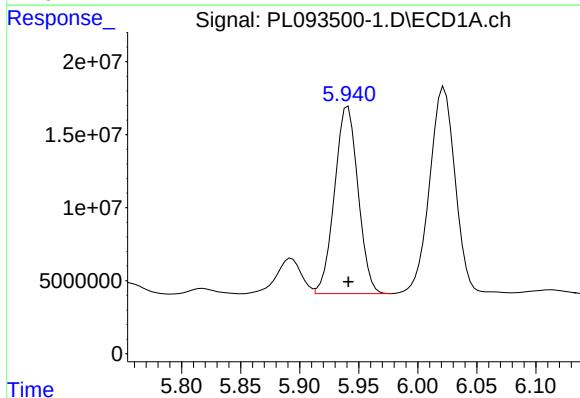


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 177623872
Conc: 497.27 ng/ml

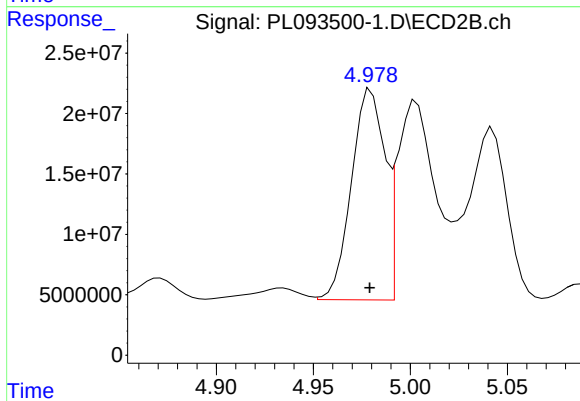

#25 Chlordane-3


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 208265211
Conc: 500.67 ng/ml

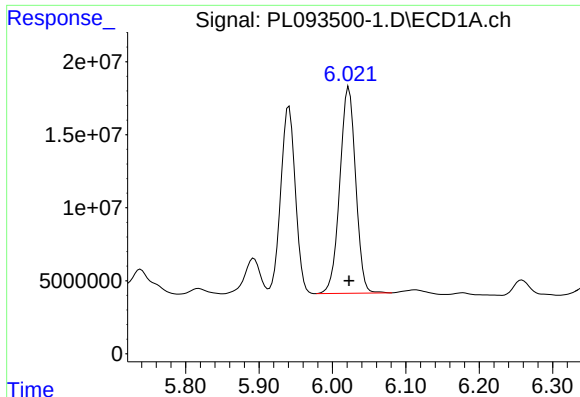

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 211991946
Conc: 494.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

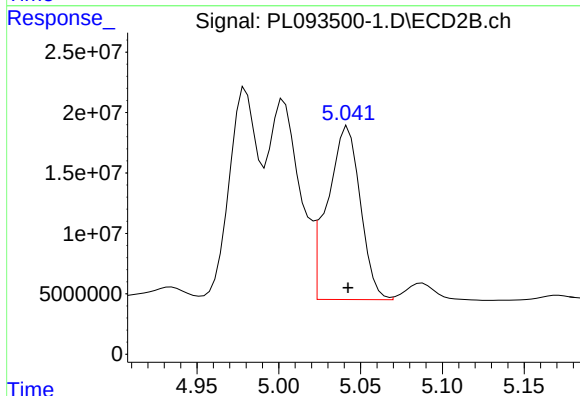


#26 Chlordane-4

R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 199489008
Conc: 489.71 ng/ml

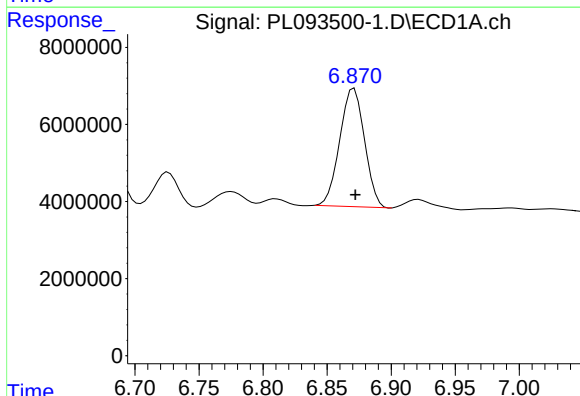


#27 Chlordane-5

R.T.: 6.871 min
Delta R.T.: -0.001 min
Response: 41102903
Conc: 496.26 ng/ml

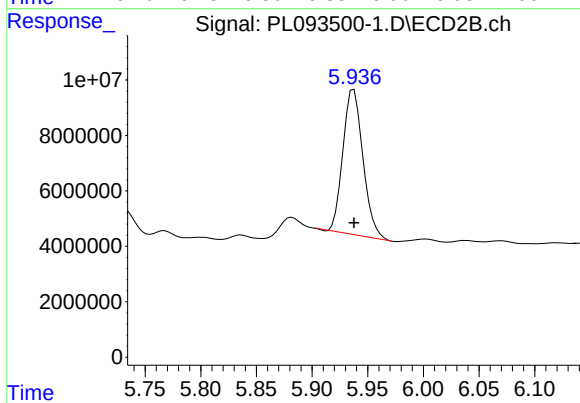

#27 Chlordane-5

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 64957816
Conc: 490.62 ng/ml

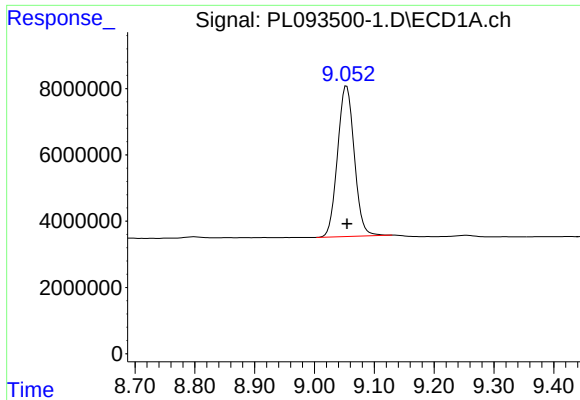

#28 Decachlorobiphenyl


R.T.: 9.054 min

Delta R.T.: 0.000 min

Response: 88395241

Conc: 50.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

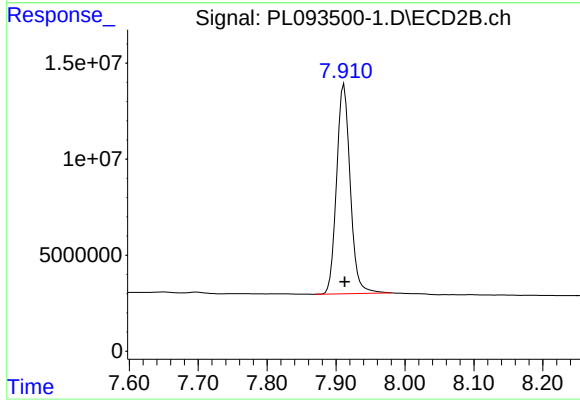

#28 Decachlorobiphenyl

R.T.: 7.912 min

Delta R.T.: 0.000 min

Response: 150059076

Conc: 50.60 ng/ml