

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
 Data File : PL093490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 14:36
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 15:22:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:21:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.776	172.0E6	264.1E6	73.882	76.369
28)	SA Decachlor...	9.054	7.912	125.9E6	220.8E6	71.661	74.475
Target Compounds							
23)	Chlordane-1	4.701	3.773	77689893	90689705	739.833	768.675
24)	Chlordane-2	5.232	4.350	75883152	102.6E6	724.821	756.497
25)	Chlordane-3	5.941	4.979	267.2E6	324.8E6	748.097	780.731
26)	Chlordane-4	6.023	5.042	319.5E6	312.6E6	744.759	767.499
27)	Chlordane-5	6.872	5.937	60463753	102.7E6	730.011	775.594



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
Data File : PL093490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 14:36
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 15:22:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:21:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

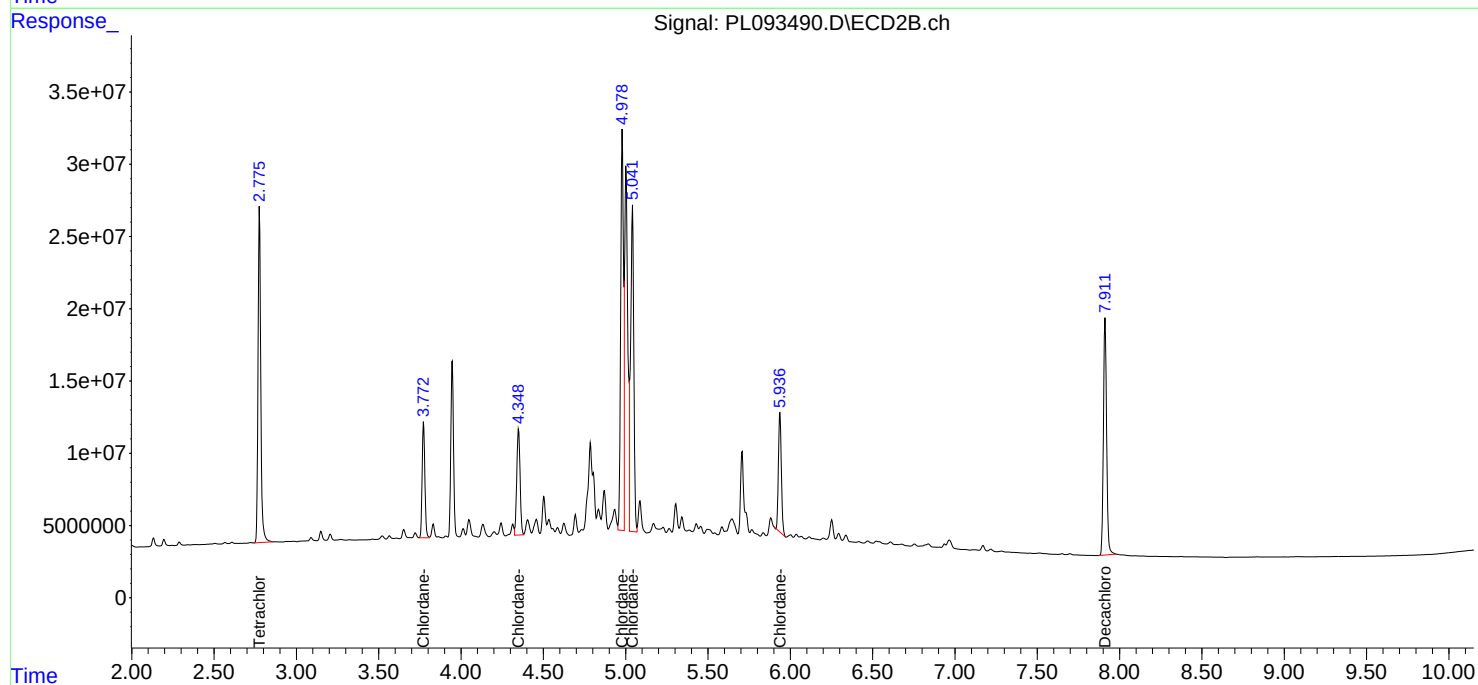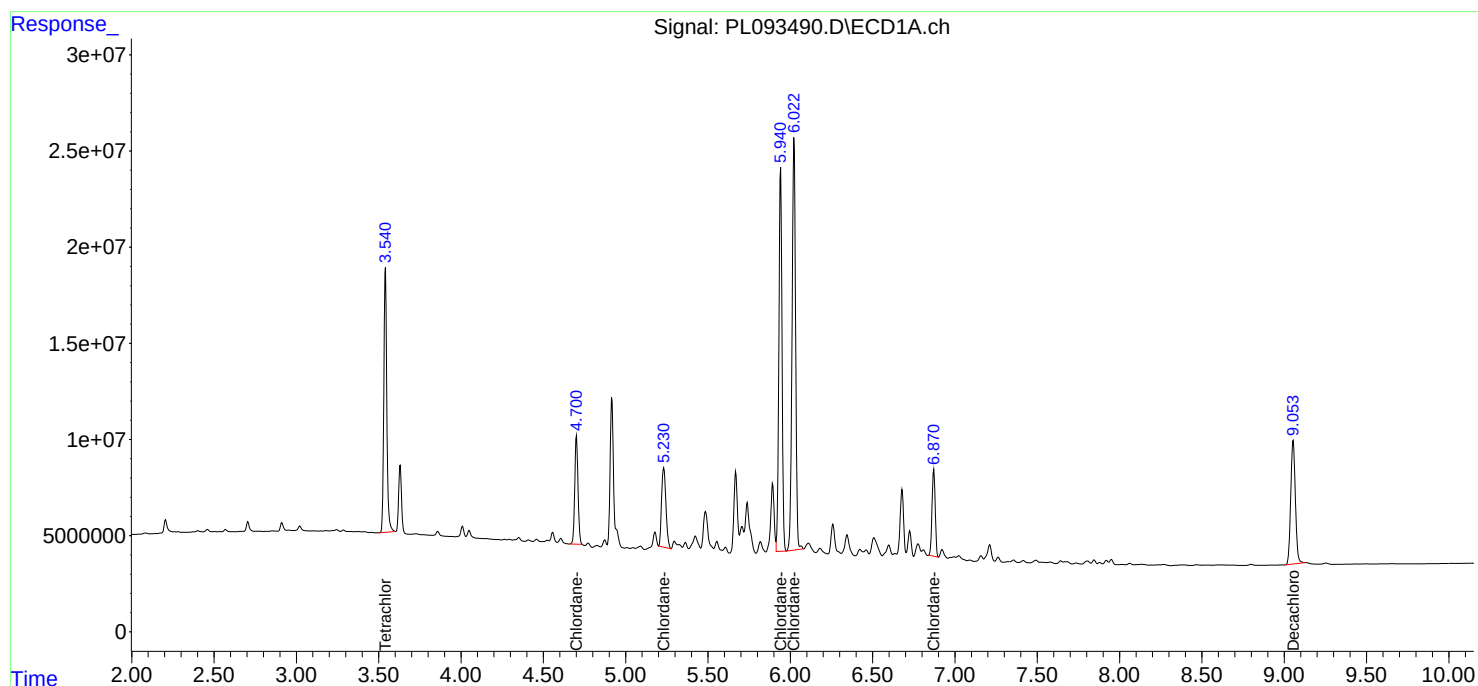


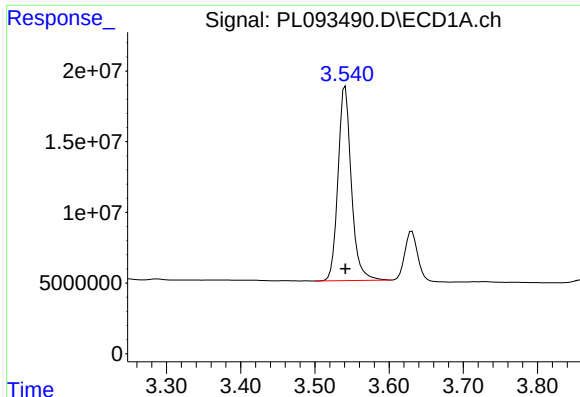

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 172009338
Conc: 73.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

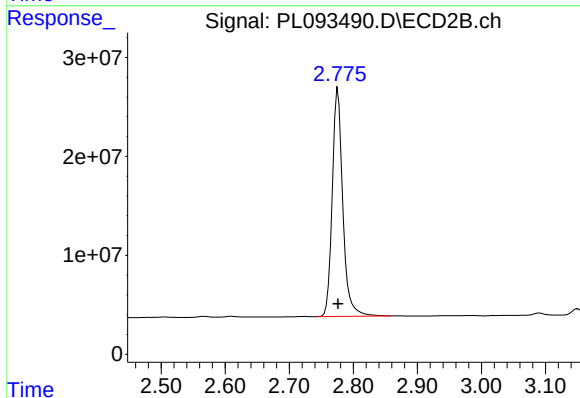


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 264127464
Conc: 76.37 ng/ml

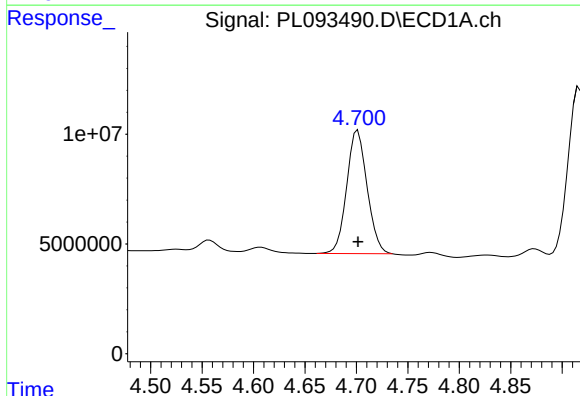


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 77689893
Conc: 739.83 ng/ml

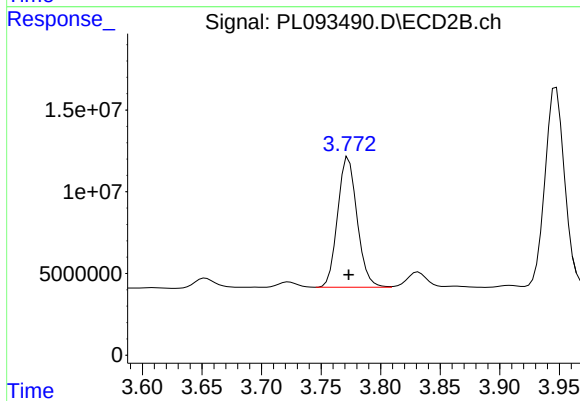

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 90689705
Conc: 768.68 ng/ml

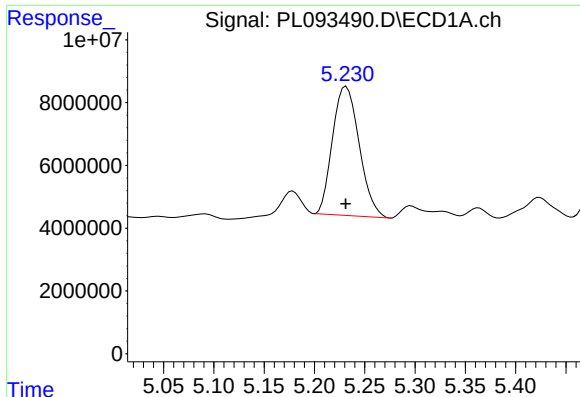

#24 Chlordane-2


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 75883152
Conc: 724.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

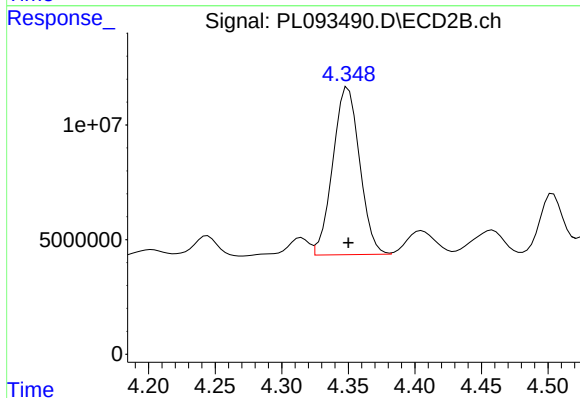


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 102601324
Conc: 756.50 ng/ml

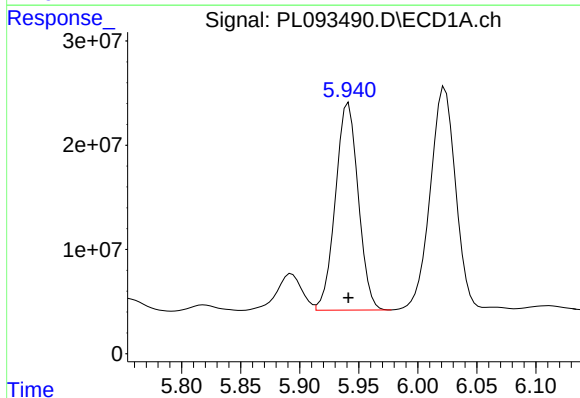


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 267220485
Conc: 748.10 ng/ml

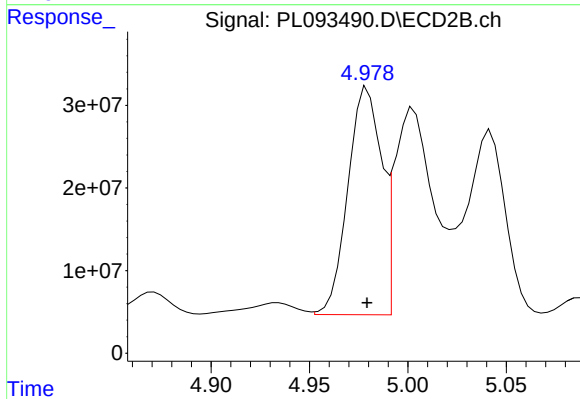

#25 Chlordane-3


R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 324763535
Conc: 780.73 ng/ml

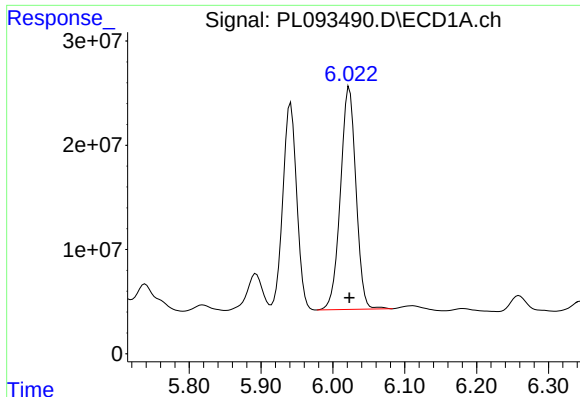

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 319514496
Conc: 744.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

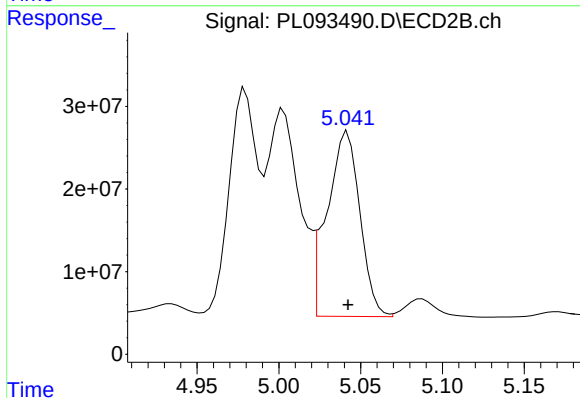


#26 Chlordane-4

R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 312648635
Conc: 767.50 ng/ml

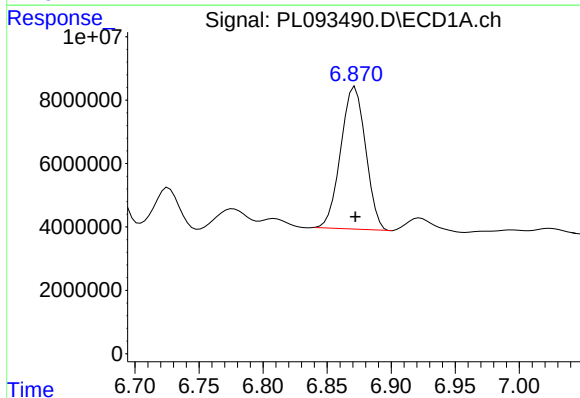


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 60463753
Conc: 730.01 ng/ml

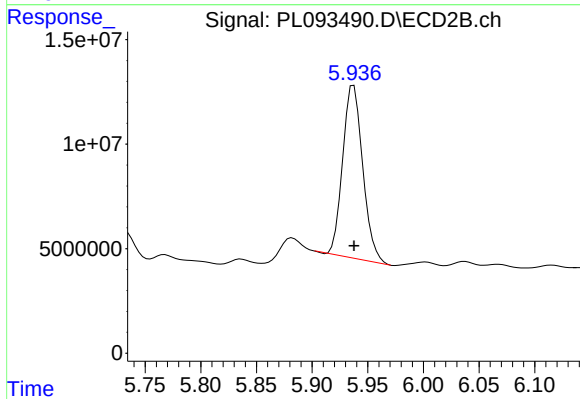

#27 Chlordane-5


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 102687486
Conc: 775.59 ng/ml

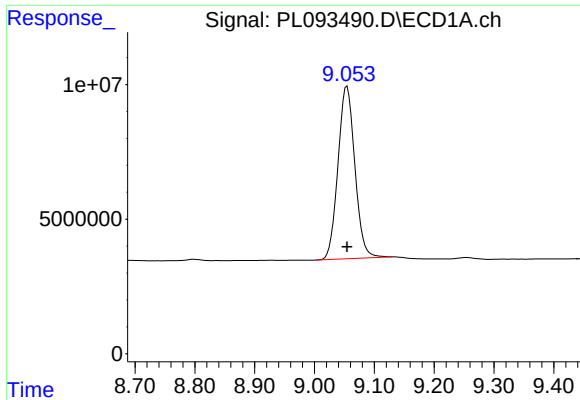

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 125852881
Conc: 71.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

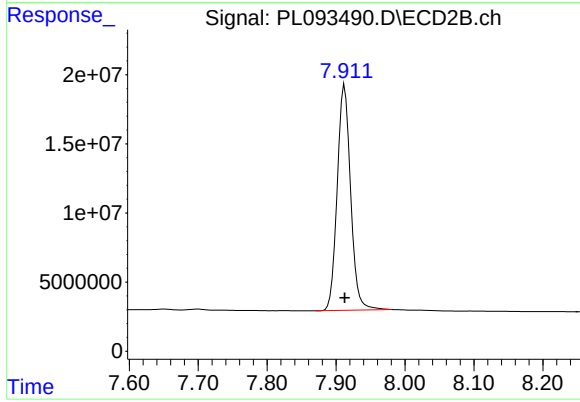

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 220841231
Conc: 74.47 ng/ml