

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
 Data File : PL093492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 15:03
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 15:22:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:21:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.776	62384510	87088559	26.795	25.181
28)	SA Decachlor...	9.054	7.912	47546039	76035961	27.073	25.642
Target Compounds							
23)	Chlordane-1	4.701	3.774	28279141	29810195	269.299	252.668
24)	Chlordane-2	5.231	4.350	28508969	35160053	272.312	259.241
25)	Chlordane-3	5.941	4.980	95183618	103.5E6	266.471	248.864
26)	Chlordane-4	6.023	5.043	114.4E6	100.2E6	266.586	245.903
27)	Chlordane-5	6.872	5.937	22602358	32803129	272.890	247.761



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122324\
Data File : PL093492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 15:03
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 15:22:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:21:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

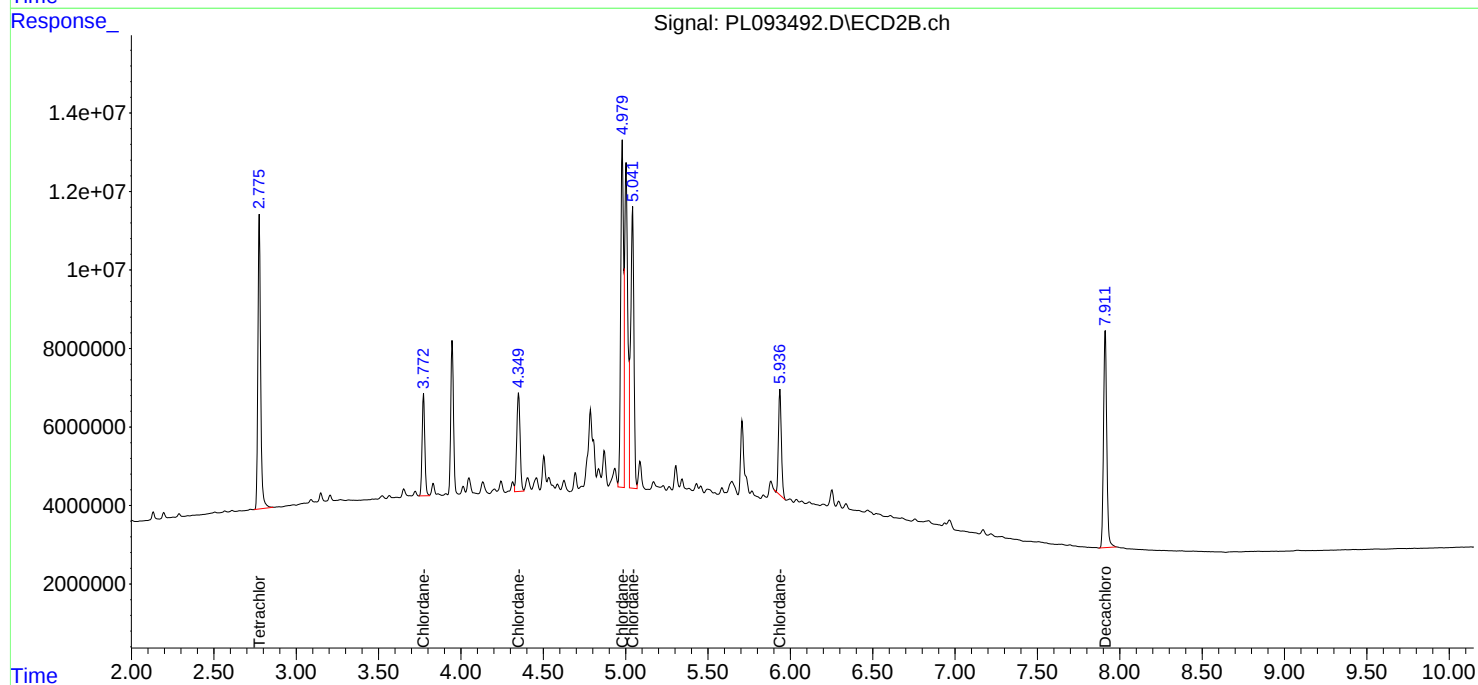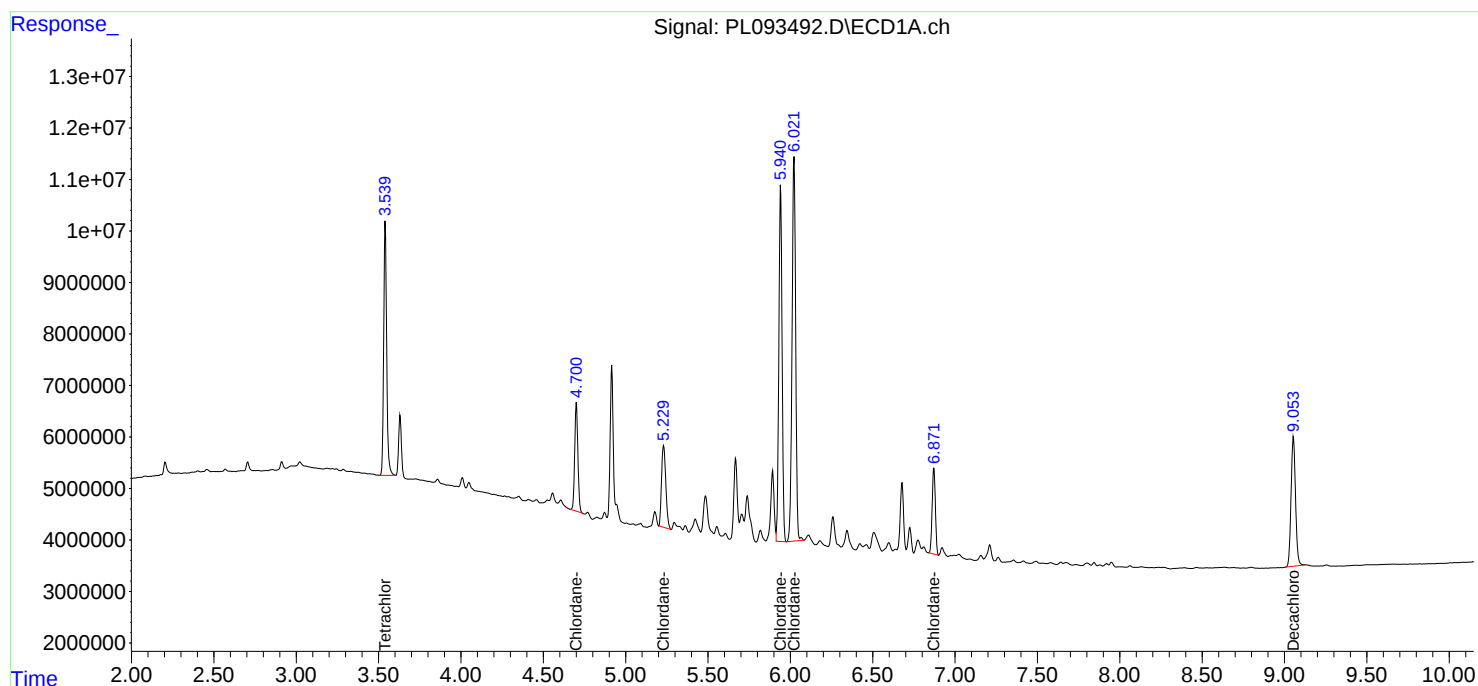


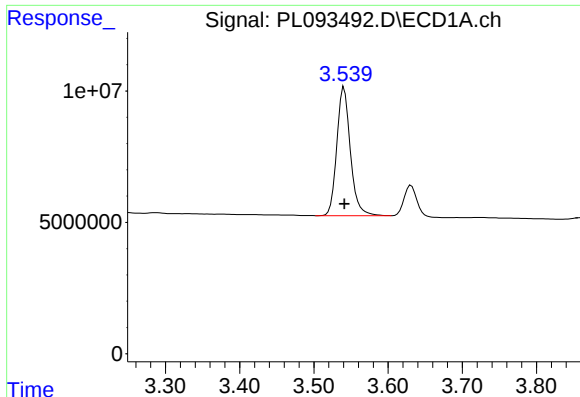

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 62384510
Conc: 26.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

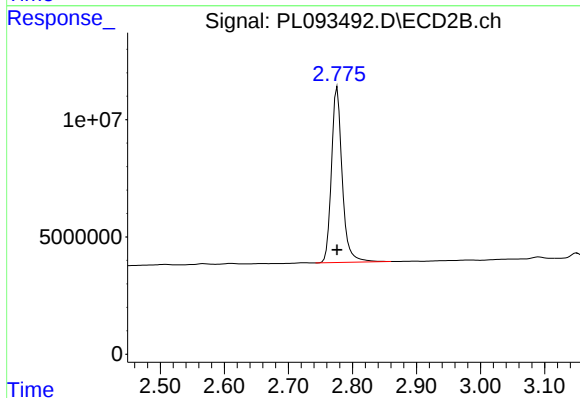


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 87088559
Conc: 25.18 ng/ml

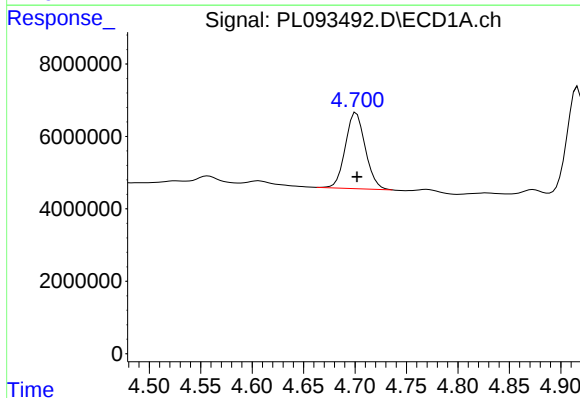


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 28279141
Conc: 269.30 ng/ml

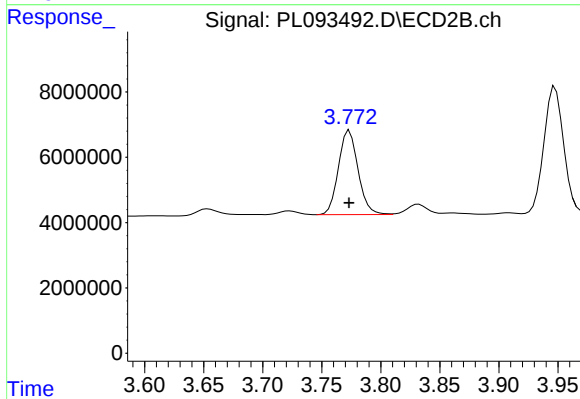

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 29810195
Conc: 252.67 ng/ml

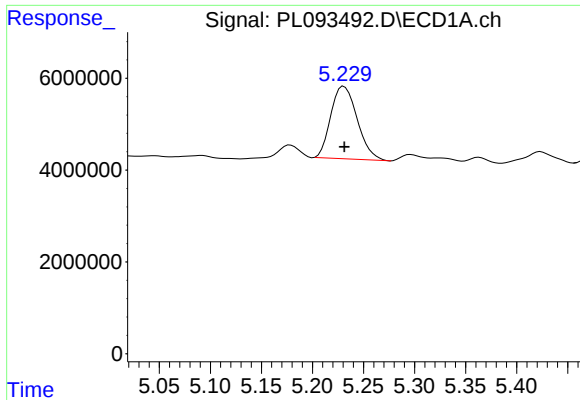

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 28508969
Conc: 272.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

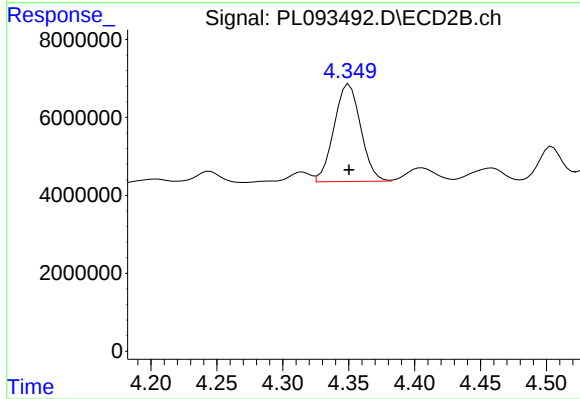


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 35160053
Conc: 259.24 ng/ml

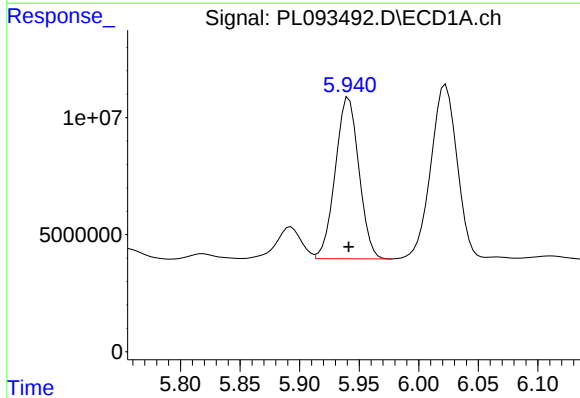


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 95183618
Conc: 266.47 ng/ml

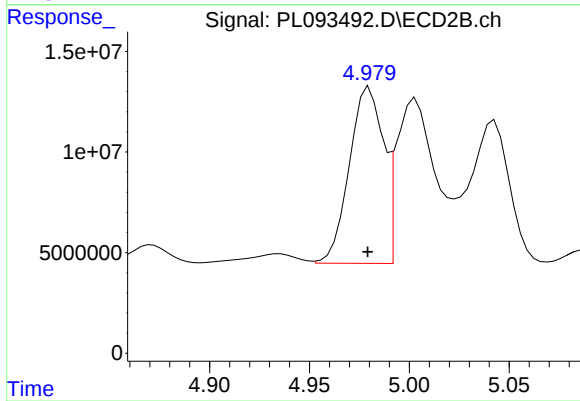

#25 Chlordane-3


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 103520950
Conc: 248.86 ng/ml

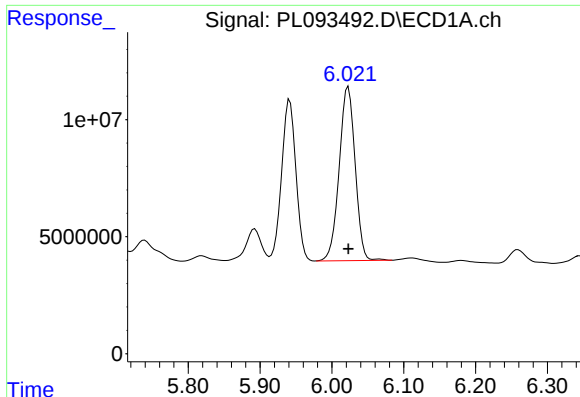

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 114369946
Conc: 266.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

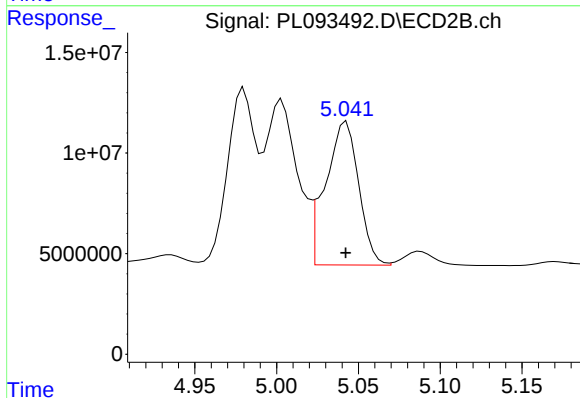


#26 Chlordane-4

R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 100171164
Conc: 245.90 ng/ml

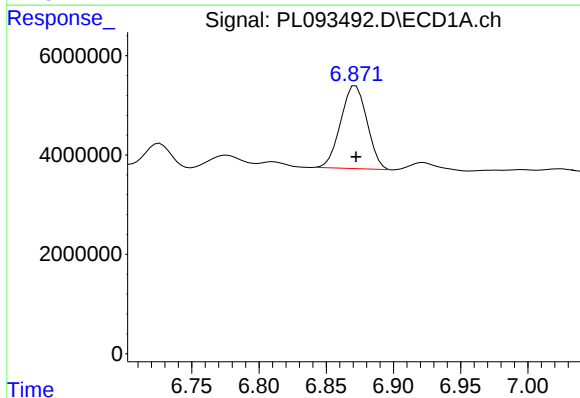


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 22602358
Conc: 272.89 ng/ml

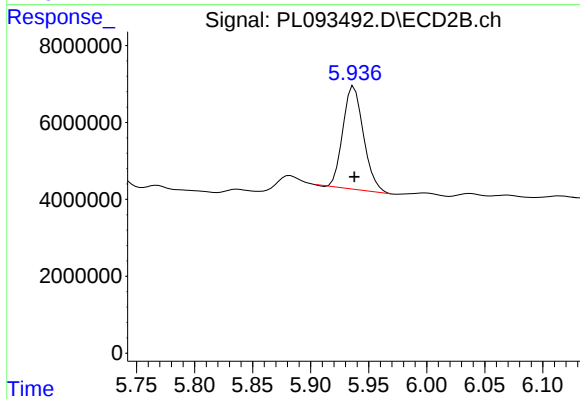

#27 Chlordane-5


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 32803129
Conc: 247.76 ng/ml

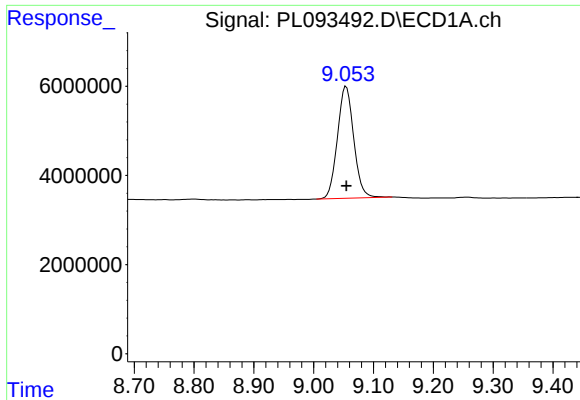

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 47546039
Conc: 27.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

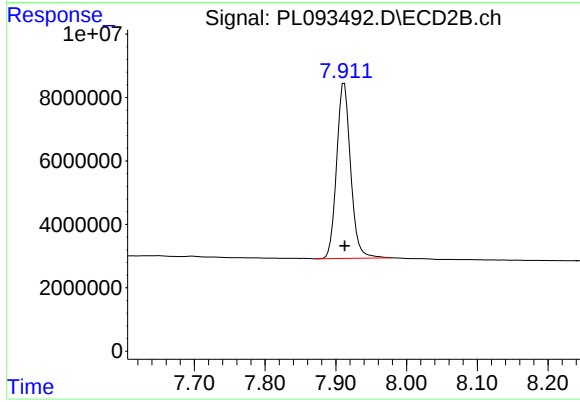

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 76035961
Conc: 25.64 ng/ml