

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL122419\  
 Data File : PL055202.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Dec 2019 08:27  
 Operator : SG\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 25 00:54:57 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL122119.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 21 05:21:06 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

#### Target Compounds

|        |              |        |       |          |          |         |         |
|--------|--------------|--------|-------|----------|----------|---------|---------|
| 8) B   | Heptachlo... | 0.000  | 5.923 | 0        | 12614126 | N.D.    | 4.949 # |
| 14) MA | Endrin       | 0.000  | 6.751 | 0        | 7287617  | N.D.    | 3.396 # |
| 27)    | Chlordane-5  | 6.421f | 0.000 | 47403988 | 0        | 121.652 | N.D. #  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL122419\  
Data File : PL055202.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Dec 2019 08:27  
Operator : SG\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 25 00:54:57 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL122119.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 21 05:21:06 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

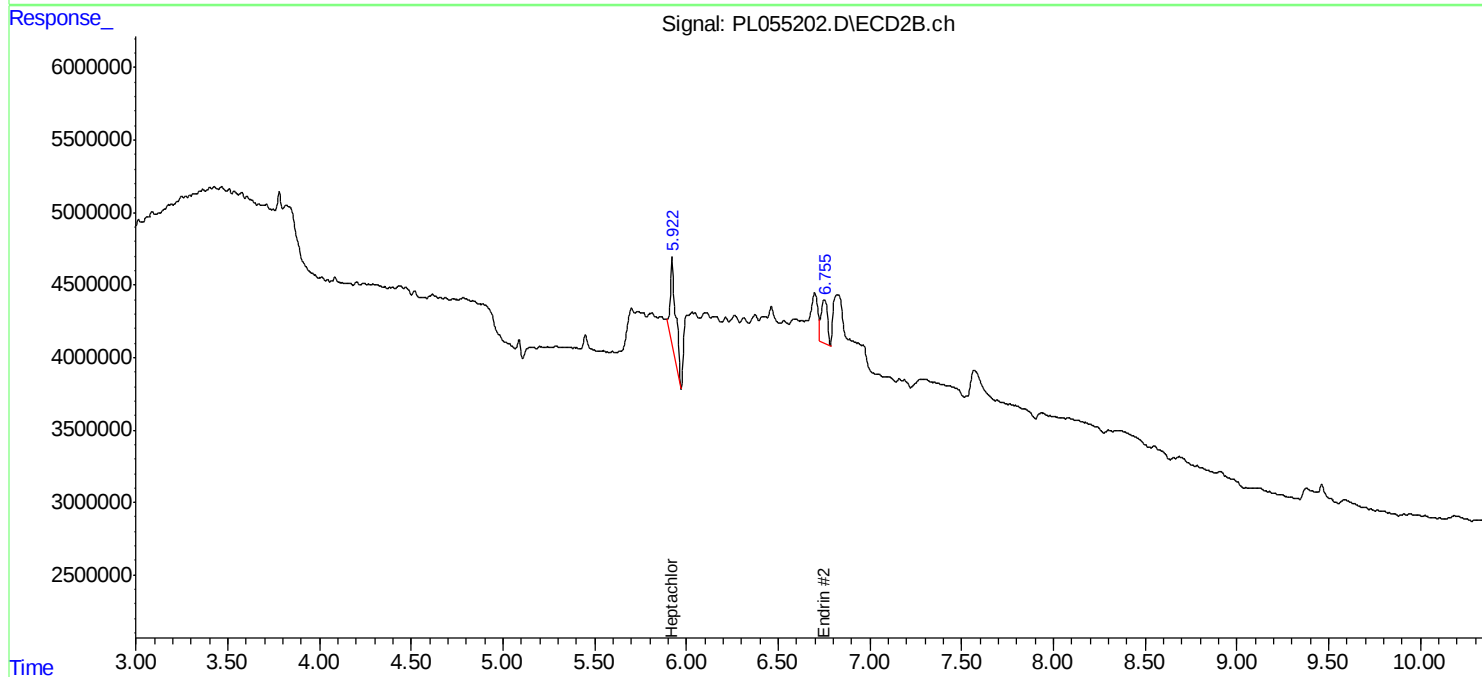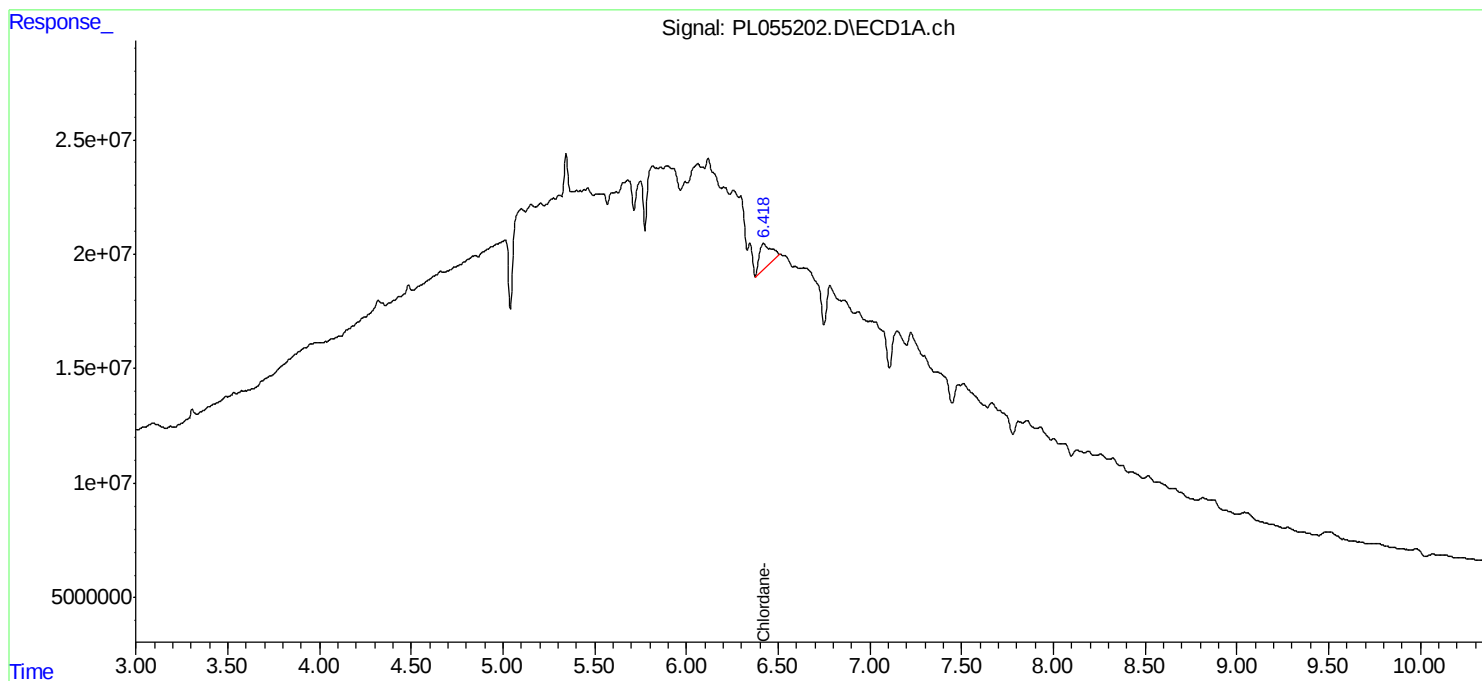


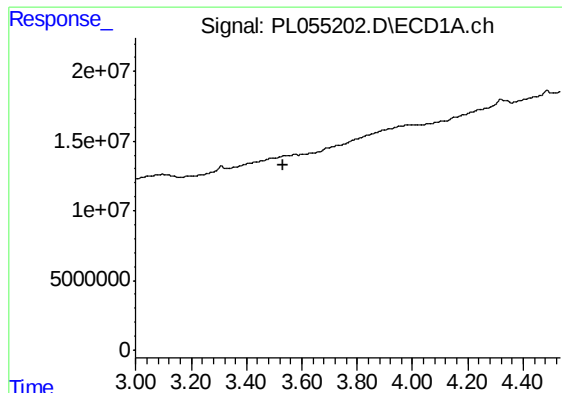

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.535 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

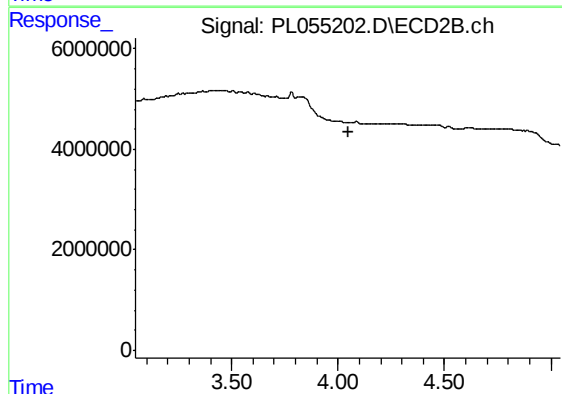


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 4.047 min  
Response: 0  
Conc: N.D.

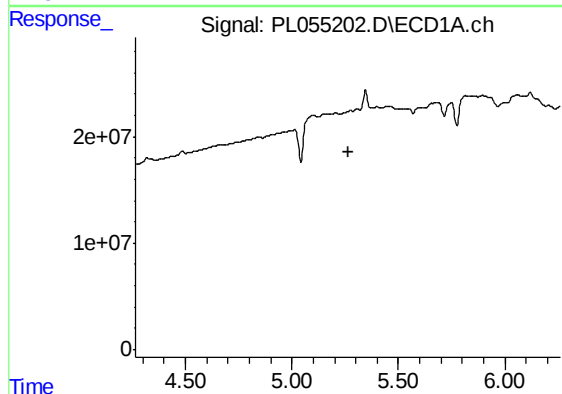


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T. : 5.265 min  
Response: 0  
Conc: N.D.

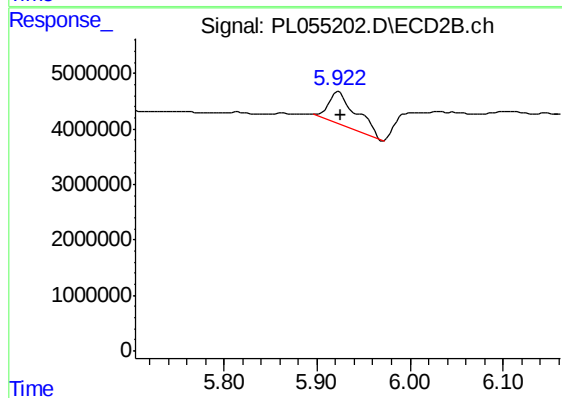

#8 Heptachlor epoxide


R.T.: 5.923 min  
Delta R.T.: -0.002 min  
Response: 12614126  
Conc: 4.95 ng/ml

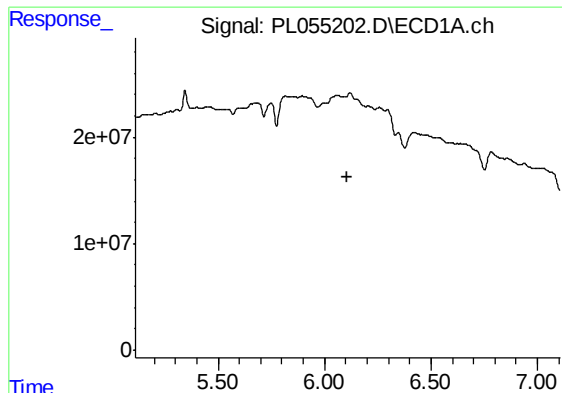

#14 Endrin


R.T.: 0.000 min  
Exp R.T. : 6.108 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

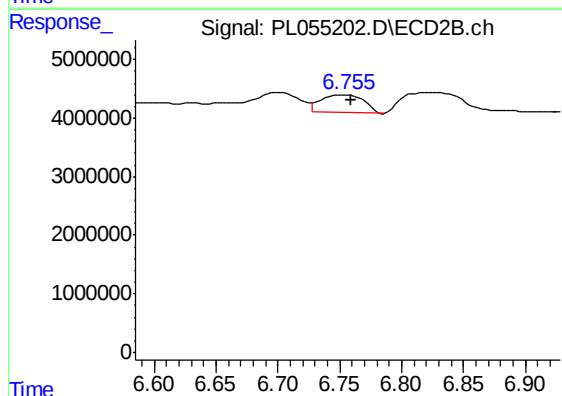


#14 Endrin

R.T.: 6.751 min  
Delta R.T.: -0.008 min  
Response: 7287617  
Conc: 3.40 ng/ml

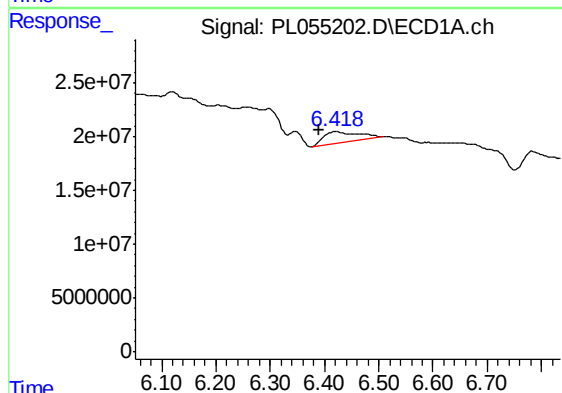


#27 Chlordane-5

R.T.: 6.421 min  
Delta R.T.: 0.030 min  
Response: 47403988  
Conc: 121.65 ng/ml

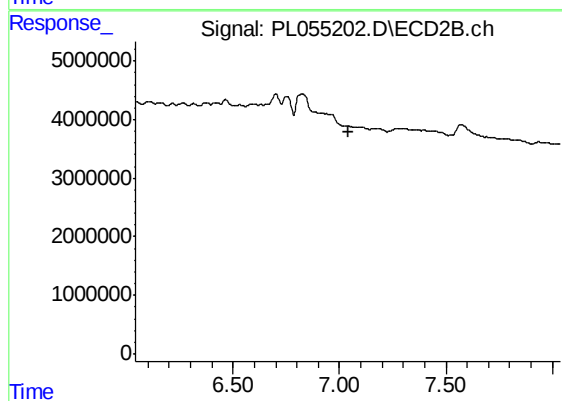

#27 Chlordane-5


R.T.: 0.000 min  
Exp R.T. : 7.041 min  
Response: 0  
Conc: N.D.

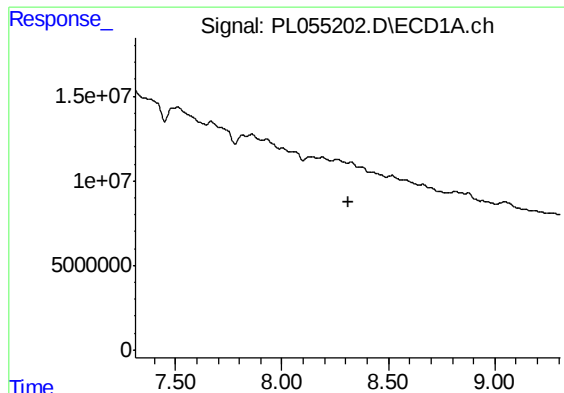

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.310 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

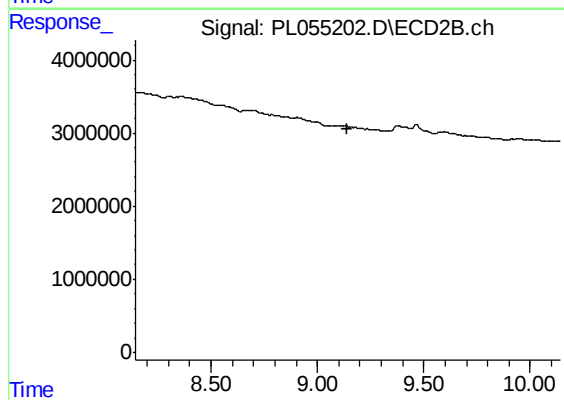

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.143 min  
Response: 0  
Conc: N.D.