

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
 Data File : PL055229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 18:18
 Operator : SG\AJ
 Sample : K6413-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 K005-AA-WC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 01:02:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	123.4E6	35338190	11.734	13.374
28)	SA Decachlor...	8.313	9.148	134.8E6	34548891	14.529	15.651
Target Compounds							
10)	B gamma-Chl...	0.000	6.162	0	1762546	N.D.	0.664 #
11)	B alpha-Chl...	0.000	6.236	0	4400327	N.D.	1.678 #
12)	B 4,4'-DDE	5.715	6.391	30534160	6639161	2.291	2.723
17)	MA 4,4'-DDT	6.473	7.183	18425981	4245065	1.830	2.163
25)	Chlordane-3	0.000	6.162	0	1762546	N.D.	5.477 #
26)	Chlordane-4	0.000	6.236	0	4400327	N.D.	11.448 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
Data File : PL055229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 18:18
Operator : SG\AJ
Sample : K6413-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 01:02:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

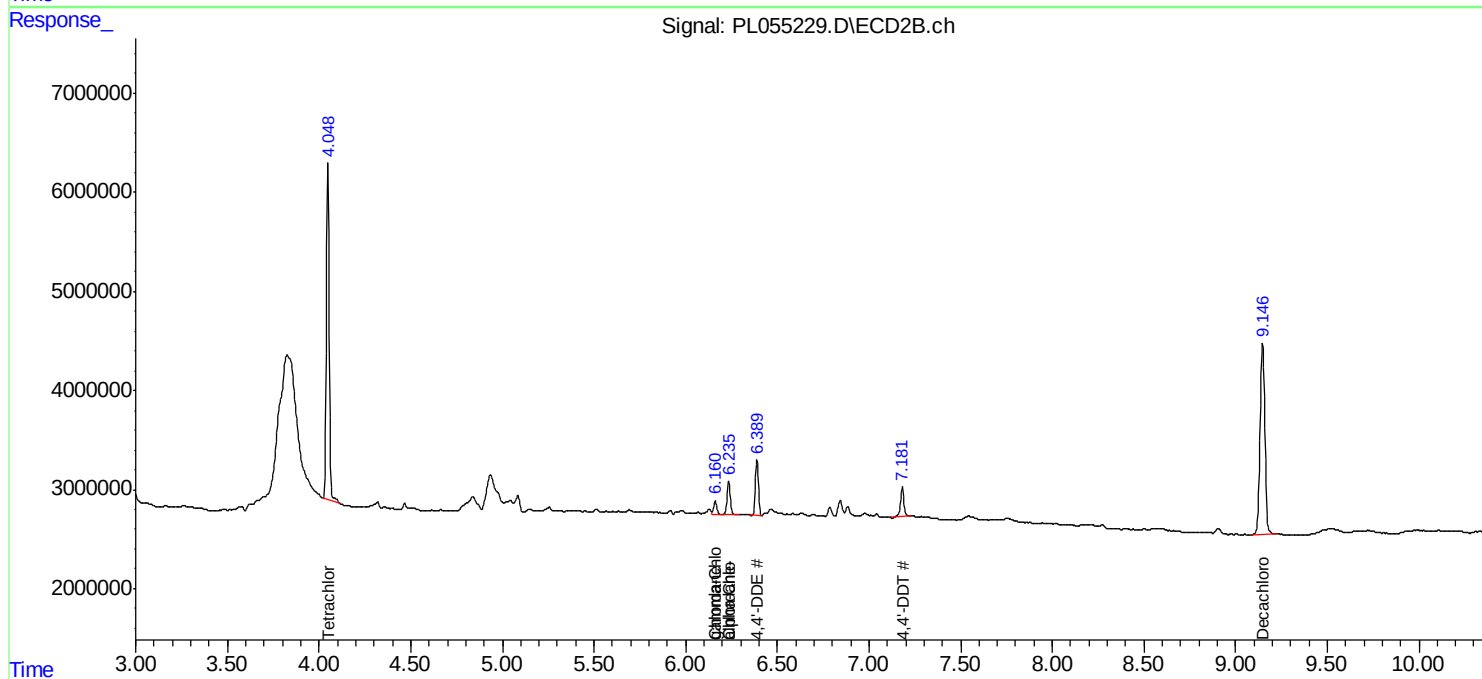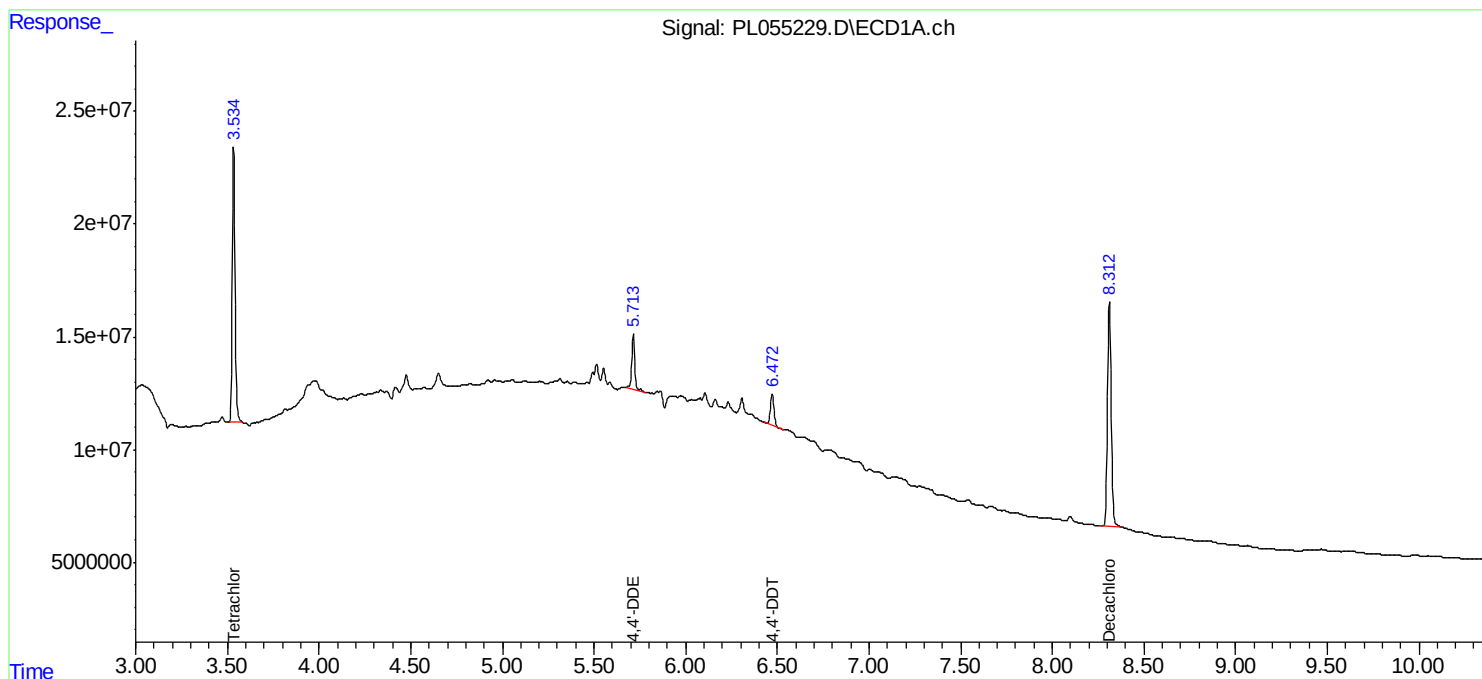


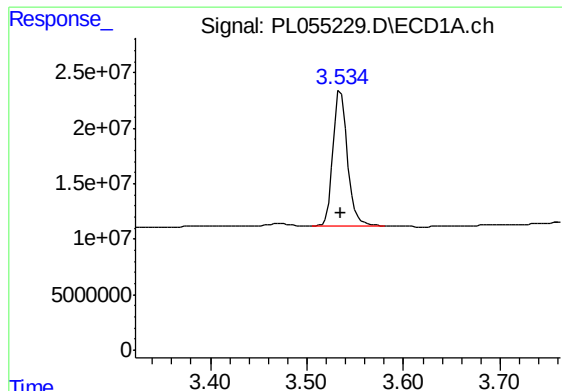

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 123398344
Conc: 11.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-2

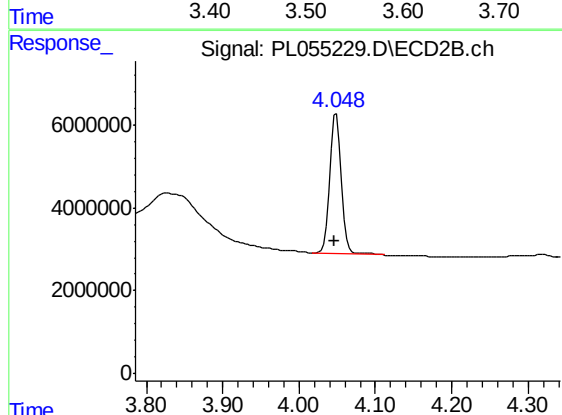


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 35338190
Conc: 13.37 ng/ml

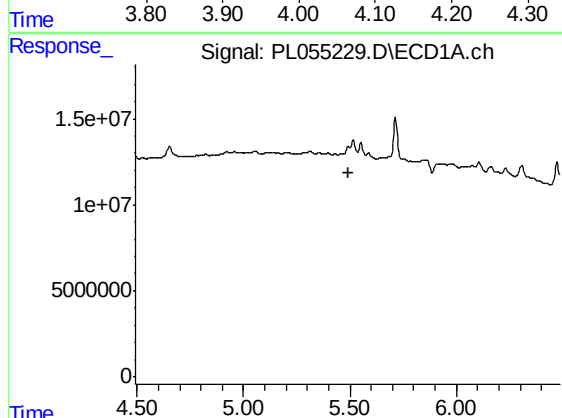


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

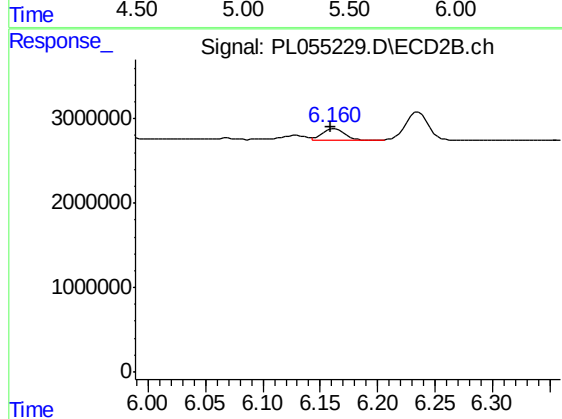

#10 gamma-Chlordane


R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 1762546
Conc: 0.66 ng/ml

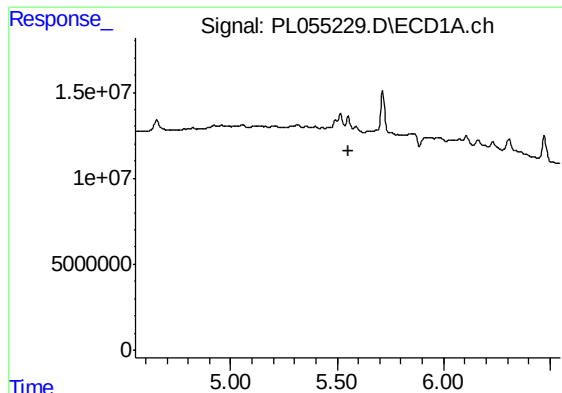

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-2

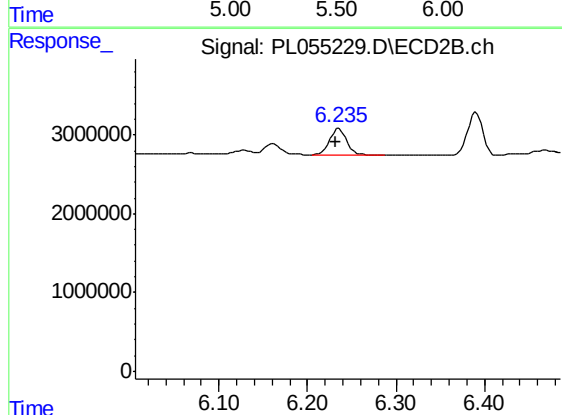


#11 alpha-Chlordane

R.T.: 6.236 min
Delta R.T.: 0.003 min
Response: 4400327
Conc: 1.68 ng/ml

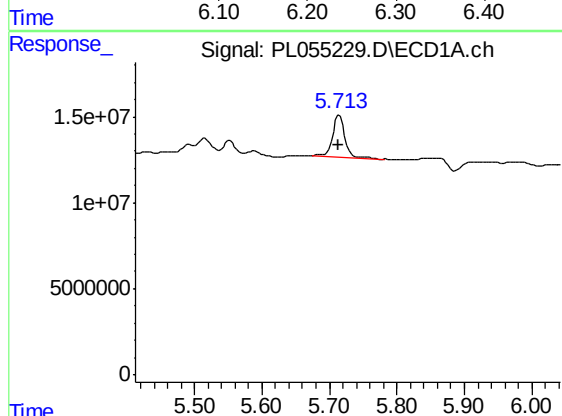


#12 4,4'-DDE

R.T.: 5.715 min
Delta R.T.: 0.001 min
Response: 30534160
Conc: 2.29 ng/ml

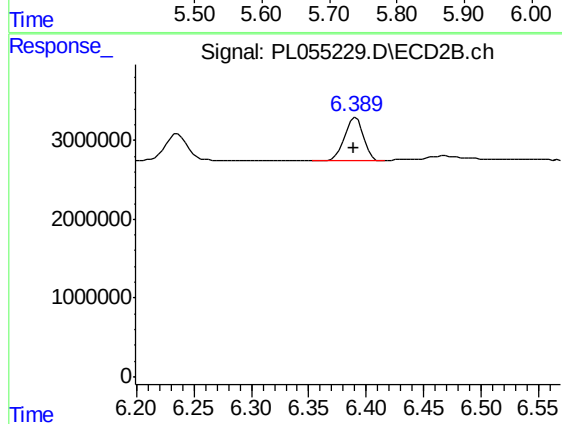

#12 4,4'-DDE


R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 6639161
Conc: 2.72 ng/ml

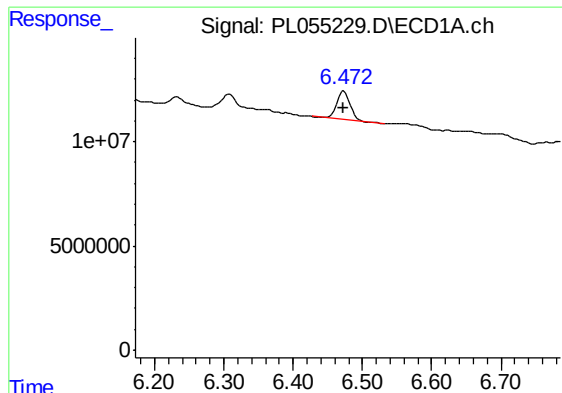

#17 4,4'-DDT


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 18425981
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-2

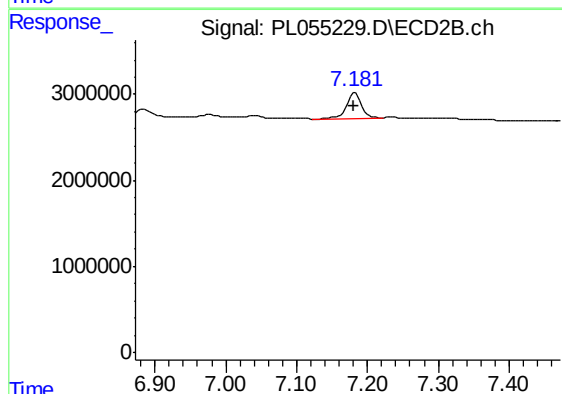


#17 4,4'-DDT

R.T.: 7.183 min
Delta R.T.: 0.003 min
Response: 4245065
Conc: 2.16 ng/ml

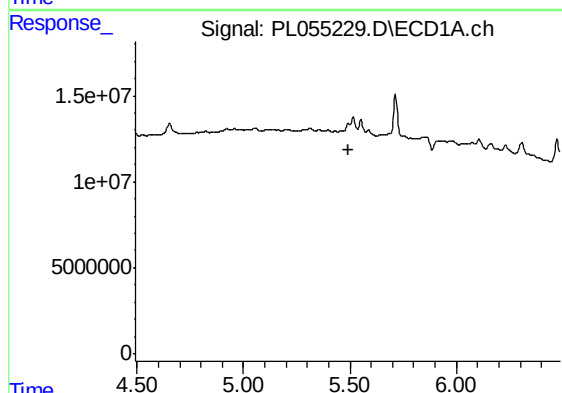


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

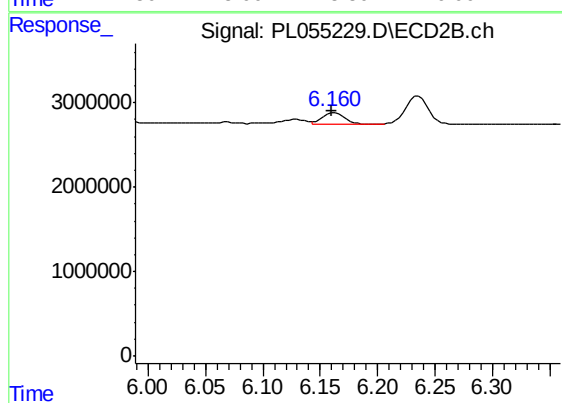

#25 Chlordane-3


R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 1762546
Conc: 5.48 ng/ml

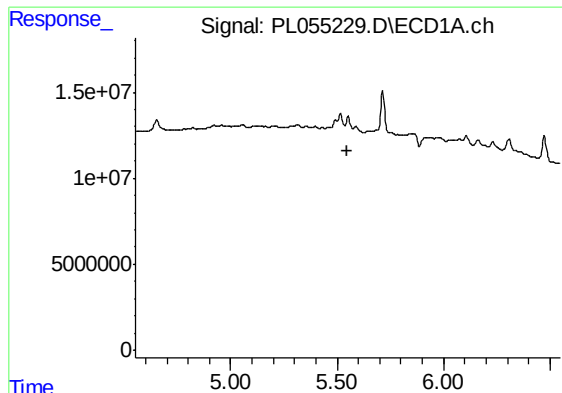

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-2

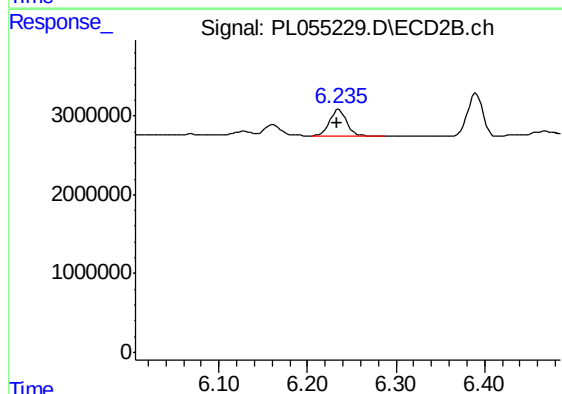


#26 Chlordane-4

R.T.: 6.236 min
Delta R.T.: 0.002 min
Response: 4400327
Conc: 11.45 ng/ml

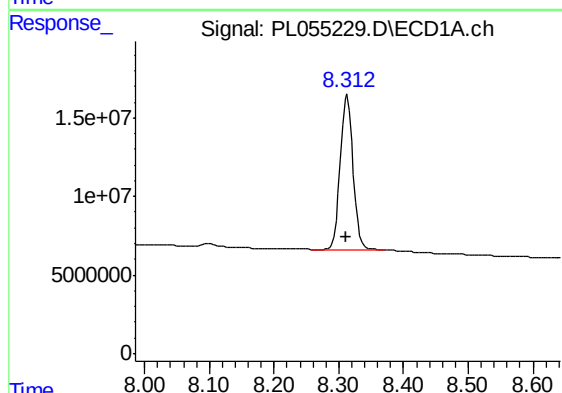

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.002 min
Response: 134807374
Conc: 14.53 ng/ml

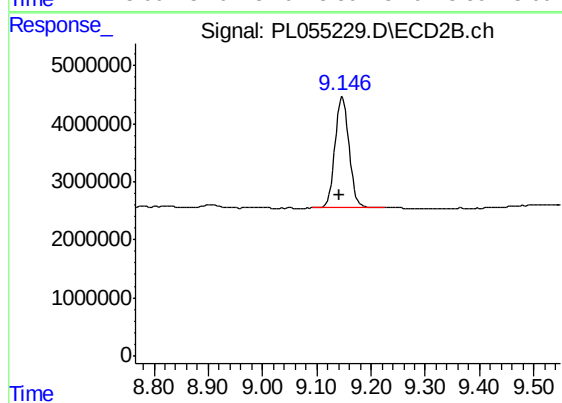

#28 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.005 min
Response: 34548891
Conc: 15.65 ng/ml