

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
 Data File : PL055230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 18:32
 Operator : SG\AJ
 Sample : K6413-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 K005-AB-WC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 01:02:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	123.5E6	35432854	11.740	13.410
28)	SA Decachlor...	8.313	9.148	132.7E6	34330079	14.299	15.552
Target Compounds							
5)	MB Aldrin	0.000	5.563f	0	1755977	N.D.	0.610 #
8)	B Heptachlo...	0.000	5.917	0	3571604	N.D.	1.401 #
11)	B alpha-Chl...	0.000	6.235	0	1461559	N.D.	0.557 #
12)	B 4,4'-DDE	5.715	6.390	23699747	7316625	1.778	3.001 #
14)	MA Endrin	0.000	6.752	0	1949053	N.D.	0.908 #
16)	A 4,4'-DDD	0.000	6.888	0	3120478	N.D.	1.641 #
17)	MA 4,4'-DDT	6.471	7.155f	14679490	2414927	1.458	1.230
26)	Chlordane-4	0.000	6.235	0	1461559	N.D.	3.802 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
Data File : PL055230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 18:32
Operator : SG\AJ
Sample : K6413-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 01:02:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

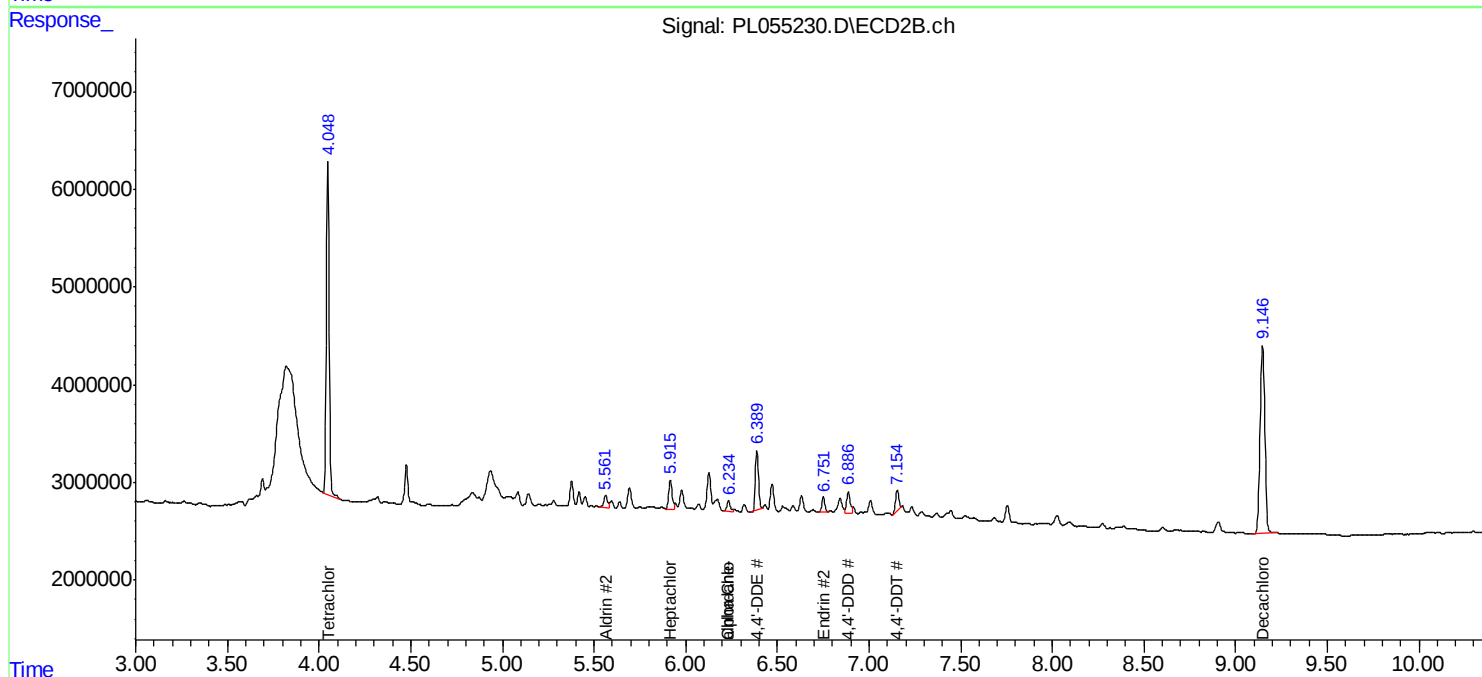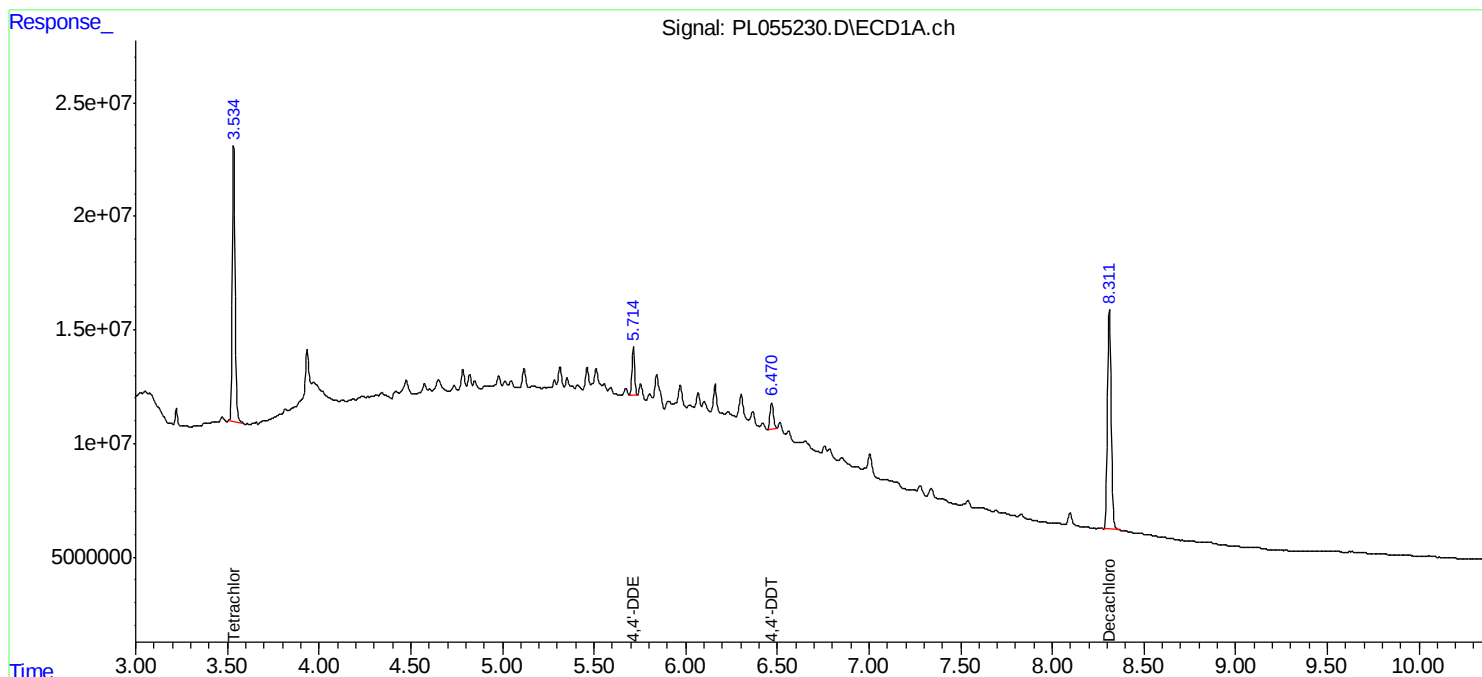


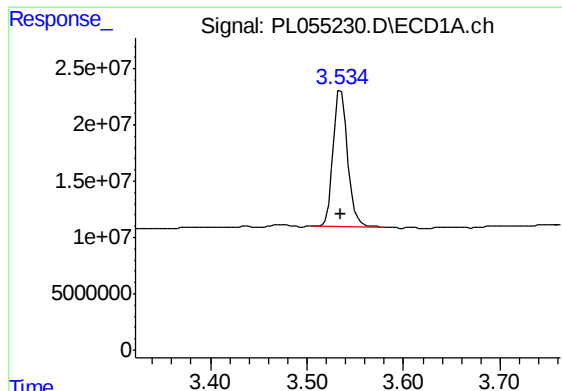

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 123467790
Conc: 11.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

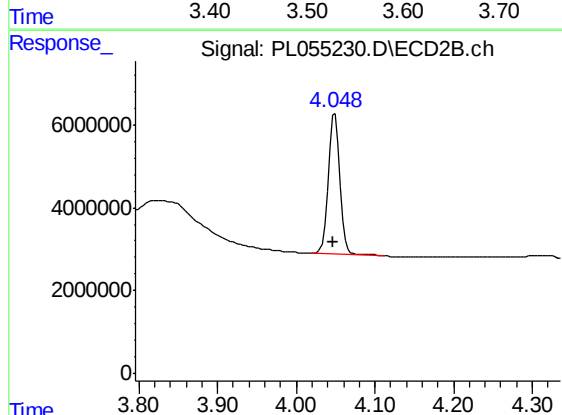


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 35432854
Conc: 13.41 ng/ml

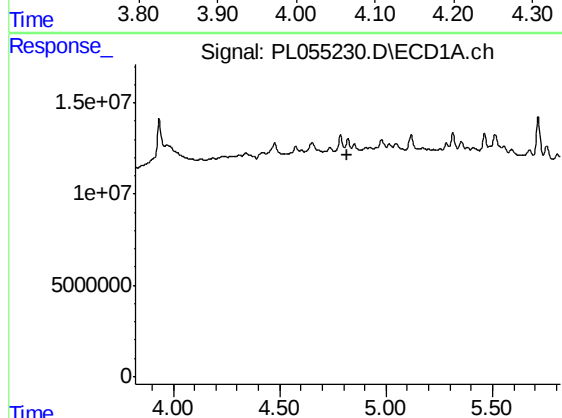


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

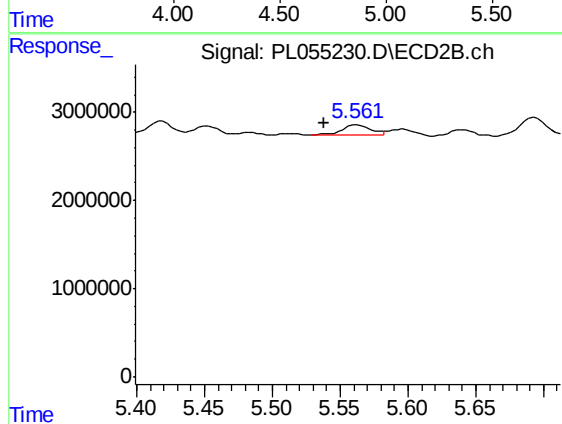

#5 Aldrin


R.T.: 5.563 min
Delta R.T.: 0.025 min
Response: 1755977
Conc: 0.61 ng/ml

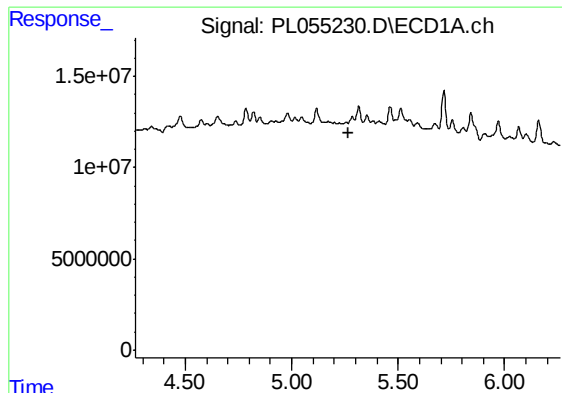

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

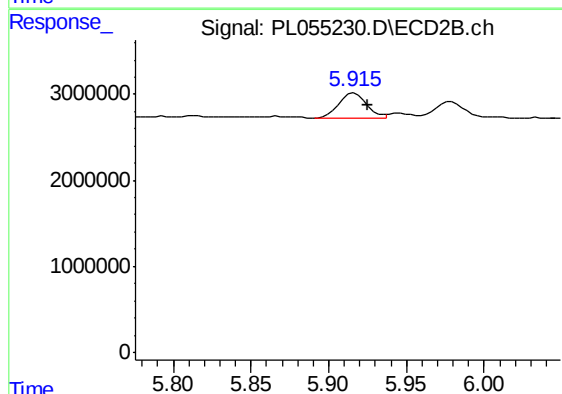


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.009 min
Response: 3571604
Conc: 1.40 ng/ml

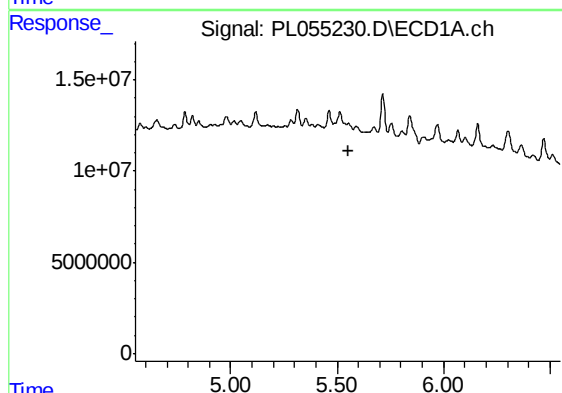


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

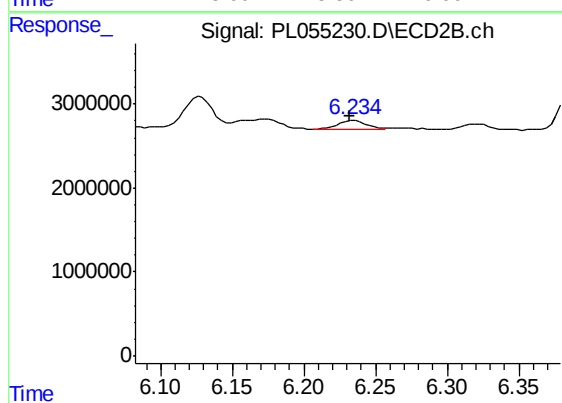

#11 alpha-Chlordane


R.T.: 6.235 min
Delta R.T.: 0.003 min
Response: 1461559
Conc: 0.56 ng/ml

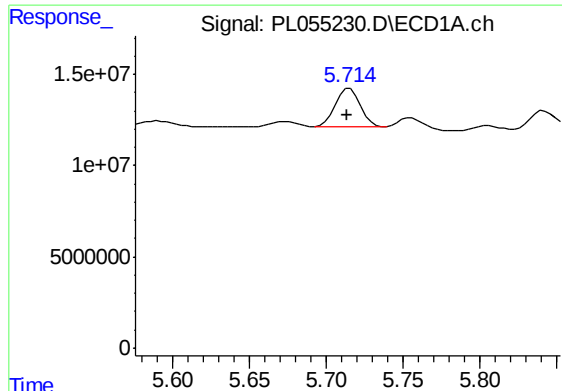

#12 4,4'-DDE


R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 23699747
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

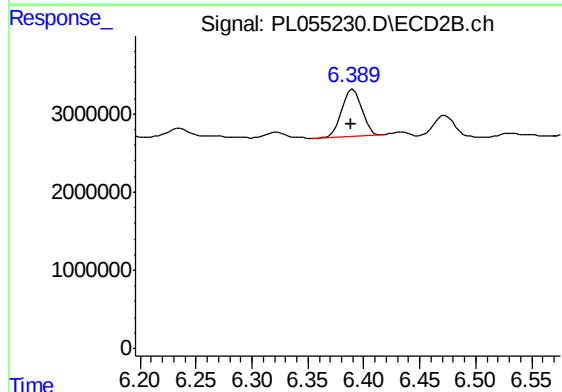


#12 4,4'-DDE

R.T.: 6.390 min
Delta R.T.: 0.001 min
Response: 7316625
Conc: 3.00 ng/ml

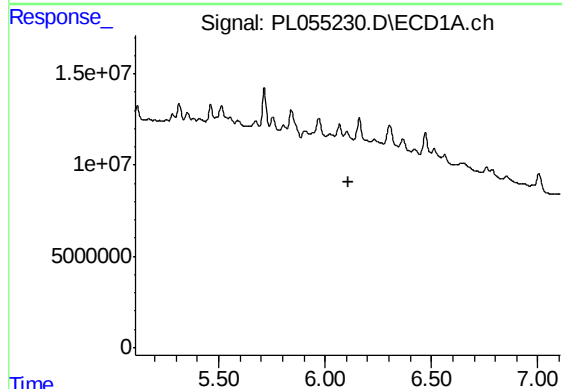


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.108 min
Response: 0
Conc: N.D.

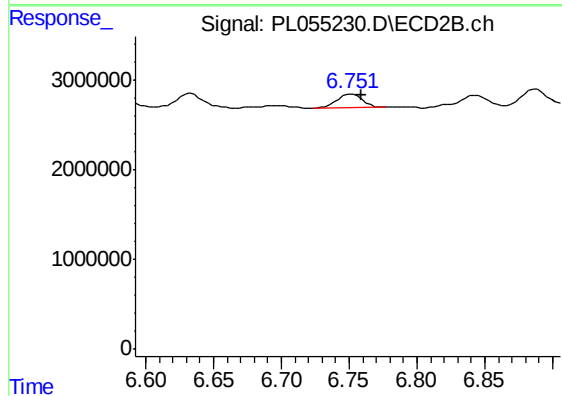

#14 Endrin


R.T.: 6.752 min
Delta R.T.: -0.007 min
Response: 1949053
Conc: 0.91 ng/ml

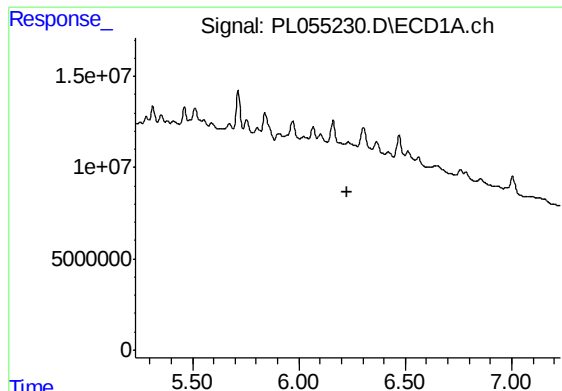

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

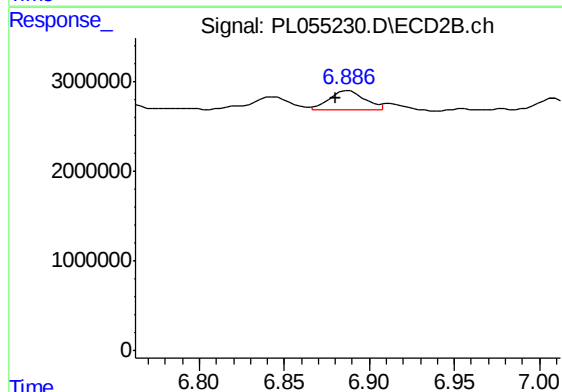


#16 4,4'-DDD

R.T.: 6.888 min
Delta R.T.: 0.007 min
Response: 3120478
Conc: 1.64 ng/ml

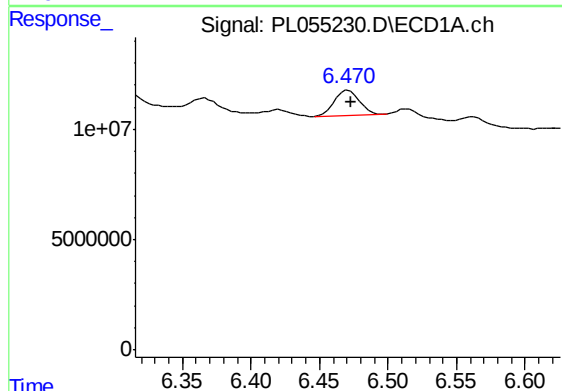


#17 4,4'-DDT

R.T.: 6.471 min
Delta R.T.: -0.002 min
Response: 14679490
Conc: 1.46 ng/ml

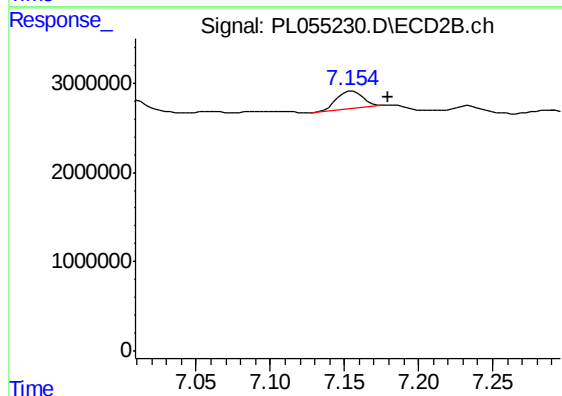

#17 4,4'-DDT


R.T.: 7.155 min
Delta R.T.: -0.025 min
Response: 2414927
Conc: 1.23 ng/ml

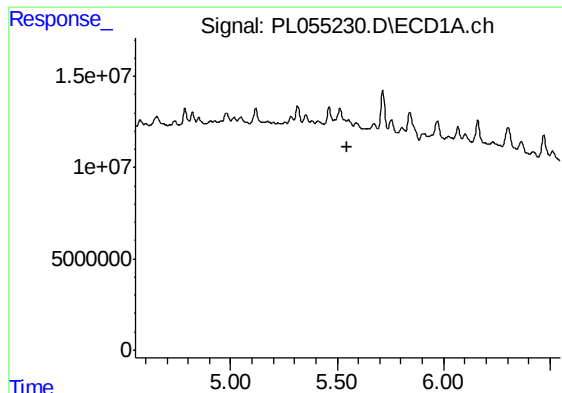

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
K005-AB-WC-1

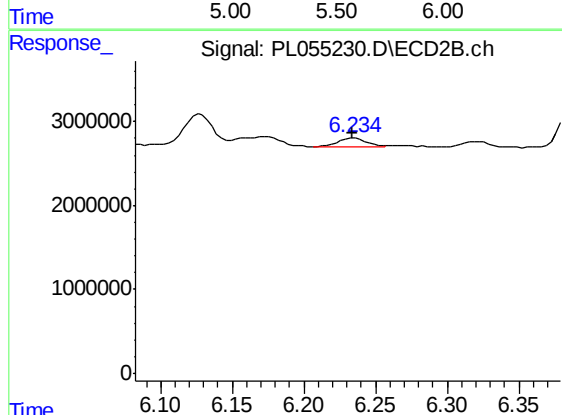


#26 Chlordane-4

R.T.: 6.235 min
Delta R.T.: 0.002 min
Response: 1461559
Conc: 3.80 ng/ml

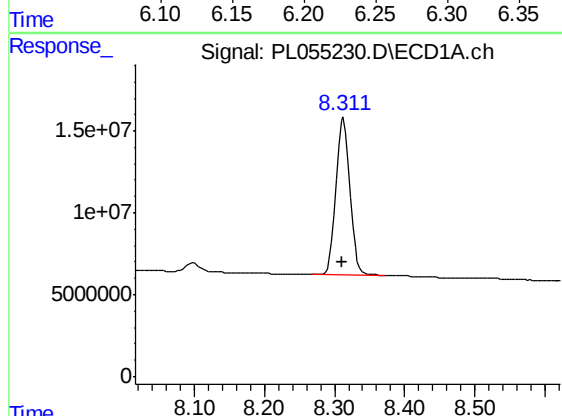

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.002 min
Response: 132672199
Conc: 14.30 ng/ml

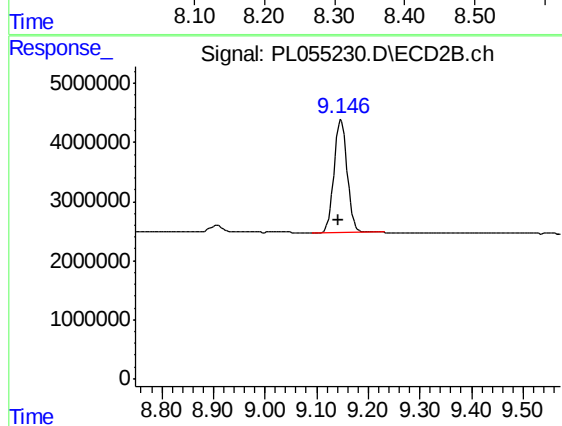

#28 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.005 min
Response: 34330079
Conc: 15.55 ng/ml