

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
 Data File : PL055232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 19:00
 Operator : SG\AJ
 Sample : K6417-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 01:03:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	120.5E6	34172504	11.457	12.933
28)	SA Decachlor...	8.311	9.147	113.1E6	28547503	12.192	12.932
Target Compounds							
8)	B Heptachlo...	0.000	5.917	0	1222089	N.D.	0.479 #
12)	B 4,4'-DDE	0.000	6.391	0	2631245	N.D.	1.079 #
13)	MA Dieldrin	5.841	6.533	28873593	2487165	2.068	0.975 #
14)	MA Endrin	0.000	6.751	0	2285195	N.D.	1.065 #
16)	A 4,4'-DDD	0.000	6.888	0	6800002	N.D.	3.577 #
17)	MA 4,4'-DDT	6.470	7.155f	58120853	13393915	5.773	6.825
19)	B Endosulfa...	0.000	7.288f	0	1418248	N.D.	0.679 #
20)	A Methoxychlor	7.004	0.000	51821878	0	10.753	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
Data File : PL055232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 19:00
Operator : SG\AJ
Sample : K6417-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 01:03:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

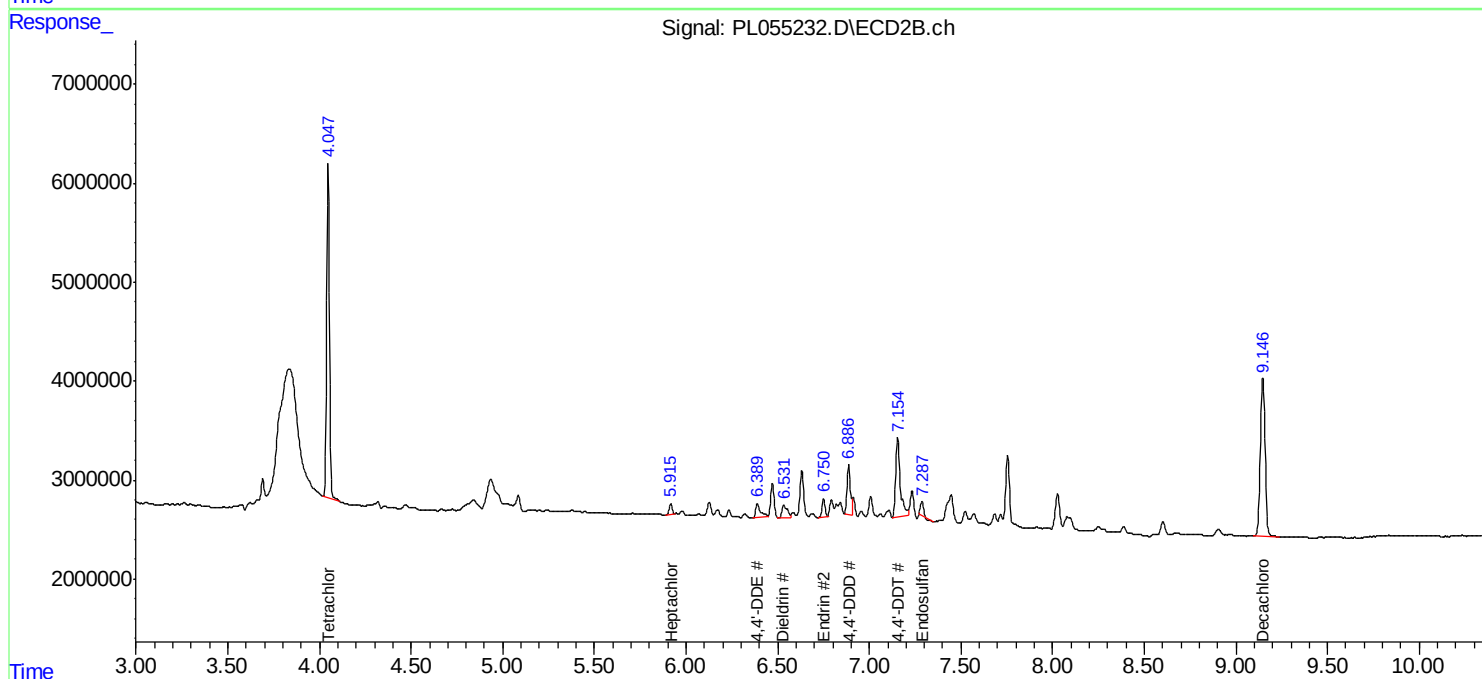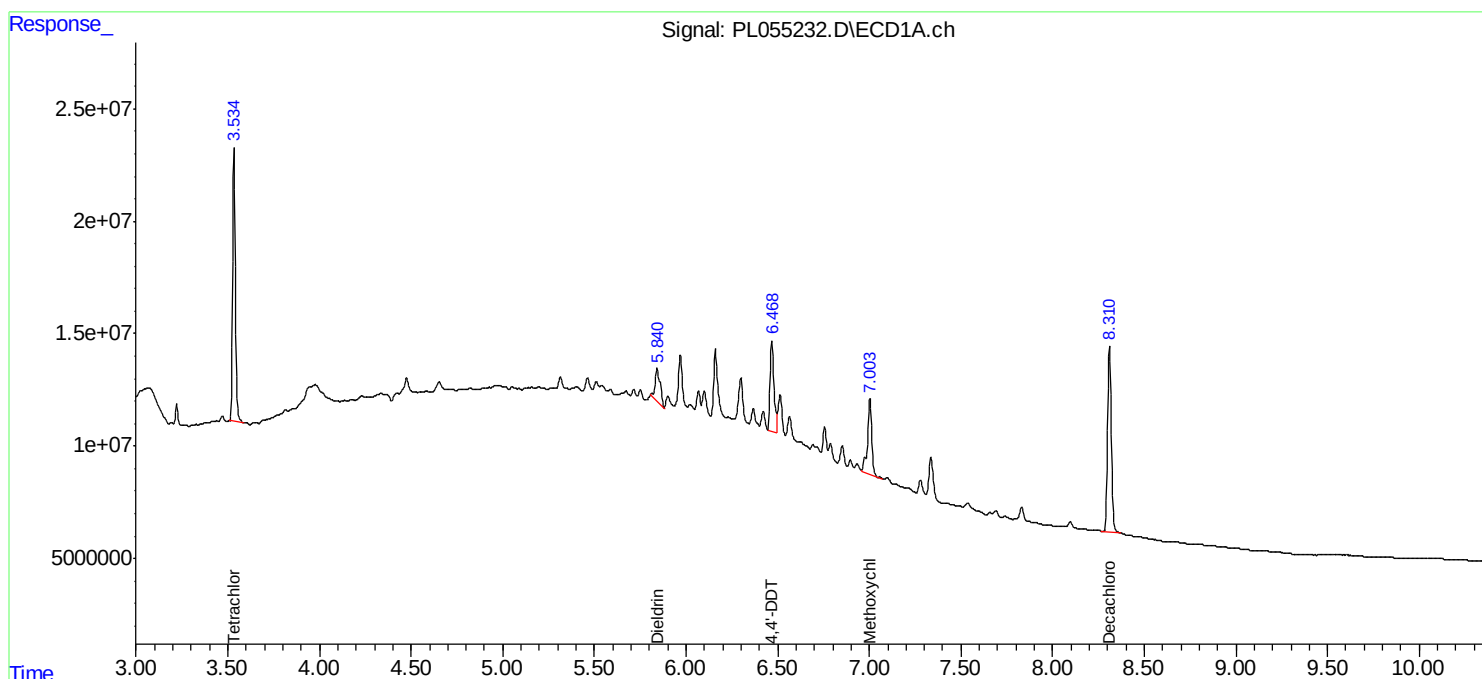


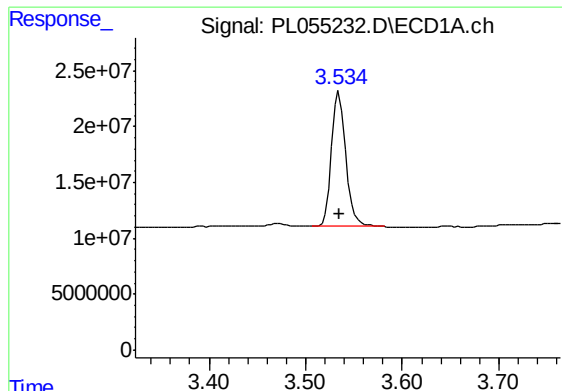

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 120492815
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

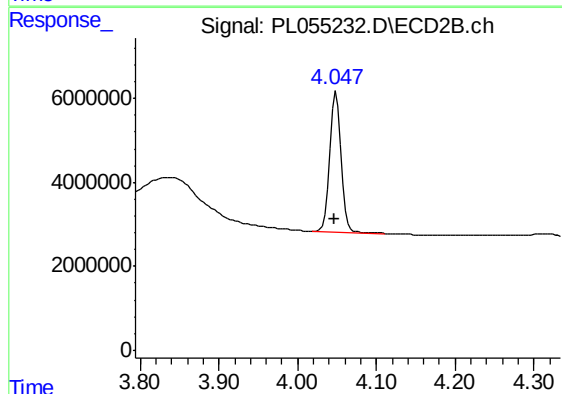


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.001 min
Response: 34172504
Conc: 12.93 ng/ml

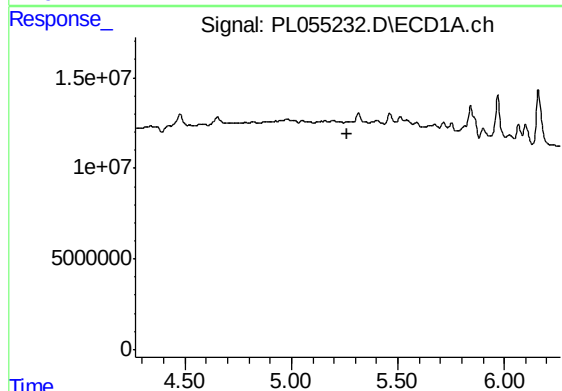


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

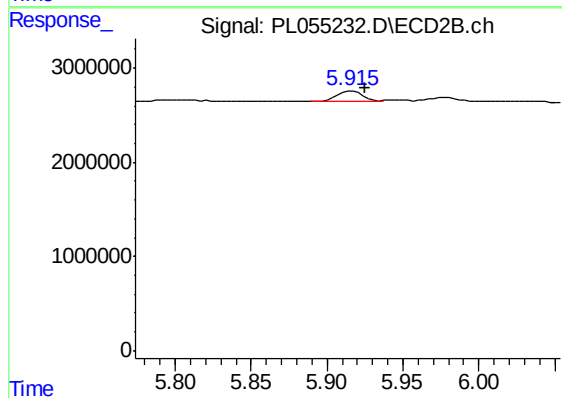

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.008 min
Response: 1222089
Conc: 0.48 ng/ml

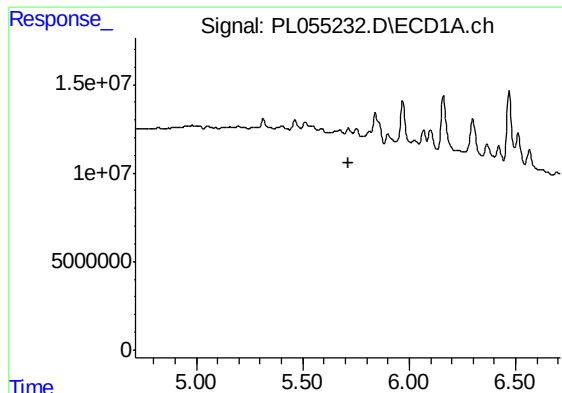

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.713 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

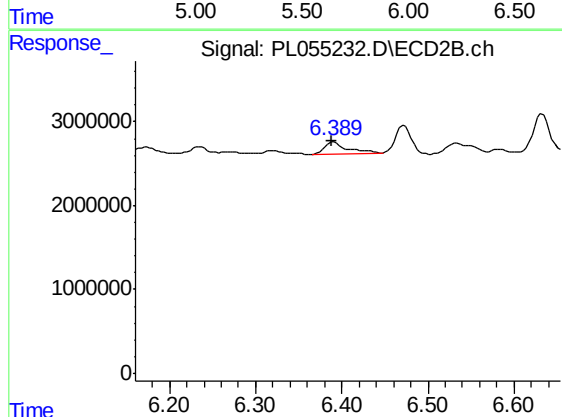


#12 4,4'-DDE

R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 2631245
Conc: 1.08 ng/ml

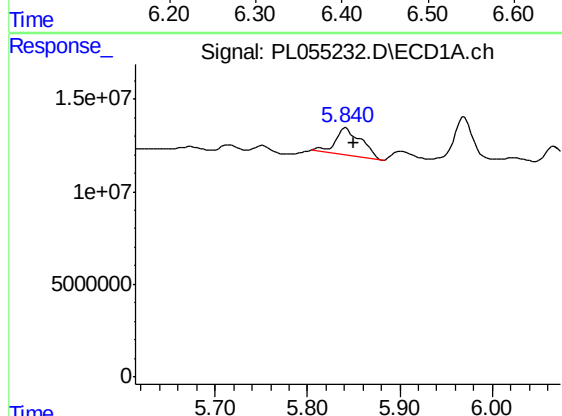


#13 Dieldrin

R.T.: 5.841 min
Delta R.T.: -0.008 min
Response: 28873593
Conc: 2.07 ng/ml

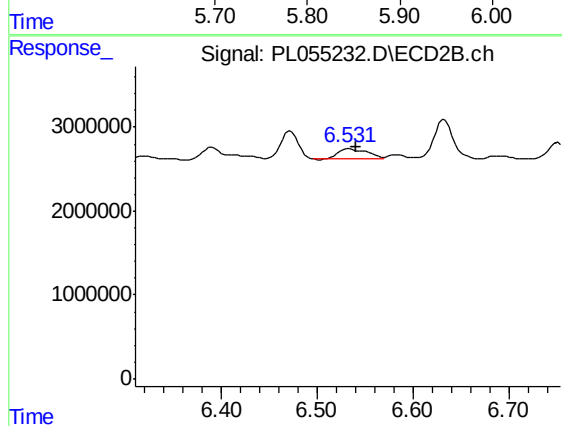

#13 Dieldrin


R.T.: 6.533 min
Delta R.T.: -0.007 min
Response: 2487165
Conc: 0.97 ng/ml

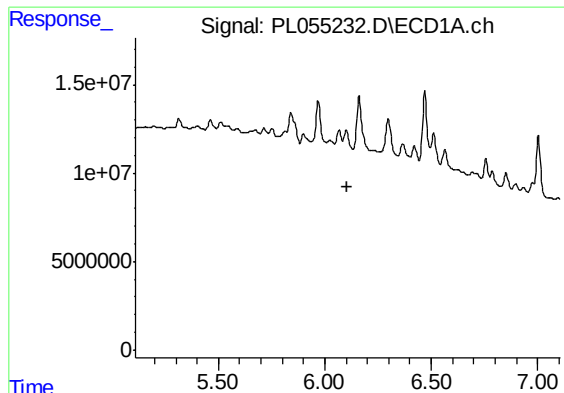

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

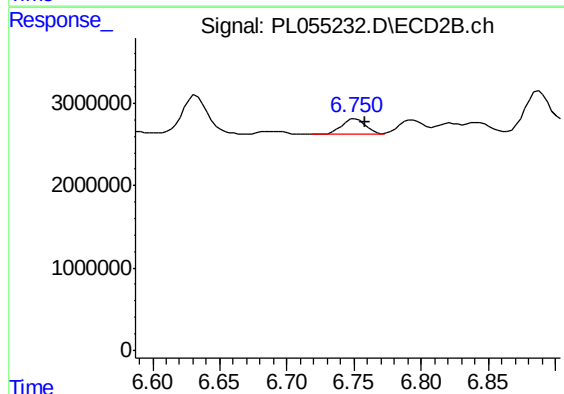


#14 Endrin

R.T.: 6.751 min
Delta R.T.: -0.007 min
Response: 2285195
Conc: 1.06 ng/ml

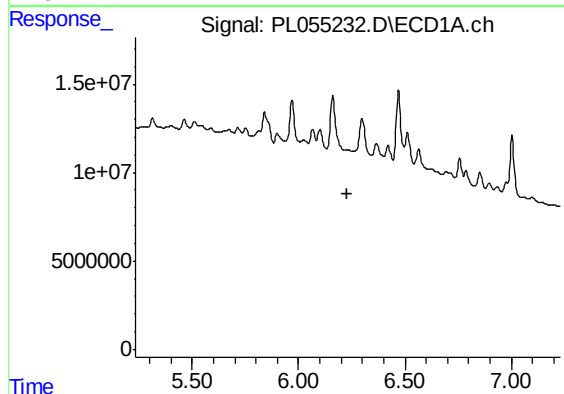


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

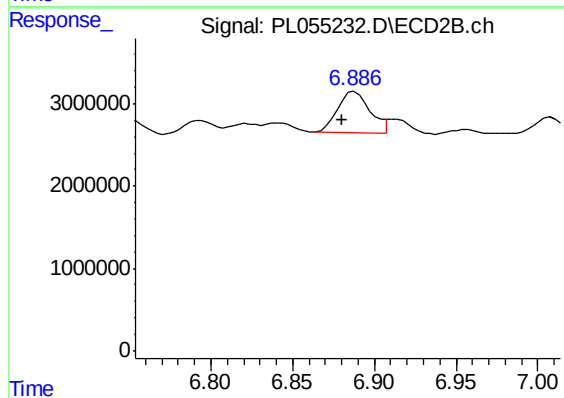

#16 4,4'-DDD


R.T.: 6.888 min
Delta R.T.: 0.007 min
Response: 6800002
Conc: 3.58 ng/ml

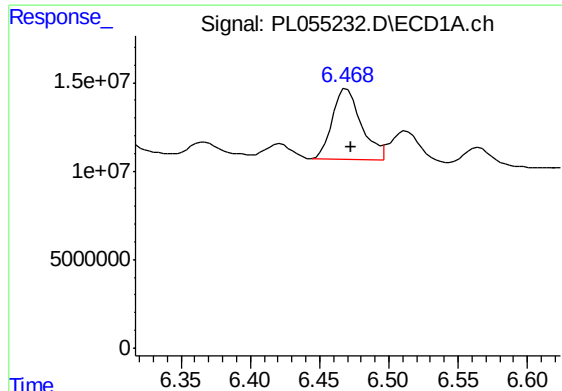

#17 4,4'-DDT


R.T.: 6.470 min
Delta R.T.: -0.004 min
Response: 58120853
Conc: 5.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

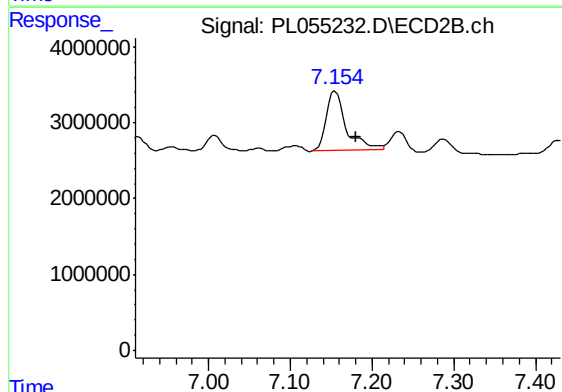


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: -0.025 min
Response: 13393915
Conc: 6.82 ng/ml

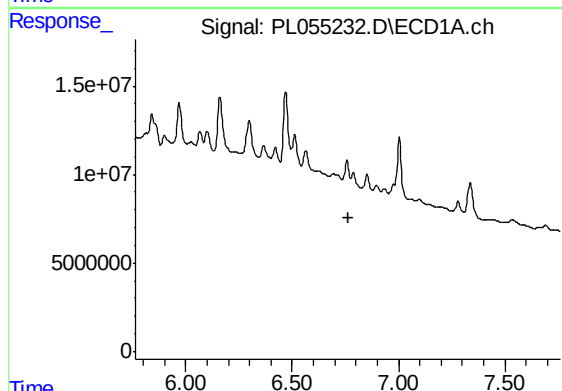


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

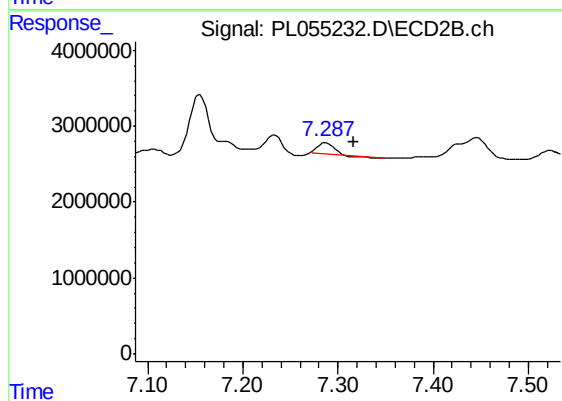

#19 Endosulfan Sulfate


R.T.: 7.288 min
Delta R.T.: -0.029 min
Response: 1418248
Conc: 0.68 ng/ml

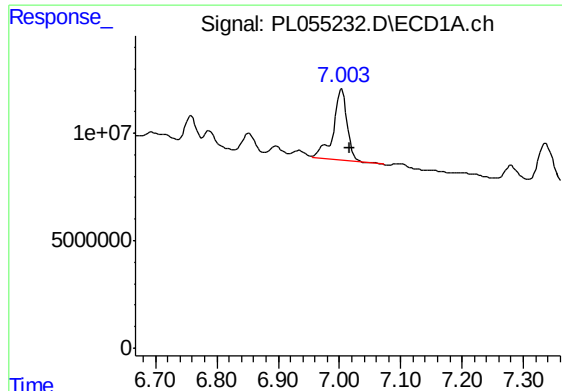

#20 Methoxychlor


R.T.: 7.004 min
Delta R.T.: -0.014 min
Response: 51821878
Conc: 10.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

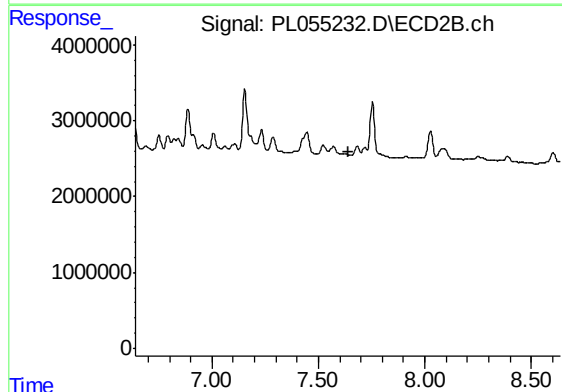


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.640 min
Response: 0
Conc: N.D.

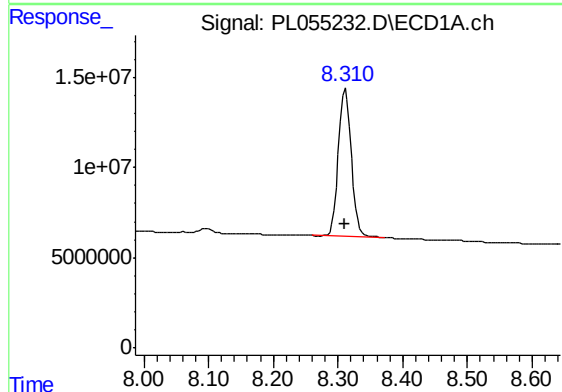

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 113130289
Conc: 12.19 ng/ml

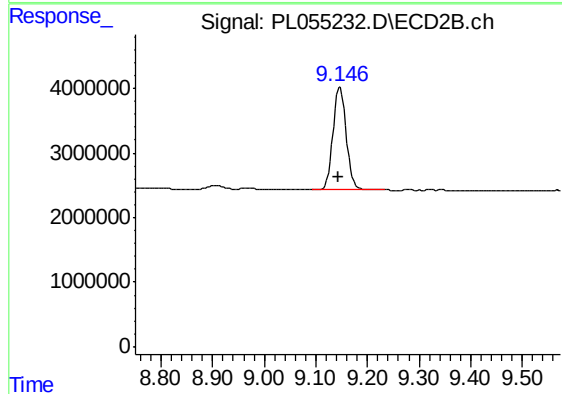

#28 Decachlorobiphenyl

R.T.: 9.147 min
Delta R.T.: 0.004 min
Response: 28547503
Conc: 12.93 ng/ml