

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
 Data File : PL055234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 19:29
 Operator : SG\AJ
 Sample : K6421-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 01:03:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	227.3E6	59203946	21.615	22.407
28)	SA Decachlor...	8.313	9.147	183.8E6	45680495	19.811	20.694
Target Compounds							
3)	MA gamma-BHC...	4.270	4.708f	9001132	8176803	0.546	2.392 #
9)	A Endosulfan I	5.629f	0.000	44734835	0	3.386	N.D. #
10)	B gamma-Chl...	0.000	6.153	0	5653640	N.D.	2.130 #
13)	MA Dieldrin	5.849	6.542	44848461	2585761	3.213	1.013 #
14)	MA Endrin	0.000	6.752	0	2013676	N.D.	0.938 #
16)	A 4,4'-DDD	0.000	6.887	0	4711955	N.D.	2.479 #
17)	MA 4,4'-DDT	6.471	7.156f	23100554	6066663	2.295	3.091 #
21)	B Endrin ke...	0.000	7.783	0	3931189	N.D.	1.765 #
25)	Chlordane-3	0.000	6.153	0	5653640	N.D.	17.568 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
Data File : PL055234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 19:29
Operator : SG\AJ
Sample : K6421-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 01:03:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

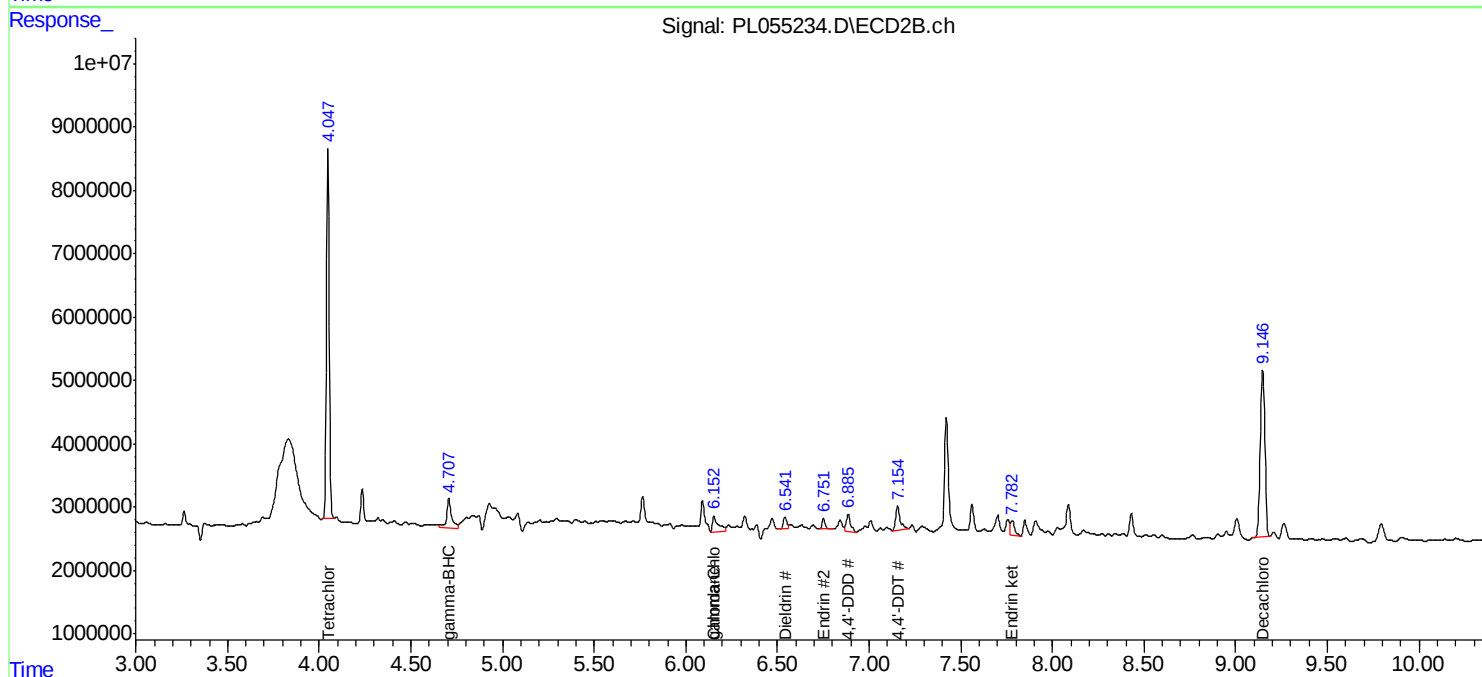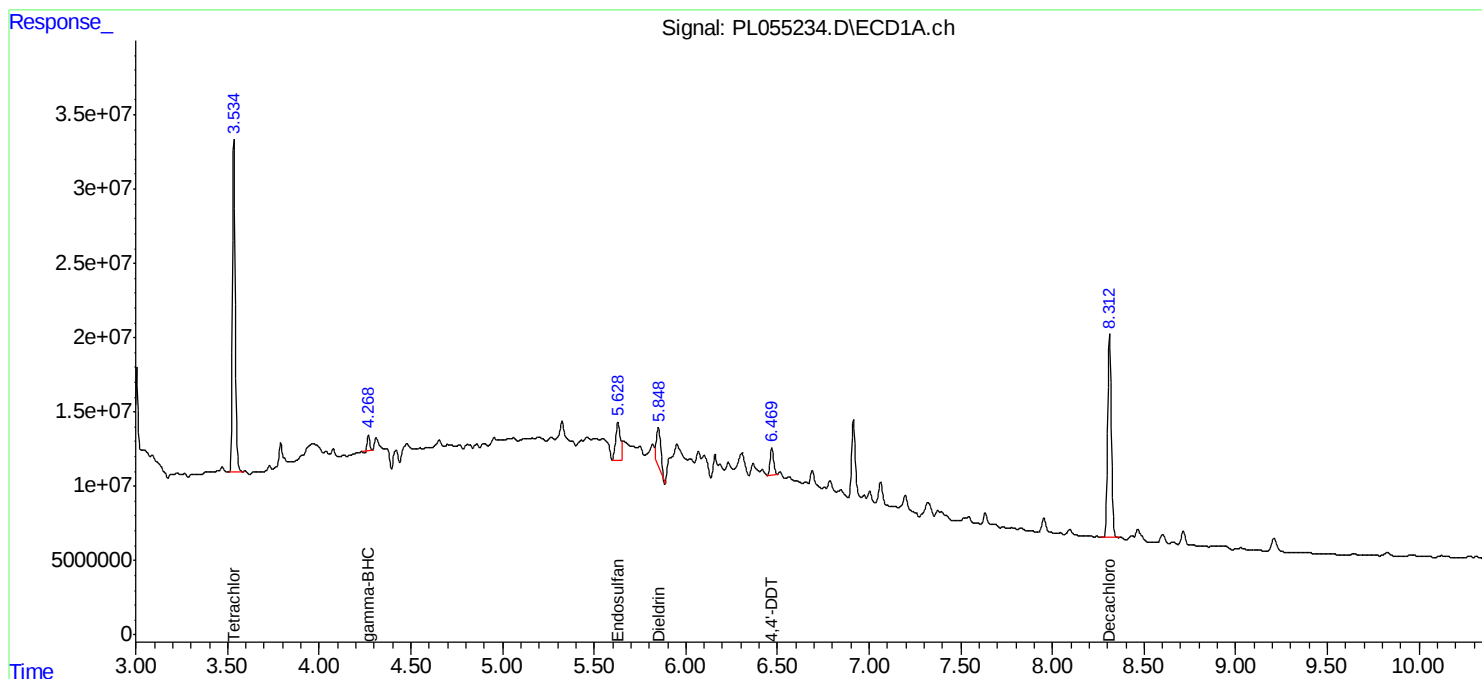


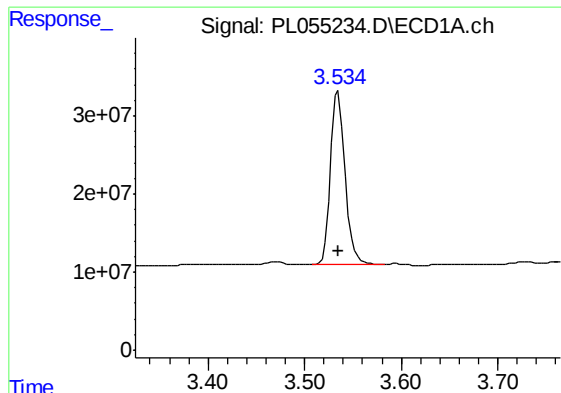

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 227318395
Conc: 21.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

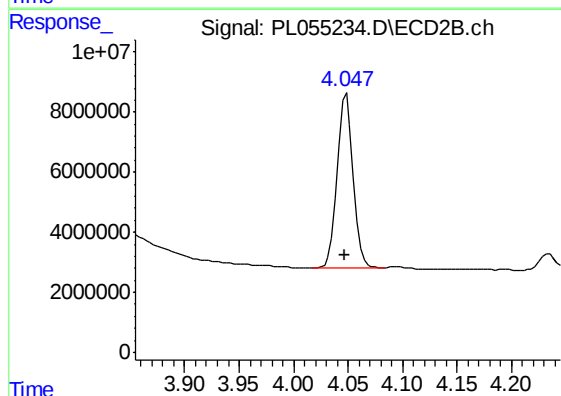


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.001 min
Response: 59203946
Conc: 22.41 ng/ml

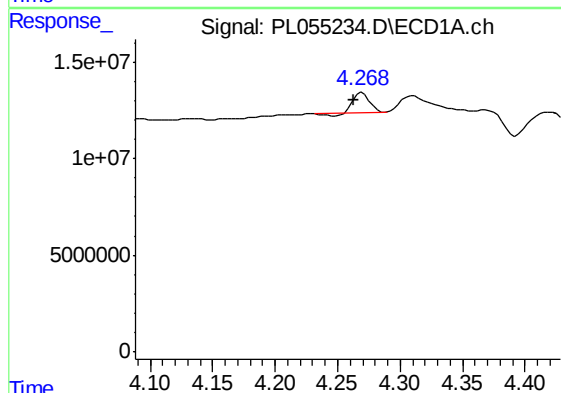


#3 gamma-BHC (Lindane)

R.T.: 4.270 min
Delta R.T.: 0.006 min
Response: 9001132
Conc: 0.55 ng/ml

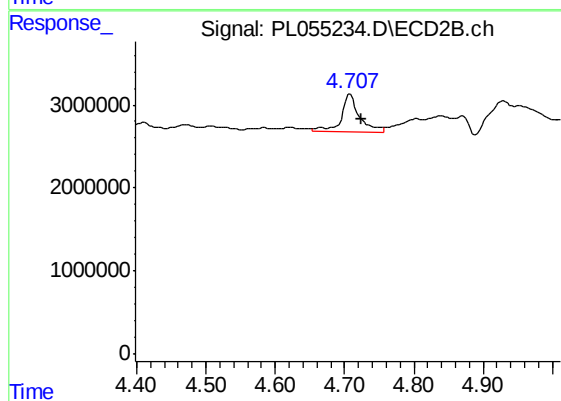

#3 gamma-BHC (Lindane)


R.T.: 4.708 min
Delta R.T.: -0.016 min
Response: 8176803
Conc: 2.39 ng/ml

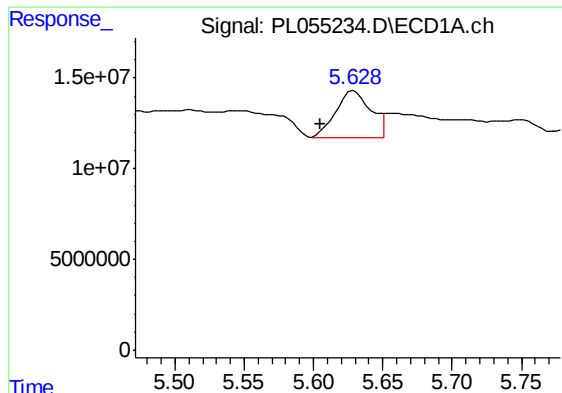

#9 Endosulfan I


R.T.: 5.629 min
Delta R.T.: 0.024 min
Response: 44734835
Conc: 3.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

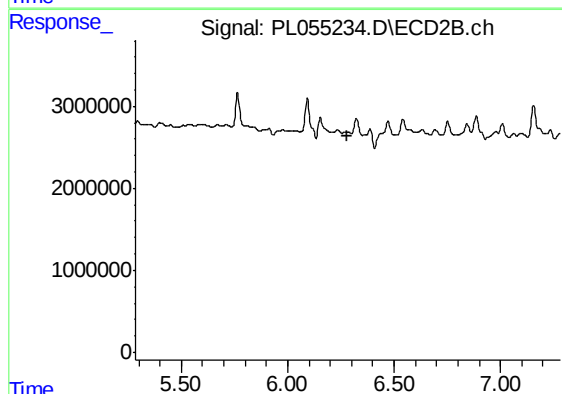


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

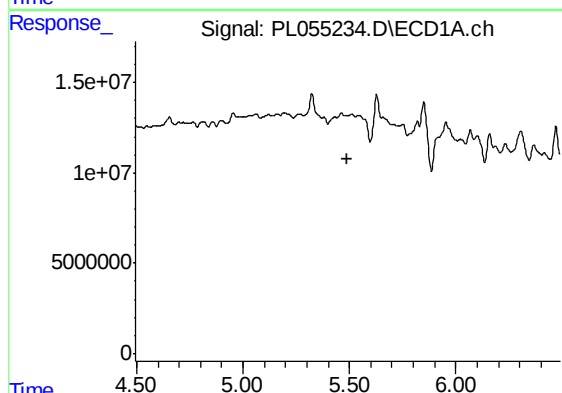


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

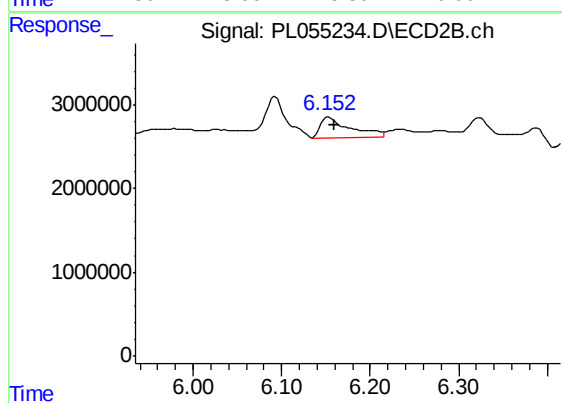

#10 gamma-Chlordane


R.T.: 6.153 min
Delta R.T.: -0.006 min
Response: 5653640
Conc: 2.13 ng/ml

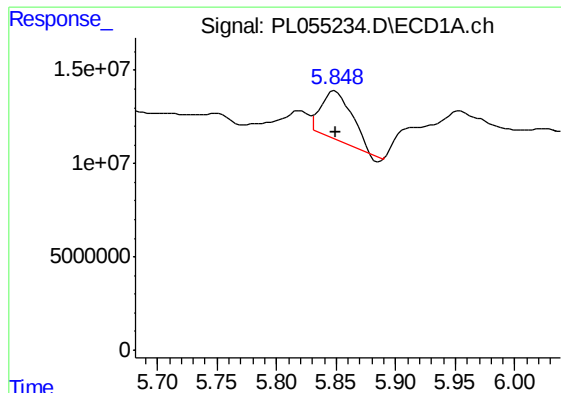

#13 Dielddrin


R.T.: 5.849 min
Delta R.T.: 0.000 min
Response: 44848461
Conc: 3.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

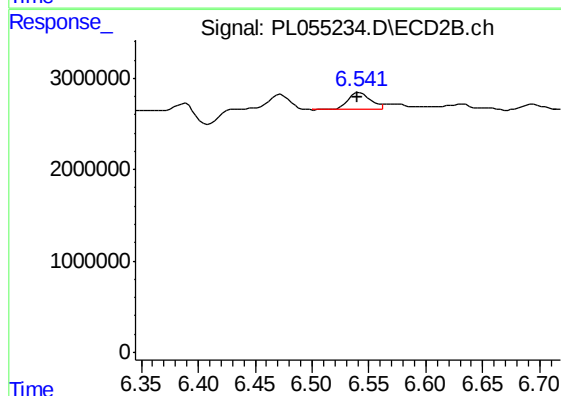


#13 Dielddrin

R.T.: 6.542 min
Delta R.T.: 0.002 min
Response: 2585761
Conc: 1.01 ng/ml

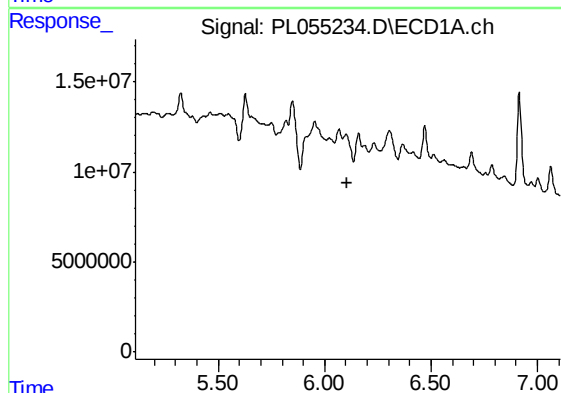


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.108 min
Response: 0
Conc: N.D.

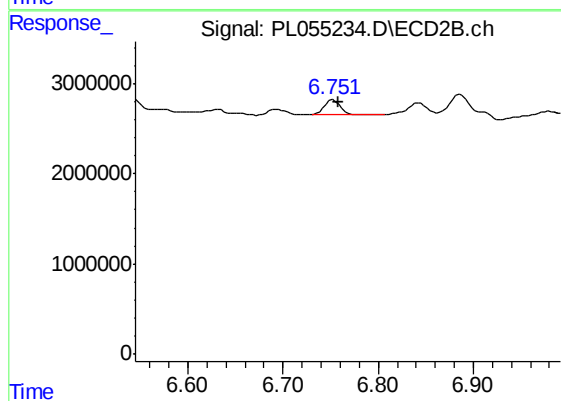

#14 Endrin


R.T.: 6.752 min
Delta R.T.: -0.006 min
Response: 2013676
Conc: 0.94 ng/ml

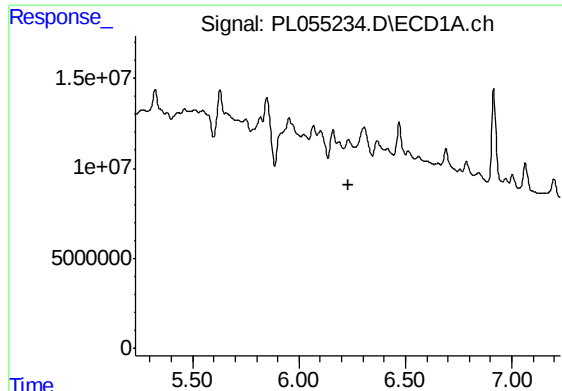

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

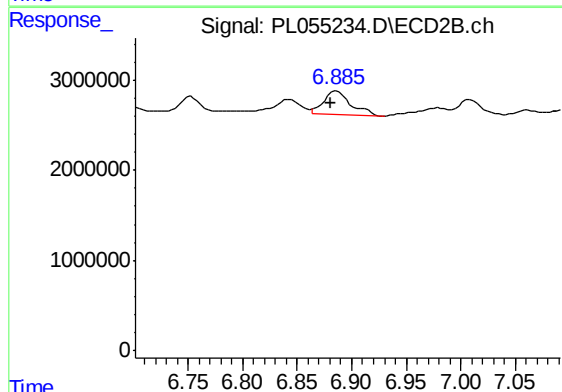


#16 4,4'-DDD

R.T.: 6.887 min
Delta R.T.: 0.006 min
Response: 4711955
Conc: 2.48 ng/ml

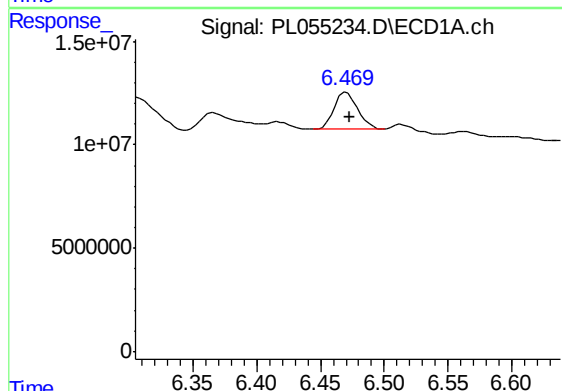


#17 4,4'-DDT

R.T.: 6.471 min
Delta R.T.: -0.003 min
Response: 23100554
Conc: 2.29 ng/ml

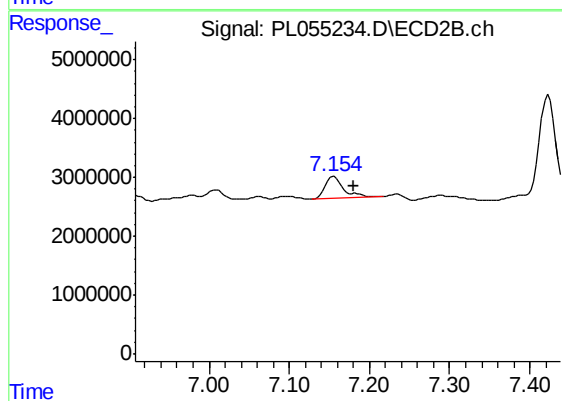

#17 4,4'-DDT


R.T.: 7.156 min
Delta R.T.: -0.024 min
Response: 6066663
Conc: 3.09 ng/ml

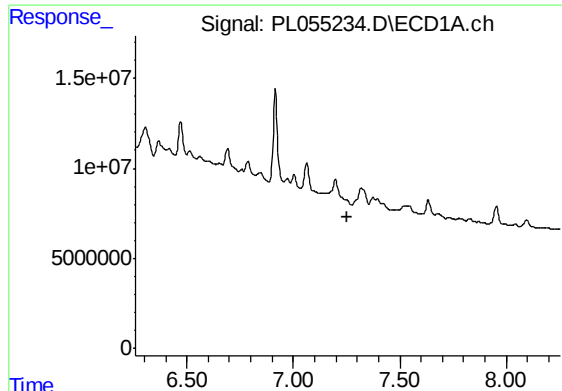

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

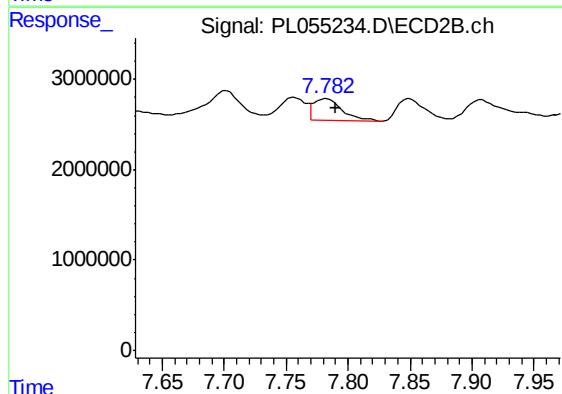


#21 Endrin ketone

R.T.: 7.783 min
Delta R.T.: -0.007 min
Response: 3931189
Conc: 1.77 ng/ml

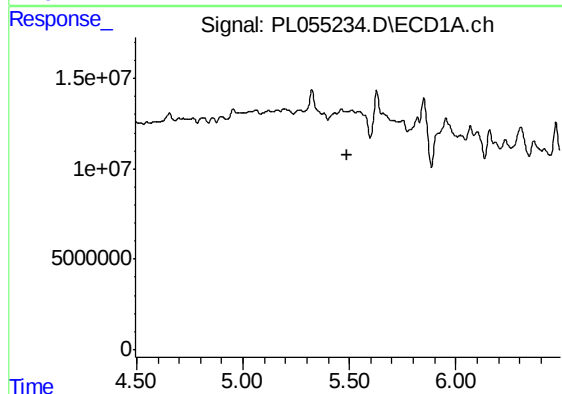


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

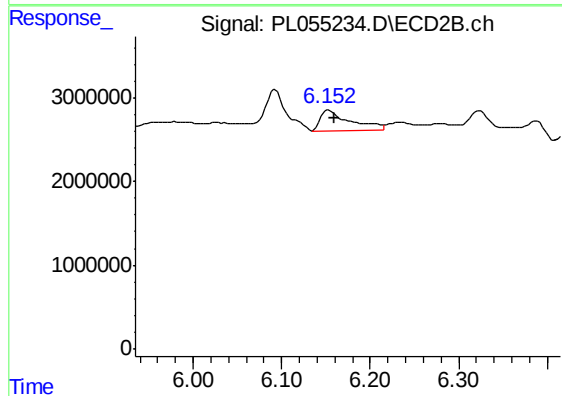

#25 Chlordane-3


R.T.: 6.153 min
Delta R.T.: -0.007 min
Response: 5653640
Conc: 17.57 ng/ml

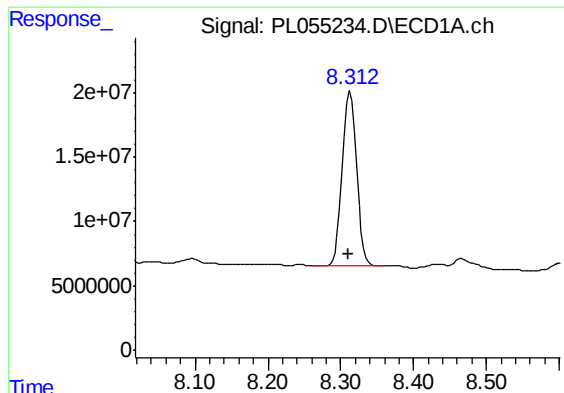

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.003 min
Response: 183820887
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

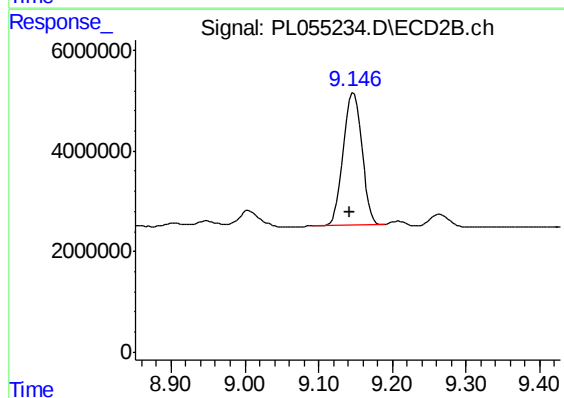

#28 Decachlorobiphenyl

R.T.: 9.147 min
Delta R.T.: 0.005 min
Response: 45680495
Conc: 20.69 ng/ml