

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
 Data File : PL055227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 17:50
 Operator : SG\AJ
 Sample : K6413-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 K005-AA-WC-1

Manual Integrations
 APPROVED

Ankita
 12/26/2019 12:25:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 01:02:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	116.5E6	33230233	11.078	12.576
28)	SA Decachlor...	8.313	9.147	121.0E6	31035591	13.043	14.059
Target Compounds							
12)	B 4,4'-DDE	5.714	6.391	14087667	3967748	1.057	1.627 #
17)	MA 4,4'-DDT	6.469	7.181	7816751	1450027	0.776m	0.739m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122419\
Data File : PL055227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 17:50
Operator : SG\AJ
Sample : K6413-06
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-1


Manual Integrations
APPROVED

Ankita
12/26/2019 12:25:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 01:02:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

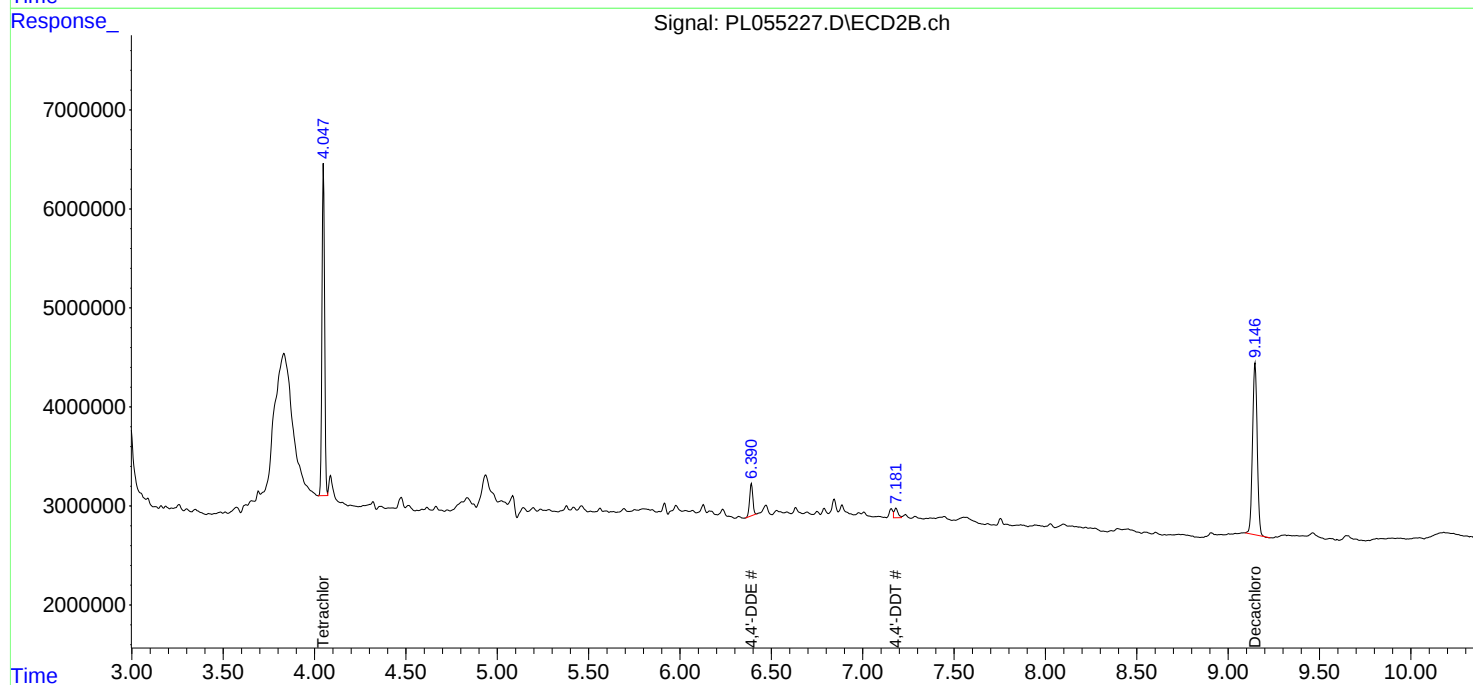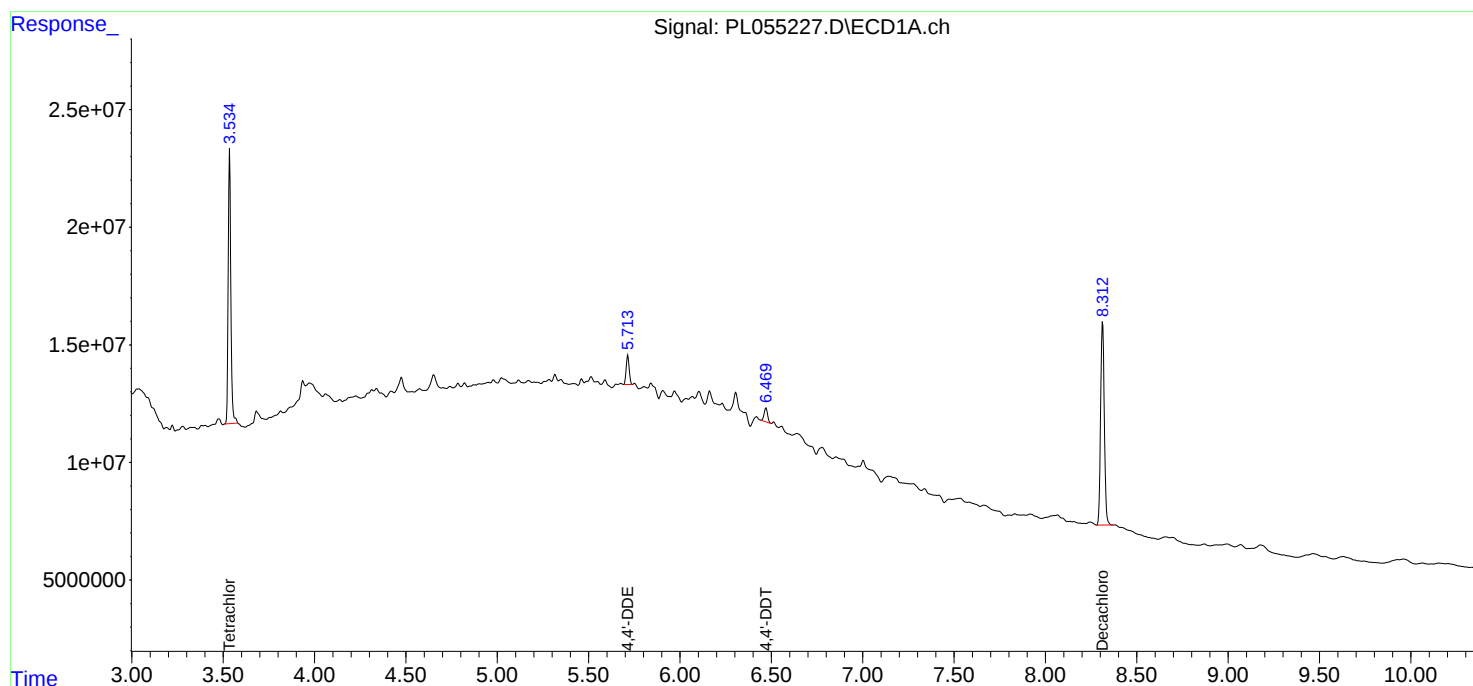

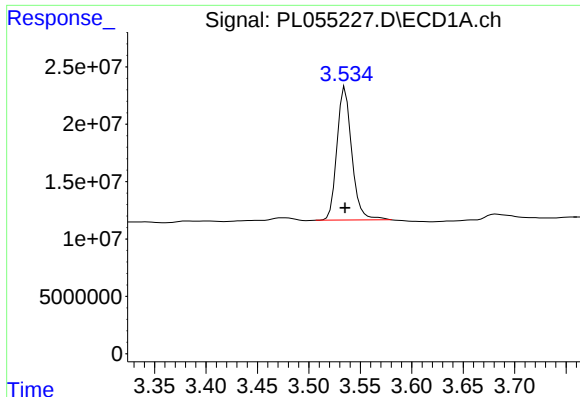


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 116502305
Conc: 11.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-1


Manual Integrations
APPROVED

Ankita
12/26/2019 12:25:47 PM

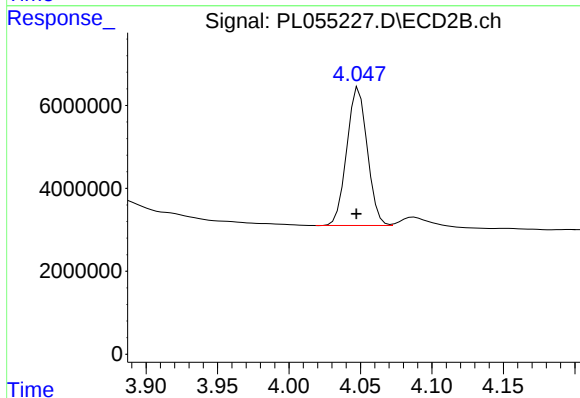


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 33230233
Conc: 12.58 ng/ml

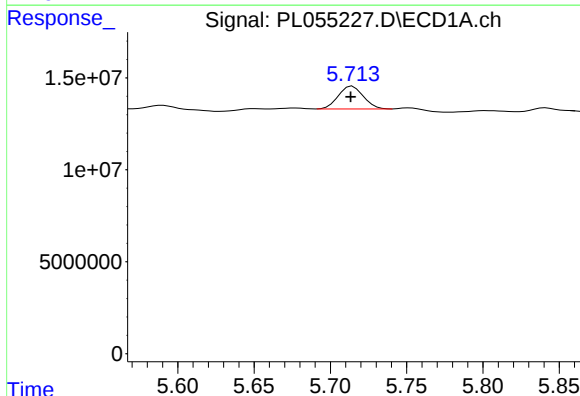


#12 4,4'-DDE

R.T.: 5.714 min
Delta R.T.: 0.001 min
Response: 14087667
Conc: 1.06 ng/ml

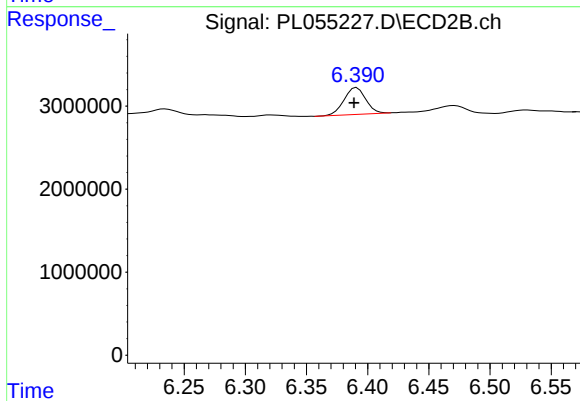

#12 4,4'-DDE

R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 3967748
Conc: 1.63 ng/ml

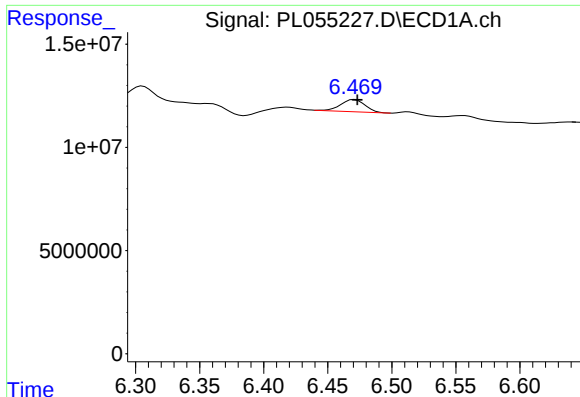


#17 4,4'-DDT

R.T.: 6.469 min
Delta R.T.: -0.004 min
Response: 7816751
Conc: 0.78 ng/ml m

Instrument :
ECD_L
ClientSampleId :
K005-AA-WC-1


Manual Integrations
APPROVED

Ankita
12/26/2019 12:25:47 PM

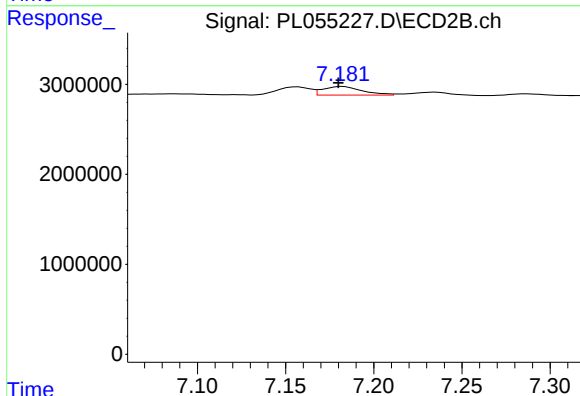


#17 4,4'-DDT

R.T.: 7.181 min
Delta R.T.: 0.001 min
Response: 1450027
Conc: 0.74 ng/ml m

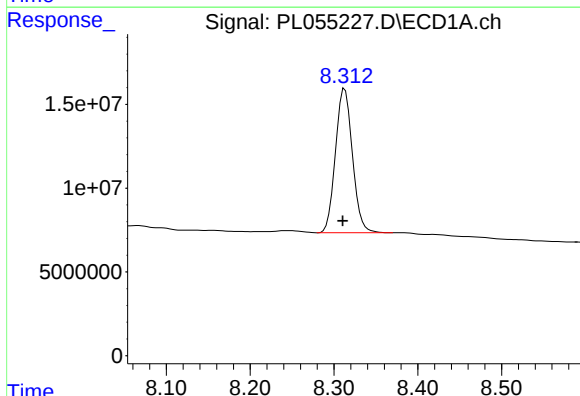

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.002 min
Response: 121024288
Conc: 13.04 ng/ml

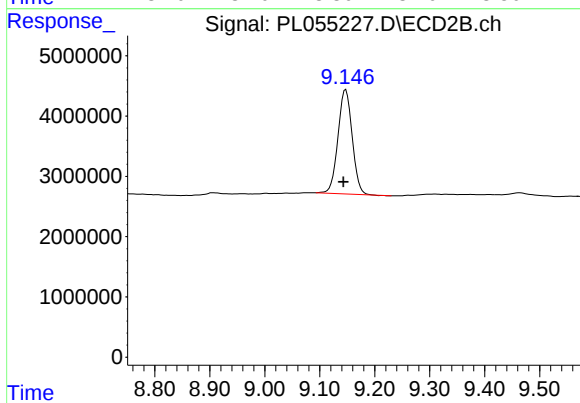

#28 Decachlorobiphenyl

R.T.: 9.147 min
Delta R.T.: 0.005 min
Response: 31035591
Conc: 14.06 ng/ml