

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
 Data File : PL063821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2020 15:12
 Operator : AR\AJ
 Sample : L5198-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 00:36:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.111	40984807	33902541	13.671	13.279
28)	SA Decachlor...	8.178	9.268	32717633	25392306	11.875	12.879
Target Compounds							
5)	MB Aldrin	4.672f	0.000	2129888	0	0.533	N.D. #
10)	B gamma-Chl...	5.390f	6.255	10785234	3172751	2.837	1.147 #
11)	B alpha-Chl...	5.425	6.327	7329200	7020466	1.954	2.543 #
12)	B 4,4'-DDE	5.592	6.484	3718853	4107802	1.082	1.663 #
17)	MA 4,4'-DDT	6.343	0.000	5488429	0	2.071	N.D. #
23)	Chlordane-1	4.302	0.000	2129377	0	20.778	N.D. #
25)	Chlordane-3	5.390f	6.255	10785234	3172751	33.006	9.260 #
26)	Chlordane-4	5.425	6.327	7329200	7020466	27.392	17.080 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
Data File : PL063821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2020 15:12
Operator : AR\AJ
Sample : L5198-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 00:36:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

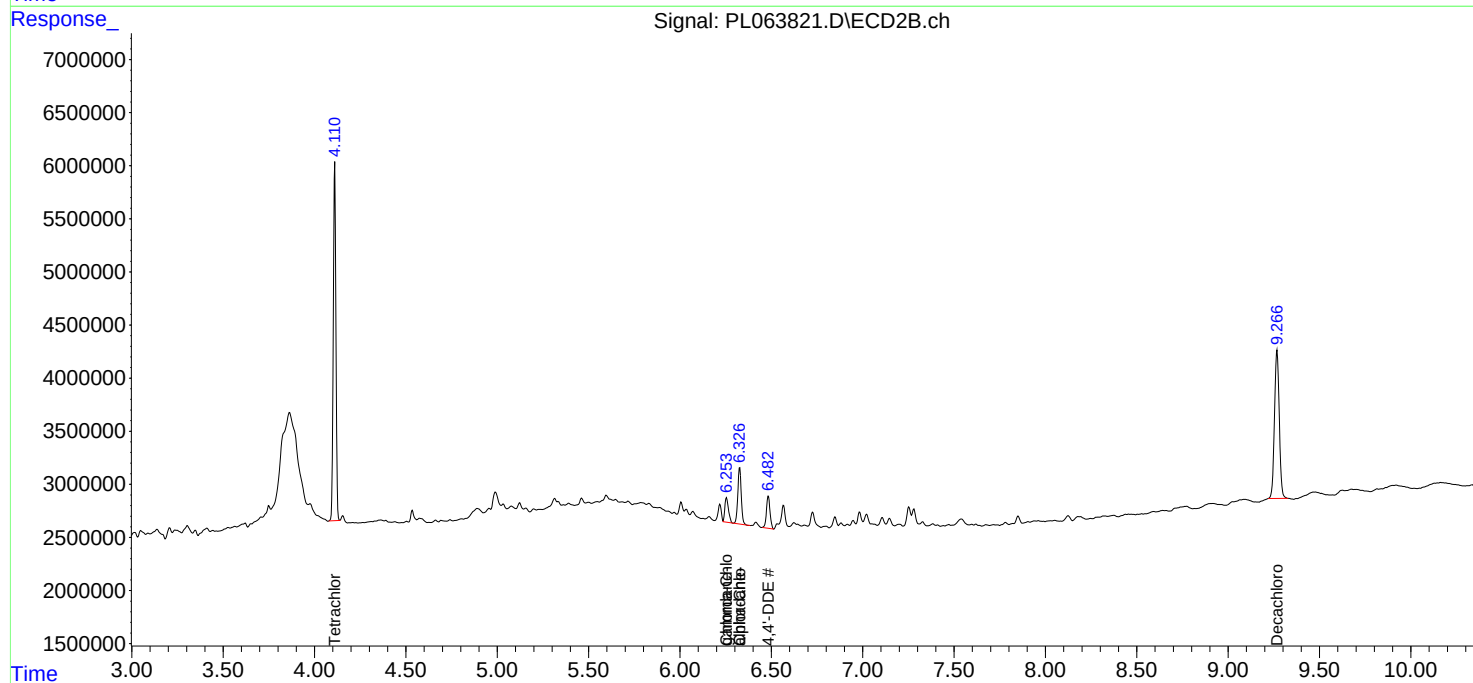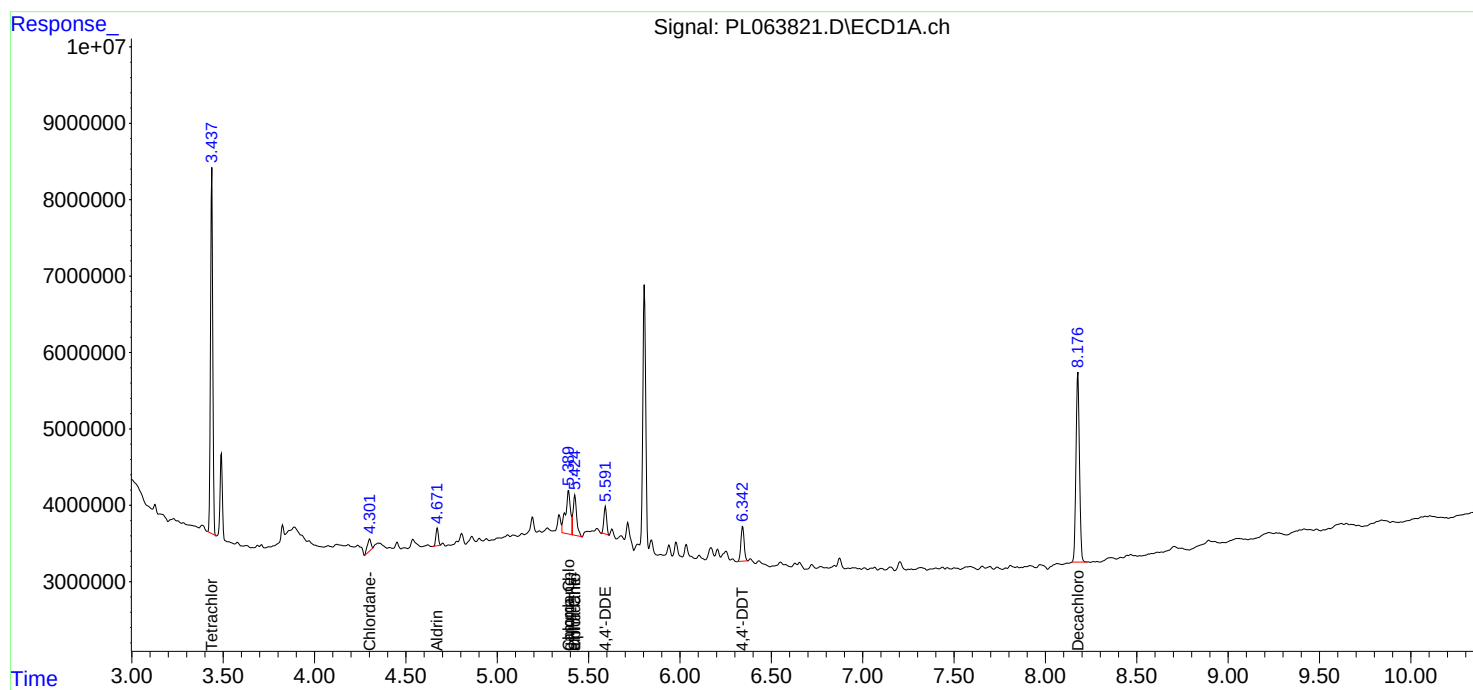


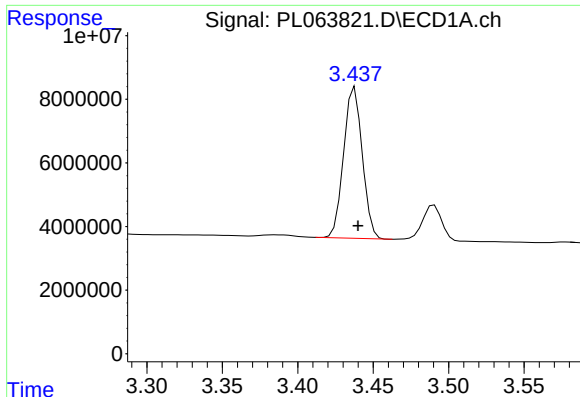

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 40984807
Conc: 13.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

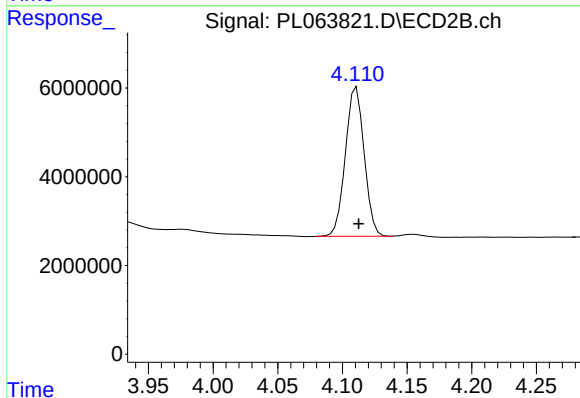


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 33902541
Conc: 13.28 ng/ml

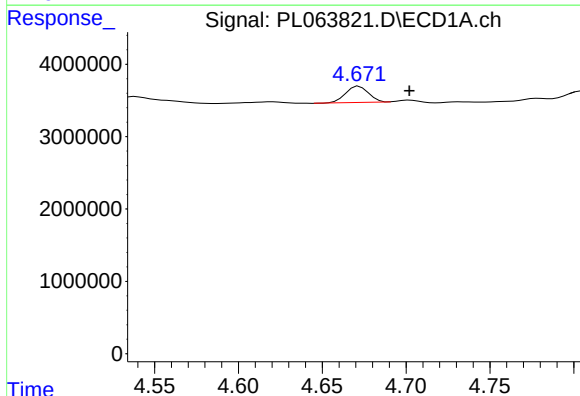


#5 Aldrin

R.T.: 4.672 min
Delta R.T.: -0.030 min
Response: 2129888
Conc: 0.53 ng/ml

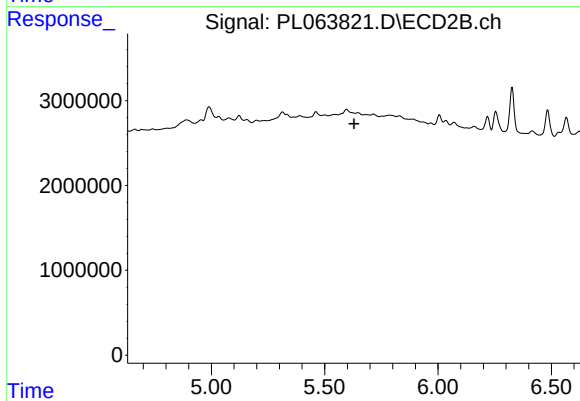

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.629 min
Response: 0
Conc: N.D.

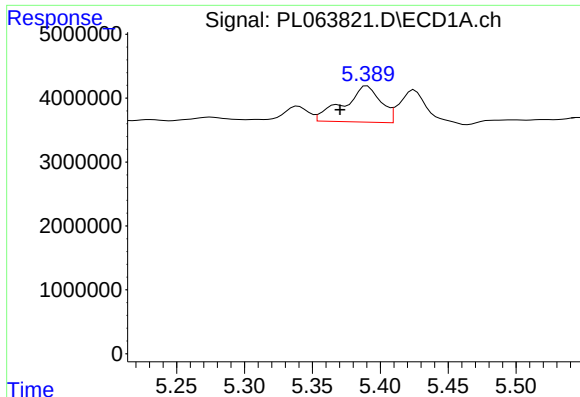

#10 gamma-Chlordane


R.T.: 5.390 min
Delta R.T.: 0.020 min
Response: 10785234
Conc: 2.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

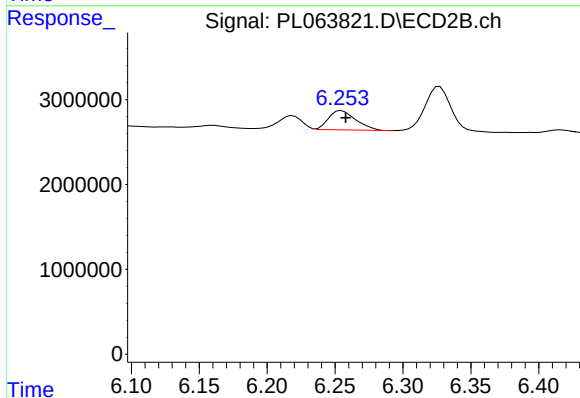


#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: -0.003 min
Response: 3172751
Conc: 1.15 ng/ml

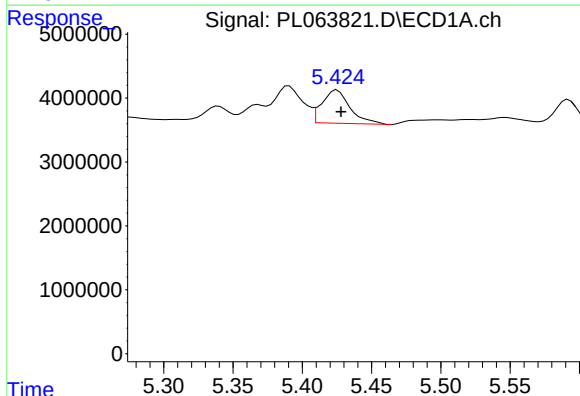


#11 alpha-Chlordane

R.T.: 5.425 min
Delta R.T.: -0.003 min
Response: 7329200
Conc: 1.95 ng/ml

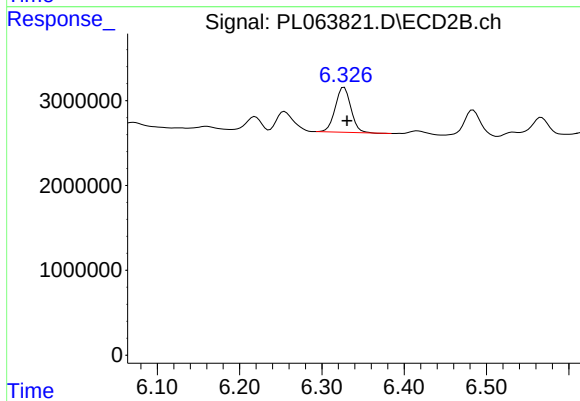

#11 alpha-Chlordane


R.T.: 6.327 min
Delta R.T.: -0.004 min
Response: 7020466
Conc: 2.54 ng/ml

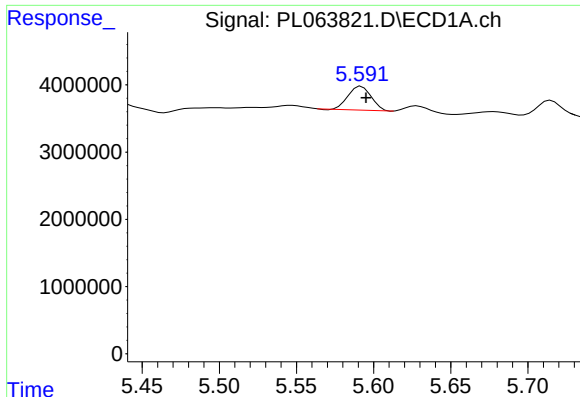

#12 4,4'-DDE


R.T.: 5.592 min
Delta R.T.: -0.003 min
Response: 3718853
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

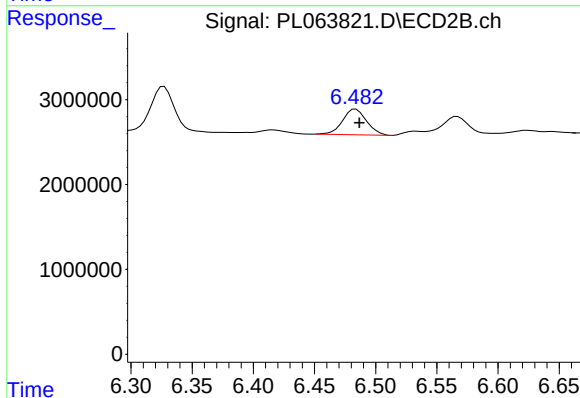


#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 4107802
Conc: 1.66 ng/ml

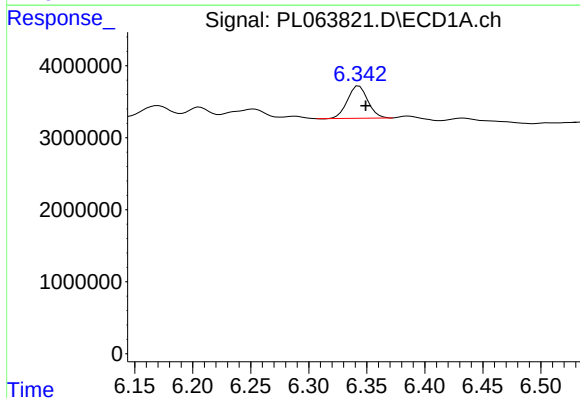


#17 4,4'-DDT

R.T.: 6.343 min
Delta R.T.: -0.006 min
Response: 5488429
Conc: 2.07 ng/ml

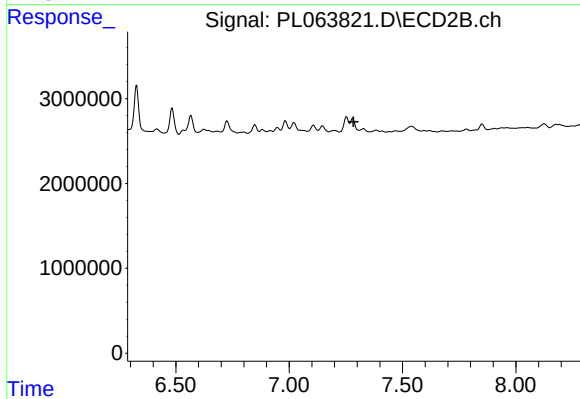

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

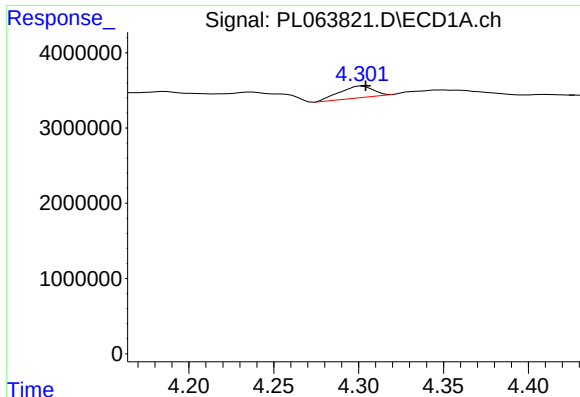

#23 Chlordane-1


R.T.: 4.302 min
Delta R.T.: -0.002 min
Response: 2129377
Conc: 20.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

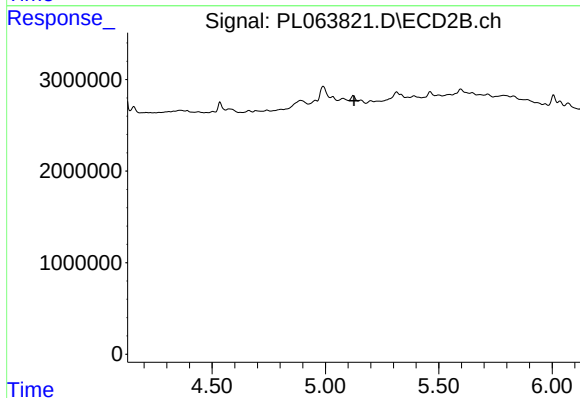


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

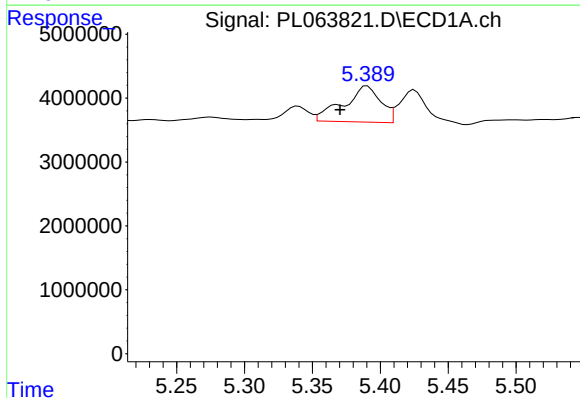


#25 Chlordane-3

R.T.: 5.390 min
Delta R.T.: 0.020 min
Response: 10785234
Conc: 33.01 ng/ml

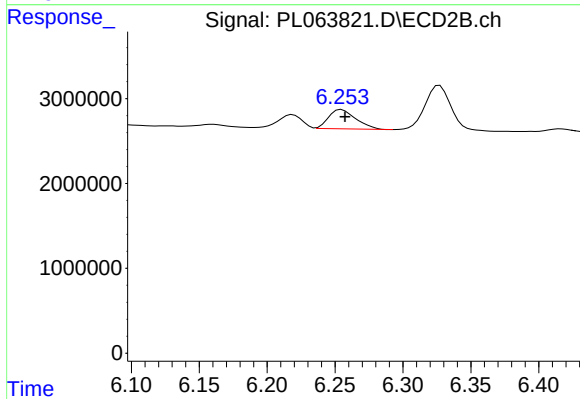

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: -0.002 min
Response: 3172751
Conc: 9.26 ng/ml

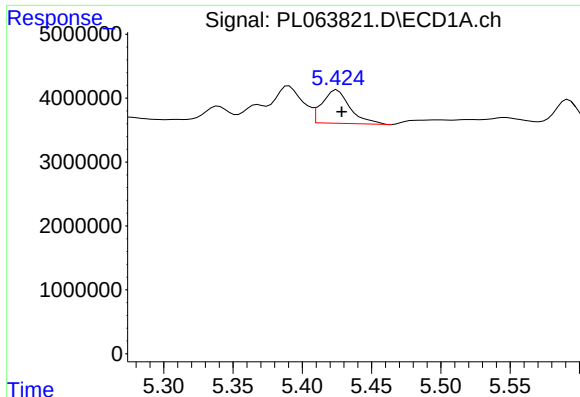

#26 Chlordane-4


R.T.: 5.425 min
Delta R.T.: -0.003 min
Response: 7329200
Conc: 27.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

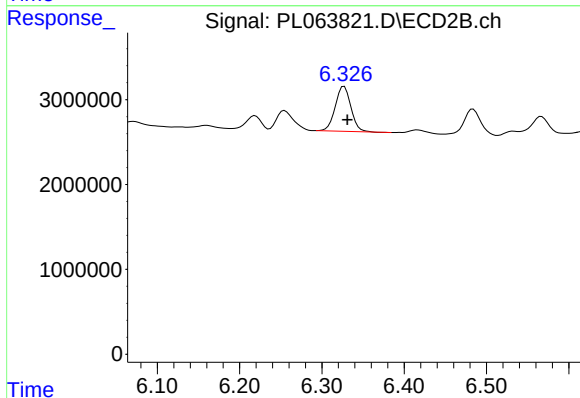


#26 Chlordane-4

R.T.: 6.327 min
Delta R.T.: -0.004 min
Response: 7020466
Conc: 17.08 ng/ml

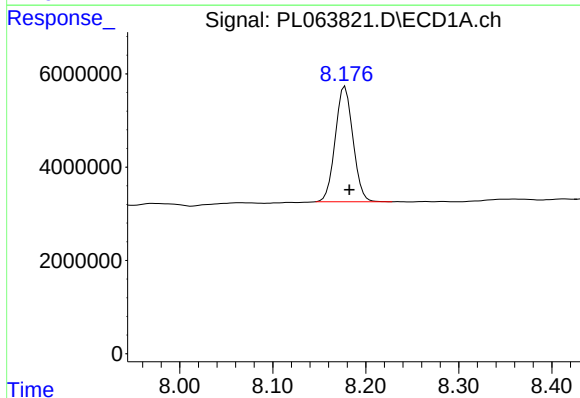

#28 Decachlorobiphenyl

R.T.: 8.178 min
Delta R.T.: -0.005 min
Response: 32717633
Conc: 11.88 ng/ml

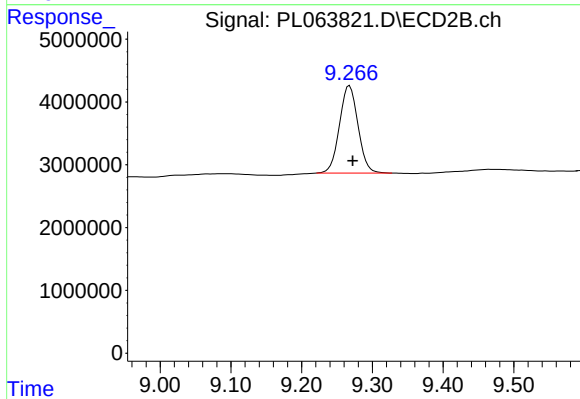

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: -0.004 min
Response: 25392306
Conc: 12.88 ng/ml