

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
 Data File : PL063822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2020 15:26
 Operator : AR\AJ
 Sample : L5199-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 00:36:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.110	36762677	29950476	12.263	11.731
28)	SA Decachlor...	8.178	9.267	28856376	21787494	10.474	11.051
Target Compounds							
5)	MB Aldrin	4.693	5.601f	4328462	10803073	1.084	3.774 #
6)	B beta-BHC	4.412	4.996	6740285	2077560	3.487	1.184 #
9)	A Endosulfan I	5.491	0.000	4256912	0	1.229	N.D. #
11)	B alpha-Chl...	0.000	6.327	0	19590971	N.D.	7.098 #
13)	MA Dieldrin	0.000	6.655	0	2725747	N.D.	1.046 #
23)	Chlordane-1	4.297	0.000	5679446	0	55.419	N.D. #
24)	Chlordane-2	0.000	5.601	0	10803073	N.D.	111.963 #
26)	Chlordane-4	0.000	6.327	0	19590971	N.D.	47.663 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
Data File : PL063822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2020 15:26
Operator : AR\AJ
Sample : L5199-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 00:36:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

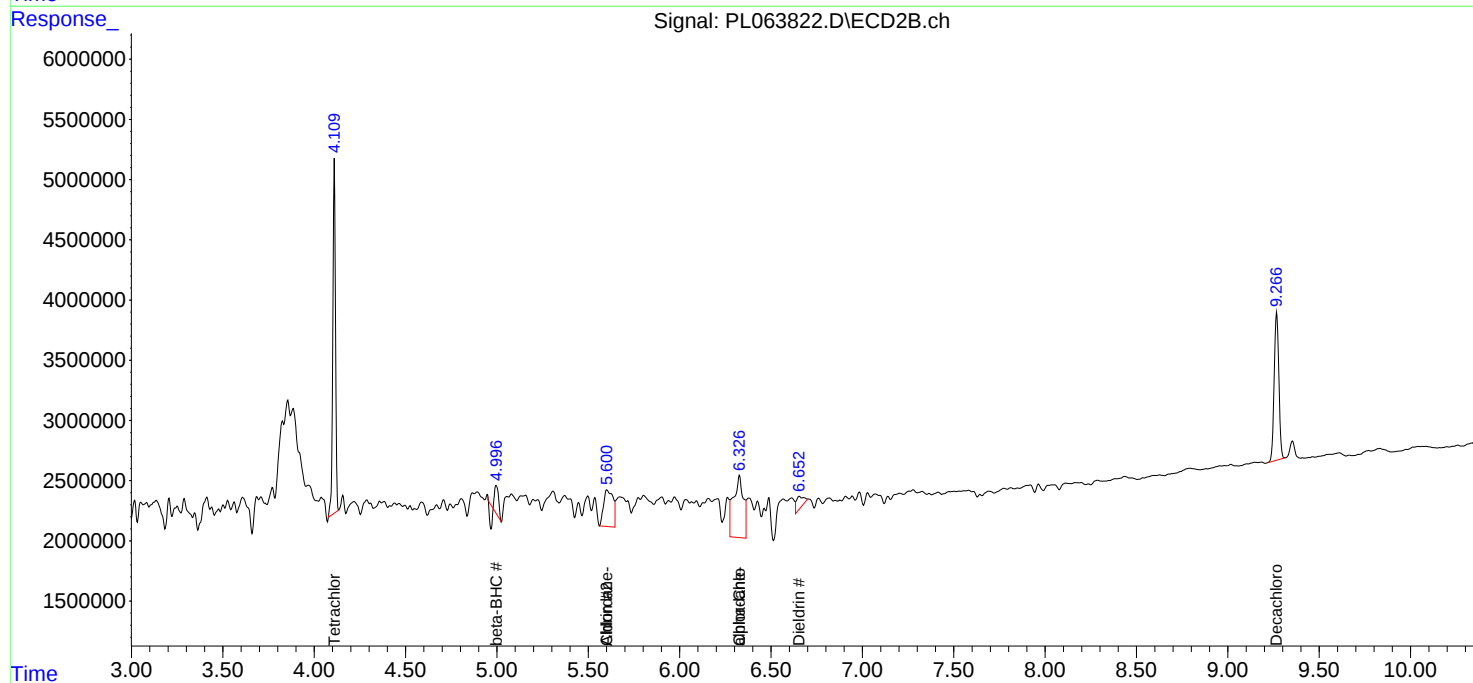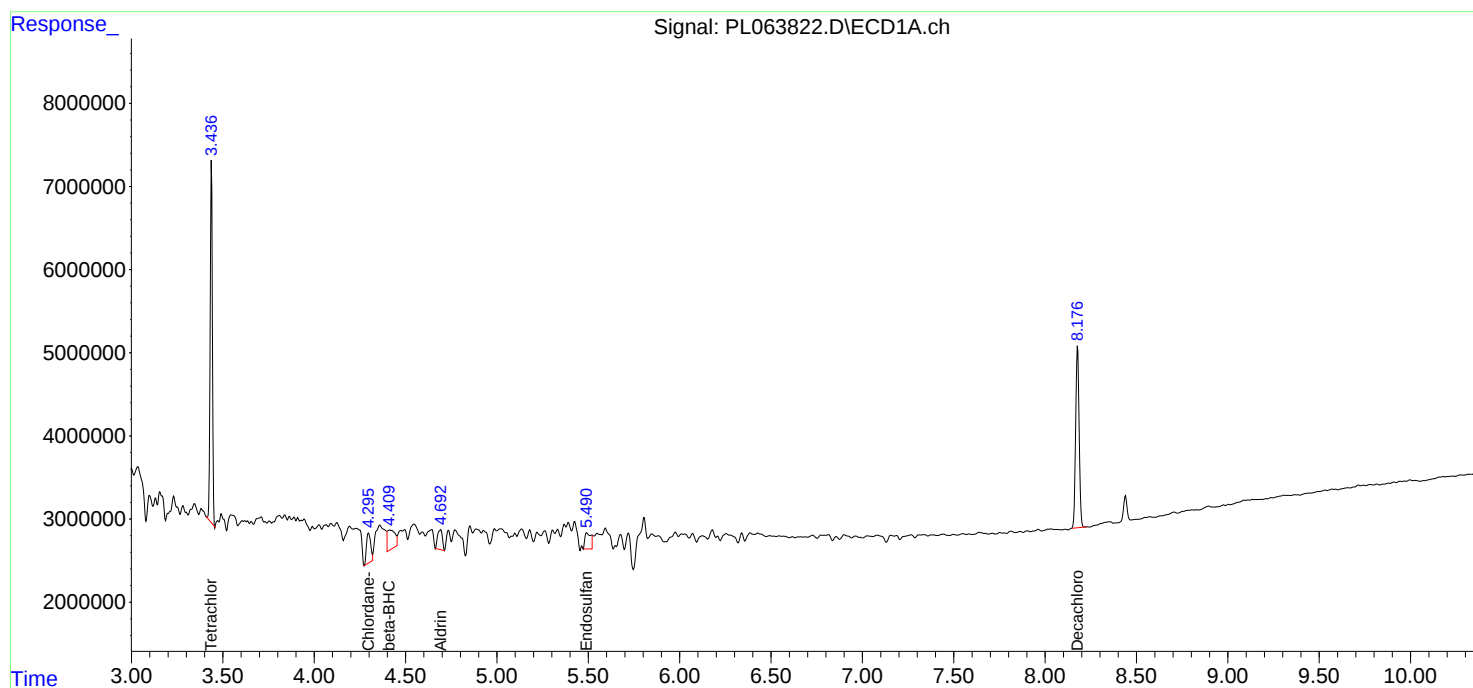


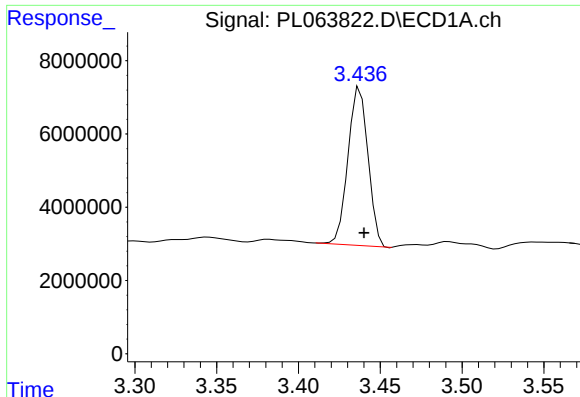

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 36762677
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

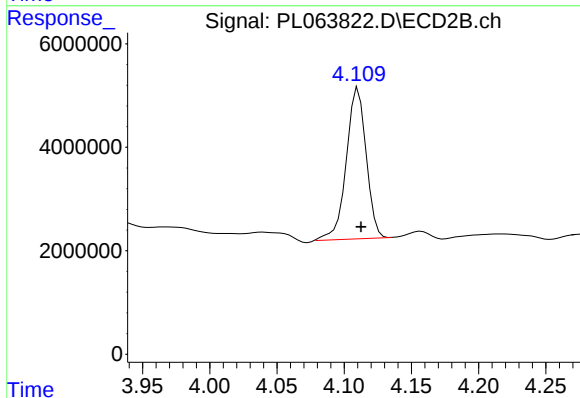


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 29950476
Conc: 11.73 ng/ml

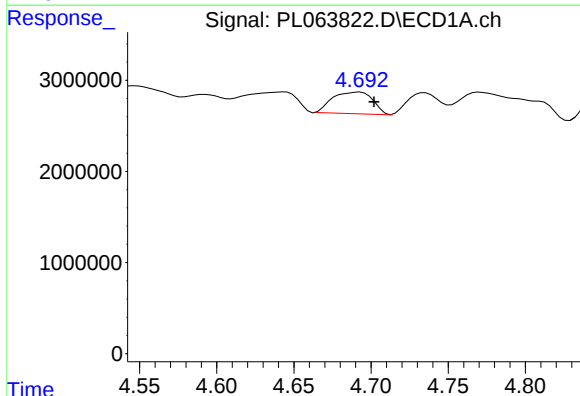


#5 Aldrin

R.T.: 4.693 min
Delta R.T.: -0.009 min
Response: 4328462
Conc: 1.08 ng/ml

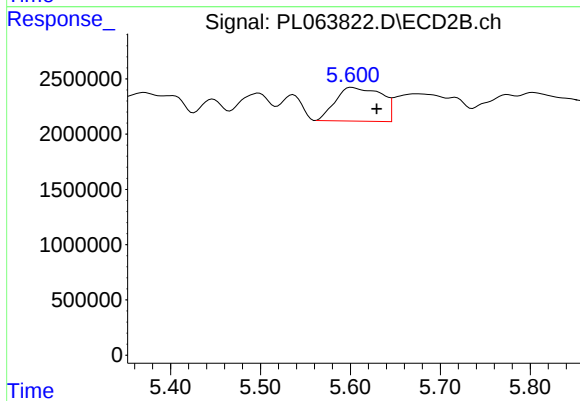

#5 Aldrin


R.T.: 5.601 min
Delta R.T.: -0.028 min
Response: 10803073
Conc: 3.77 ng/ml

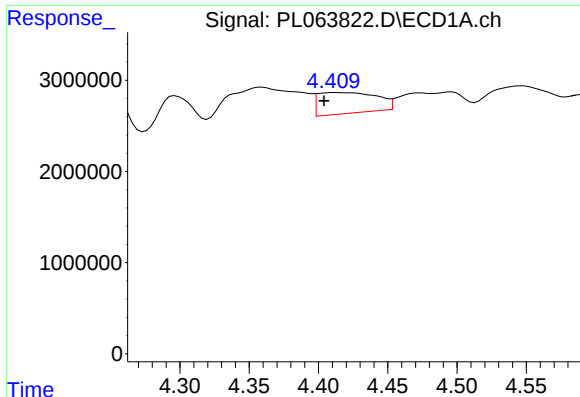

#6 beta-BHC


R.T.: 4.412 min
Delta R.T.: 0.008 min
Response: 6740285
Conc: 3.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

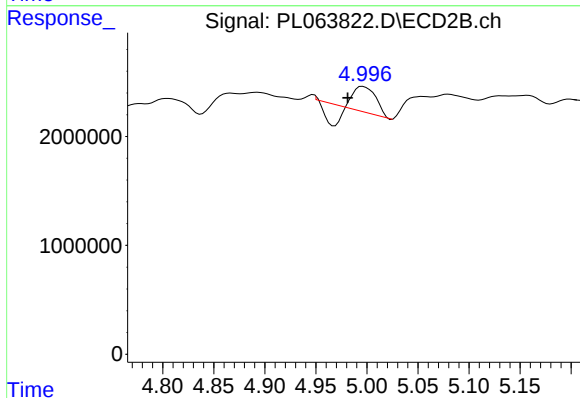


#6 beta-BHC

R.T.: 4.996 min
Delta R.T.: 0.015 min
Response: 2077560
Conc: 1.18 ng/ml

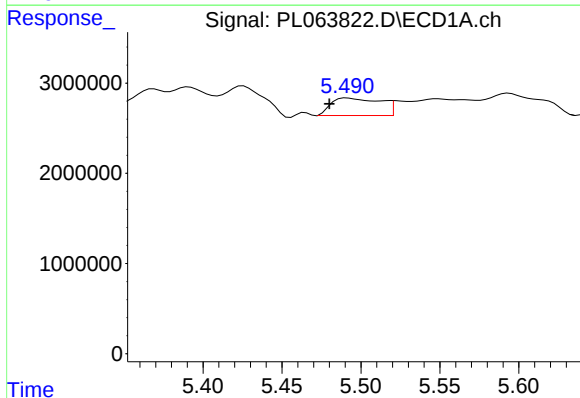


#9 Endosulfan I

R.T.: 5.491 min
Delta R.T.: 0.011 min
Response: 4256912
Conc: 1.23 ng/ml

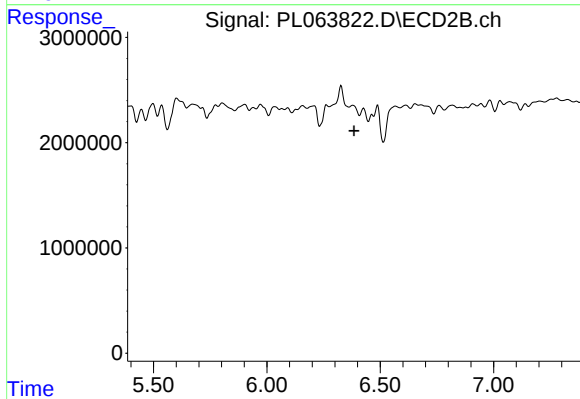

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

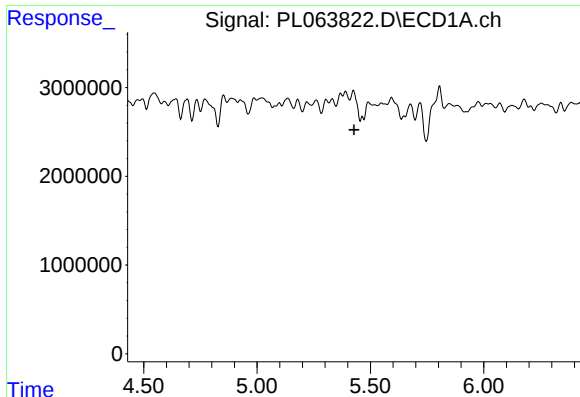

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

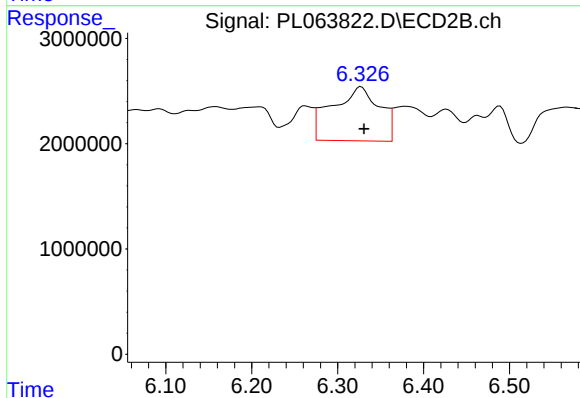


#11 alpha-Chlordane

R.T.: 6.327 min
Delta R.T.: -0.003 min
Response: 19590971
Conc: 7.10 ng/ml

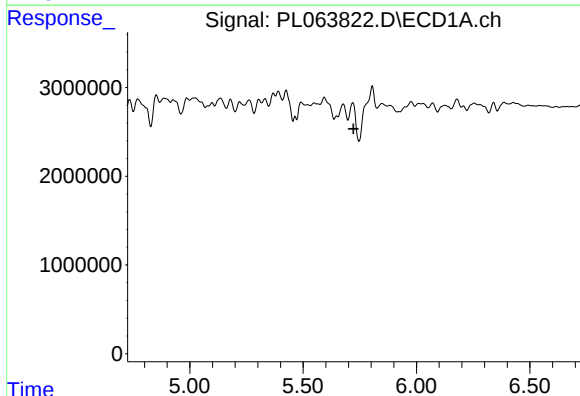


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.723 min
Response: 0
Conc: N.D.

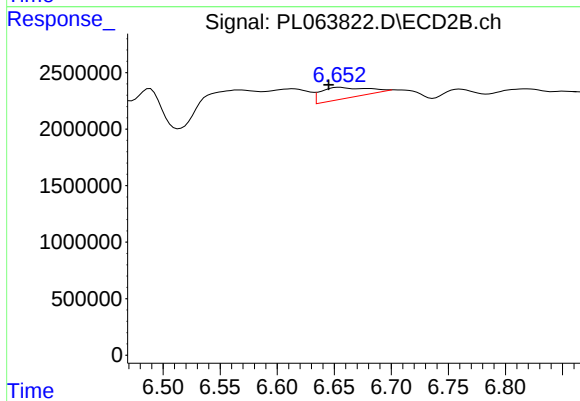

#13 Dieldrin


R.T.: 6.655 min
Delta R.T.: 0.009 min
Response: 2725747
Conc: 1.05 ng/ml

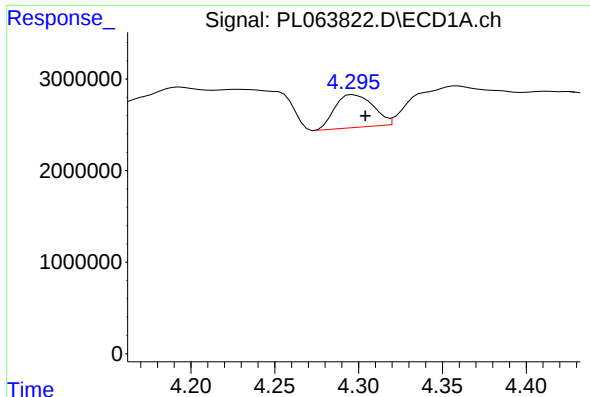

#23 Chlordane-1


R.T.: 4.297 min
Delta R.T.: -0.007 min
Response: 5679446
Conc: 55.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

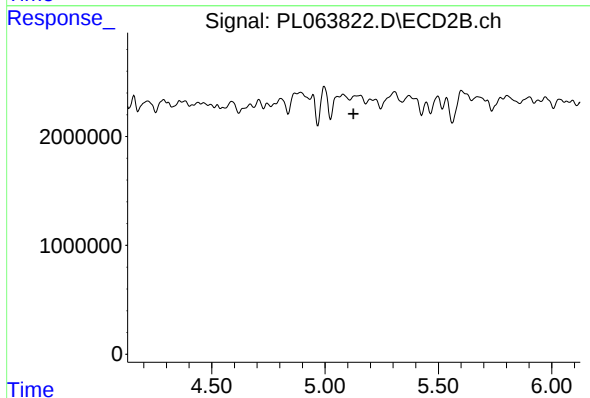


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

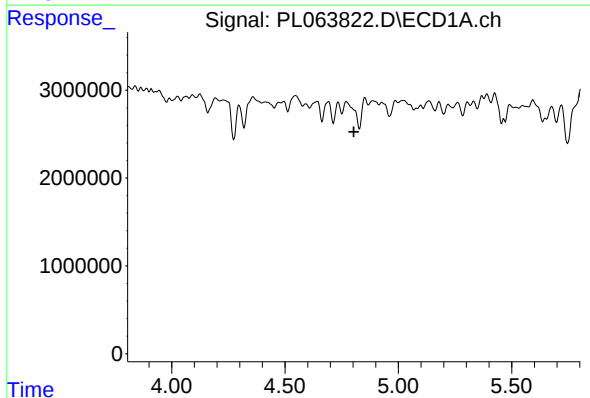


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

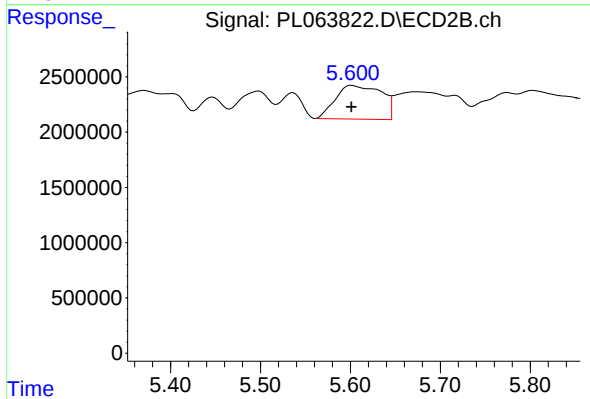

#24 Chlordane-2


R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 10803073
Conc: 111.96 ng/ml

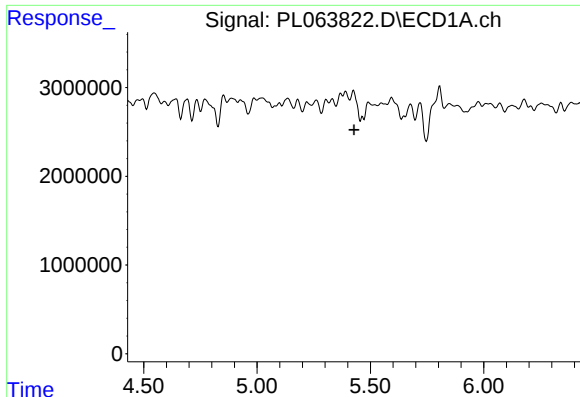

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

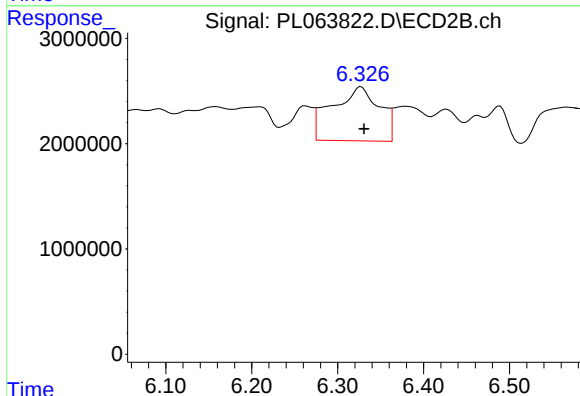


#26 Chlordane-4

R.T.: 6.327 min
Delta R.T.: -0.003 min
Response: 19590971
Conc: 47.66 ng/ml

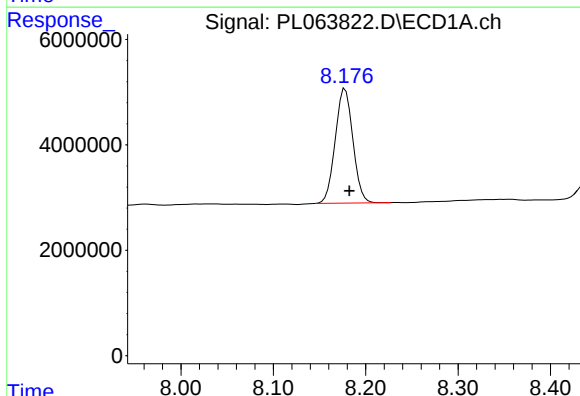

#28 Decachlorobiphenyl

R.T.: 8.178 min
Delta R.T.: -0.004 min
Response: 28856376
Conc: 10.47 ng/ml

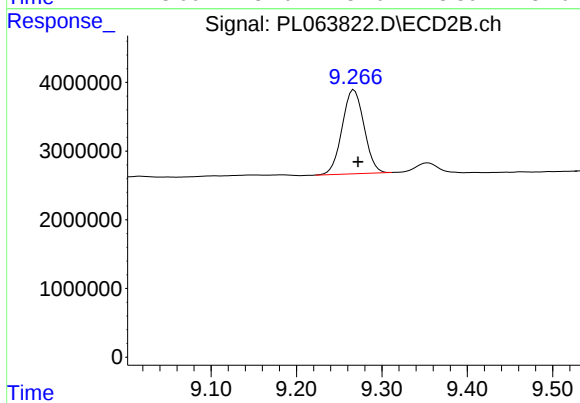

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.005 min
Response: 21787494
Conc: 11.05 ng/ml