

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
 Data File : PL063825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2020 16:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 00:37:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.111	78200367	63576352	26.084	24.902
28)	SA Decachlor...	8.179	9.268	55248312	38895584	20.053	19.728
Target Compounds							
8)	B Heptachlo...	0.000	6.013	0	6056058	N.D.	2.182 #
14)	MA Endrin	5.979	6.890f	3889502	562471	1.335	0.290 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
Data File : PL063825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2020 16:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 00:37:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

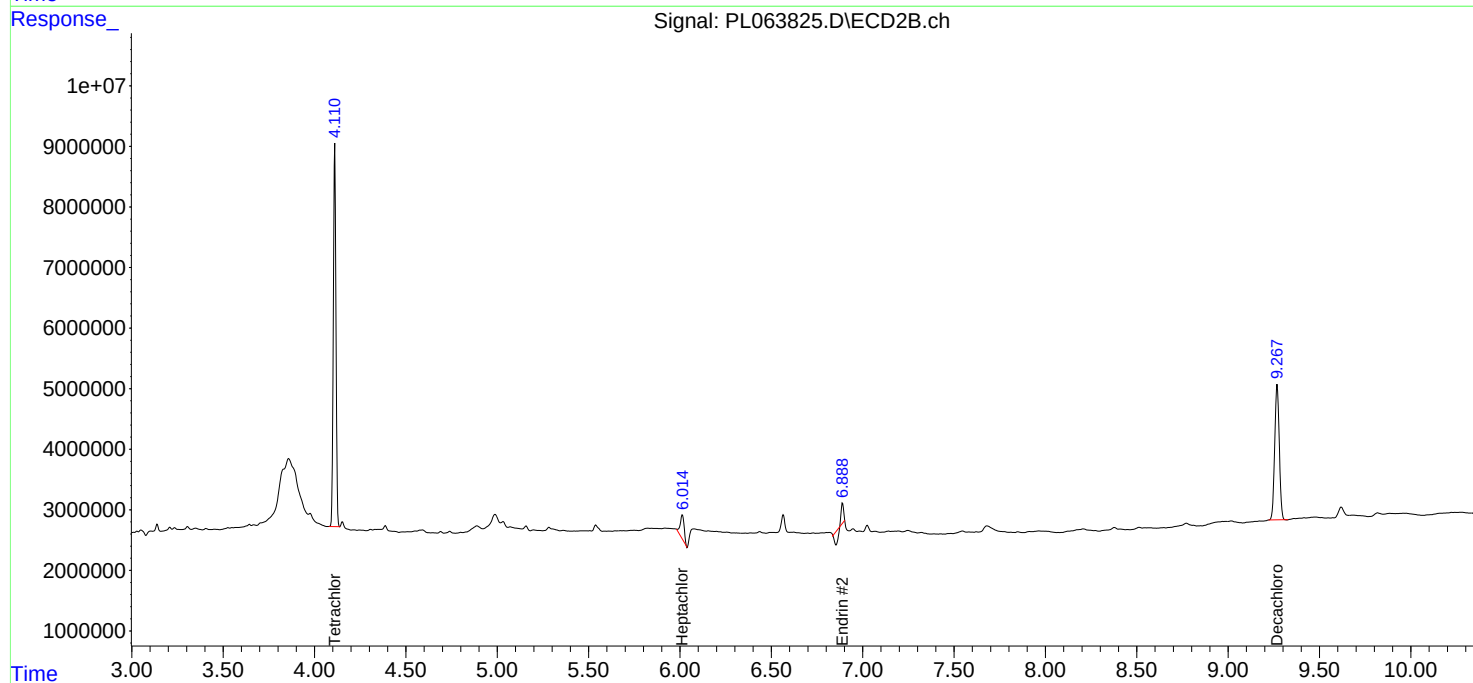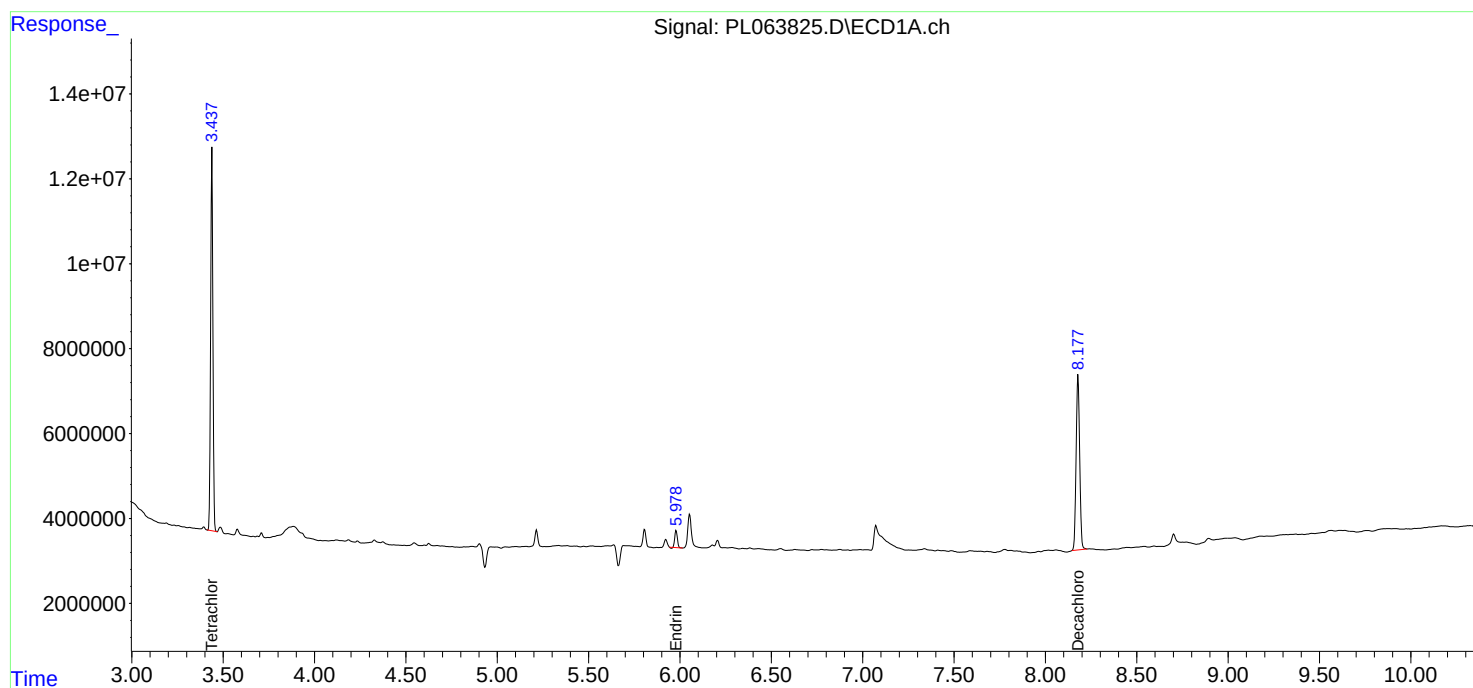


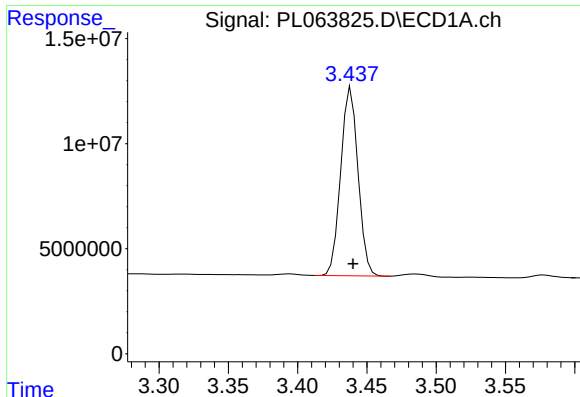

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 78200367
Conc: 26.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

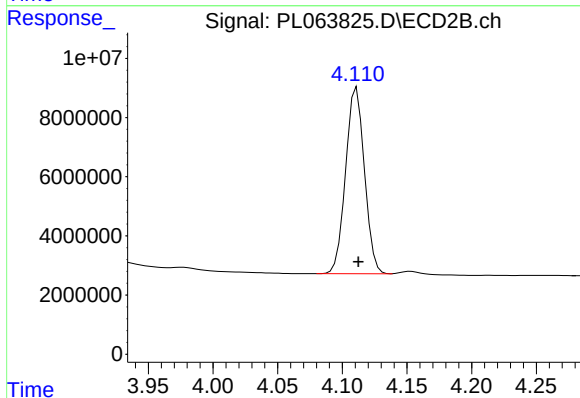


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 63576352
Conc: 24.90 ng/ml

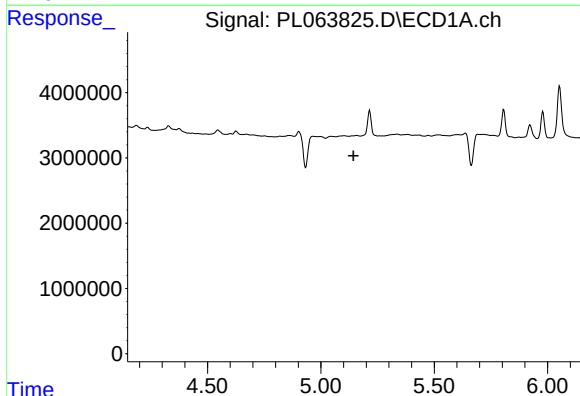


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.144 min
Response: 0
Conc: N.D.

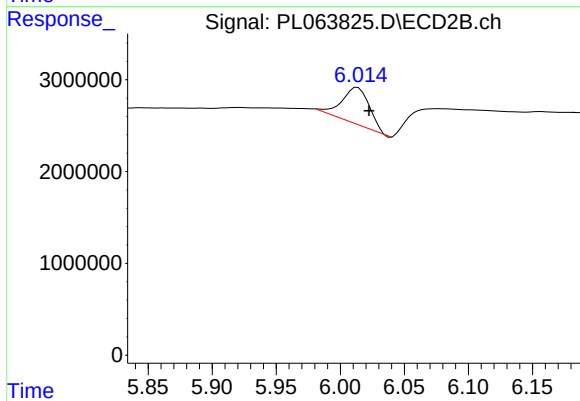

#8 Heptachlor epoxide


R.T.: 6.013 min
Delta R.T.: -0.009 min
Response: 6056058
Conc: 2.18 ng/ml

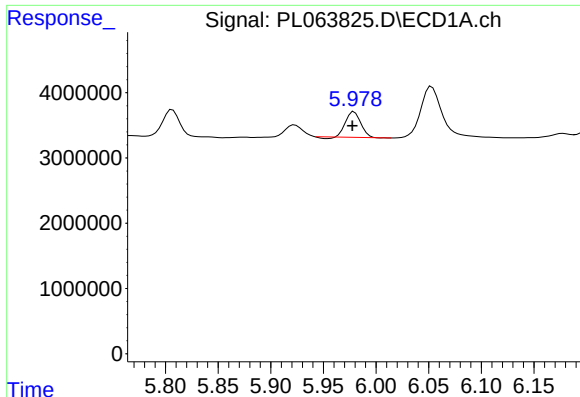

#14 Endrin


R.T.: 5.979 min
Delta R.T.: 0.002 min
Response: 3889502
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

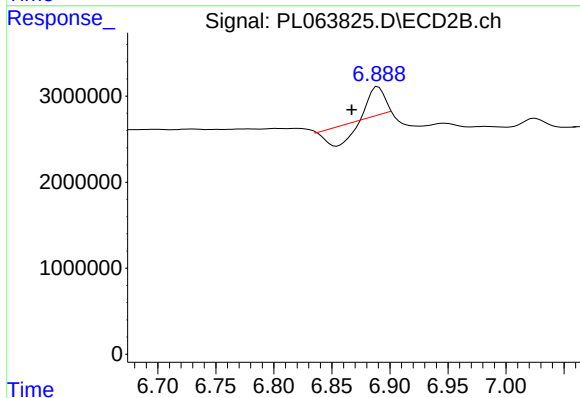


#14 Endrin

R.T.: 6.890 min
Delta R.T.: 0.023 min
Response: 562471
Conc: 0.29 ng/ml

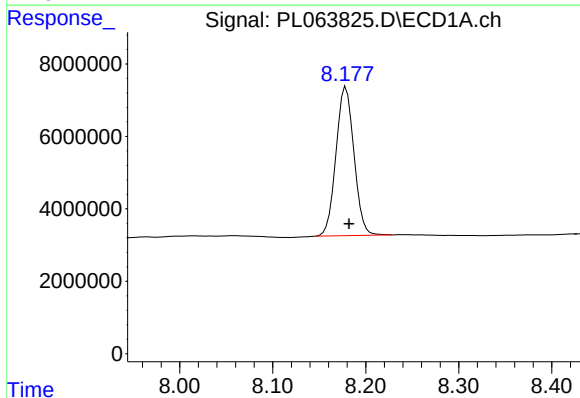

#28 Decachlorobiphenyl

R.T.: 8.179 min
Delta R.T.: -0.003 min
Response: 55248312
Conc: 20.05 ng/ml

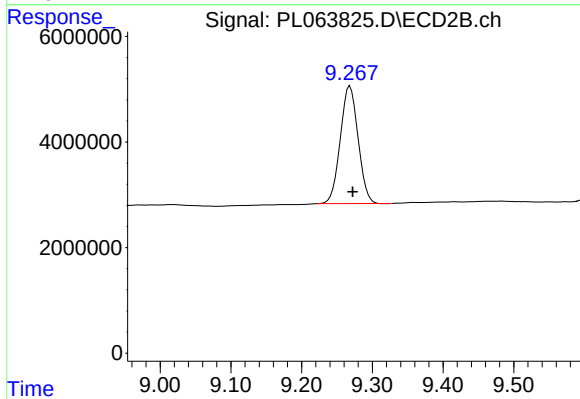

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: -0.004 min
Response: 38895584
Conc: 19.73 ng/ml