

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
 Data File : PL063814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2020 10:20
 Operator : AR\AJ
 Sample : L5189-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 08

Manual Integrations
 APPROVED

Ankita
 12/28/2020 12:52:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 00:34:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.111	35019038	29485778	11.681	11.549
28)	SA Decachlor...	8.165f	9.267	55053731	13903742	19.982m	7.052 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122420\
Data File : PL063814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2020 10:20
Operator : AR\AJ
Sample : L5189-16
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
08


Manual Integrations
APPROVED

Ankita
12/28/2020 12:52:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 00:34:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

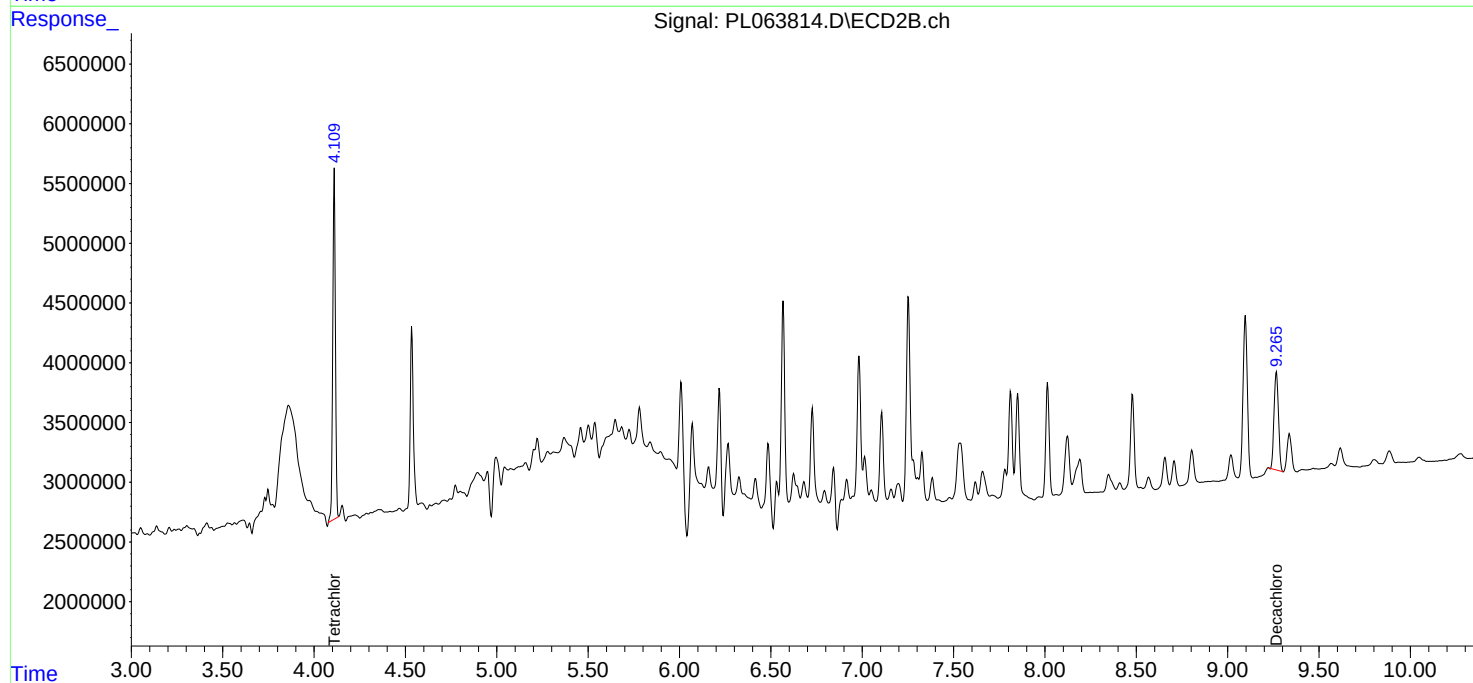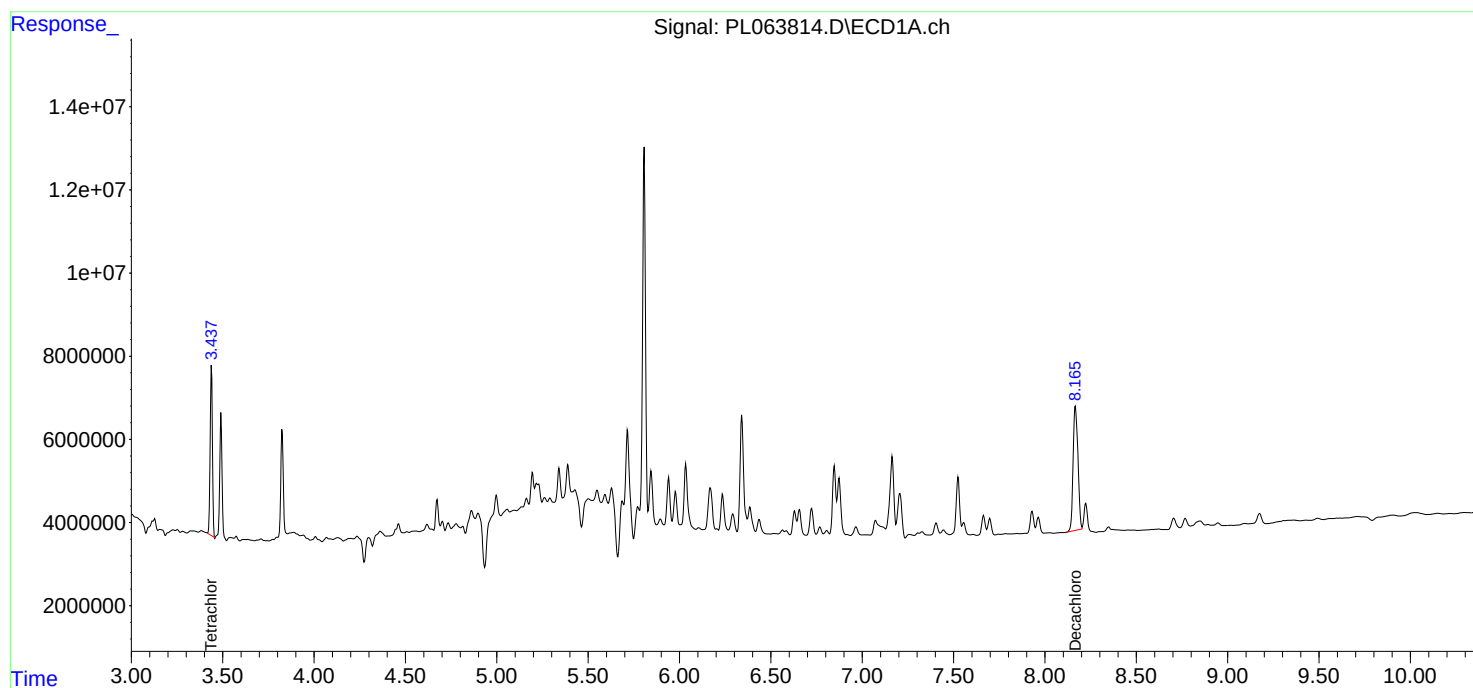

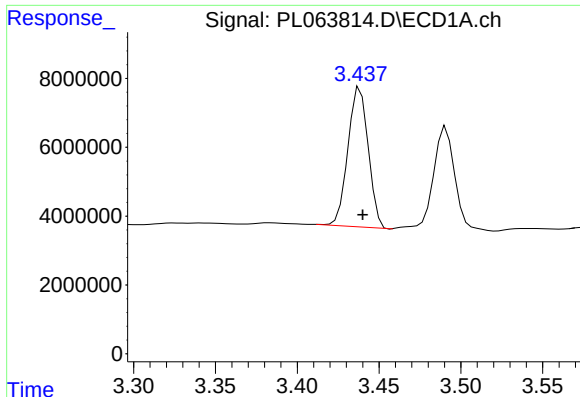


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 35019038
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
08


Manual Integrations
APPROVED

Ankita
12/28/2020 12:52:10 PM

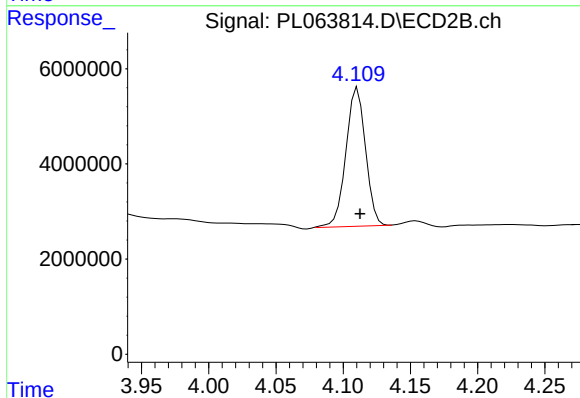


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 29485778
Conc: 11.55 ng/ml

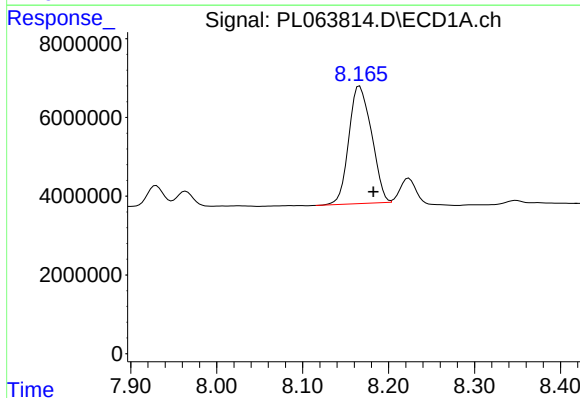

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.017 min
Response: 55053731
Conc: 19.98 ng/ml m

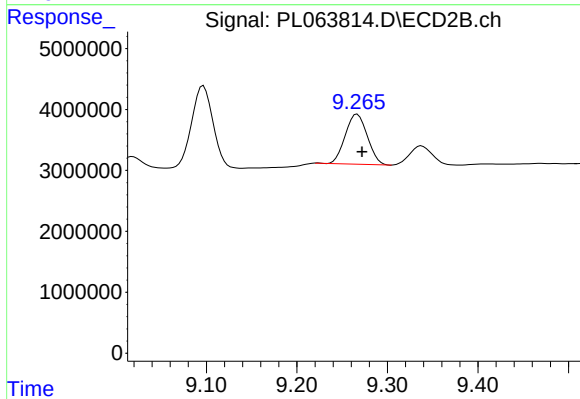

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.005 min
Response: 13903742
Conc: 7.05 ng/ml