

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
 Data File : PL087436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 18:08
 Operator : AR\AJ
 Sample : 05899-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GHL-SS-02

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2023
 Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:30:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.675	46075728	18228265	12.243m	10.829m
2) SA Decachlor...	8.976	7.863	50067670	19435530	14.683m	11.507m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
Data File : PL087436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 18:08
Operator : AR\AJ
Sample : 05899-12
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GHL-SS-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:30:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

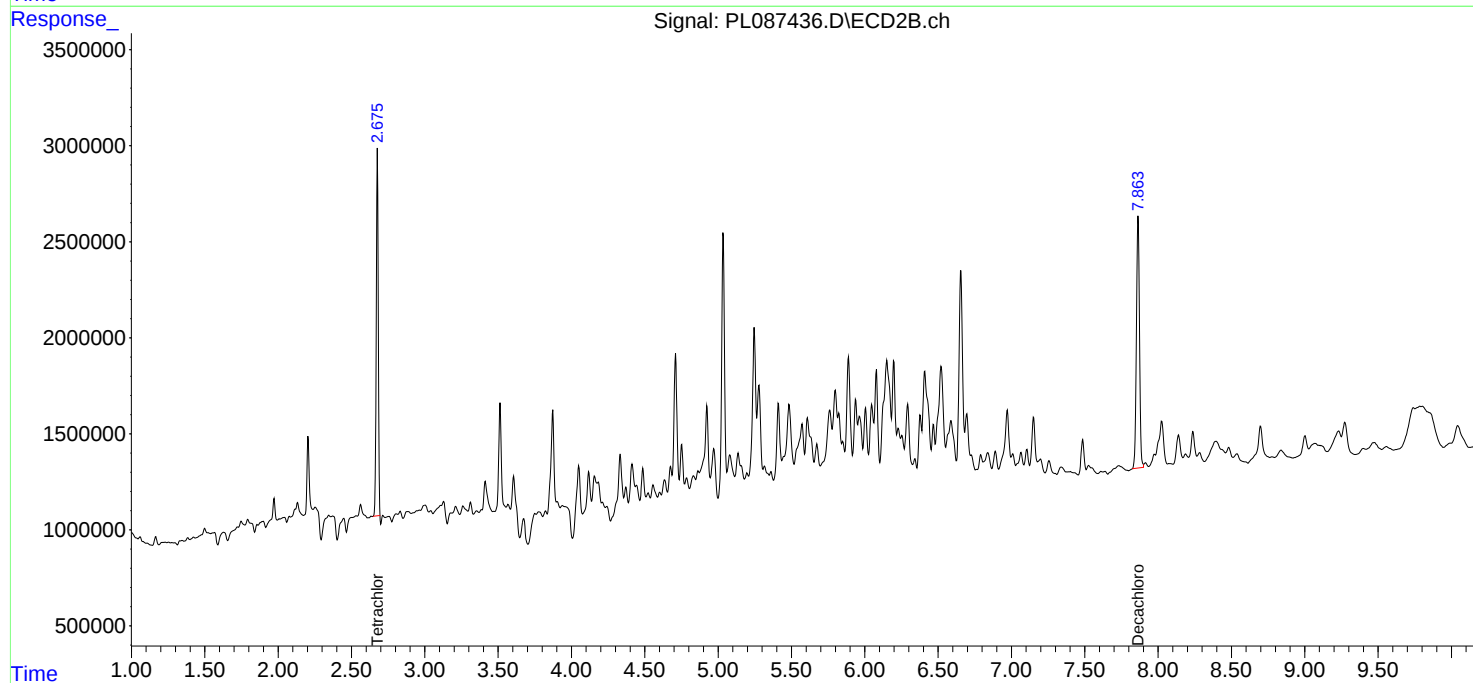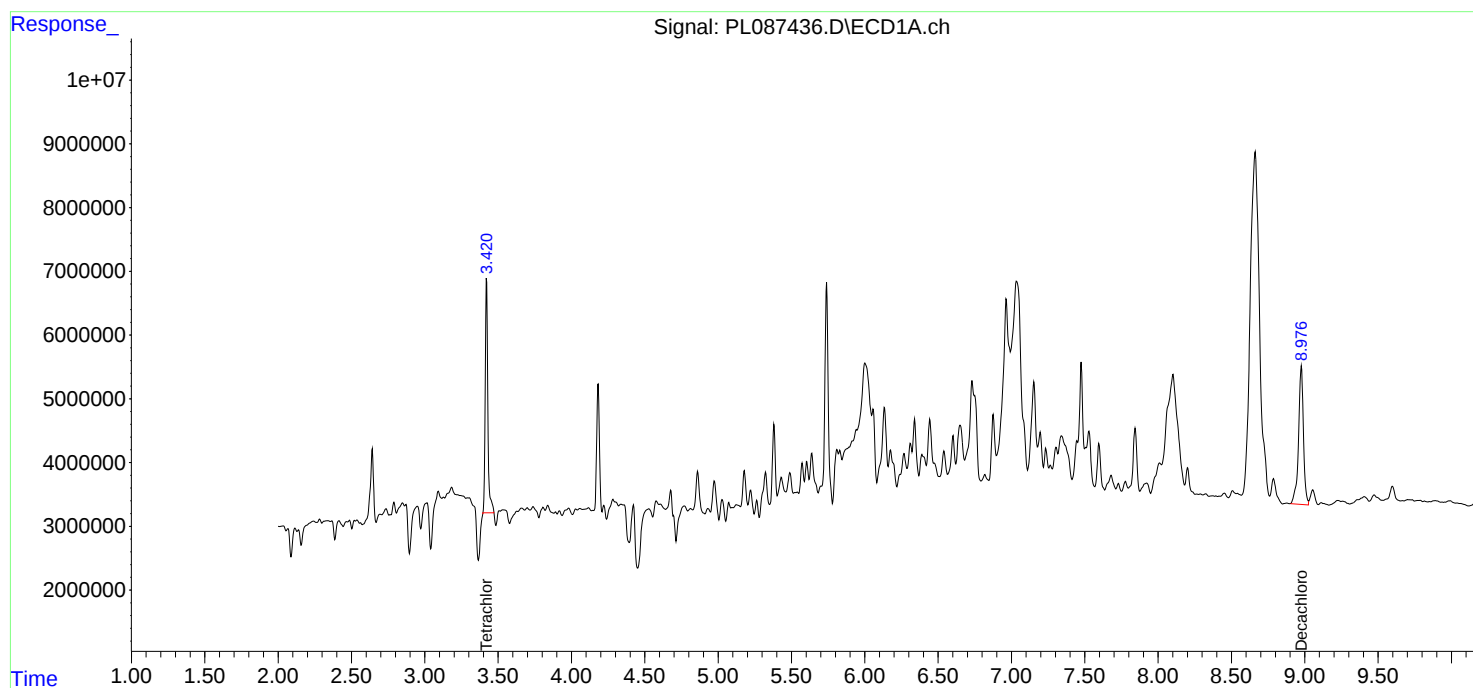

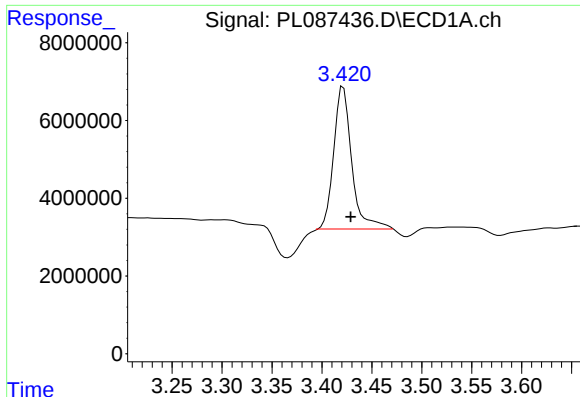


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: -0.009 min
Response: 46075728
Conc: 12.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SS-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

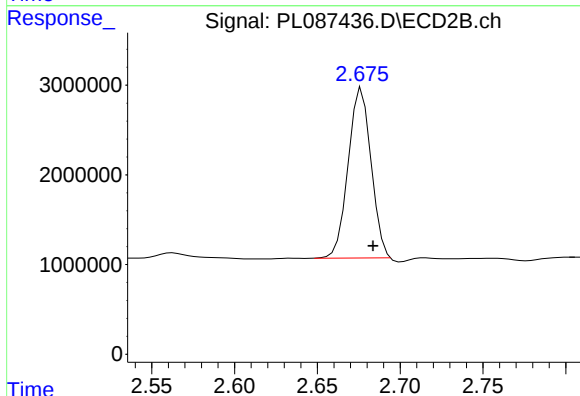


#1 Tetrachloro-m-xylene

R.T.: 2.675 min
Delta R.T.: -0.008 min
Response: 18228265
Conc: 10.83 ng/ml m

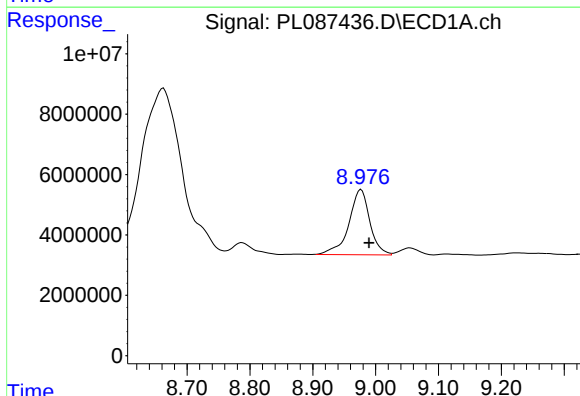

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.014 min
Response: 50067670
Conc: 14.68 ng/ml m

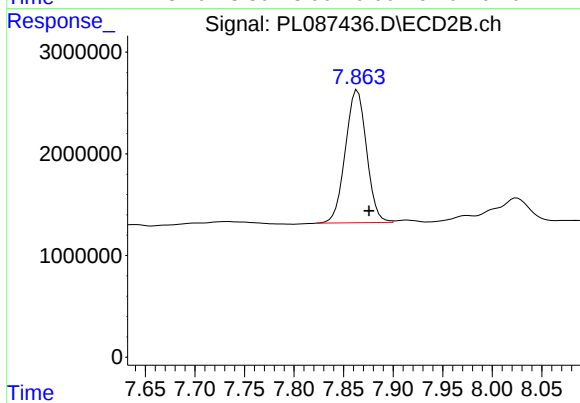

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.013 min
Response: 19435530
Conc: 11.51 ng/ml m