

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
 Data File : PL087447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 21:09
 Operator : AR\AJ
 Sample : 06011-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-03-122223

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:34:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.421	2.676	28210043	12556508	7.496	7.460
28) SA Decachlor...	8.977	7.862	28256292	12454526	8.286	7.374m
Target Compounds						
12) B 4,4'-DDE	6.094	5.157	5078587	1411087	1.226m	0.711 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
Data File : PL087447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 21:09
Operator : AR\AJ
Sample : 06011-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-03-122223


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:34:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

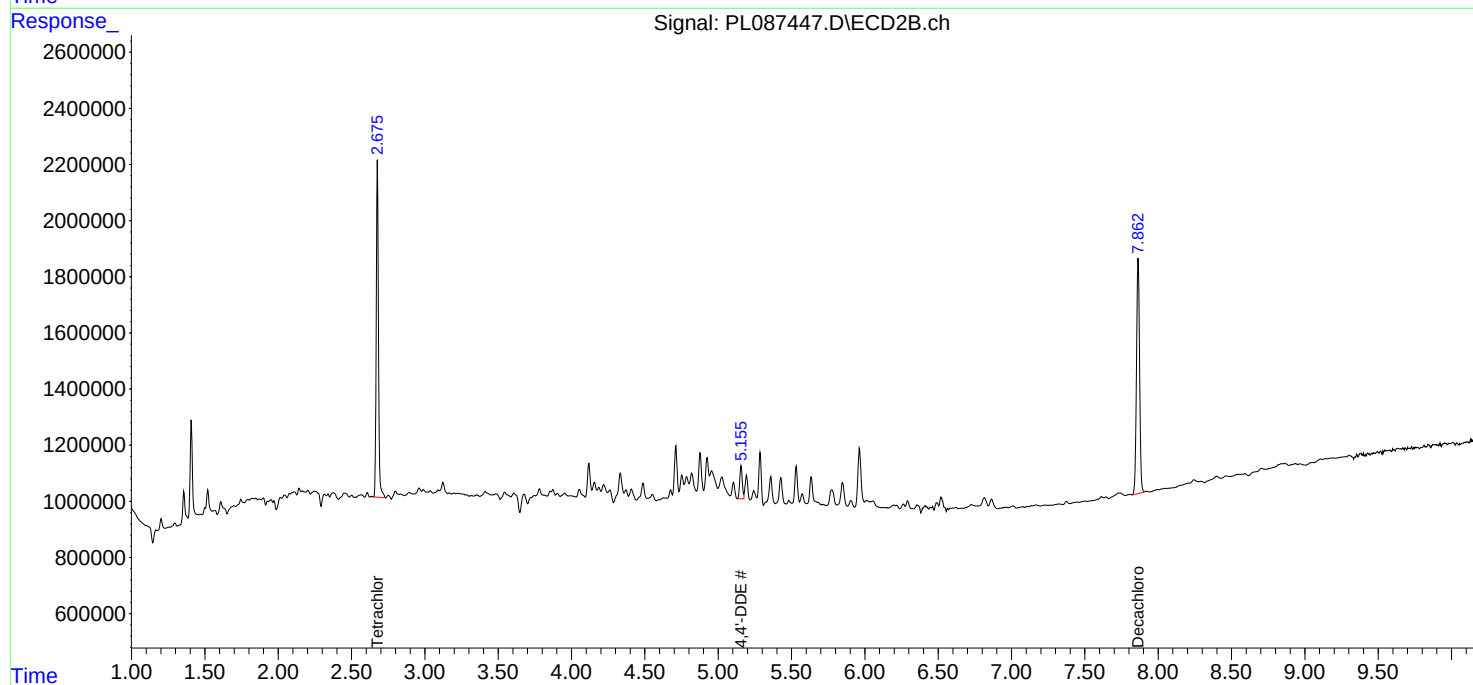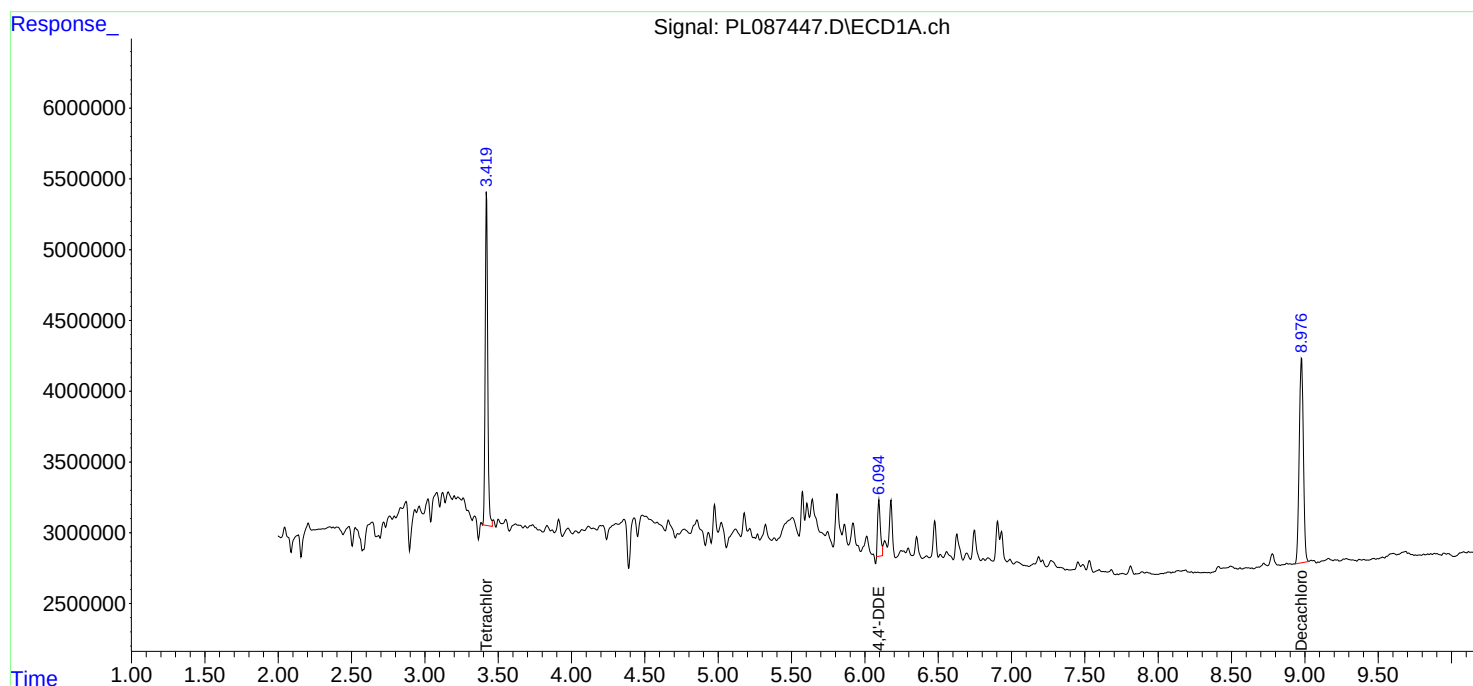

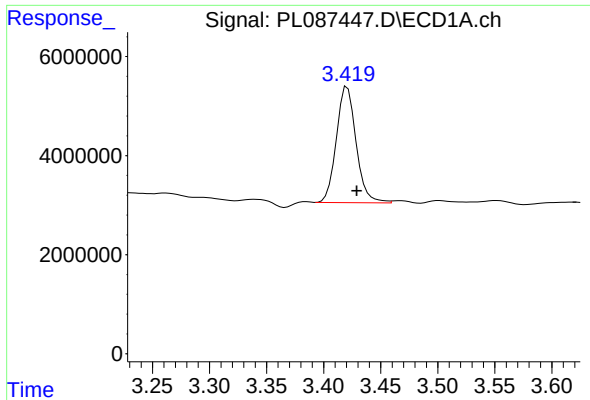


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: -0.008 min
Response: 28210043
Conc: 7.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-122223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

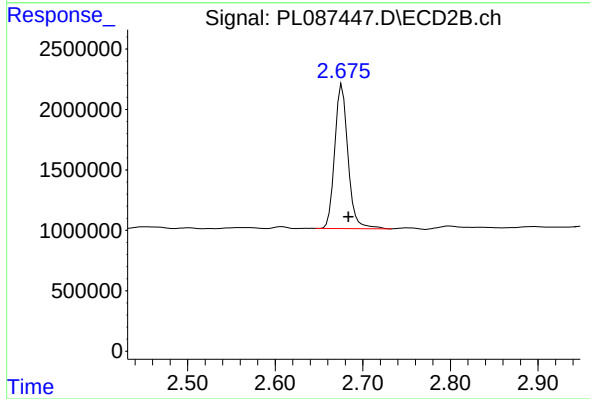


#1 Tetrachloro-m-xylene

R.T.: 2.676 min
Delta R.T.: -0.007 min
Response: 12556508
Conc: 7.46 ng/ml

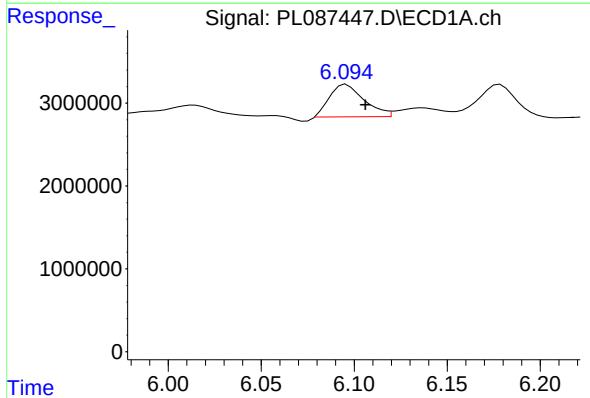


#12 4,4'-DDE

R.T.: 6.094 min
Delta R.T.: -0.012 min
Response: 5078587
Conc: 1.23 ng/ml m

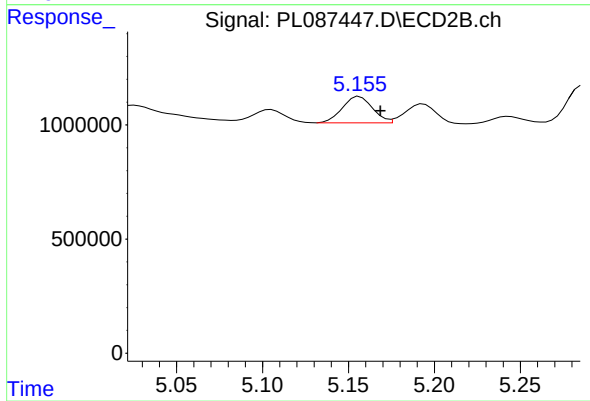

#12 4,4'-DDE

R.T.: 5.157 min
Delta R.T.: -0.012 min
Response: 1411087
Conc: 0.71 ng/ml

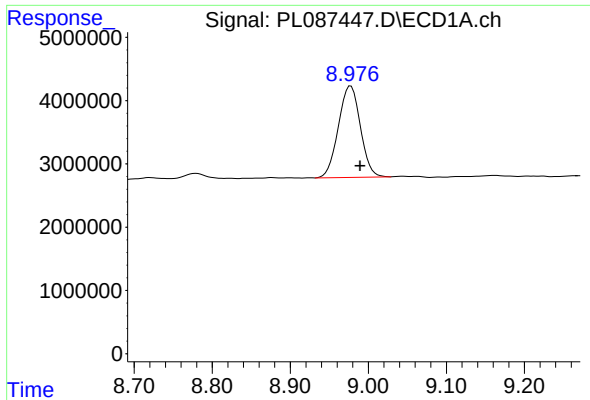


#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.012 min
Response: 28256292
Conc: 8.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-122223

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

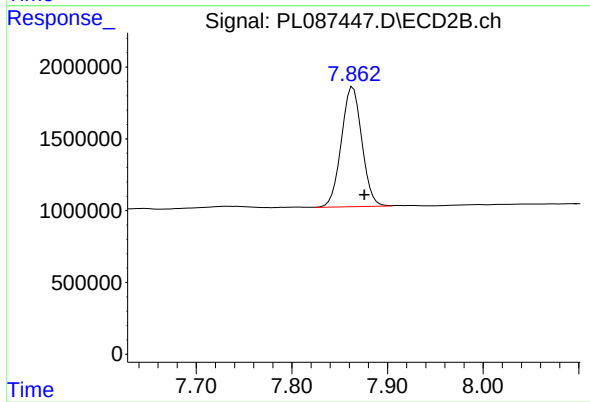

#28 Decachlorobiphenyl

R.T.: 7.862 min
Delta R.T.: -0.013 min
Response: 12454526
Conc: 7.37 ng/ml m