

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
 Data File : PL087457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 23:28
 Operator : AR\AJ
 Sample : 05932-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT-MW-06-121923

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 03:00:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.678	44130212	18971886	11.726	11.271
28)	SA Decachlor...	8.977	7.865	20786396	8865596	6.096	5.249

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122523\
Data File : PL087457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 23:28
Operator : AR\AJ
Sample : 05932-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RT-MW-06-121923

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 03:00:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

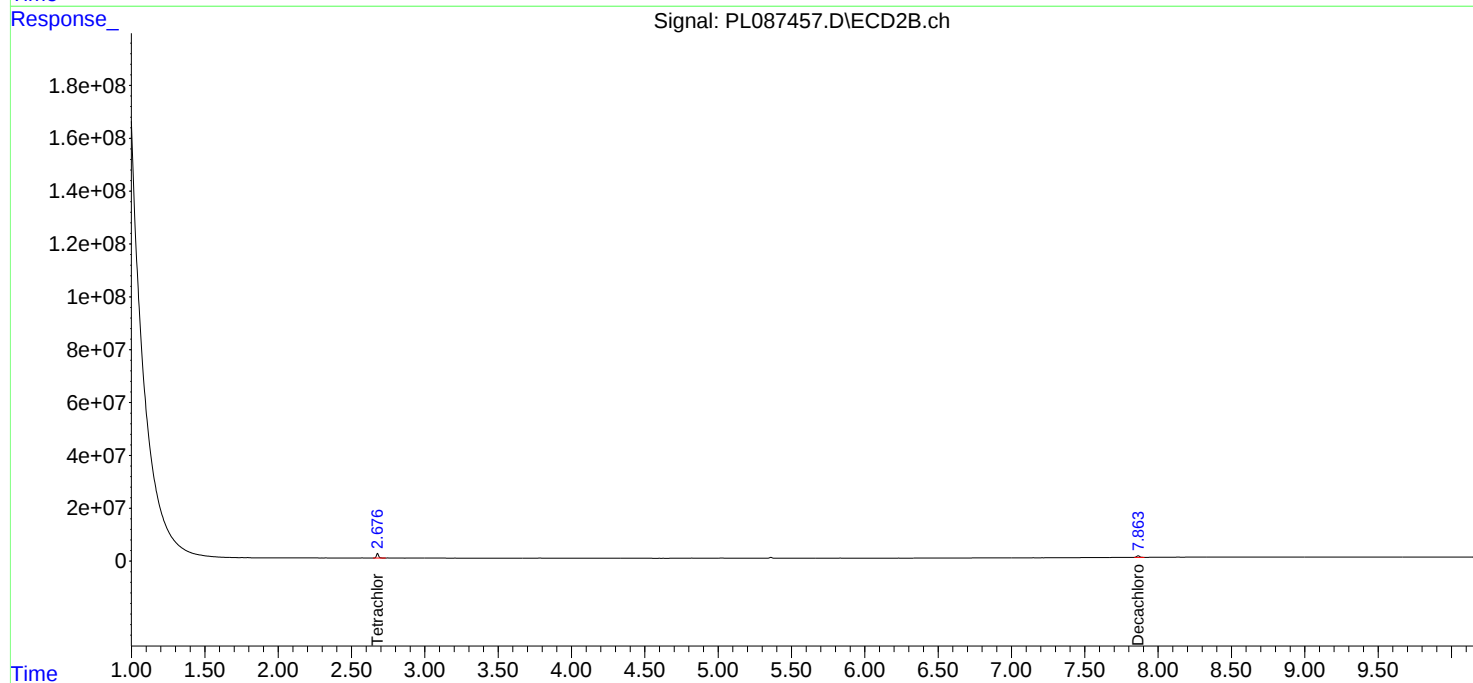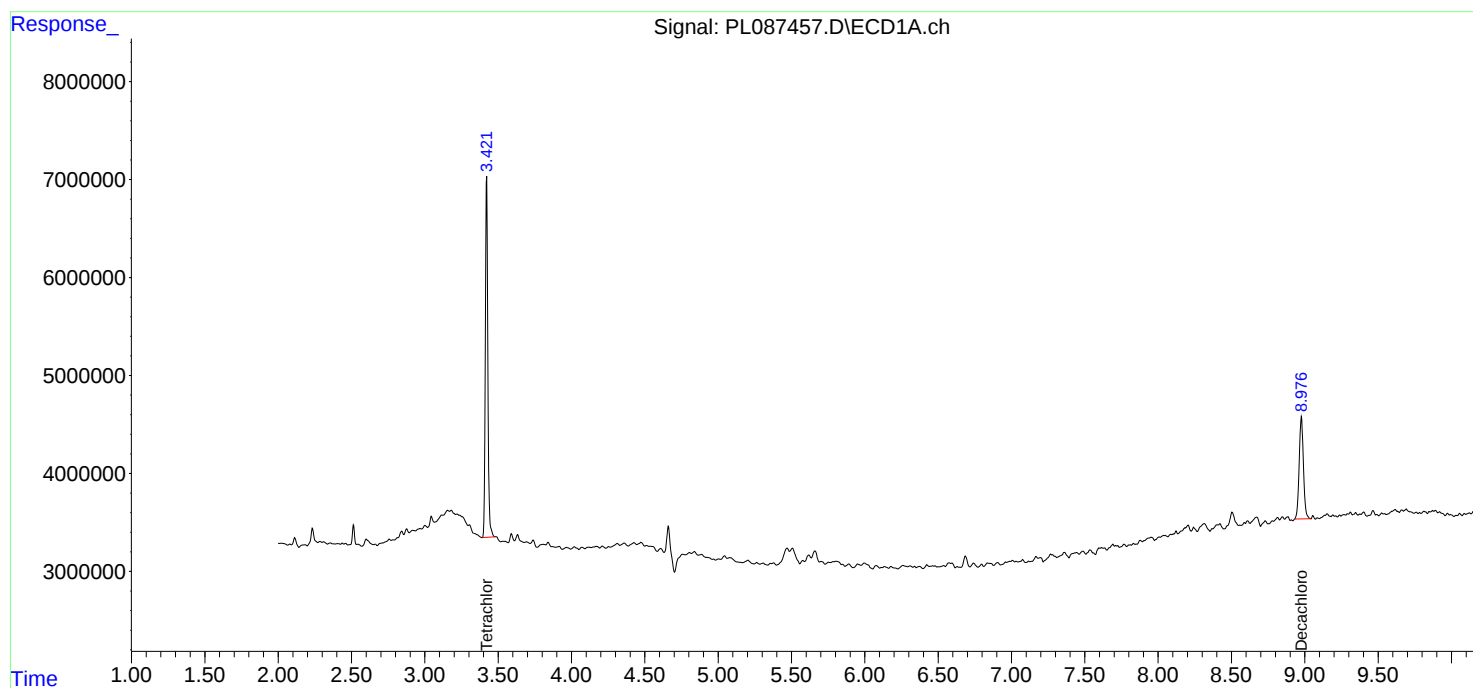


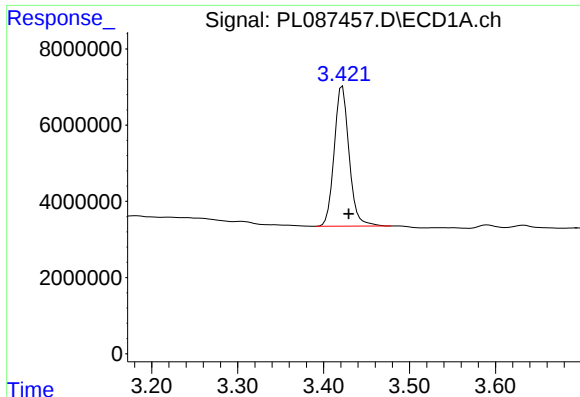

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 44130212
Conc: 11.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-MW-06-121923

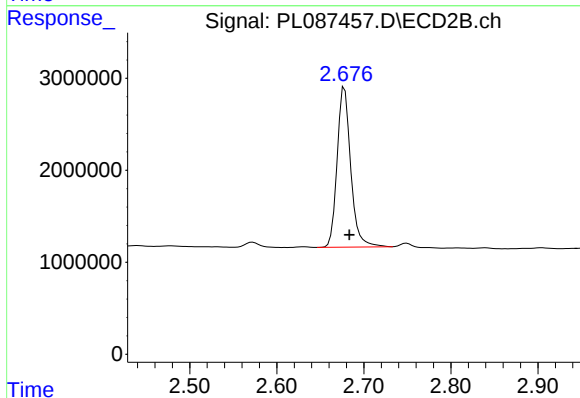


#1 Tetrachloro-m-xylene

R.T.: 2.678 min
Delta R.T.: -0.006 min
Response: 18971886
Conc: 11.27 ng/ml

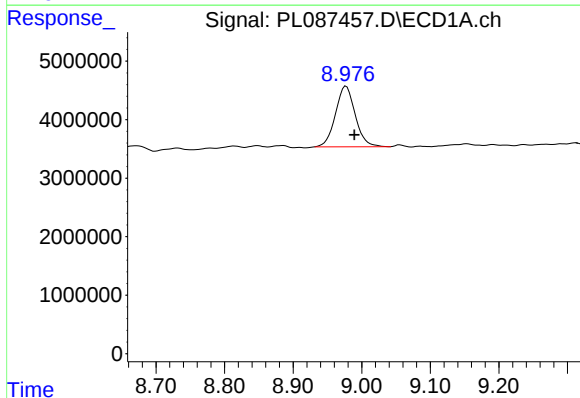

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.012 min
Response: 20786396
Conc: 6.10 ng/ml

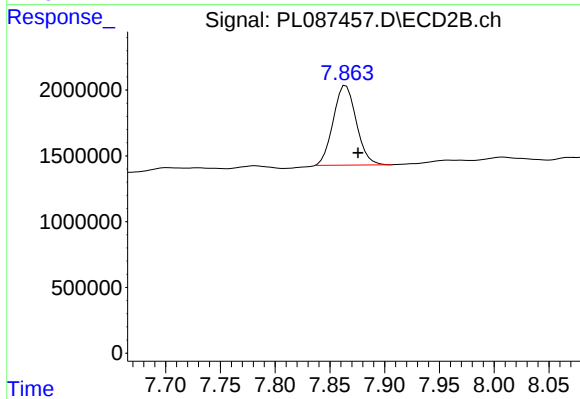

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.011 min
Response: 8865596
Conc: 5.25 ng/ml