

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122619\
 Data File : PL055240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2019 09:11
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 04:38:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.134	0	7014326	N.D.	3.178 #
Target Compounds							
6)	B beta-BHC	4.487f	0.000	9617076	0	1.402	N.D. #
7)	B delta-BHC	4.731	0.000	26362256	0	1.742	N.D. #
8)	B Heptachlo...	0.000	5.922	0	44484101	N.D.	17.453 #
9)	A Endosulfan I	5.615	6.273	11635439	5981656	0.881	2.415 #
10)	B gamma-Chl...	5.509f	6.157	111.8E6	11631791	7.675	4.383 #
11)	B alpha-Chl...	0.000	6.224	0	13734258	N.D.	5.237 #
14)	MA Endrin	6.118	6.754	17436796	14432039	1.372	6.725 #
25)	Chlordane-3	5.509f	6.157	111.8E6	11631791	88.222	36.144 #
26)	Chlordane-4	0.000	6.224	0	13734258	N.D.	35.731 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122619\
Data File : PL055240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2019 09:11
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 04:38:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

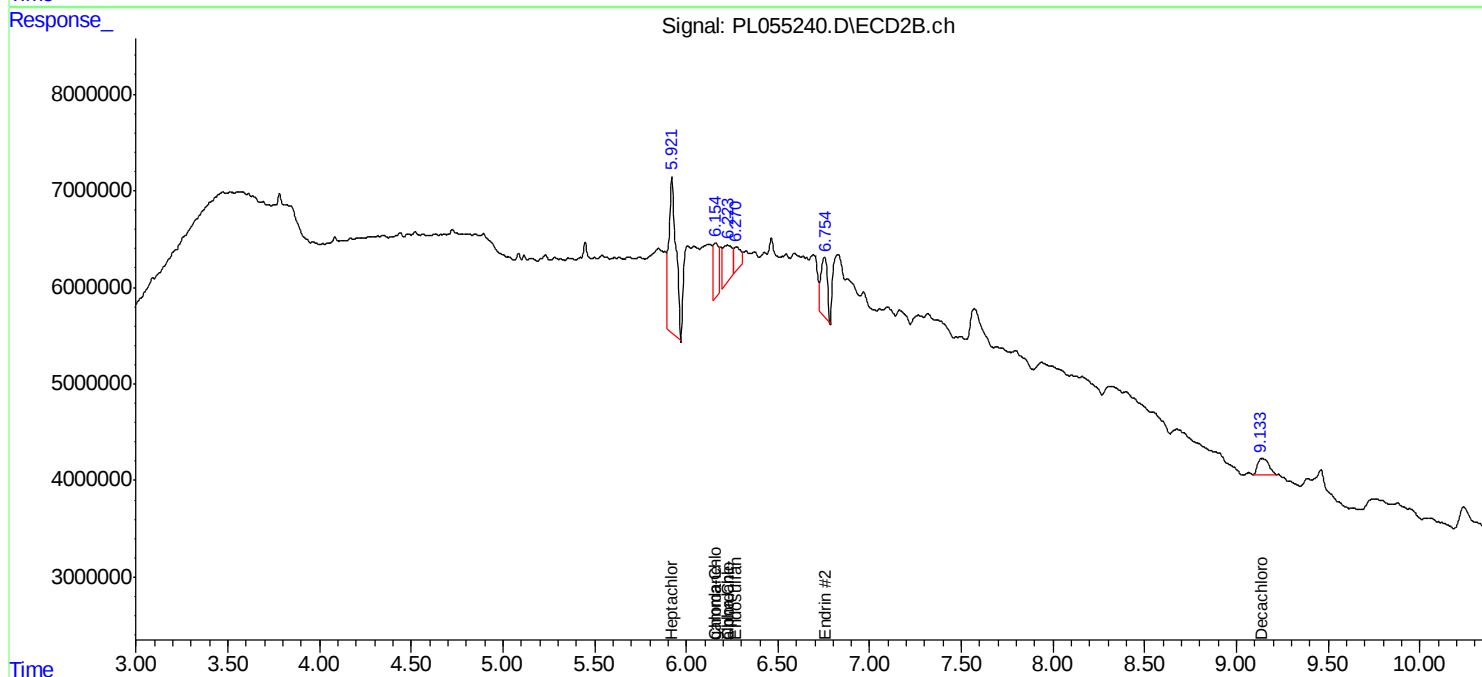


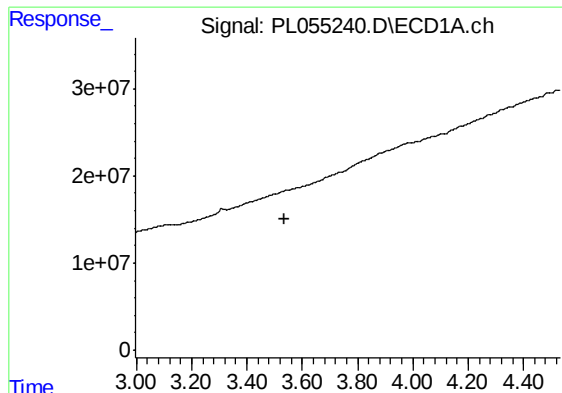

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

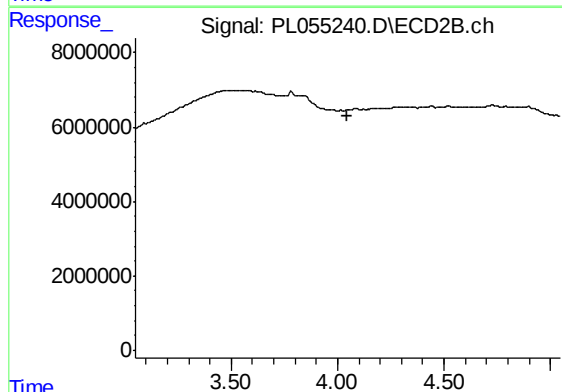


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

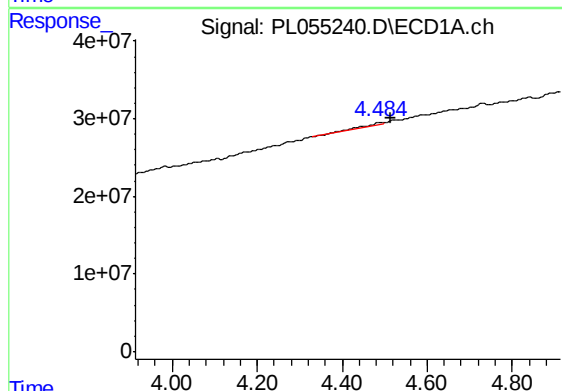


#6 beta-BHC

R.T.: 4.487 min
Delta R.T.: -0.027 min
Response: 9617076
Conc: 1.40 ng/ml

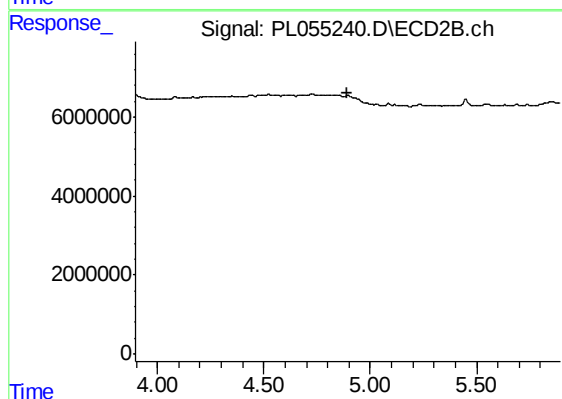

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

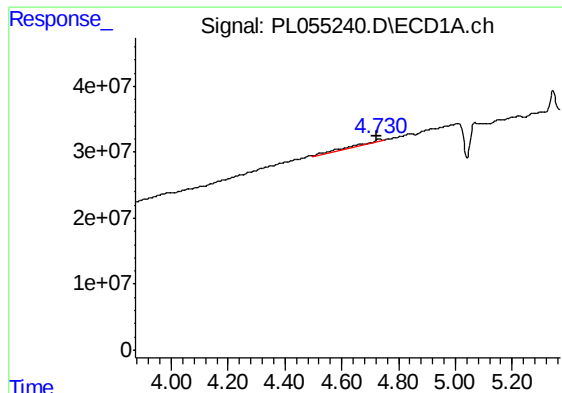

#7 delta-BHC


R.T.: 4.731 min
Delta R.T.: 0.010 min
Response: 26362256
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

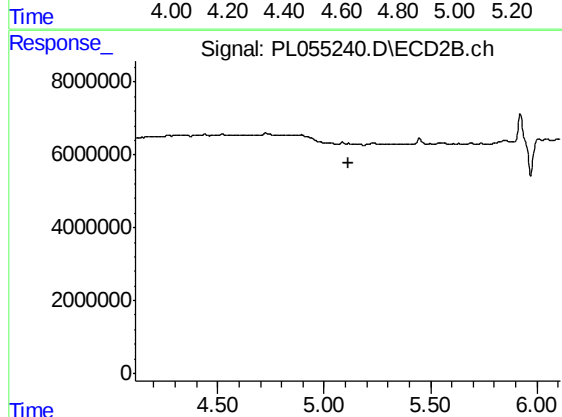


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

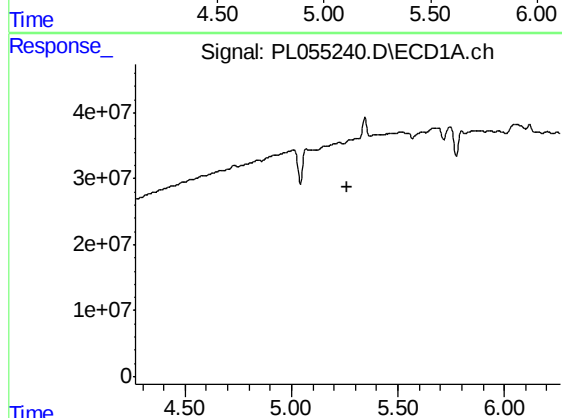


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

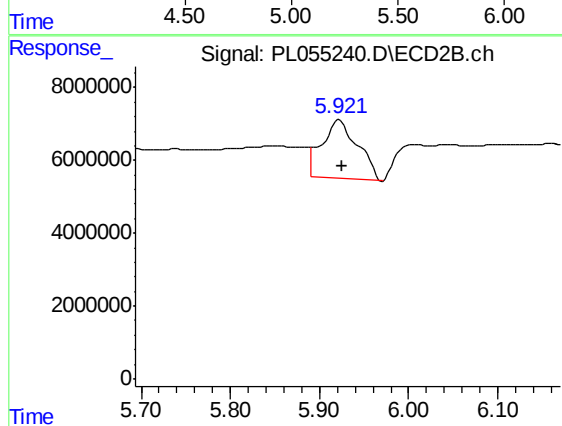

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.003 min
Response: 44484101
Conc: 17.45 ng/ml

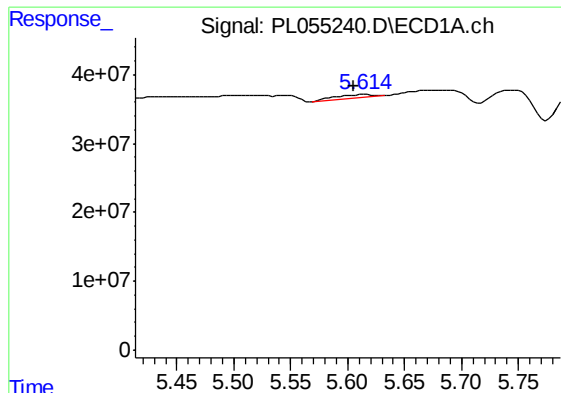

#9 Endosulfan I


R.T.: 5.615 min
Delta R.T.: 0.010 min
Response: 11635439
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

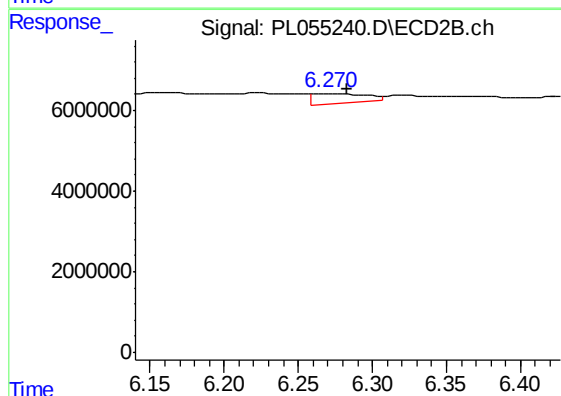


#9 Endosulfan I

R.T.: 6.273 min
Delta R.T.: -0.010 min
Response: 5981656
Conc: 2.42 ng/ml

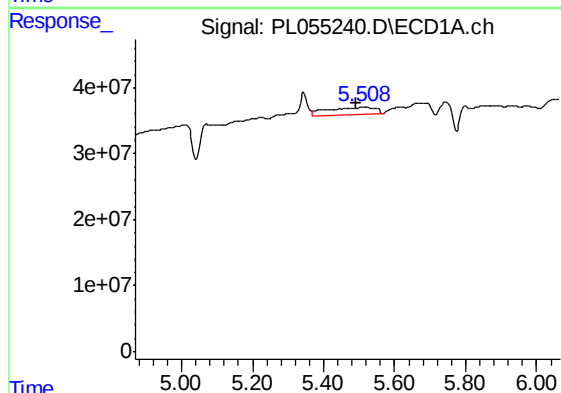


#10 gamma-Chlordane

R.T.: 5.509 min
Delta R.T.: 0.017 min
Response: 111818245
Conc: 7.67 ng/ml

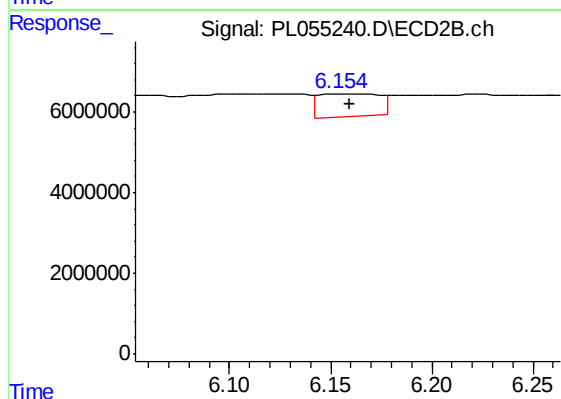

#10 gamma-Chlordane


R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 11631791
Conc: 4.38 ng/ml

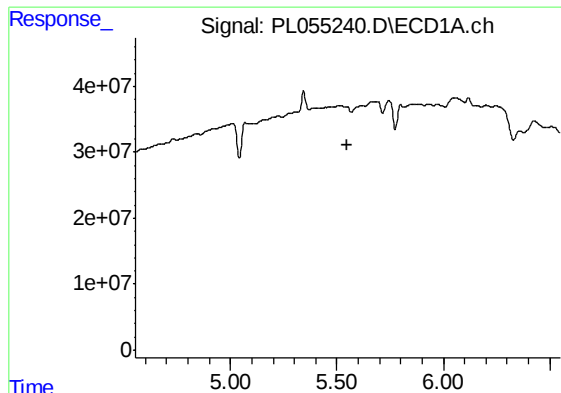

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

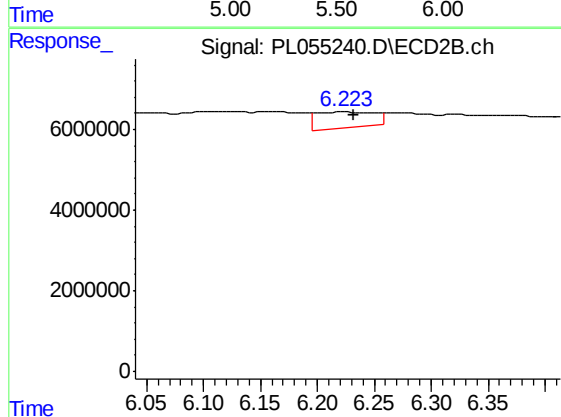


#11 alpha-Chlordane

R.T.: 6.224 min
Delta R.T.: -0.008 min
Response: 13734258
Conc: 5.24 ng/ml

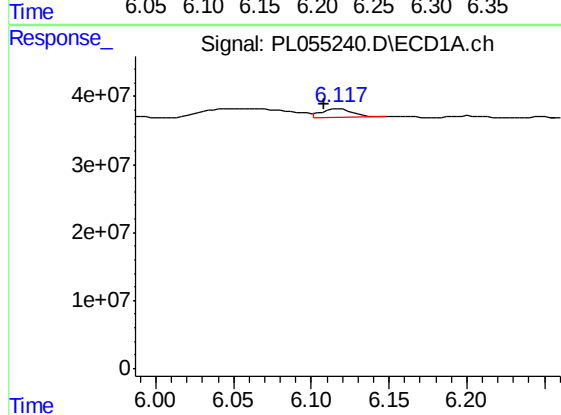


#14 Endrin

R.T.: 6.118 min
Delta R.T.: 0.010 min
Response: 17436796
Conc: 1.37 ng/ml

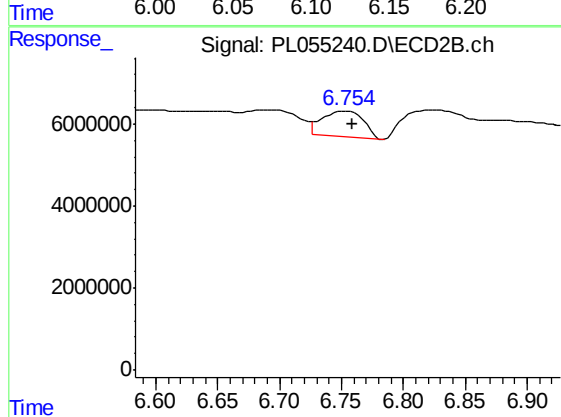

#14 Endrin


R.T.: 6.754 min
Delta R.T.: -0.005 min
Response: 14432039
Conc: 6.73 ng/ml

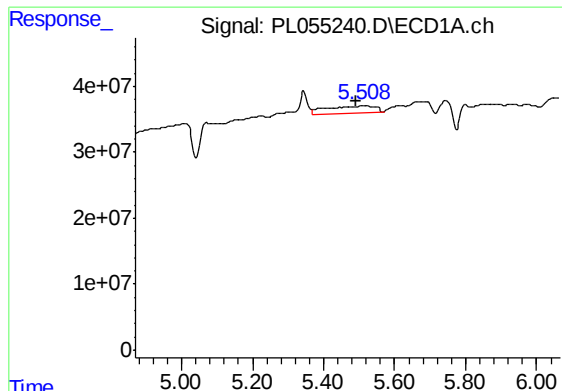

#25 Chlordane-3


R.T.: 5.509 min
Delta R.T.: 0.017 min
Response: 111818245
Conc: 88.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

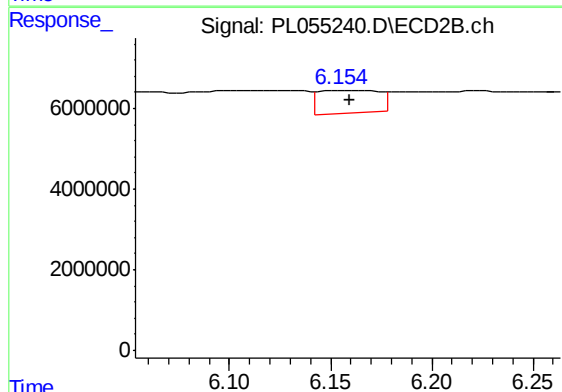


#25 Chlordane-3

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 11631791
Conc: 36.14 ng/ml

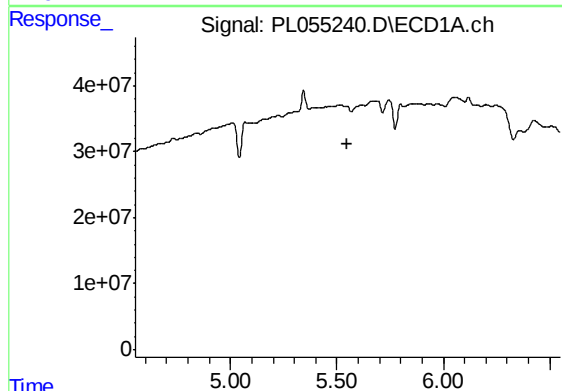


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

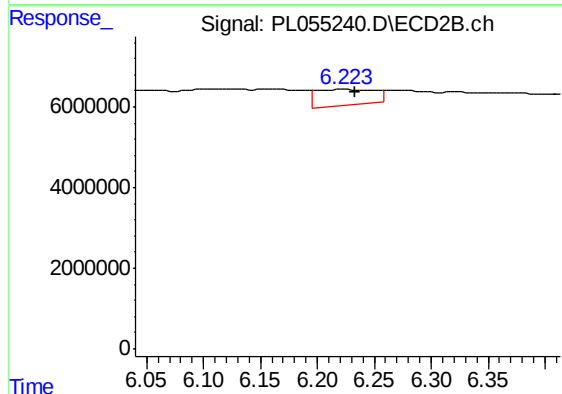

#26 Chlordane-4


R.T.: 6.224 min
Delta R.T.: -0.009 min
Response: 13734258
Conc: 35.73 ng/ml

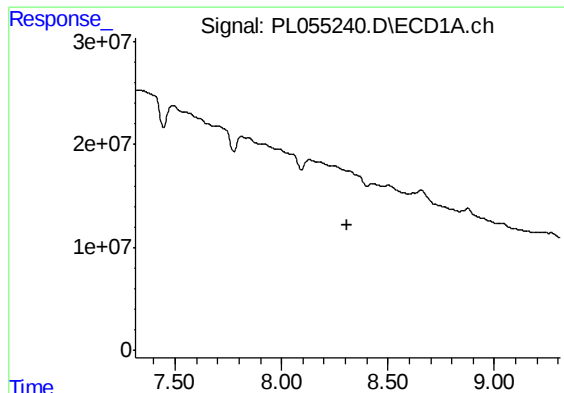

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.310 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

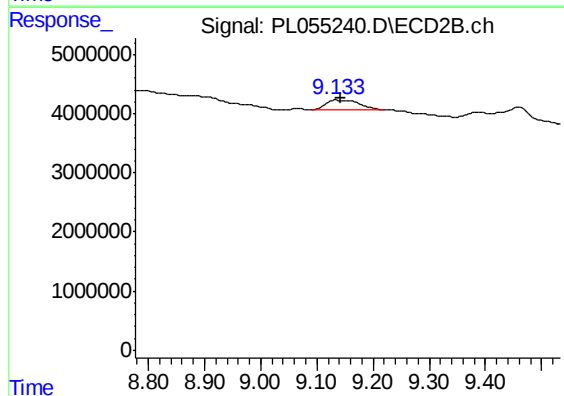

#28 Decachlorobiphenyl

R.T.: 9.134 min
Delta R.T.: -0.009 min
Response: 7014326
Conc: 3.18 ng/ml