

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122619\
 Data File : PL055286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 04:08
 Operator : SG\AJ
 Sample : K6431-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-1-(0-2)

Manual Integrations
 APPROVED

Ankita
 12/27/2019 12:34:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 04:53:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.534	4.048	228.0E6	62709768	21.683	23.733
28) SA Decachlor...	8.309	9.145	132.2E6	41418818	14.247m	18.763 #
Target Compounds						
12) B 4,4'-DDE	5.712	6.389	61143198	17658767	4.588m	7.242 #
17) MA 4,4'-DDT	6.472	7.181	49755669	13488565	4.942	6.873 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122619\
Data File : PL055286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 04:08
Operator : SG\AJ
Sample : K6431-12
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-1-(0-2)


Manual Integrations
APPROVED

Ankita
12/27/2019 12:34:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 04:53:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

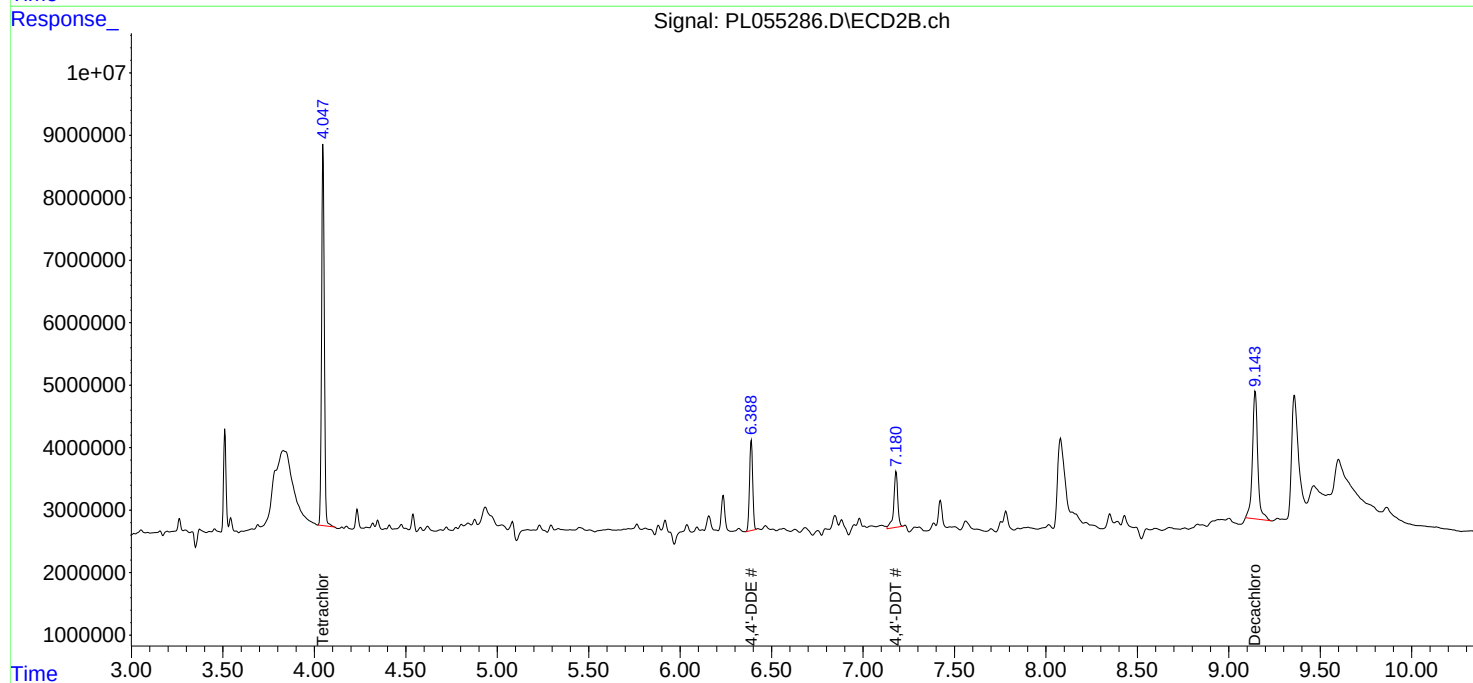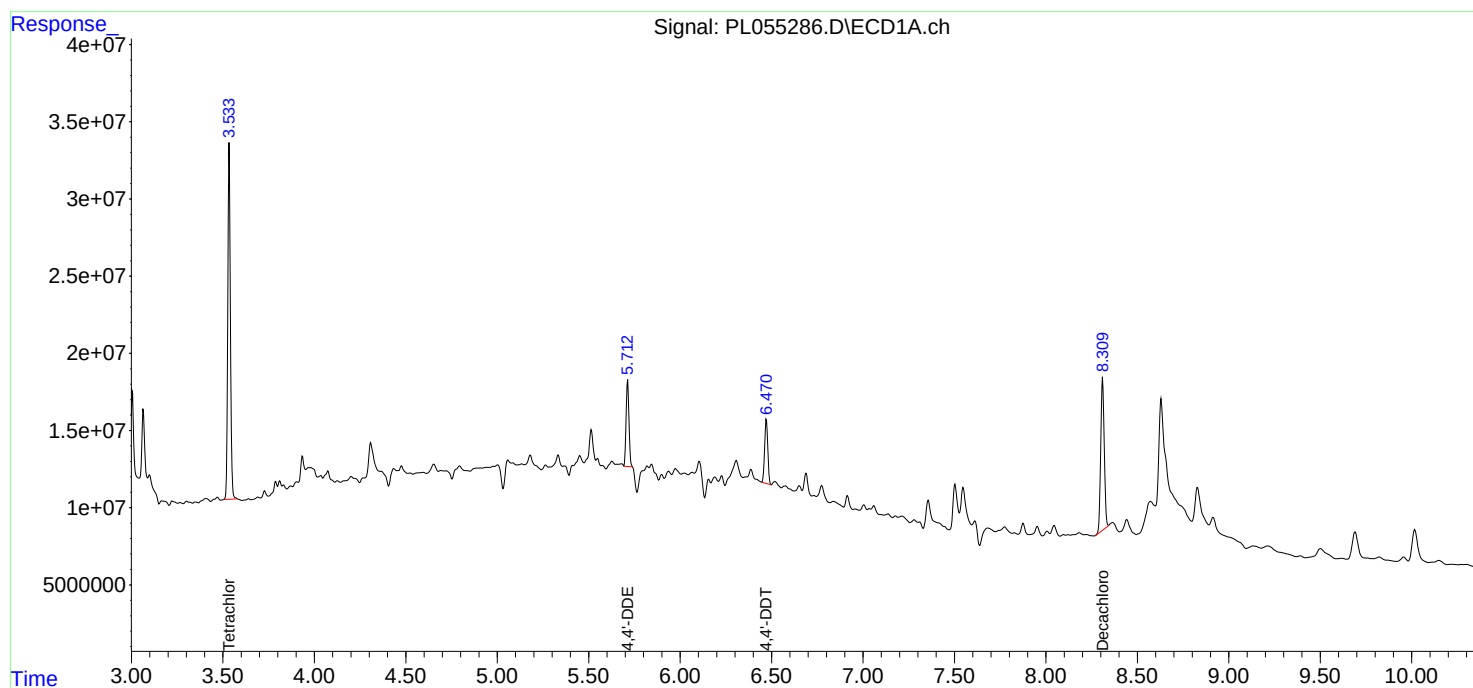

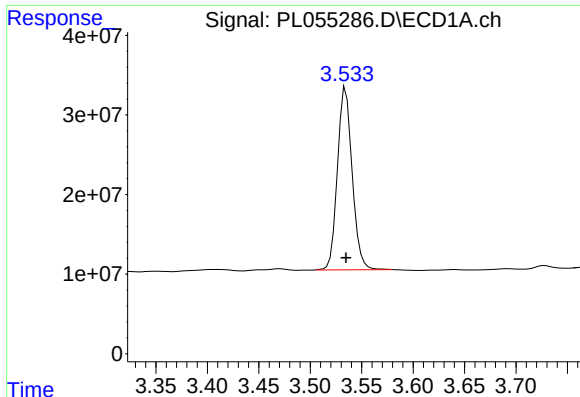


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 228027820
Conc: 21.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1-(0-2)


Manual Integrations
APPROVED

Ankita
12/27/2019 12:34:27 PM

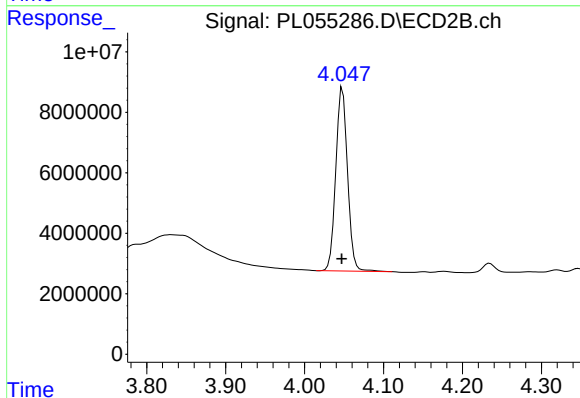


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 62709768
Conc: 23.73 ng/ml

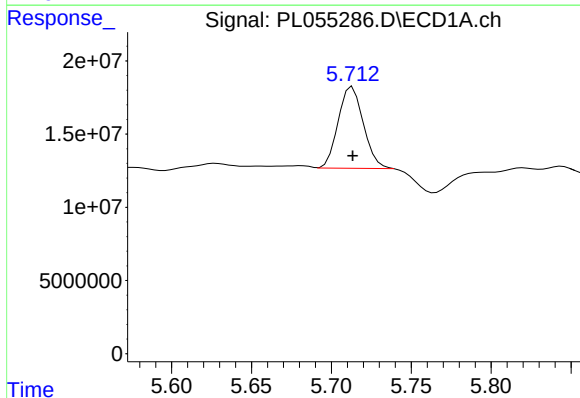


#12 4,4'-DDE

R.T.: 5.712 min
Delta R.T.: -0.002 min
Response: 61143198
Conc: 4.59 ng/ml m

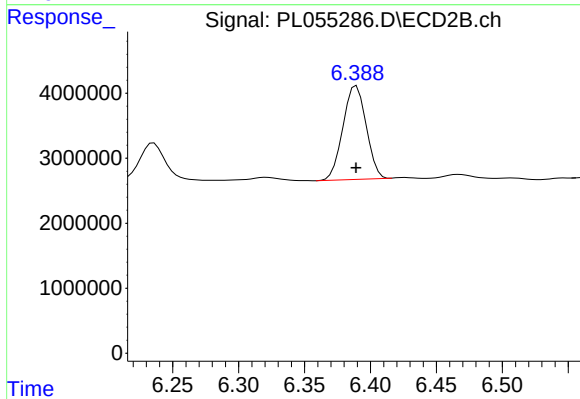

#12 4,4'-DDE

R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 17658767
Conc: 7.24 ng/ml

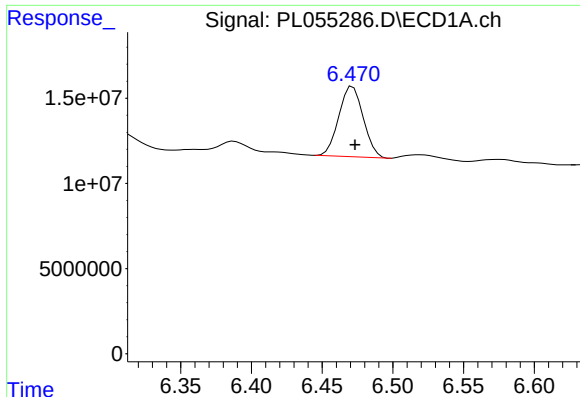


#17 4,4'-DDT

R.T.: 6.472 min
Delta R.T.: -0.002 min
Response: 49755669
Conc: 4.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1-(0-2)


Manual Integrations
APPROVED

Ankita
12/27/2019 12:34:27 PM

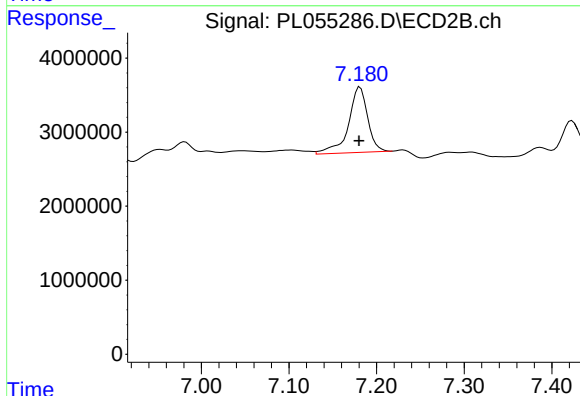


#17 4,4'-DDT

R.T.: 7.181 min
Delta R.T.: 0.001 min
Response: 13488565
Conc: 6.87 ng/ml

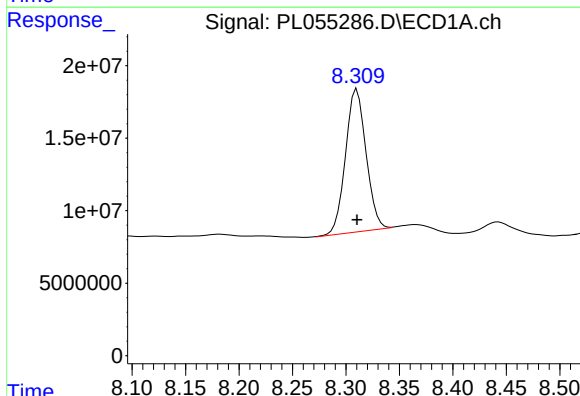

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: -0.002 min
Response: 132197910
Conc: 14.25 ng/ml m

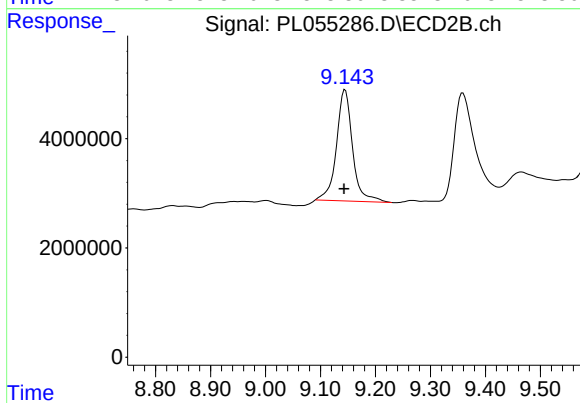

#28 Decachlorobiphenyl

R.T.: 9.145 min
Delta R.T.: 0.002 min
Response: 41418818
Conc: 18.76 ng/ml