

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122623\
 Data File : PL087494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 16:11
 Operator : AR\AJ
 Sample : 06018-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/28/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:35:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	2.677	32763306	13821375	8.706	8.211
28) SA Decachlor...	8.978	7.863	31764871	14356871	9.315	8.500m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122623\
Data File : PL087494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 16:11
Operator : AR\AJ
Sample : 06018-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/28/2023
Supervised By : Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:35:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

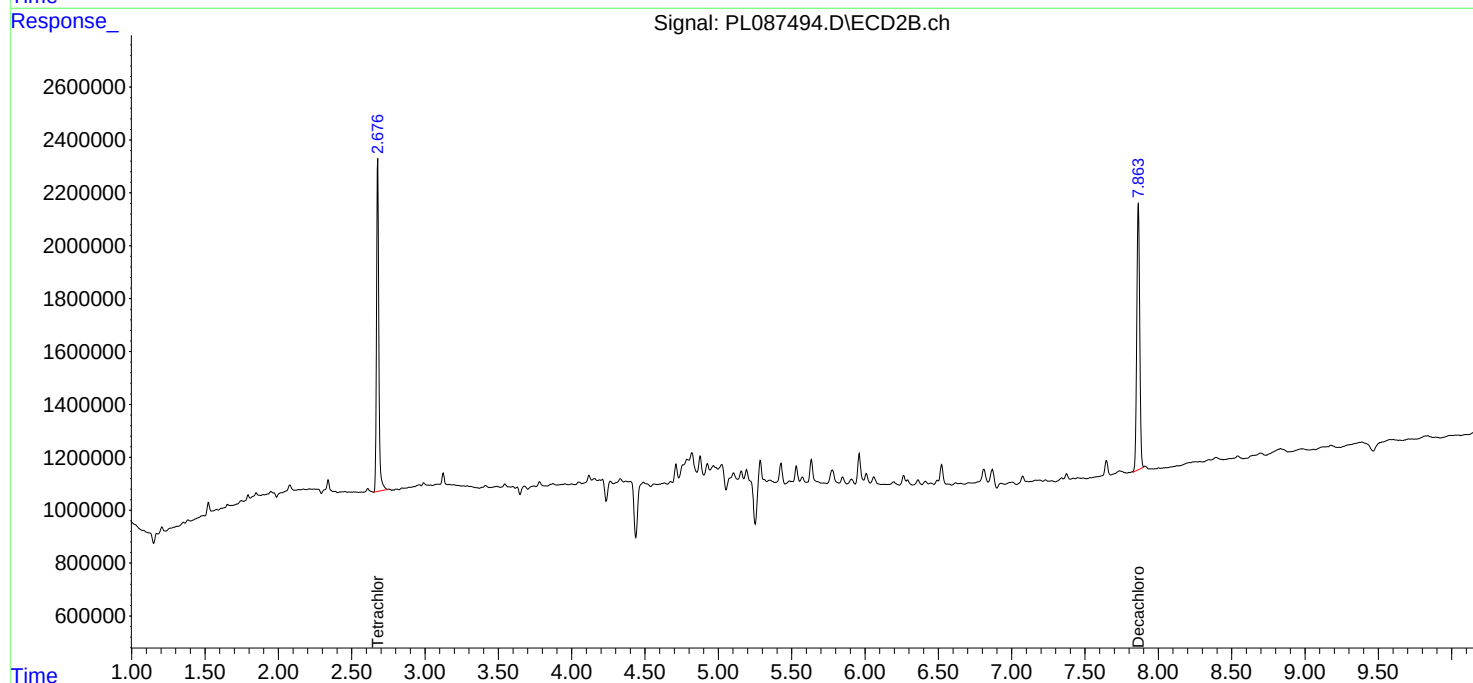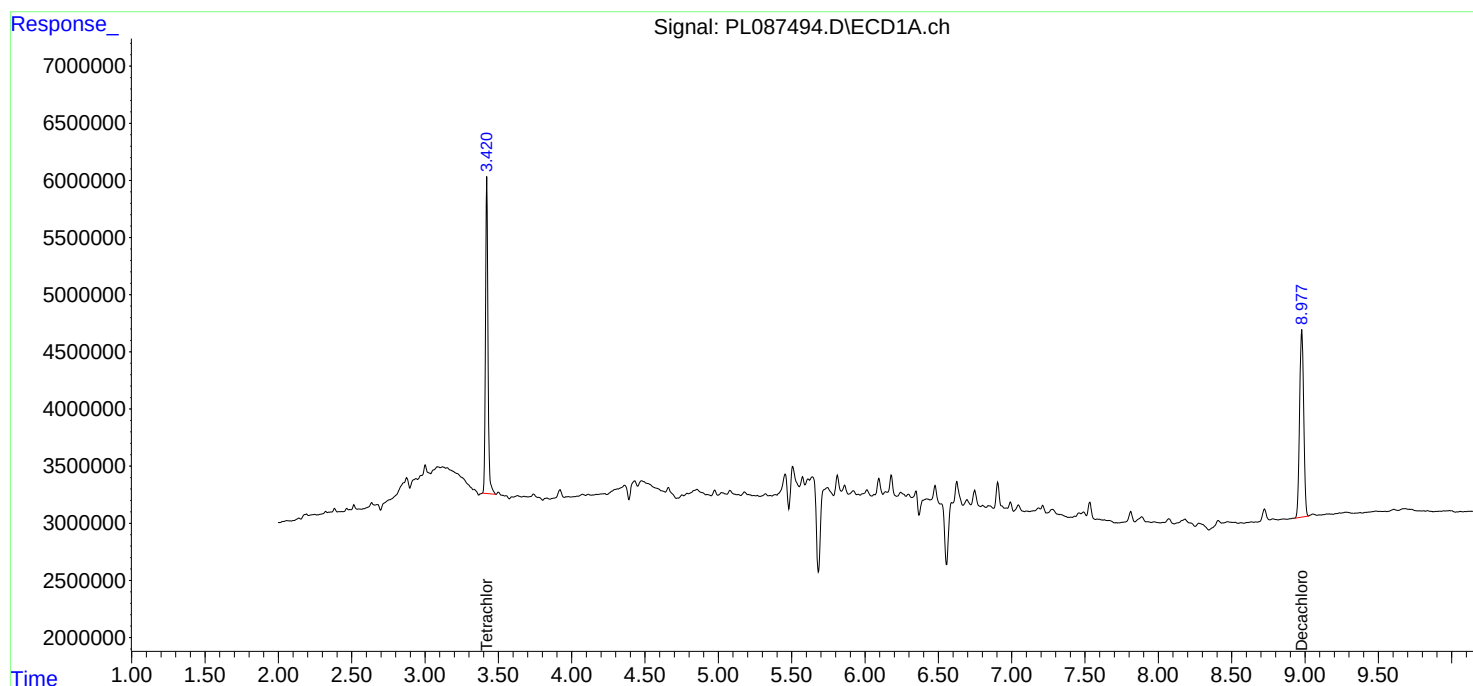

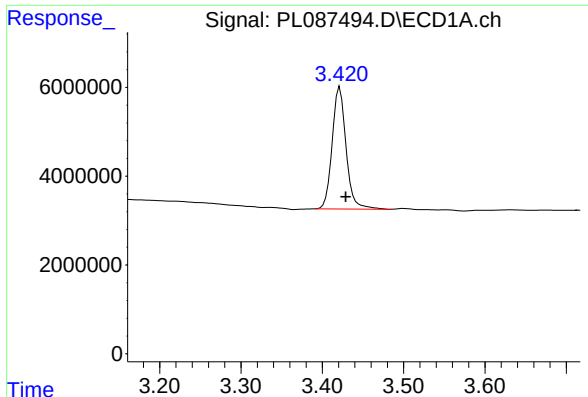


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 32763306
Conc: 8.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

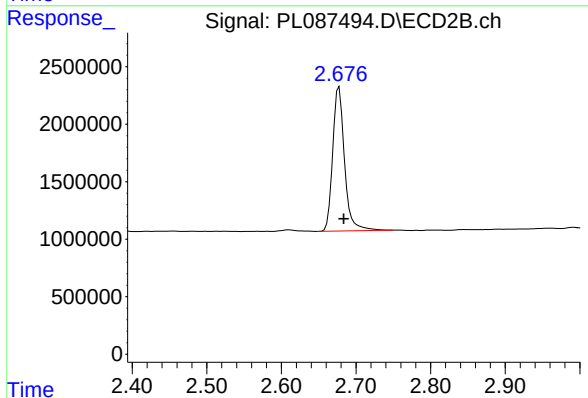


#1 Tetrachloro-m-xylene

R.T.: 2.677 min
Delta R.T.: -0.006 min
Response: 13821375
Conc: 8.21 ng/ml

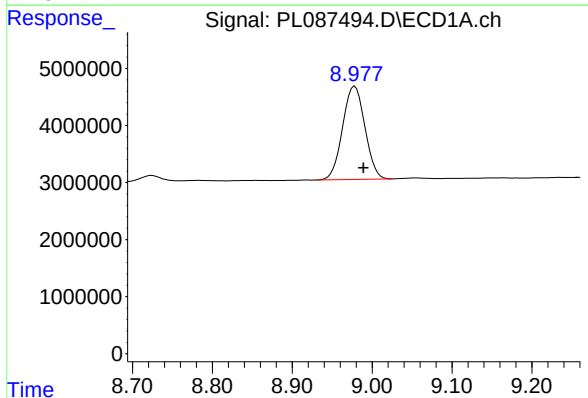

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.011 min
Response: 31764871
Conc: 9.32 ng/ml

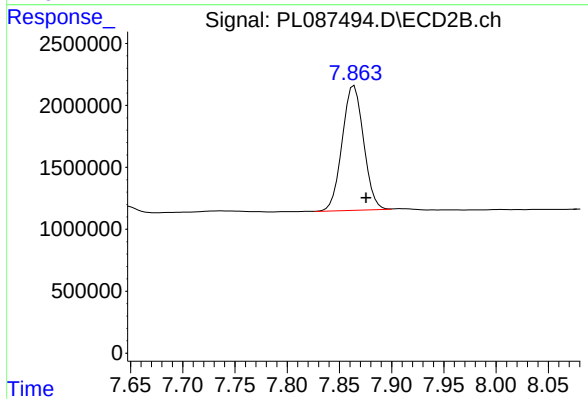

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.013 min
Response: 14356871
Conc: 8.50 ng/ml m