

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122623\
 Data File : PL087501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 19:17
 Operator : AR\AJ
 Sample : 05948-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/28/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:39:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.677	37603954	19121229	9.992	11.359
28)	SA Decachlor...	8.981	7.864	93516946	13172556	27.425	7.799m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122623\
Data File : PL087501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 19:17
Operator : AR\AJ
Sample : 05948-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:39:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

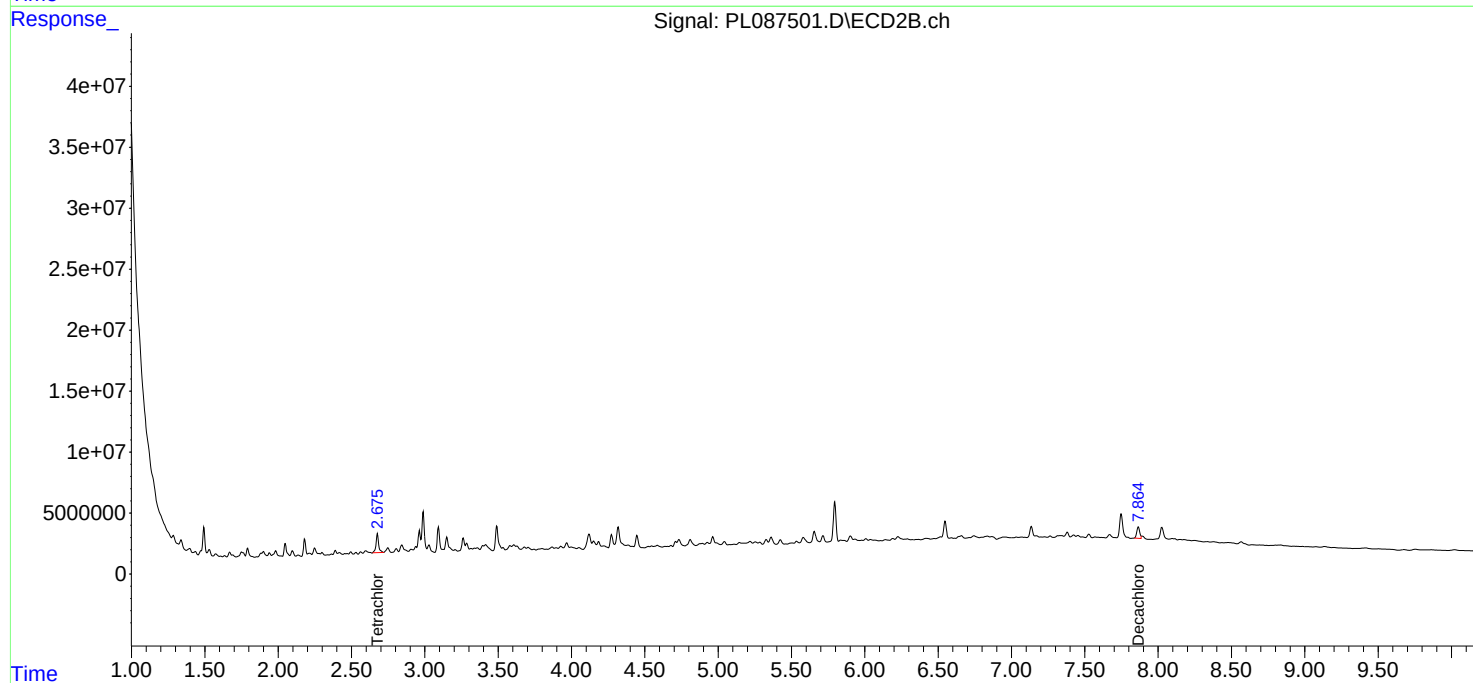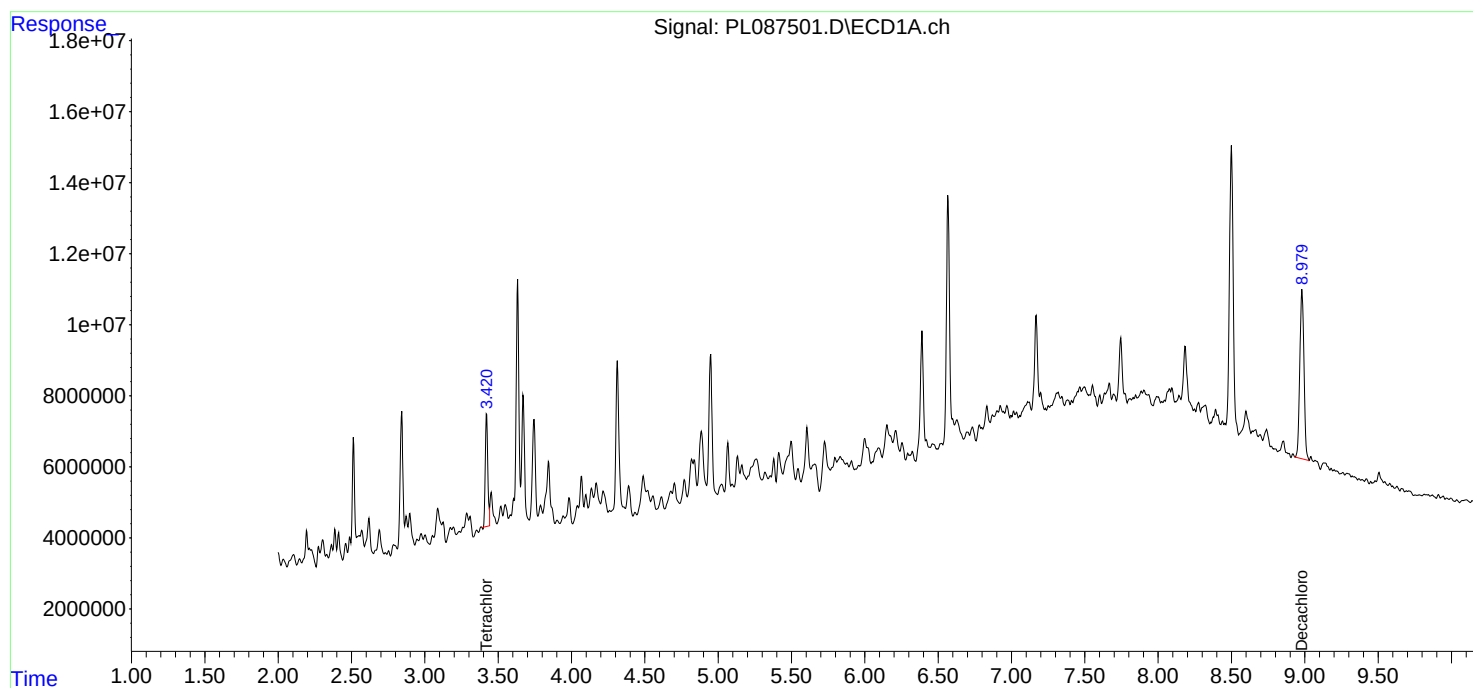

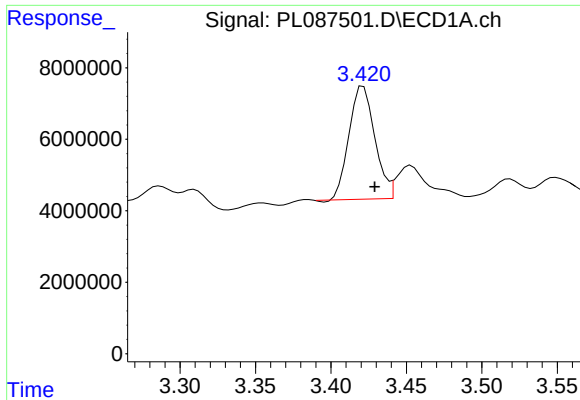


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 37603954
Conc: 9.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

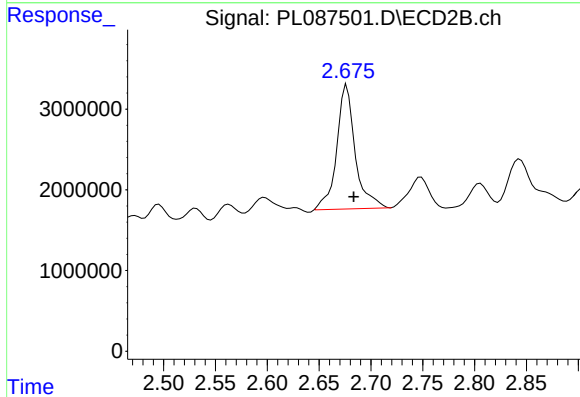


#1 Tetrachloro-m-xylene

R.T.: 2.677 min
Delta R.T.: -0.007 min
Response: 19121229
Conc: 11.36 ng/ml

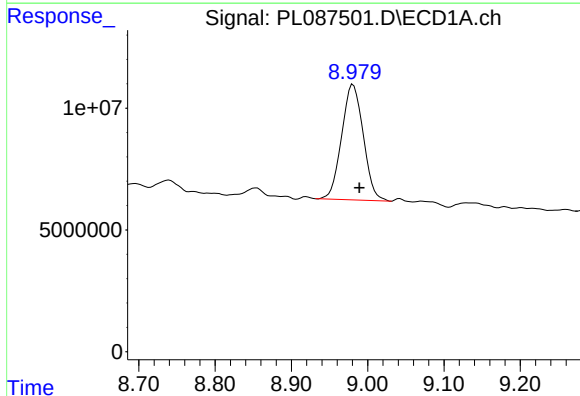

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: -0.008 min
Response: 93516946
Conc: 27.42 ng/ml

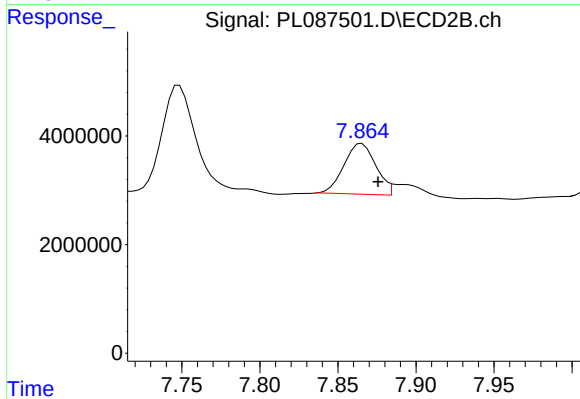

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: -0.012 min
Response: 13172556
Conc: 7.80 ng/ml m