

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122624\
 Data File : PL093521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 13:33
 Operator : AR\AJ
 Sample : P5382-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/27/2024
 Supervised By : Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 03:59:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.773	53787474	60205803	21.726m	20.681
28) SA Decachlor...	9.051	7.910	39546131	59608024	21.388m	19.963m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122624\
Data File : PL093521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 13:33
Operator : AR\AJ
Sample : P5382-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/27/2024
Supervised By : Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 03:59:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

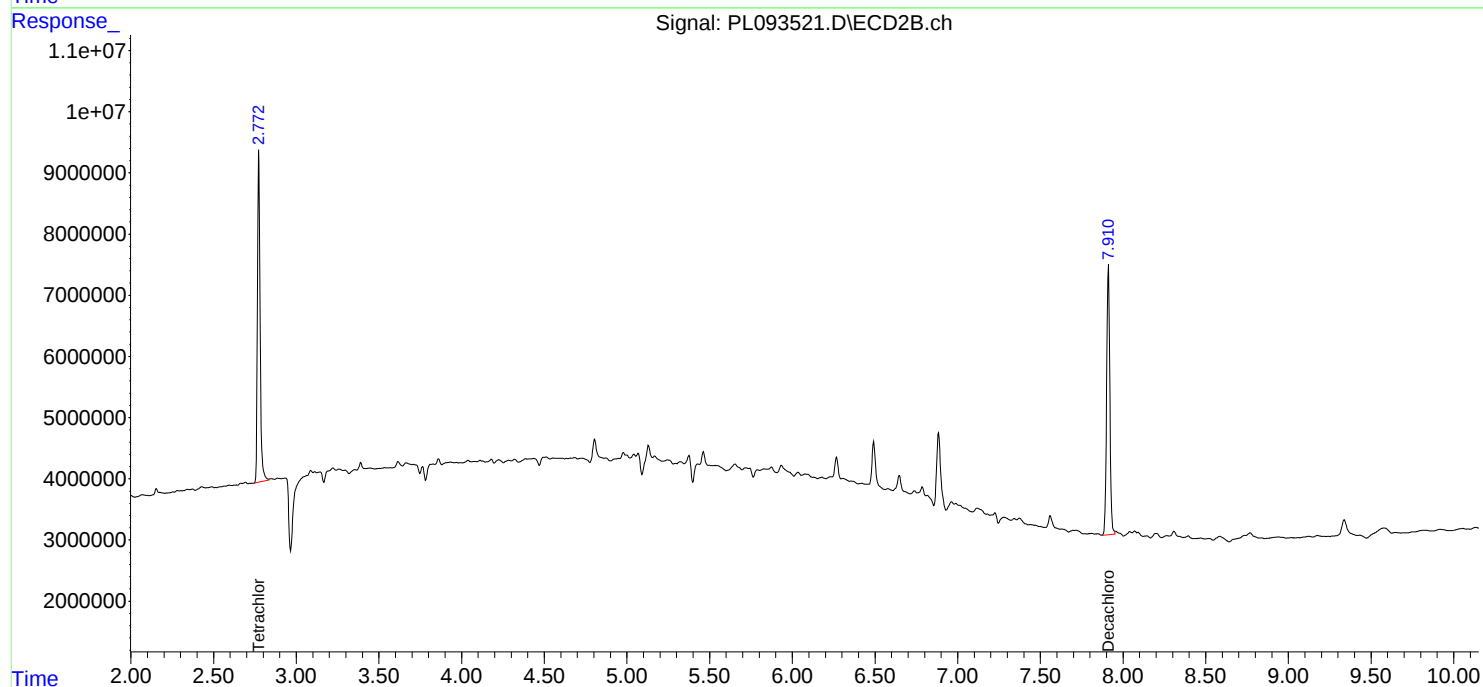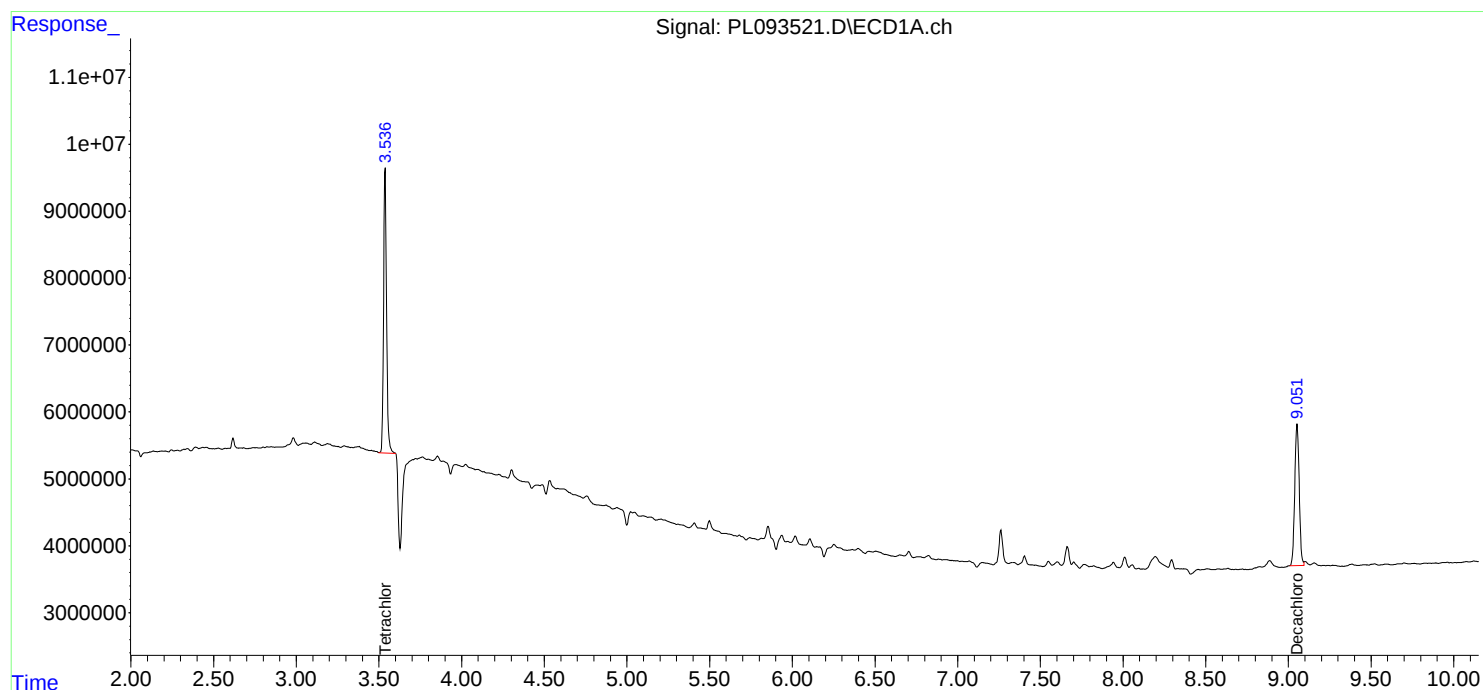

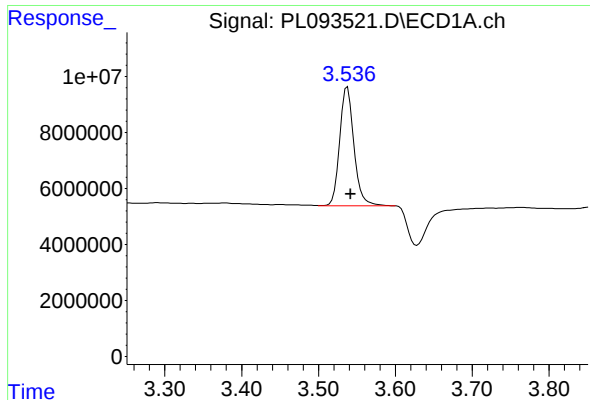


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.006 min
Response: 53787474
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

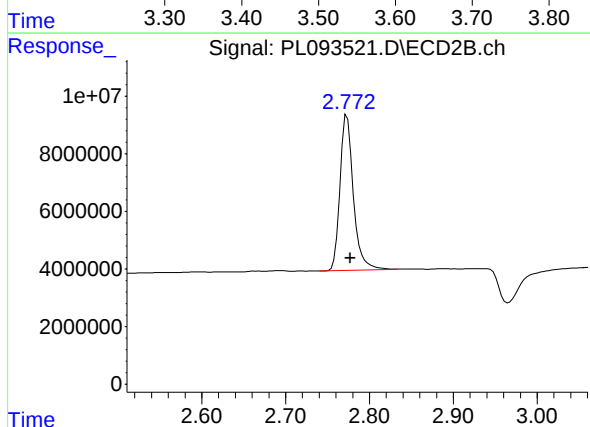


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: -0.004 min
Response: 60205803
Conc: 20.68 ng/ml

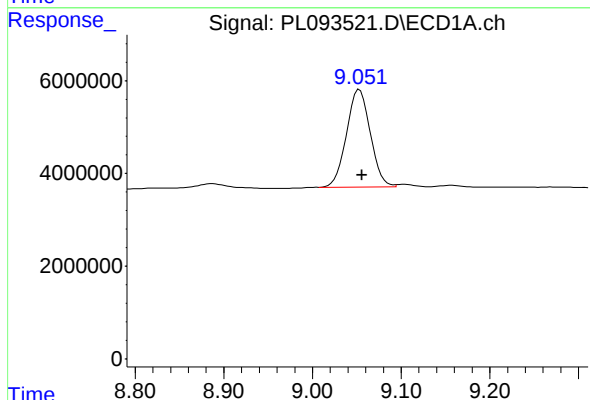

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.004 min
Response: 39546131
Conc: 21.39 ng/ml m

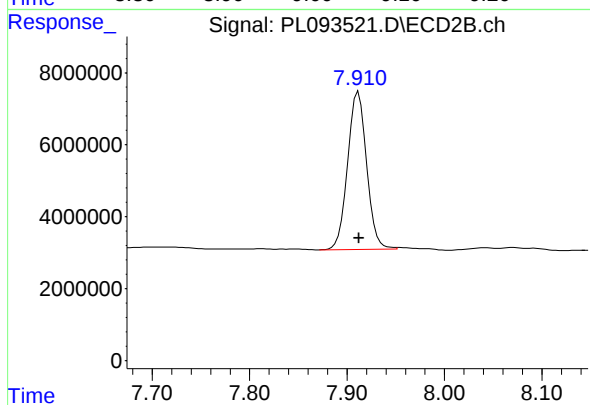

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 59608024
Conc: 19.96 ng/ml m