

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
 Data File : PL043438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2018 11:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:06:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.098	133.5E6	66566942	21.773	22.459
28)	SA Decachlor...	8.195	9.223	130.1E6	52550901	19.929	20.146
Target Compounds							
6)	B beta-BHC	4.394f	0.000	1538833	0	0.417	N.D. #
8)	B Heptachlo...	0.000	6.008	0	2209472	N.D.	0.583 #
14)	MA Endrin	0.000	6.853	0	11117782	N.D.	3.561 #
15)	B Endosulfa...	6.318f	7.099f	949141	1395649	0.143	0.461 #
16)	A 4,4'-DDD	6.081f	0.000	26566708	0	4.685	N.D. #
17)	MA 4,4'-DDT	6.318f	0.000	949141	0	0.160	N.D. #
18)	B Endrin al...	0.000	7.099f	0	1395649	N.D.	0.556 #
23)	Chlordane-1	4.358	0.000	558974	0	2.080	N.D. #
24)	Chlordane-2	0.000	5.546	0	352975	N.D.	2.461 #
27)	Chlordane-5	6.318	7.099	949141	1395649	3.957	11.904 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
Data File : PL043438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2018 11:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:06:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

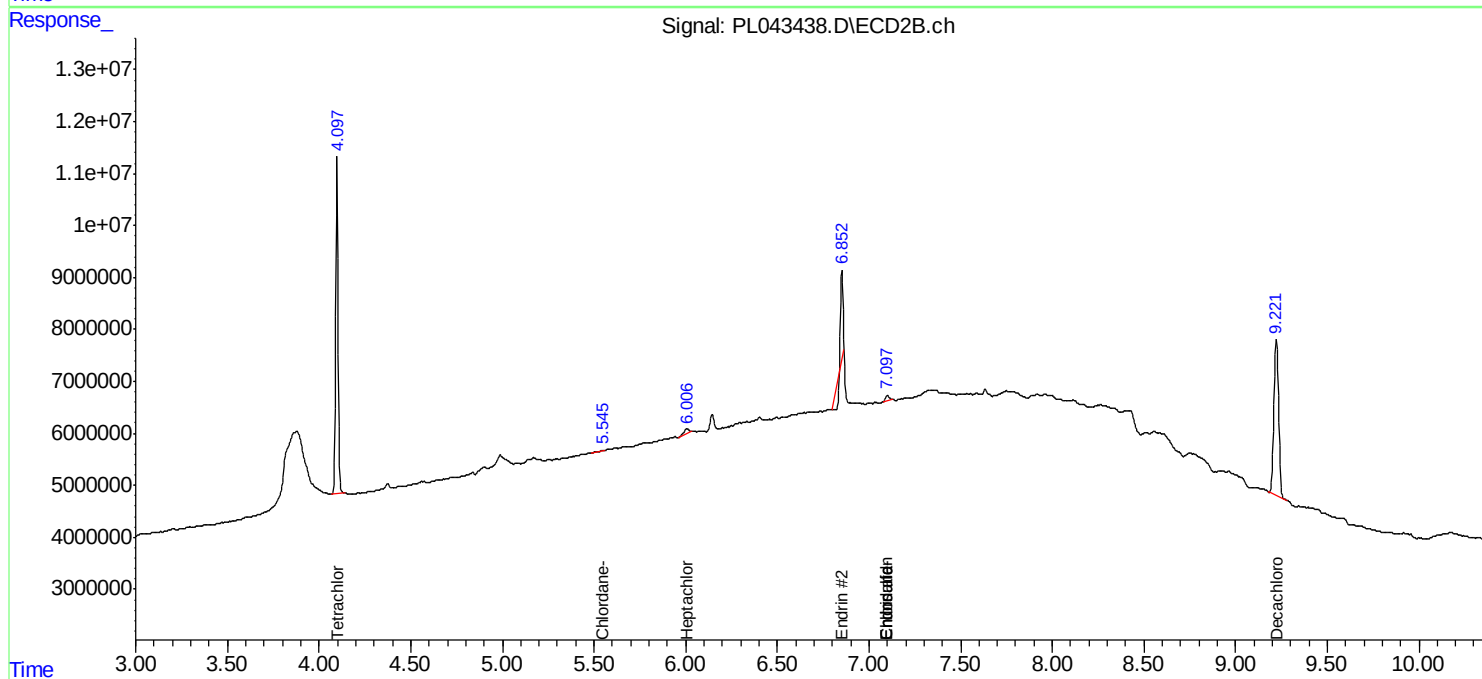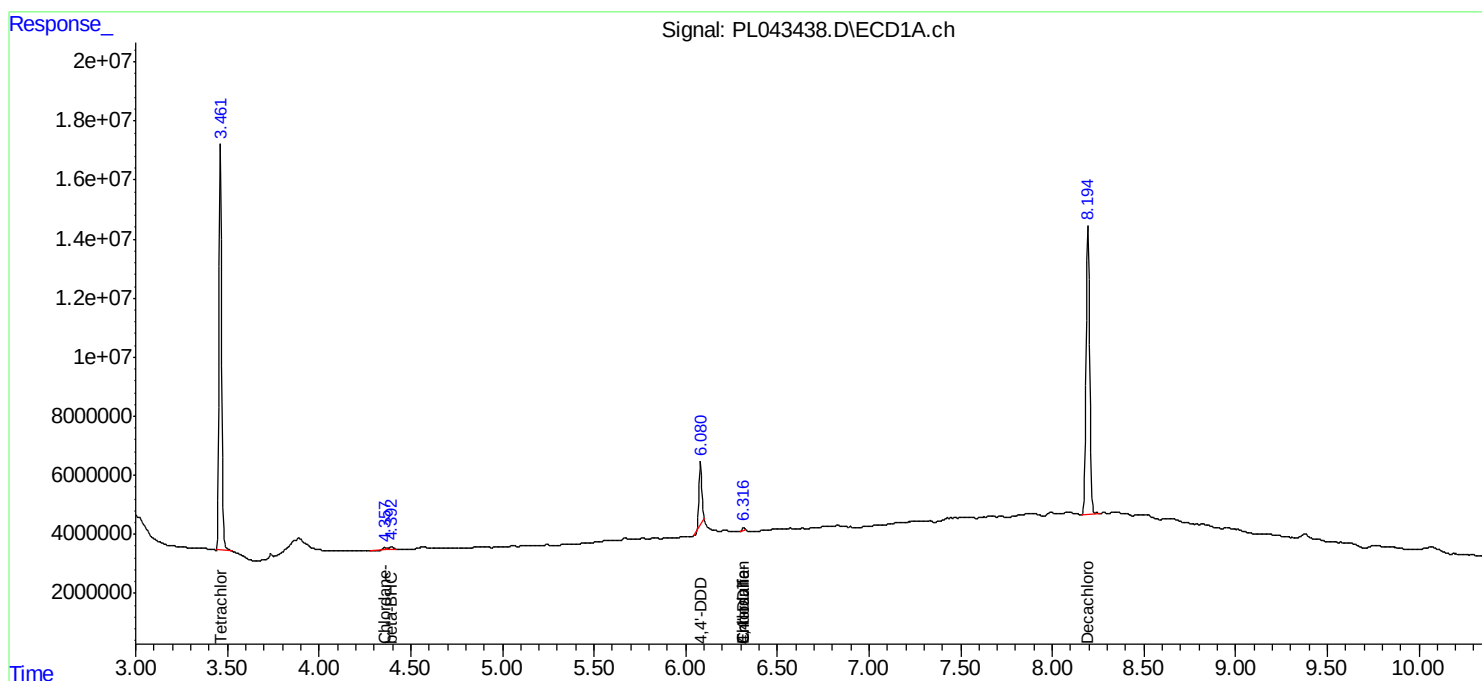


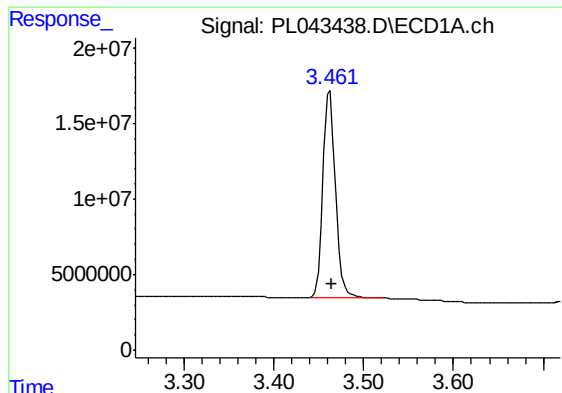

#1 Tetrachloro-m-xylene


R.T.: 3.462 min
Delta R.T.: -0.002 min
Response: 133533570
Conc: 21.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

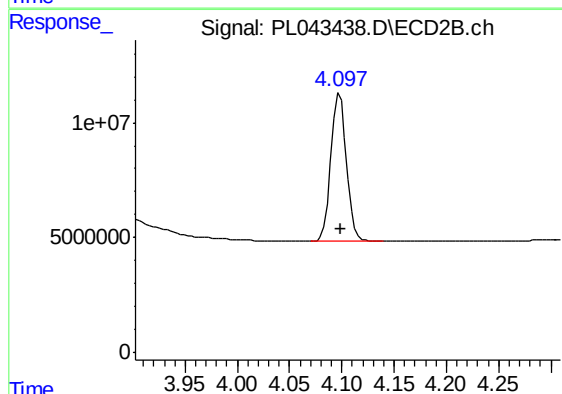


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 66566942
Conc: 22.46 ng/ml

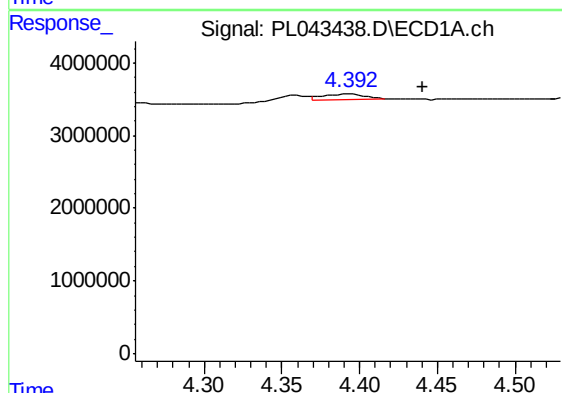


#6 beta-BHC

R.T.: 4.394 min
Delta R.T.: -0.047 min
Response: 1538833
Conc: 0.42 ng/ml

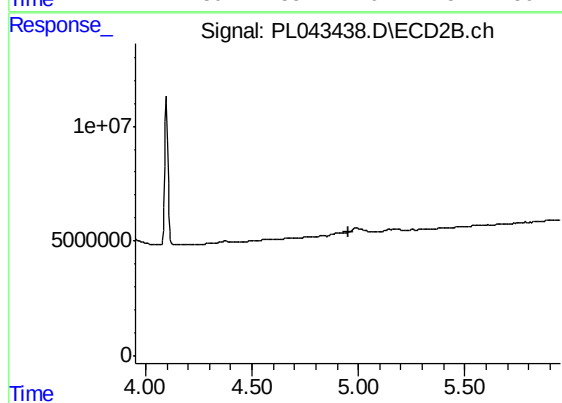

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

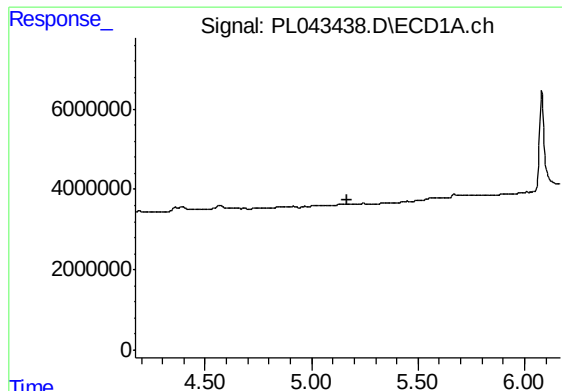

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

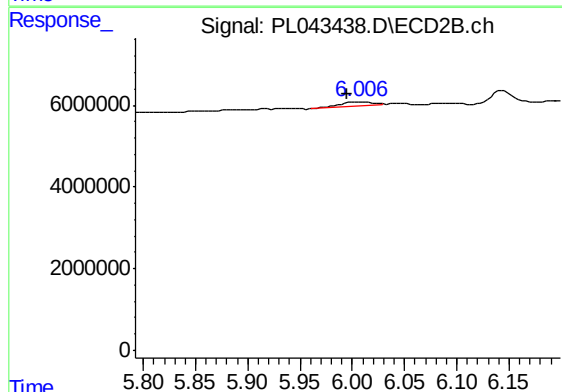


#8 Heptachlor epoxide

R.T.: 6.008 min
Delta R.T.: 0.013 min
Response: 2209472
Conc: 0.58 ng/ml

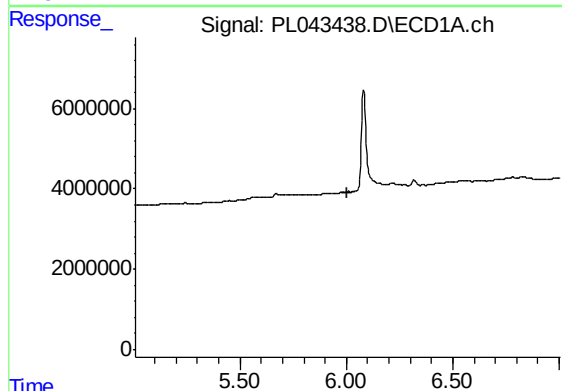


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.007 min
Response: 0
Conc: N.D.

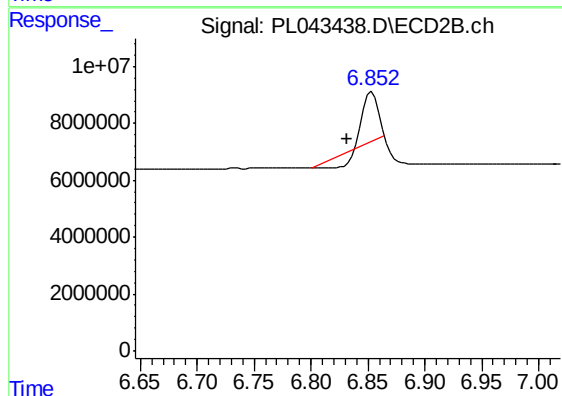

#14 Endrin


R.T.: 6.853 min
Delta R.T.: 0.021 min
Response: 11117782
Conc: 3.56 ng/ml

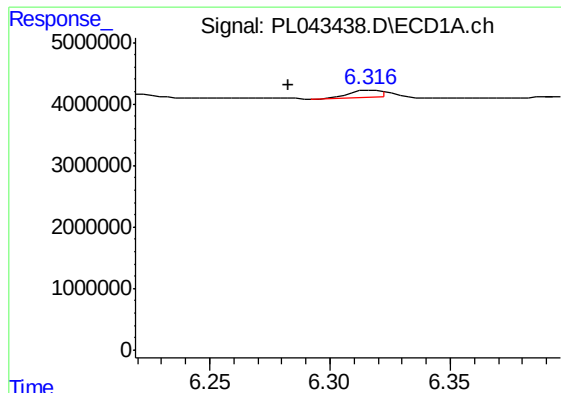

#15 Endosulfan II


R.T.: 6.318 min
Delta R.T.: 0.035 min
Response: 949141
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

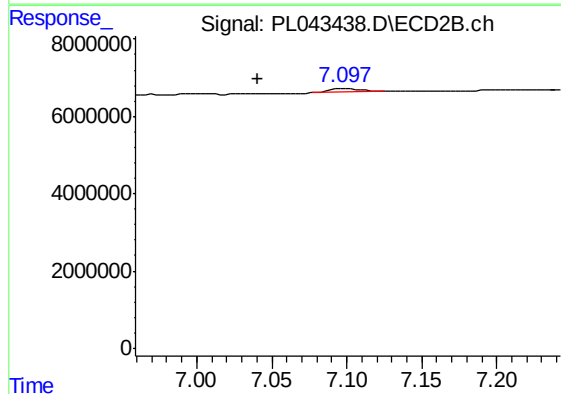


#15 Endosulfan II

R.T.: 7.099 min
Delta R.T.: 0.058 min
Response: 1395649
Conc: 0.46 ng/ml

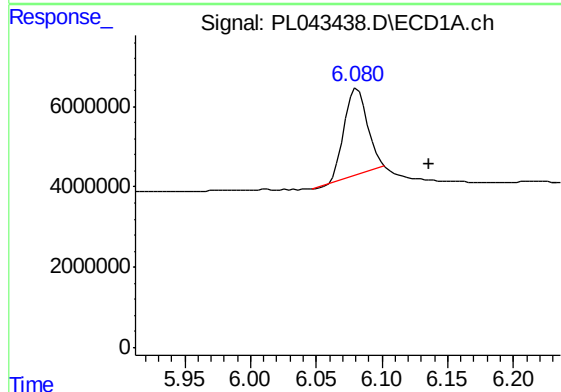


#16 4,4'-DDD

R.T.: 6.081 min
Delta R.T.: -0.055 min
Response: 26566708
Conc: 4.68 ng/ml

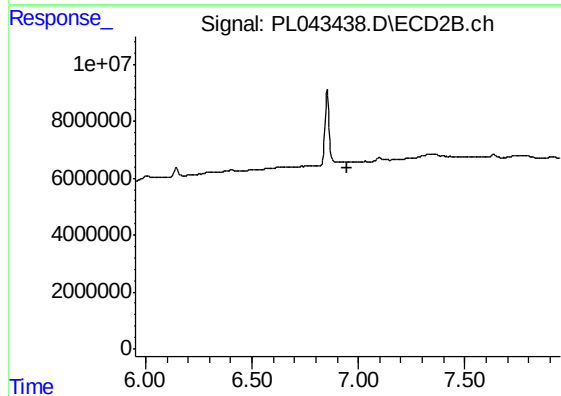

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

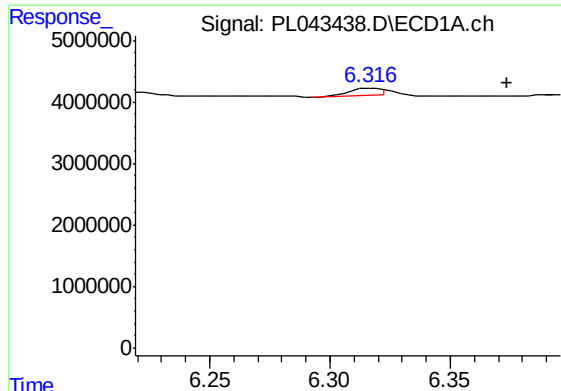

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: -0.056 min
Response: 949141
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

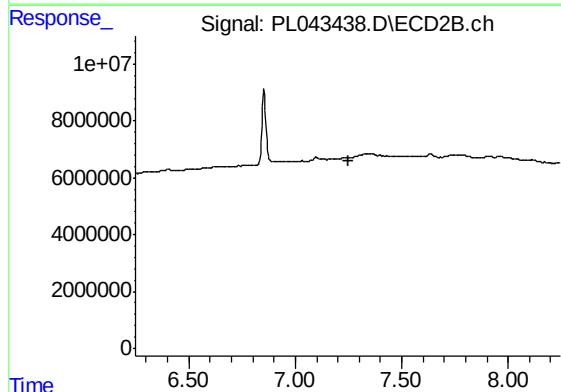


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

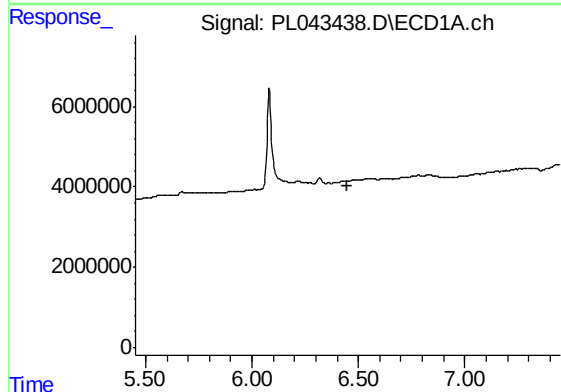


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.450 min
Response: 0
Conc: N.D.

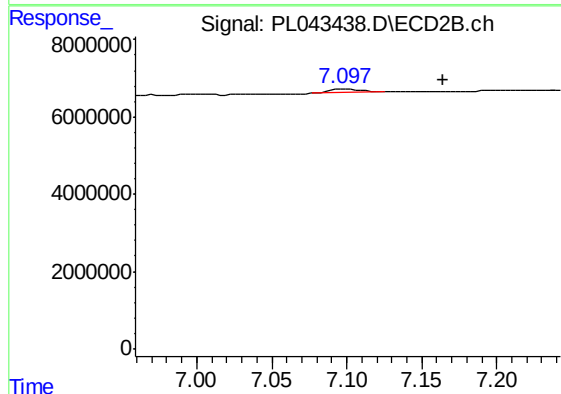

#18 Endrin aldehyde


R.T.: 7.099 min
Delta R.T.: -0.066 min
Response: 1395649
Conc: 0.56 ng/ml

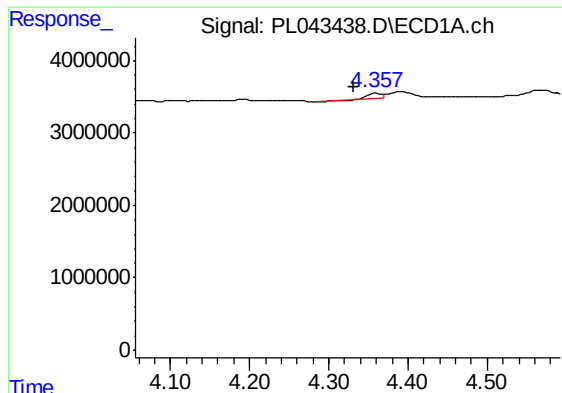

#23 Chlordane-1


R.T.: 4.358 min
Delta R.T.: 0.026 min
Response: 558974
Conc: 2.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

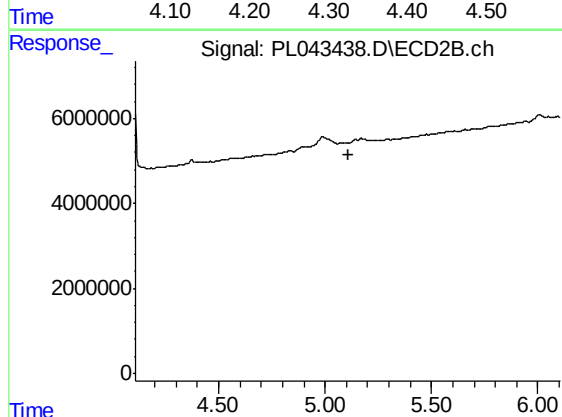


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

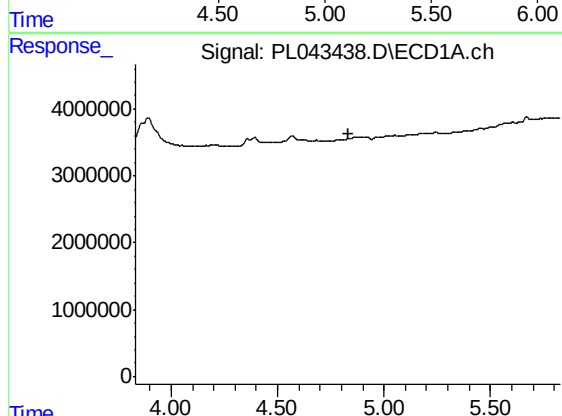


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

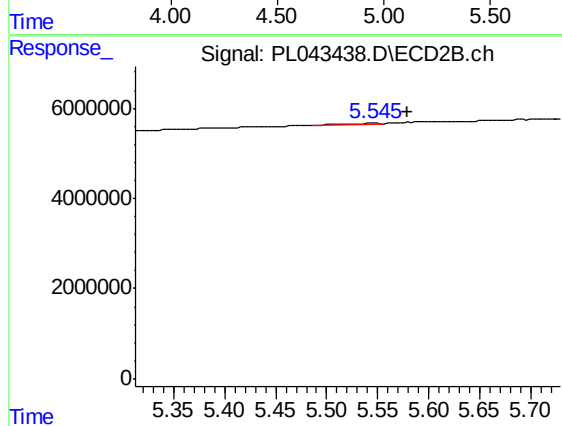

#24 Chlordane-2


R.T.: 5.546 min
Delta R.T.: -0.033 min
Response: 352975
Conc: 2.46 ng/ml

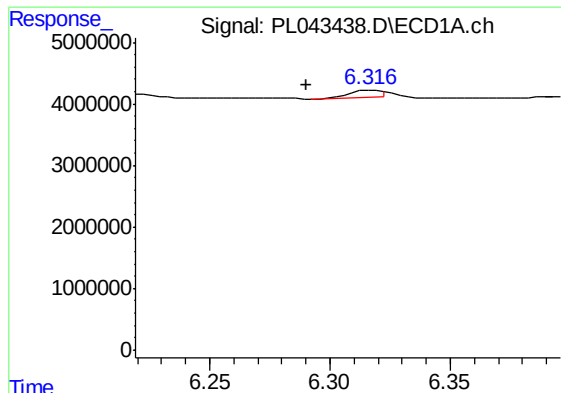

#27 Chlordane-5


R.T.: 6.318 min
Delta R.T.: 0.028 min
Response: 949141
Conc: 3.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

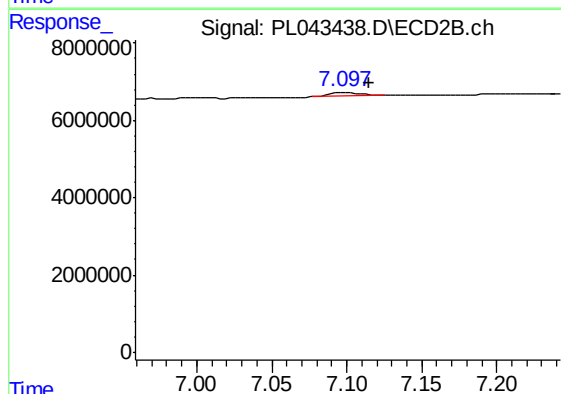


#27 Chlordane-5

R.T.: 7.099 min
Delta R.T.: -0.016 min
Response: 1395649
Conc: 11.90 ng/ml

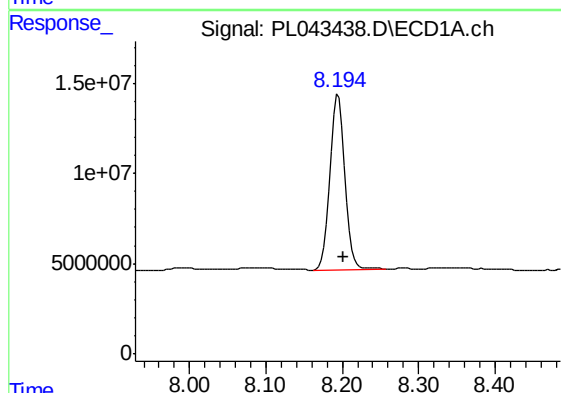

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: -0.006 min
Response: 130138225
Conc: 19.93 ng/ml

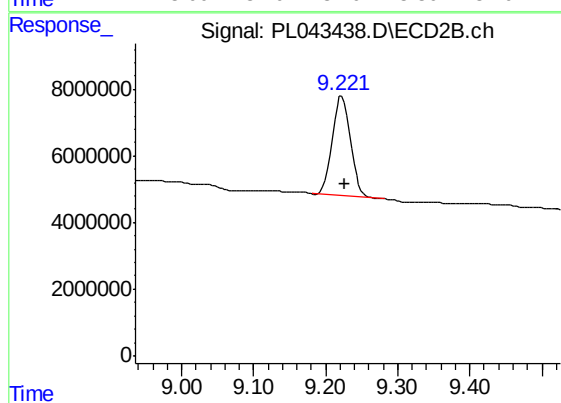

#28 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 52550901
Conc: 20.15 ng/ml