

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
 Data File : PL043440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2018 14:05
 Operator : AJ\SJ
 Sample : PB116007BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB116007BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:07:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.098	130.1E6	64226459	21.211	21.670
28)	SA Decachlor...	8.199	9.226	136.0E6	55266495	20.829	21.187
Target Compounds							
6)	B beta-BHC	4.411f	4.982f	697547	3584481	0.189	2.117 #
7)	B delta-BHC	0.000	5.143f	0	1591521	N.D.	0.370 #
8)	B Heptachlo...	0.000	6.003	0	2780103	N.D.	0.733 #
9)	A Endosulfan I	0.000	6.363	0	779988	N.D.	0.230 #
11)	B alpha-Chl...	0.000	6.363f	0	779988	N.D.	0.217 #
19)	B Endosulfa...	0.000	7.381	0	3652633	N.D.	1.215 #
20)	A Methoxychlor	0.000	7.643f	0	3041685	N.D.	2.017 #
21)	B Endrin ke...	7.195f	0.000	1088773	0	0.151	N.D. #
23)	Chlordane-1	4.363	5.143	203020	1591521	0.756	11.261 #
26)	Chlordane-4	0.000	6.363	0	779988	N.D.	1.367 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
Data File : PL043440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2018 14:05
Operator : AJ\SJ
Sample : PB116007BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB116007BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:07:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

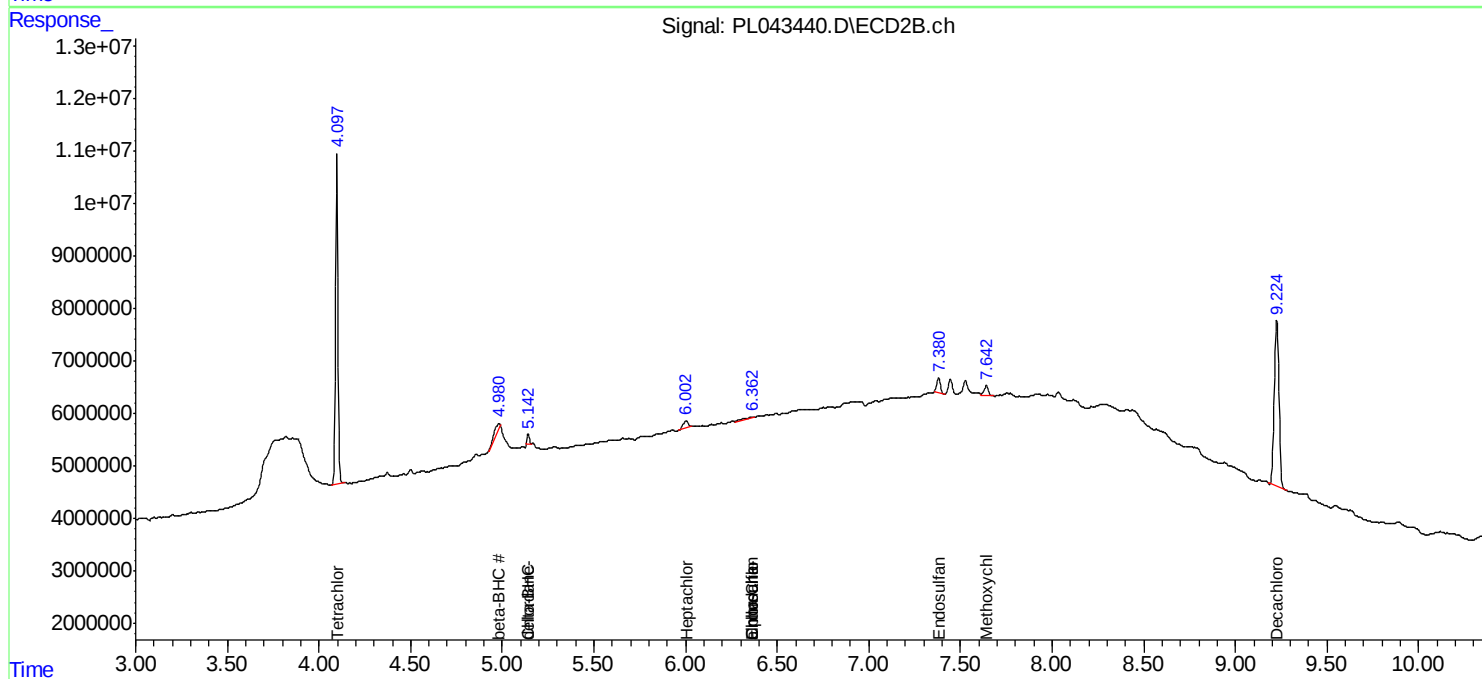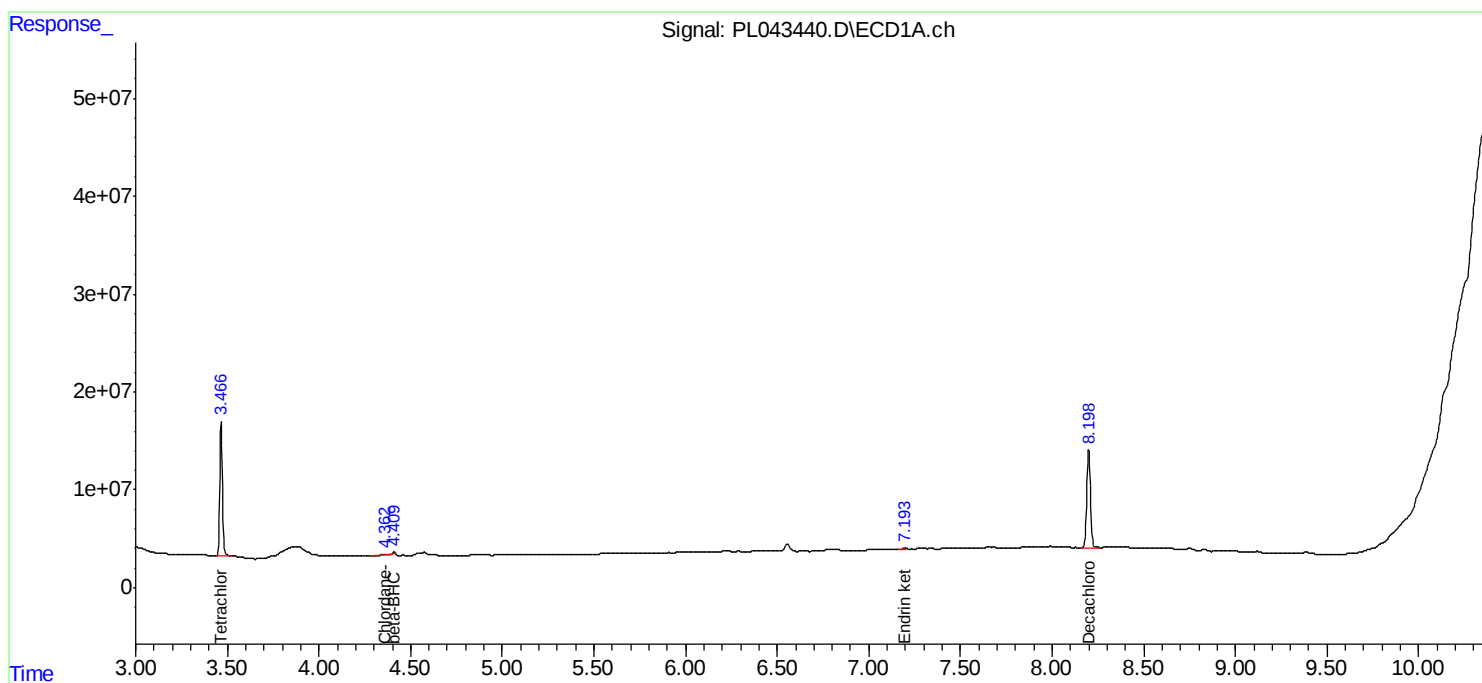


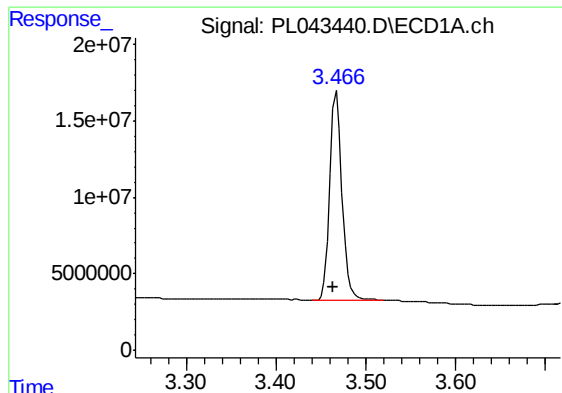

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.003 min
Response: 130087794
Conc: 21.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB116007BL

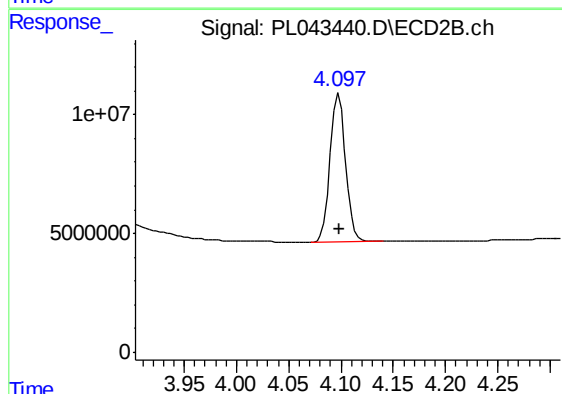


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 64226459
Conc: 21.67 ng/ml

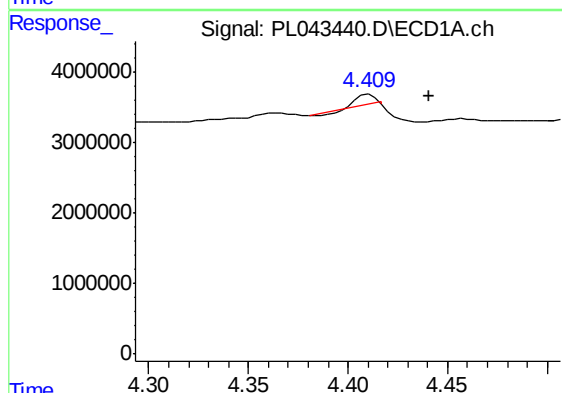


#6 beta-BHC

R.T.: 4.411 min
Delta R.T.: -0.030 min
Response: 697547
Conc: 0.19 ng/ml

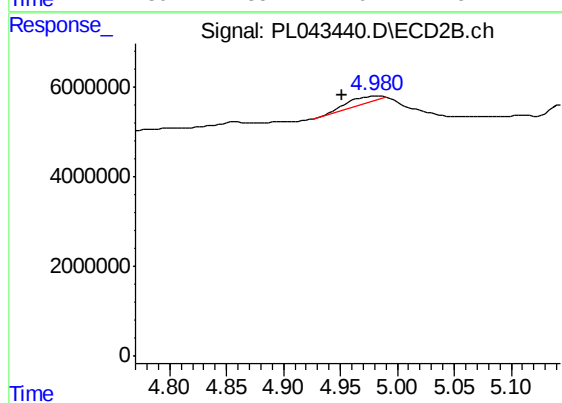

#6 beta-BHC


R.T.: 4.982 min
Delta R.T.: 0.030 min
Response: 3584481
Conc: 2.12 ng/ml

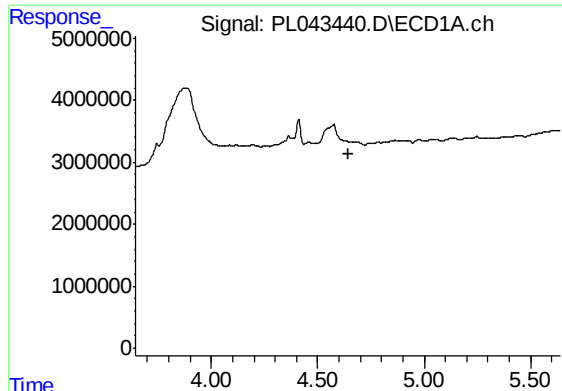

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB116007BL

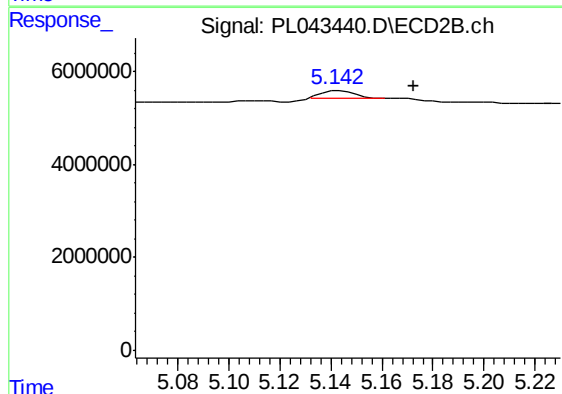


#7 delta-BHC

R.T.: 5.143 min
Delta R.T.: -0.030 min
Response: 1591521
Conc: 0.37 ng/ml

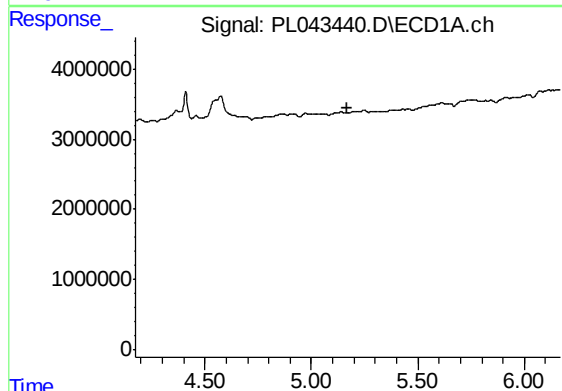


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

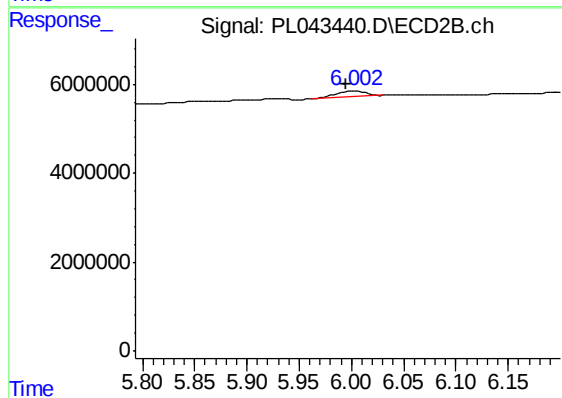

#8 Heptachlor epoxide


R.T.: 6.003 min
Delta R.T.: 0.008 min
Response: 2780103
Conc: 0.73 ng/ml

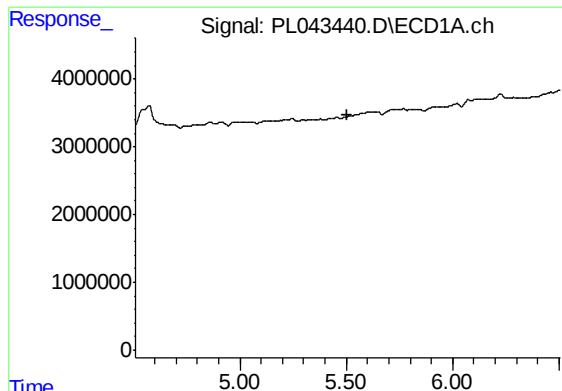

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB116007BL

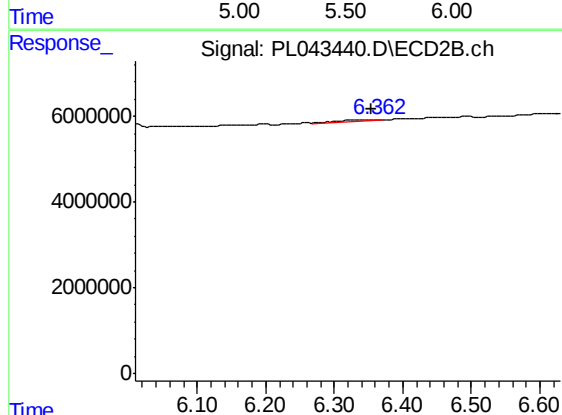


#9 Endosulfan I

R.T.: 6.363 min
Delta R.T.: 0.008 min
Response: 779988
Conc: 0.23 ng/ml

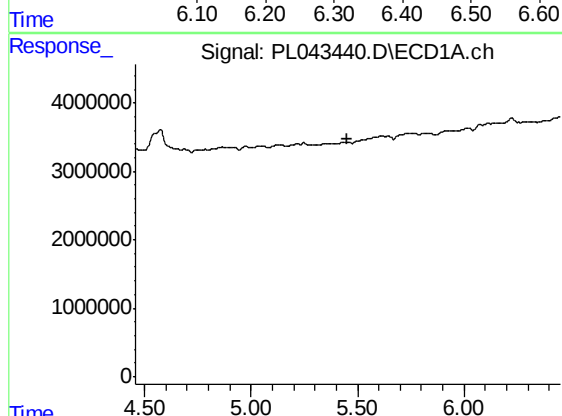


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.454 min
Response: 0
Conc: N.D.

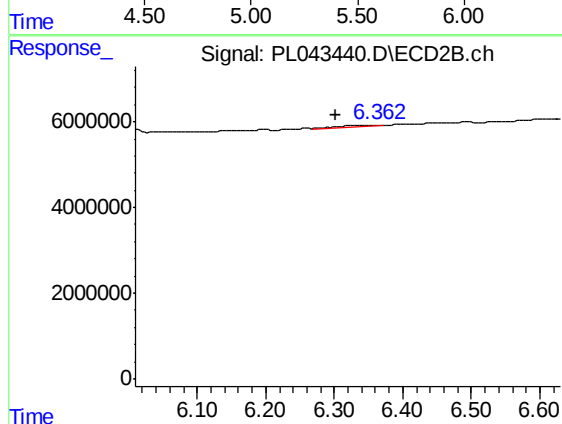

#11 alpha-Chlordane


R.T.: 6.363 min
Delta R.T.: 0.060 min
Response: 779988
Conc: 0.22 ng/ml

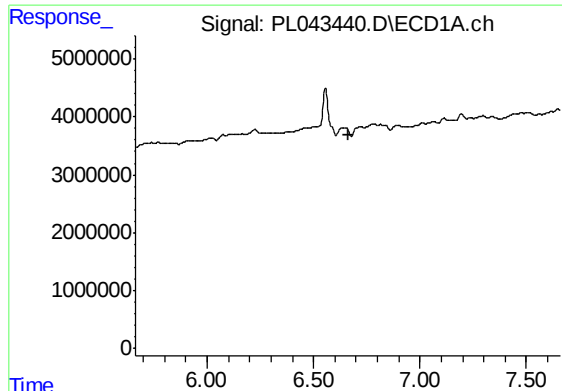

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB116007BL

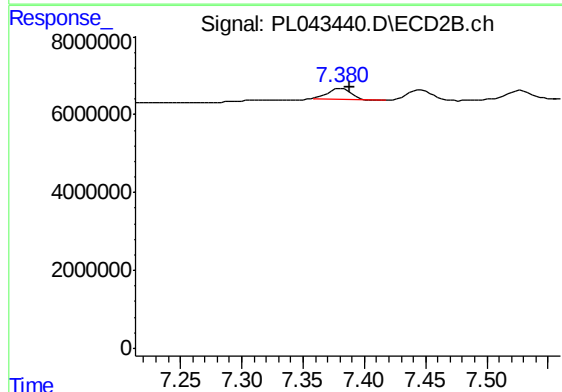


#19 Endosulfan Sulfate

R.T.: 7.381 min
Delta R.T.: -0.008 min
Response: 3652633
Conc: 1.21 ng/ml

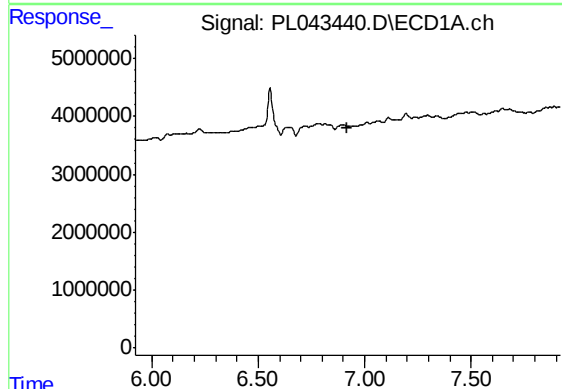


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

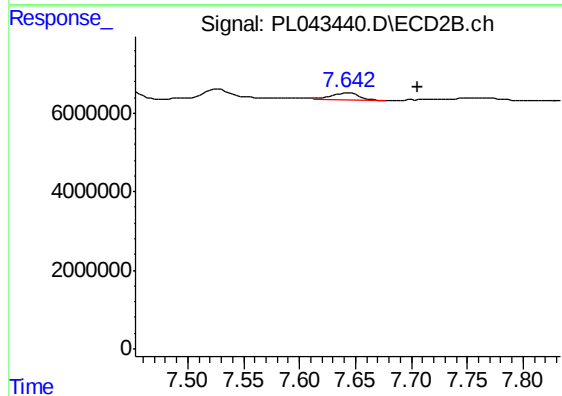

#20 Methoxychlor


R.T.: 7.643 min
Delta R.T.: -0.062 min
Response: 3041685
Conc: 2.02 ng/ml

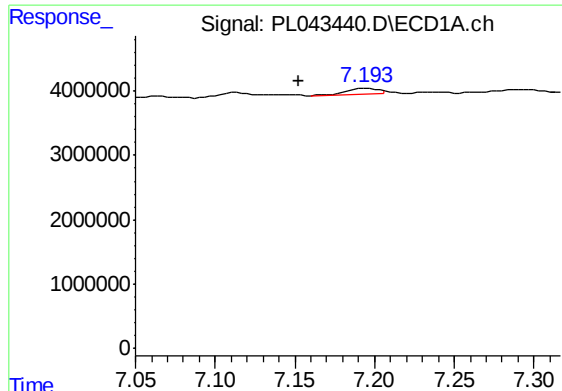

#21 Endrin ketone


R.T.: 7.195 min
Delta R.T.: 0.042 min
Response: 1088773
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB116007BL

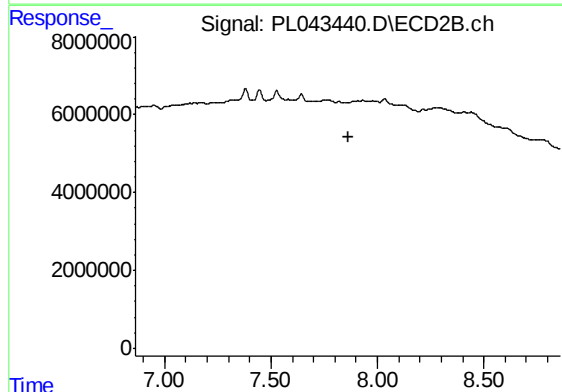


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.863 min
Response: 0
Conc: N.D.

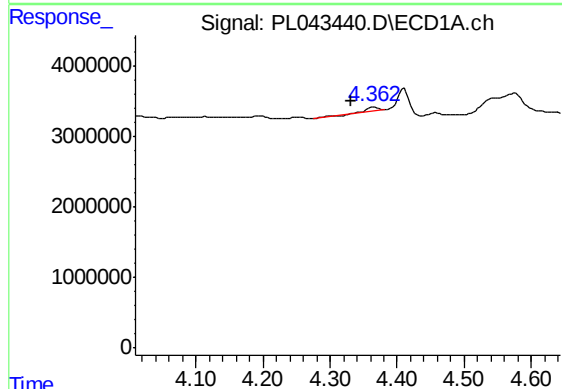


#23 Chlordane-1

R.T.: 4.363 min
Delta R.T.: 0.031 min
Response: 203020
Conc: 0.76 ng/ml

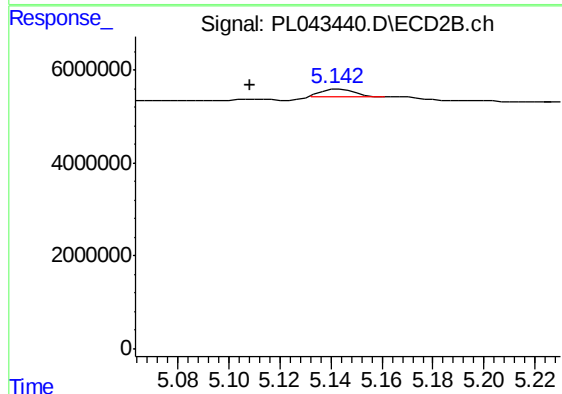

#23 Chlordane-1


R.T.: 5.143 min
Delta R.T.: 0.035 min
Response: 1591521
Conc: 11.26 ng/ml

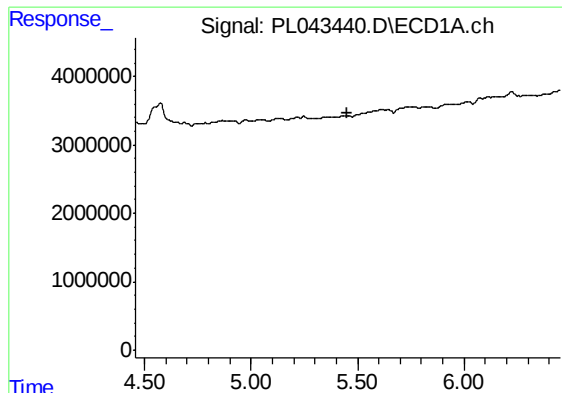

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB116007BL

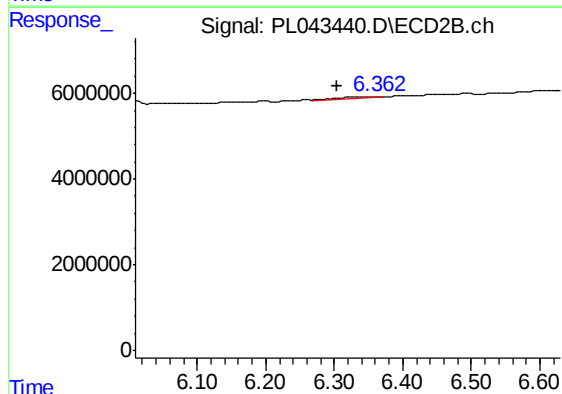


#26 Chlordane-4

R.T.: 6.363 min
Delta R.T.: 0.058 min
Response: 779988
Conc: 1.37 ng/ml

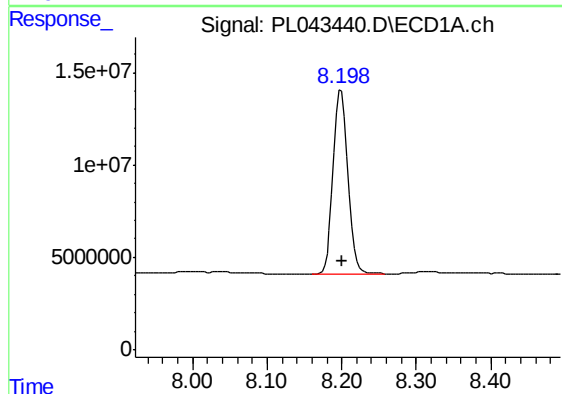

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 136011817
Conc: 20.83 ng/ml

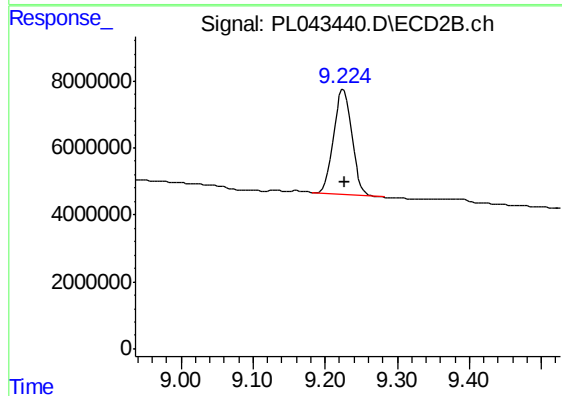

#28 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: -0.001 min
Response: 55266495
Conc: 21.19 ng/ml