

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
 Data File : PL043481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 00:25
 Operator : AJ\SJ
 Sample : J6195-12
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-01-122618-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:09:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	143.3E6	71953508	23.372	24.277
28)	SA Decachlor...	8.196	9.226	138.8E6	60228526	21.261	23.089
Target Compounds							
2)	A alpha-BHC	3.896	4.501	4271857	937665	0.452	0.207 #
7)	B delta-BHC	0.000	5.144f	0	10523000	N.D.	2.449 #
8)	B Heptachlo...	5.239f	6.000	2535798	3627276	0.320	0.957 #
19)	B Endosulfa...	6.657	7.382	1724586	15656905	0.257	5.208 #
20)	A Methoxychlor	6.884f	7.644f	-1648559	13269733	N.D.	8.798
21)	B Endrin ke...	7.190f	0.000	4104386	0	0.568	N.D. #
23)	Chlordane-1	4.361	5.113	222240	50003	0.827	0.354 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122718\
Data File : PL043481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 00:25
Operator : AJ\SJ
Sample : J6195-12
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:09:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

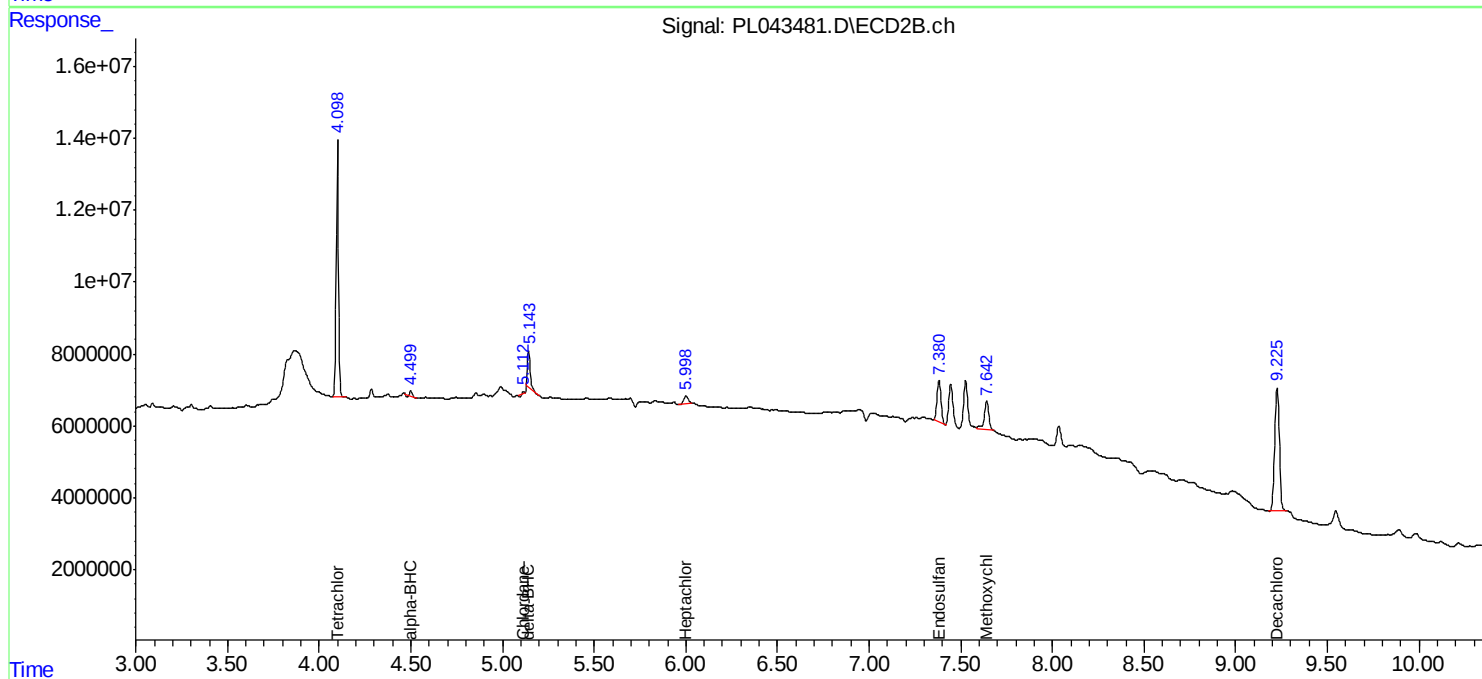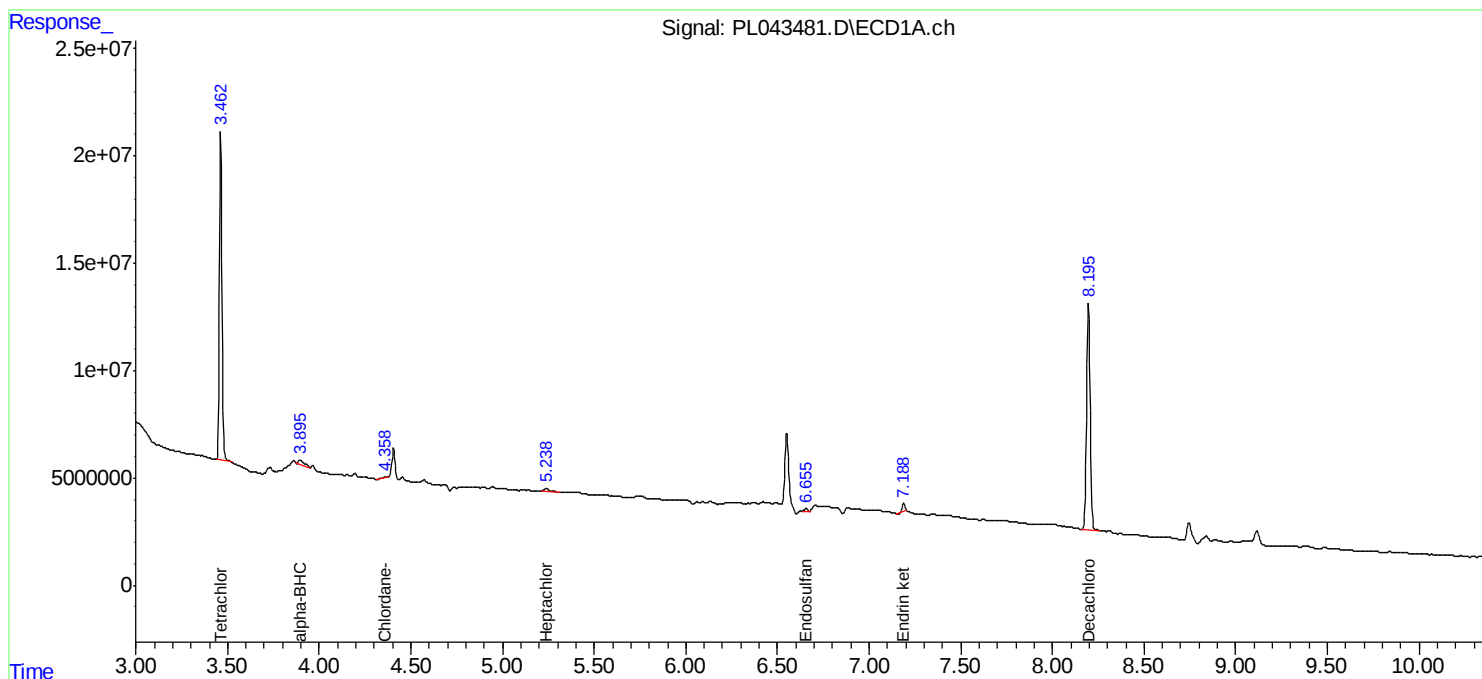


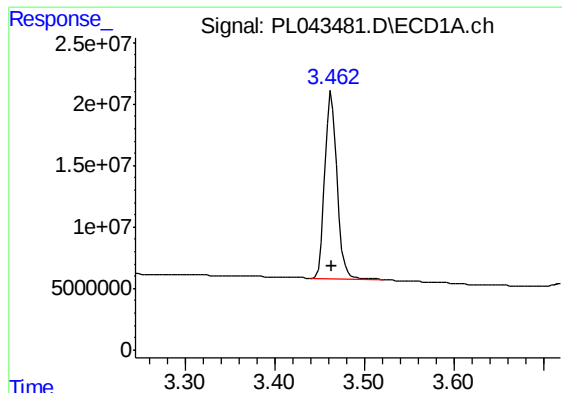

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 143340370
Conc: 23.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

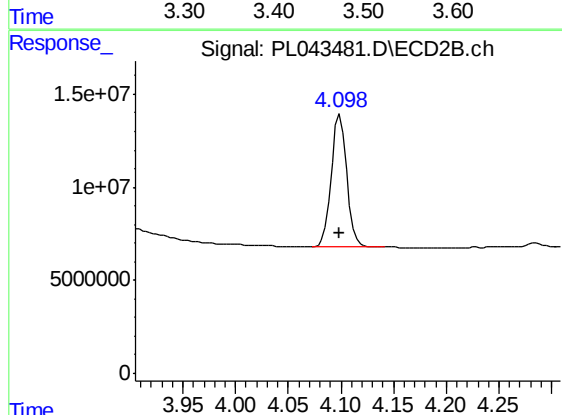


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 71953508
Conc: 24.28 ng/ml

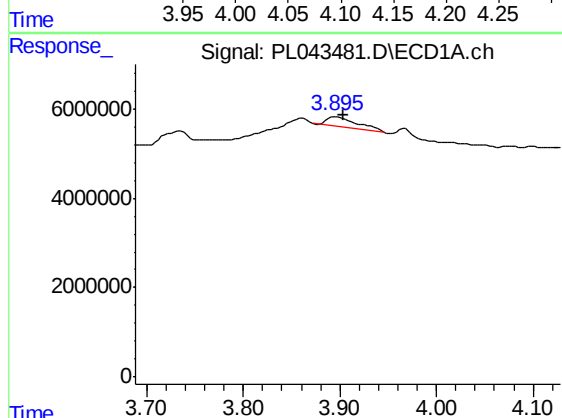


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: -0.009 min
Response: 4271857
Conc: 0.45 ng/ml

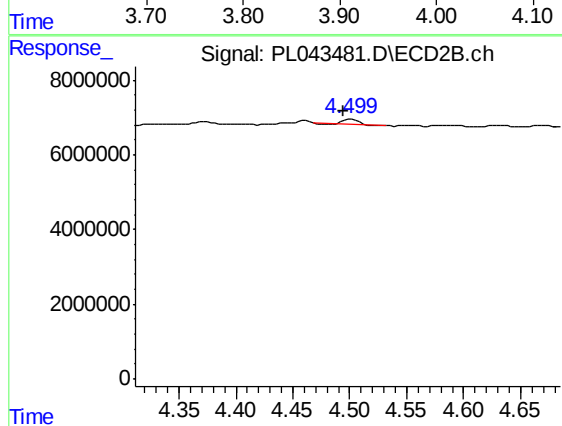

#2 alpha-BHC


R.T.: 4.501 min
Delta R.T.: 0.006 min
Response: 937665
Conc: 0.21 ng/ml

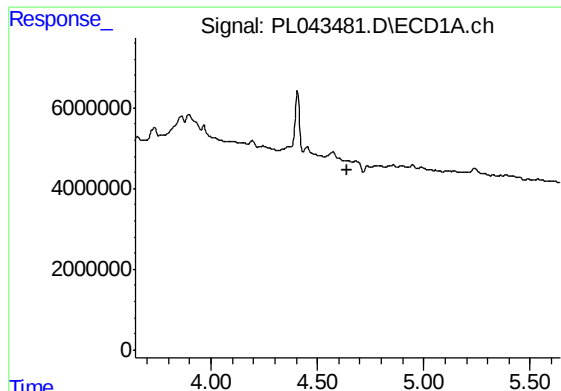

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

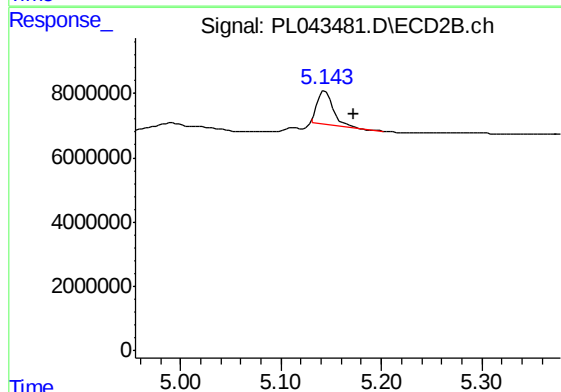


#7 delta-BHC

R.T.: 5.144 min
Delta R.T.: -0.029 min
Response: 10523000
Conc: 2.45 ng/ml

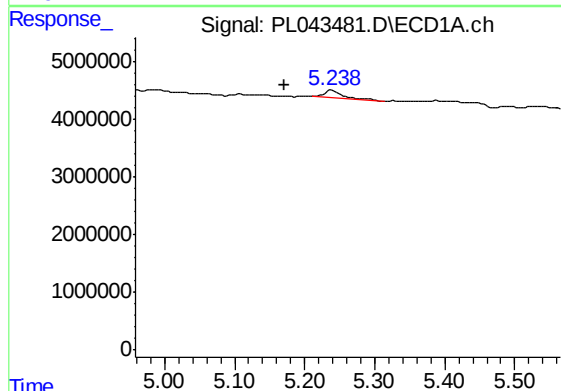


#8 Heptachlor epoxide

R.T.: 5.239 min
Delta R.T.: 0.069 min
Response: 2535798
Conc: 0.32 ng/ml

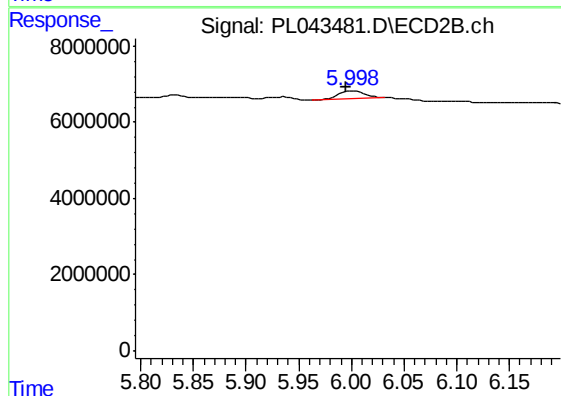

#8 Heptachlor epoxide


R.T.: 6.000 min
Delta R.T.: 0.005 min
Response: 3627276
Conc: 0.96 ng/ml

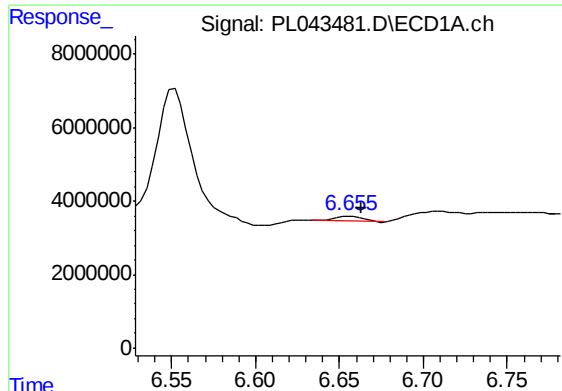

#19 Endosulfan Sulfate


R.T.: 6.657 min
Delta R.T.: -0.006 min
Response: 1724586
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

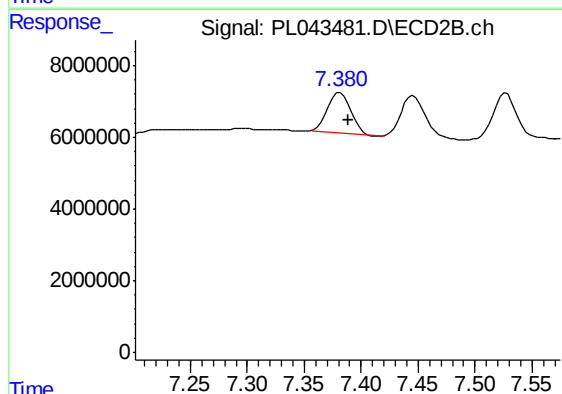


#19 Endosulfan Sulfate

R.T.: 7.382 min
Delta R.T.: -0.007 min
Response: 15656905
Conc: 5.21 ng/ml

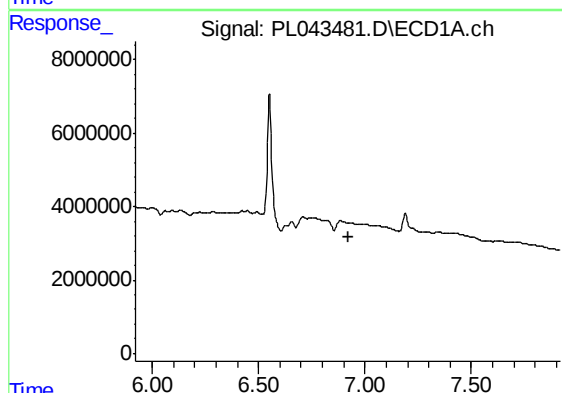


#20 Methoxychlor

R.T.: 6.884 min
Delta R.T.: -0.036 min
Response: -1648559
Conc: N.D.

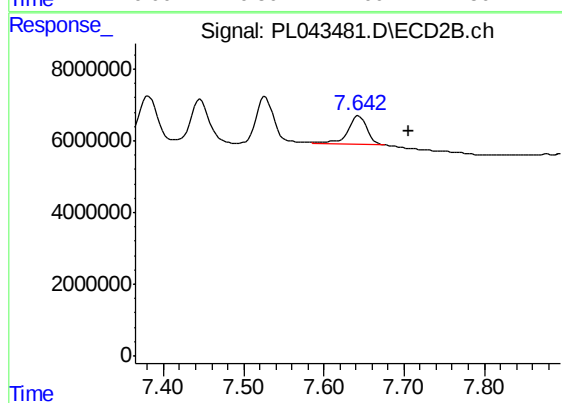

#20 Methoxychlor


R.T.: 7.644 min
Delta R.T.: -0.062 min
Response: 13269733
Conc: 8.80 ng/ml

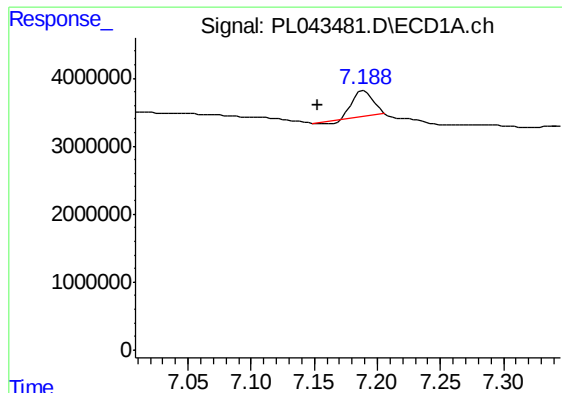

#21 Endrin ketone


R.T.: 7.190 min
Delta R.T.: 0.037 min
Response: 4104386
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

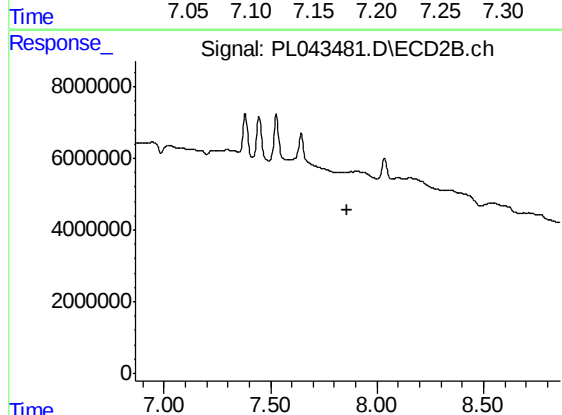


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.863 min
Response: 0
Conc: N.D.

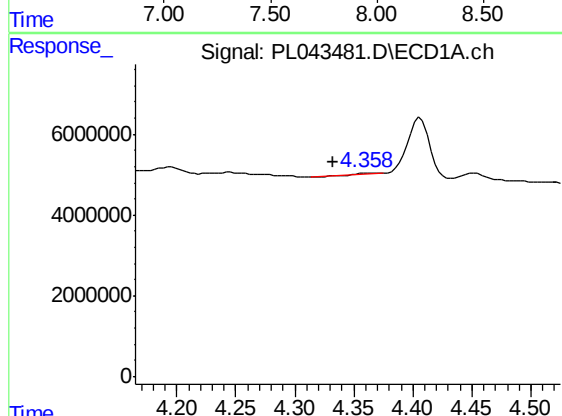


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.029 min
Response: 222240
Conc: 0.83 ng/ml

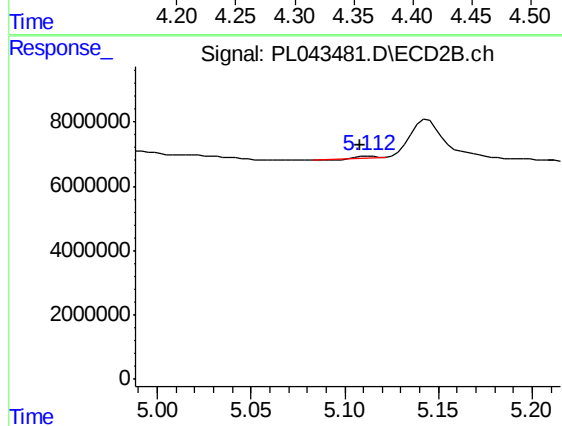

#23 Chlordane-1


R.T.: 5.113 min
Delta R.T.: 0.005 min
Response: 50003
Conc: 0.35 ng/ml

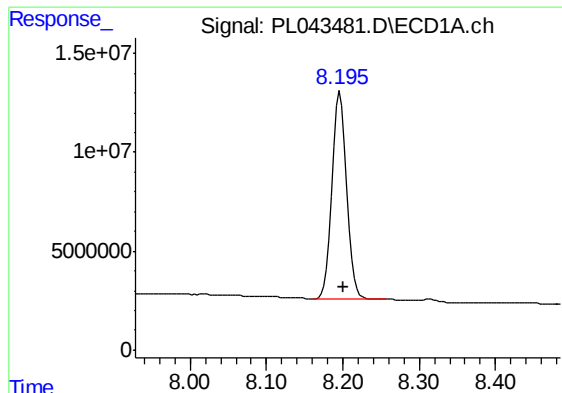

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: -0.005 min
Response: 138834853
Conc: 21.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-122618-A

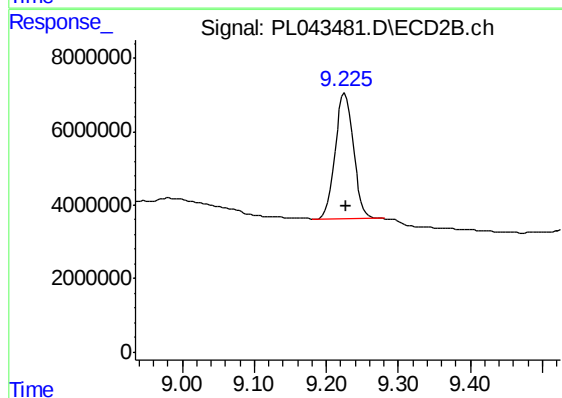

#28 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 60228526
Conc: 23.09 ng/ml