

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122719\
 Data File : PL055346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 22:18
 Operator : SG\AJ
 Sample : K6443-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:37:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	134.5E6	34702701	12.788	13.134
28)	SA Decachlor...	8.312	9.146	129.5E6	35231879	13.956	15.960
Target Compounds							
10)	B gamma-Chl...	0.000	6.172	0	4129066	N.D.	1.556 #
12)	B 4,4'-DDE	0.000	6.388	0	4474853	N.D.	1.835 #
16)	A 4,4'-DDD	0.000	6.887	0	3464682	N.D.	1.822 #
17)	MA 4,4'-DDT	6.470	7.153f	15694911	3930812	1.559	2.003 #
19)	B Endosulfa...	6.758	7.287f	33167103	1526003	3.297	0.731 #
20)	A Methoxychlor	7.003	0.000	53786126	0	11.160	N.D. #
21)	B Endrin ke...	7.279f	0.000	69425540	0	6.624	N.D. #
22)	Mirex	0.000	8.273f	0	5025324	N.D.	3.031 #
25)	Chlordane-3	0.000	6.172	0	4129066	N.D.	12.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122719\
Data File : PL055346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 22:18
Operator : SG\AJ
Sample : K6443-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:37:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

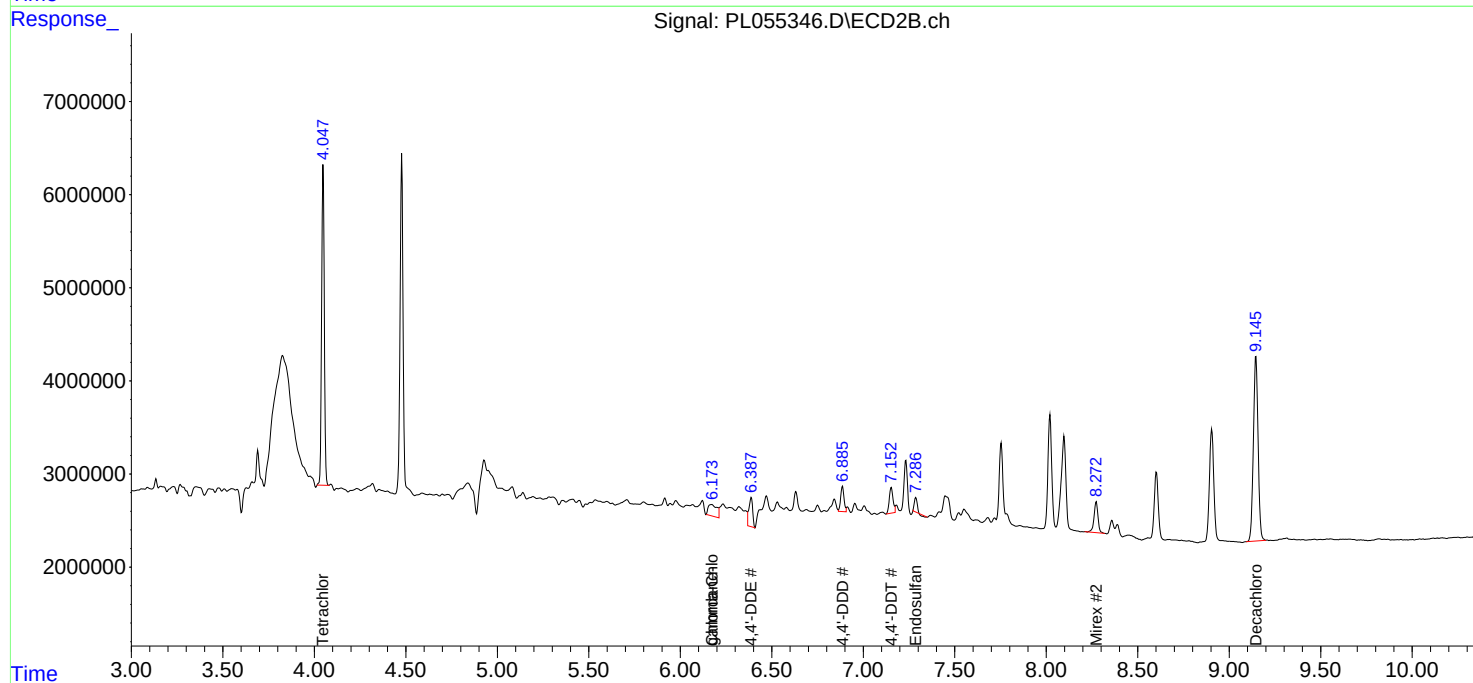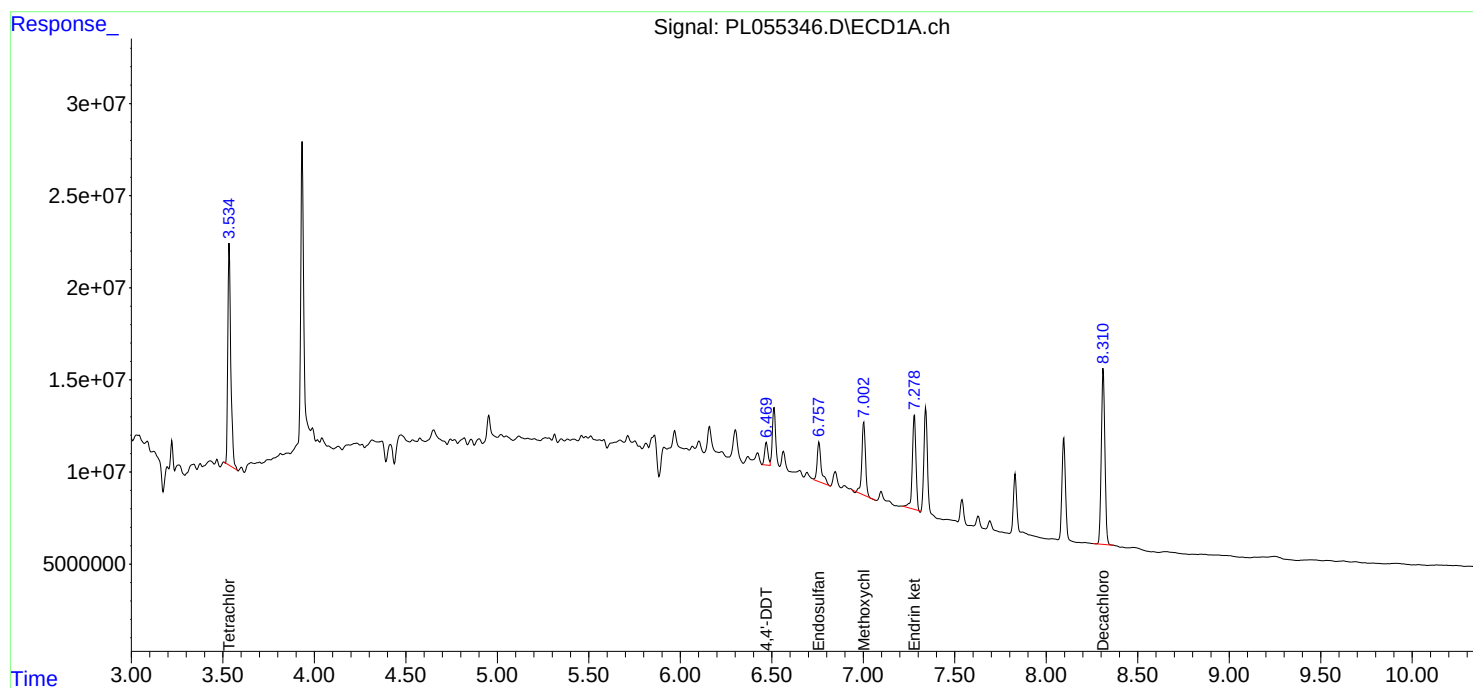


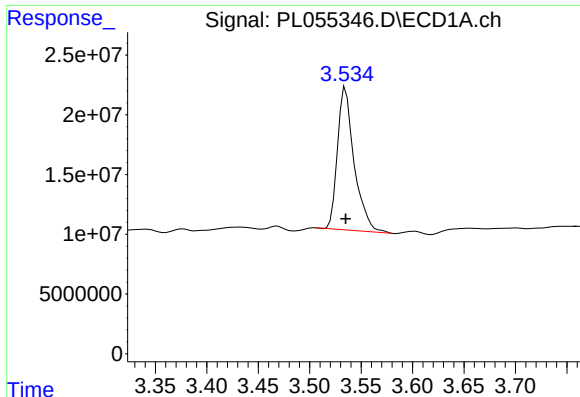

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 134481840
Conc: 12.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

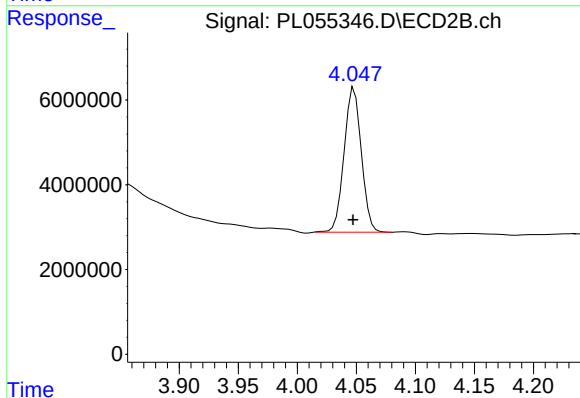


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.001 min
Response: 34702701
Conc: 13.13 ng/ml

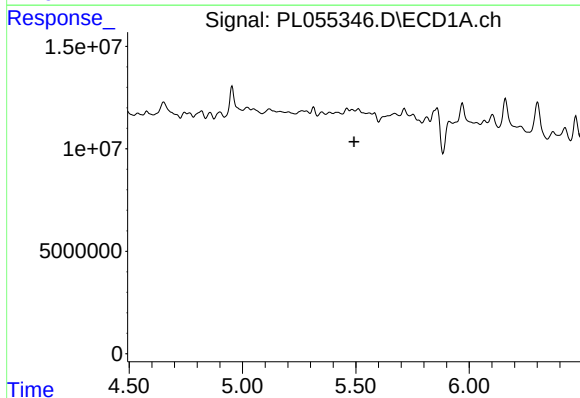


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

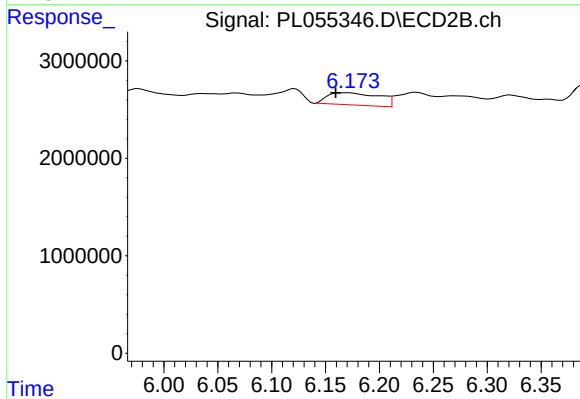

#10 gamma-Chlordane


R.T.: 6.172 min
Delta R.T.: 0.013 min
Response: 4129066
Conc: 1.56 ng/ml

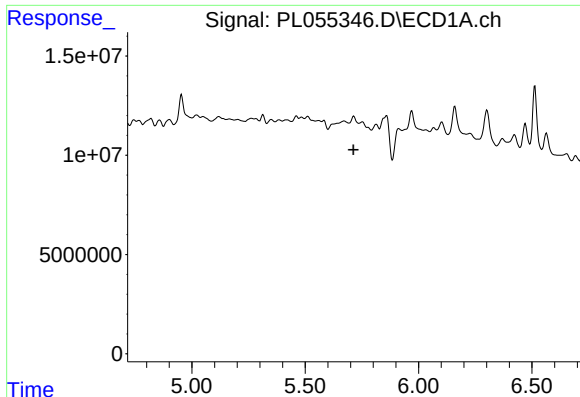

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.713 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

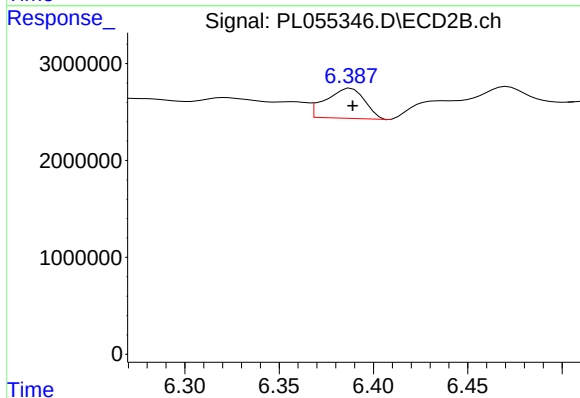


#12 4,4'-DDE

R.T.: 6.388 min
Delta R.T.: 0.000 min
Response: 4474853
Conc: 1.84 ng/ml

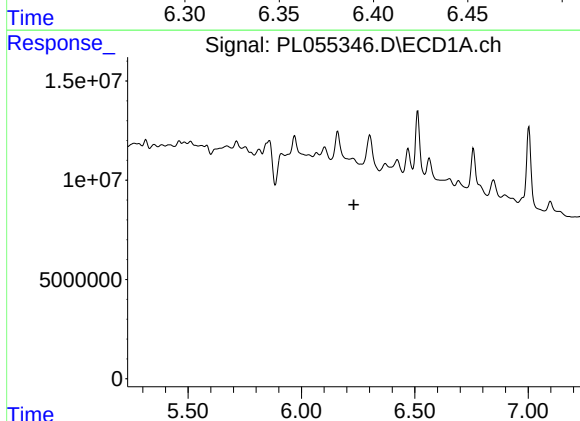


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

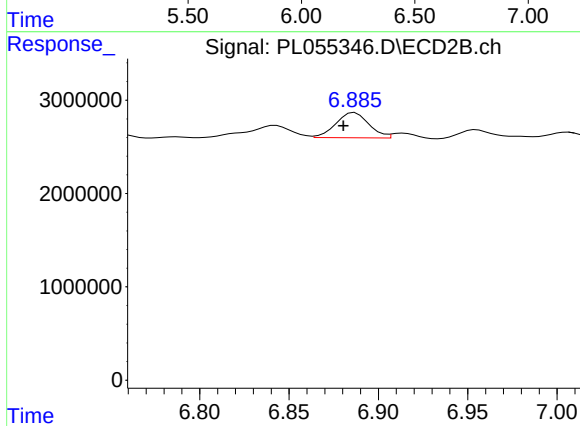

#16 4,4'-DDD


R.T.: 6.887 min
Delta R.T.: 0.006 min
Response: 3464682
Conc: 1.82 ng/ml

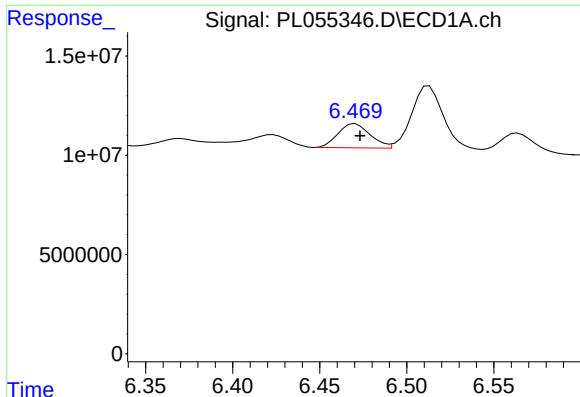

#17 4,4'-DDT


R.T.: 6.470 min
Delta R.T.: -0.003 min
Response: 15694911
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

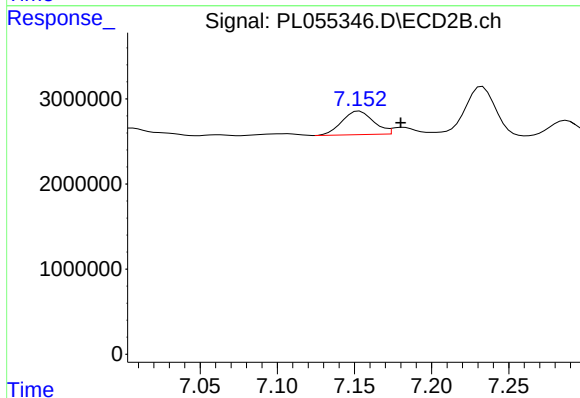


#17 4,4'-DDT

R.T.: 7.153 min
Delta R.T.: -0.027 min
Response: 3930812
Conc: 2.00 ng/ml

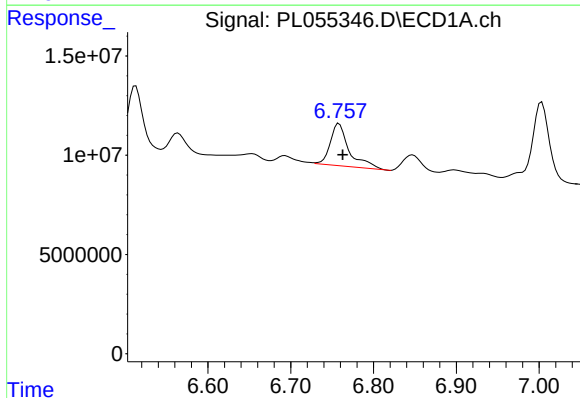


#19 Endosulfan Sulfate

R.T.: 6.758 min
Delta R.T.: -0.004 min
Response: 33167103
Conc: 3.30 ng/ml

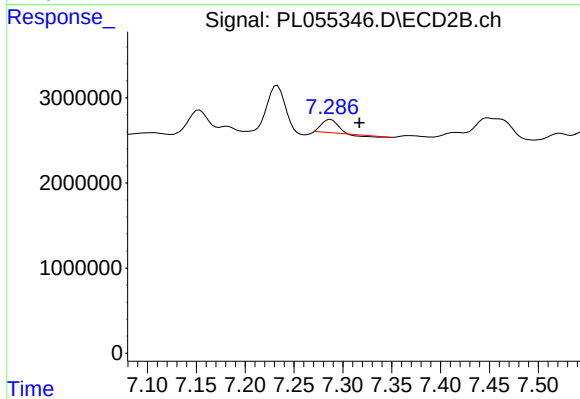

#19 Endosulfan Sulfate


R.T.: 7.287 min
Delta R.T.: -0.030 min
Response: 1526003
Conc: 0.73 ng/ml

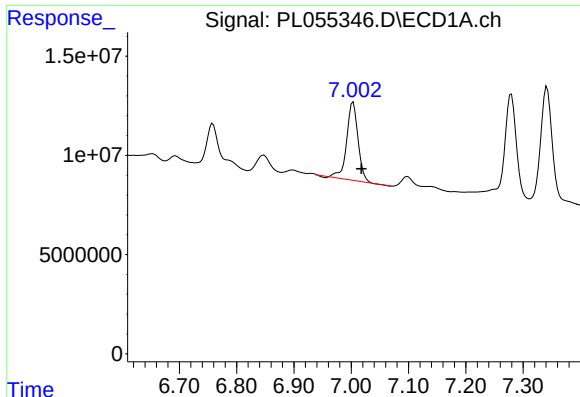

#20 Methoxychlor


R.T.: 7.003 min
Delta R.T.: -0.014 min
Response: 53786126
Conc: 11.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

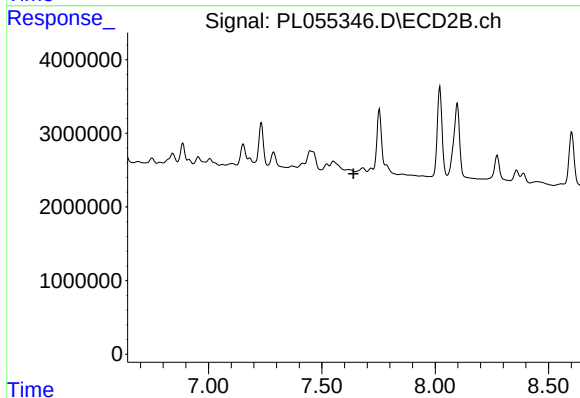


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.640 min
Response: 0
Conc: N.D.

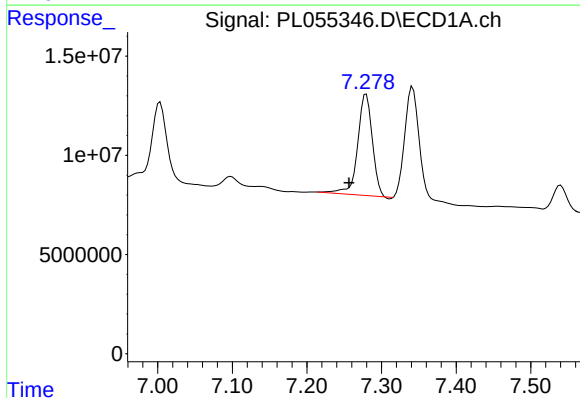


#21 Endrin ketone

R.T.: 7.279 min
Delta R.T.: 0.023 min
Response: 69425540
Conc: 6.62 ng/ml

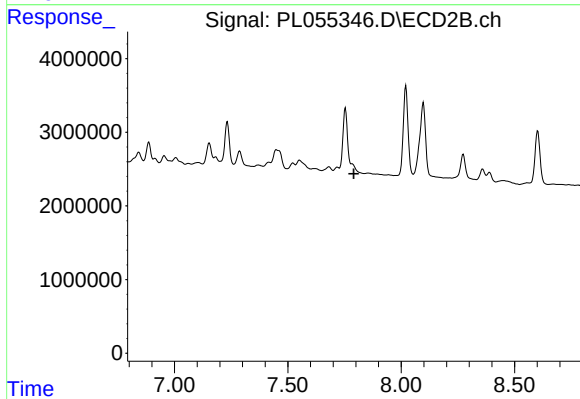

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.790 min
Response: 0
Conc: N.D.

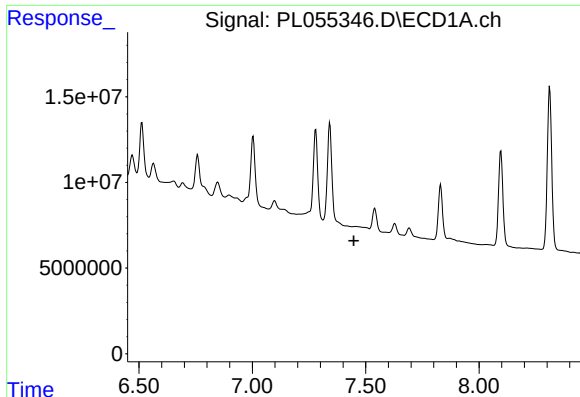

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

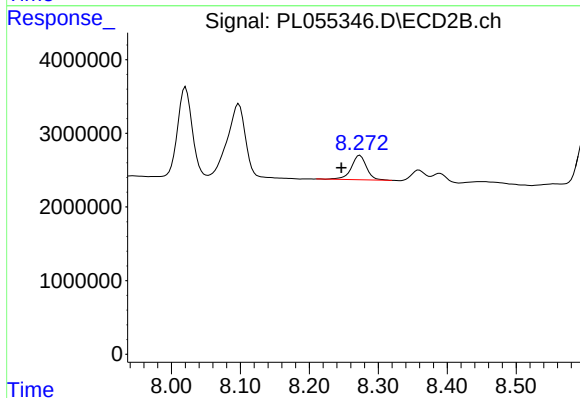


#22 Mirex

R.T.: 8.273 min
Delta R.T.: 0.027 min
Response: 5025324
Conc: 3.03 ng/ml

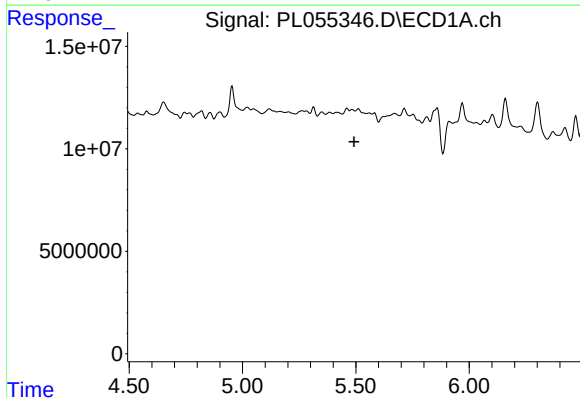


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

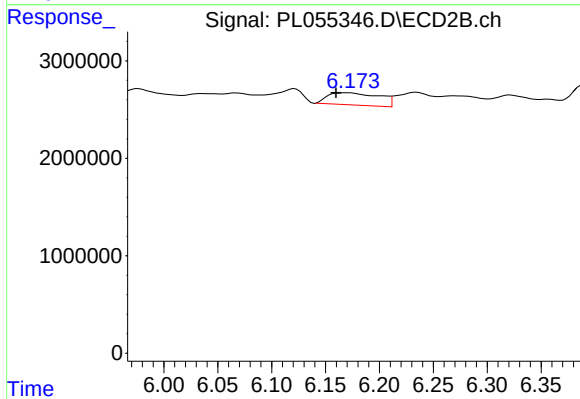

#25 Chlordane-3

R.T.: 6.172 min
Delta R.T.: 0.012 min
Response: 4129066
Conc: 12.83 ng/ml

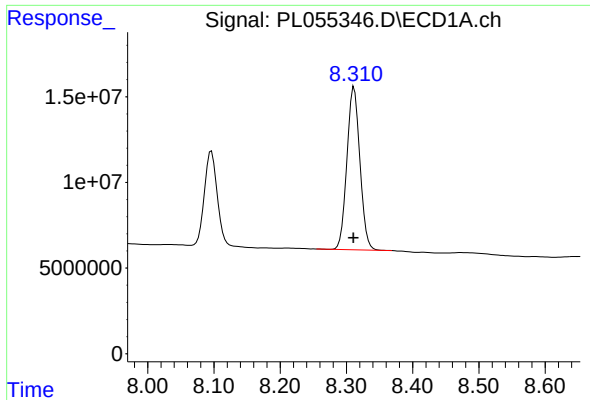

#28 Decachlorobiphenyl


R.T.: 8.312 min

Delta R.T.: 0.001 min

Response: 129495216

Conc: 13.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

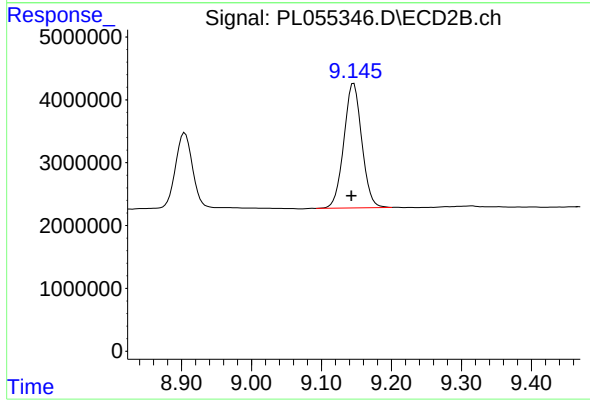

#28 Decachlorobiphenyl

R.T.: 9.146 min

Delta R.T.: 0.003 min

Response: 35231879

Conc: 15.96 ng/ml