

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 12:41
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 13:45:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 13:44:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.499	65714586	165.9E6	98.024	98.336
28)	SA Decachlor...	10.325	11.392	68007276	119.1E6	90.820	94.118
Target Compounds							
23)	Chlordane-1	5.889	6.881	24713014	67502196	998.504	971.173
24)	Chlordane-2	6.578	7.473	29601603	69647774	929.241	958.452
25)	Chlordane-3	7.277	8.230	86304731	277.8E6	992.149	997.851
26)	Chlordane-4	7.346	8.312	92020436	320.5E6	994.338	985.334
27)	Chlordane-5	8.295	9.198	29883710	52067535	969.311	963.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 12:41
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 13:45:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 13:44:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

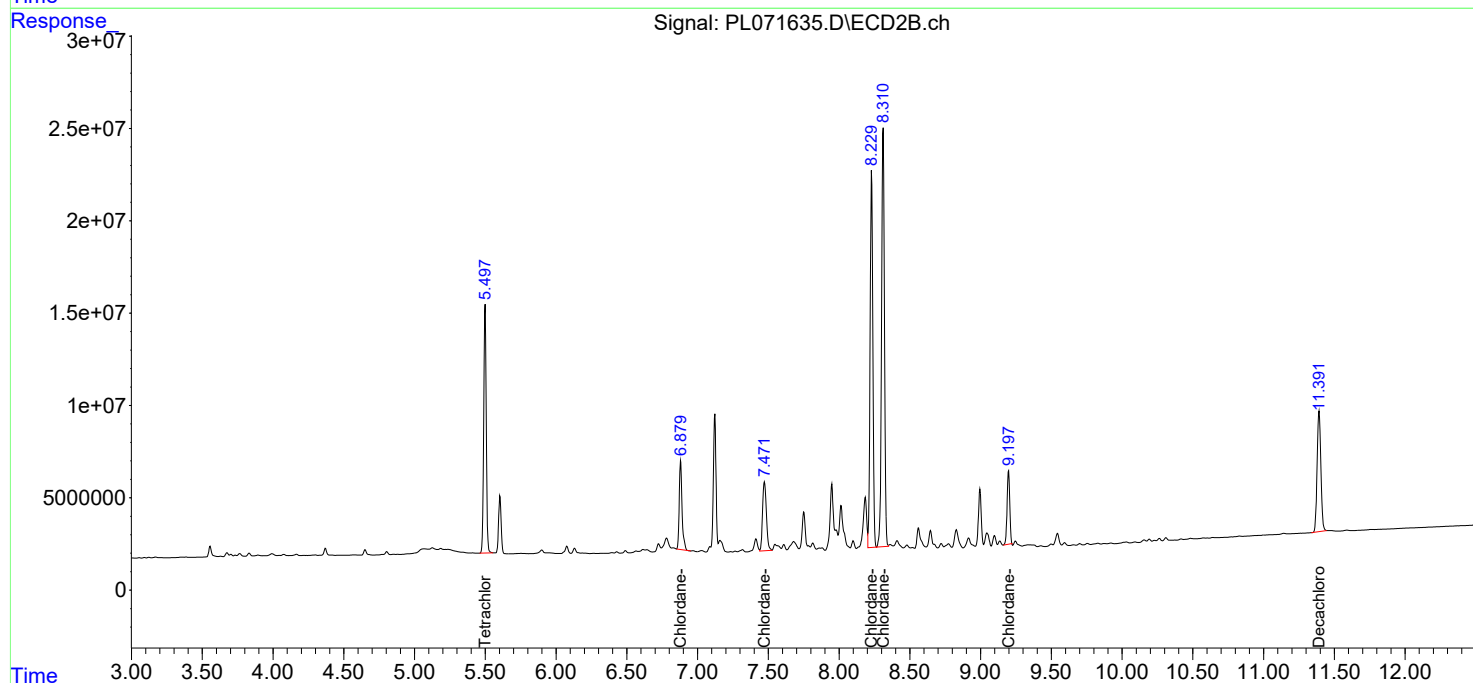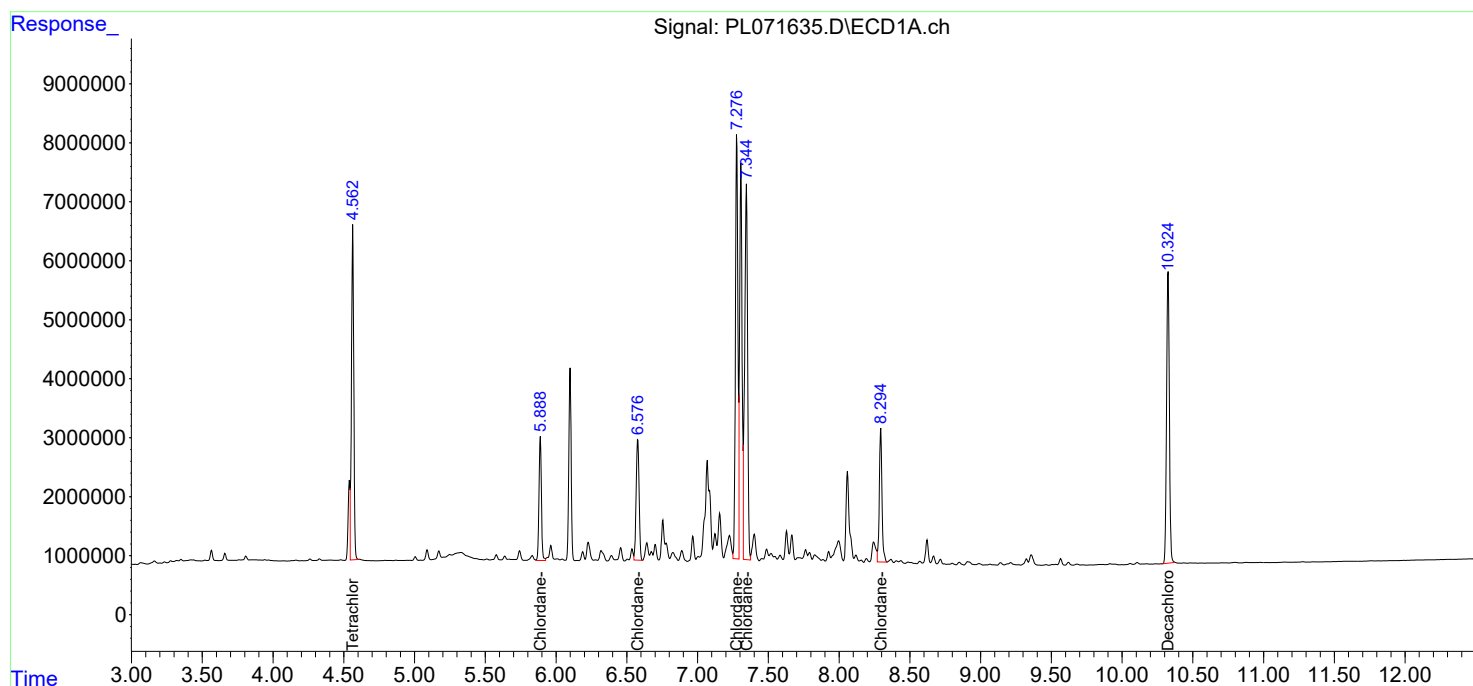


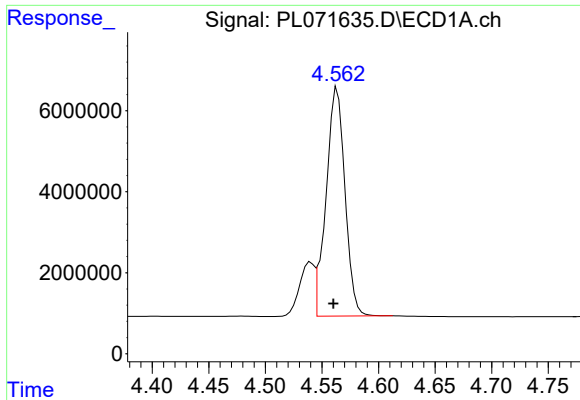

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.004 min
Response: 65714586
Conc: 98.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

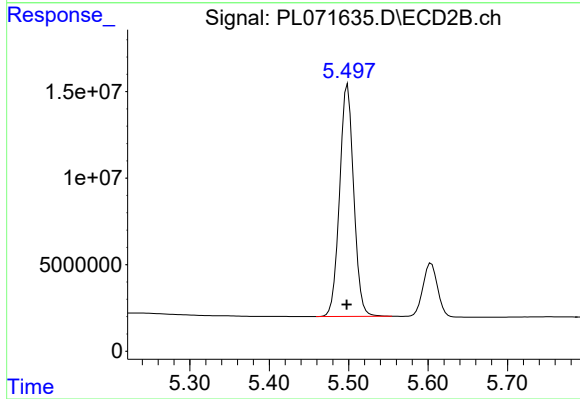


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: 0.001 min
Response: 165865821
Conc: 98.34 ng/ml

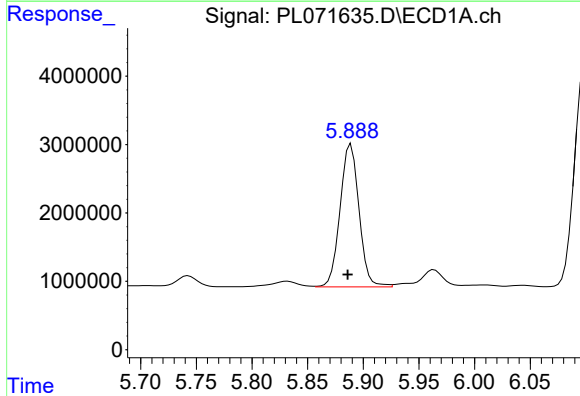


#23 Chlordane-1

R.T.: 5.889 min
Delta R.T.: 0.003 min
Response: 24713014
Conc: 998.50 ng/ml

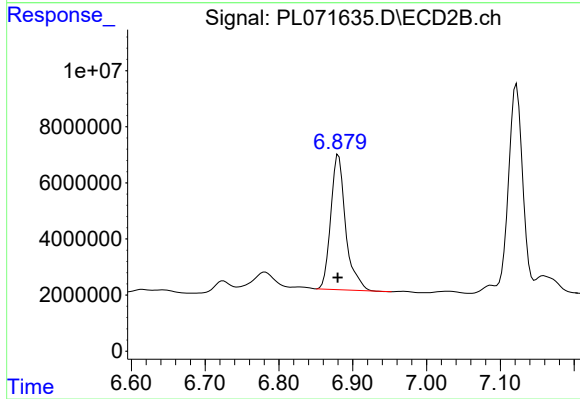

#23 Chlordane-1


R.T.: 6.881 min
Delta R.T.: 0.001 min
Response: 67502196
Conc: 971.17 ng/ml

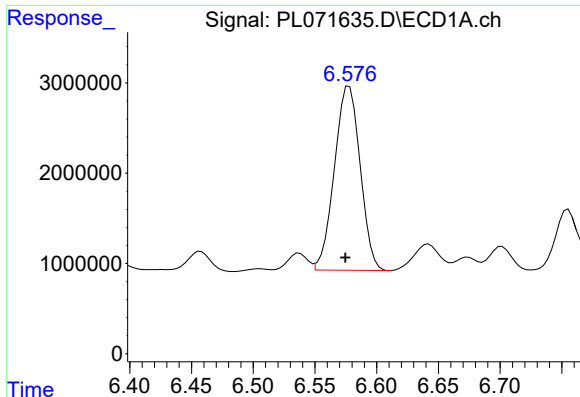

#24 Chlordane-2


R.T.: 6.578 min
Delta R.T.: 0.003 min
Response: 29601603
Conc: 929.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

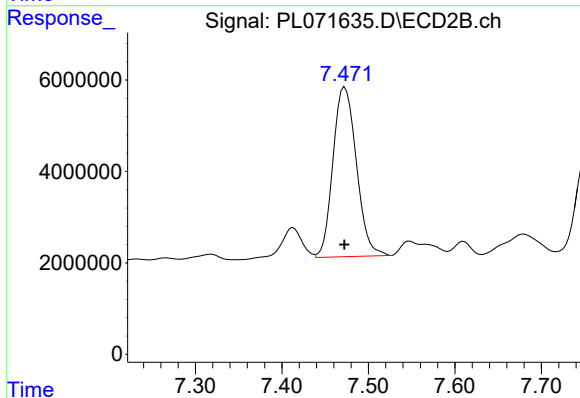


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 69647774
Conc: 958.45 ng/ml

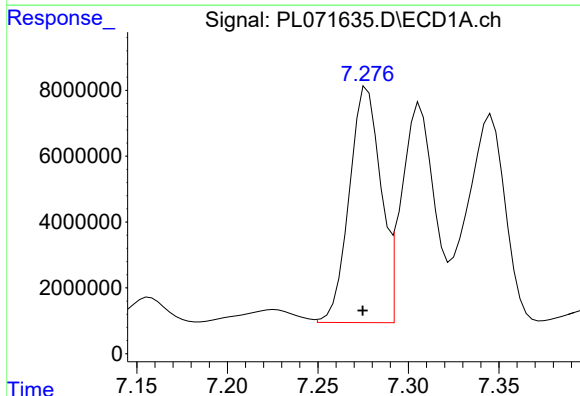


#25 Chlordane-3

R.T.: 7.277 min
Delta R.T.: 0.003 min
Response: 86304731
Conc: 992.15 ng/ml

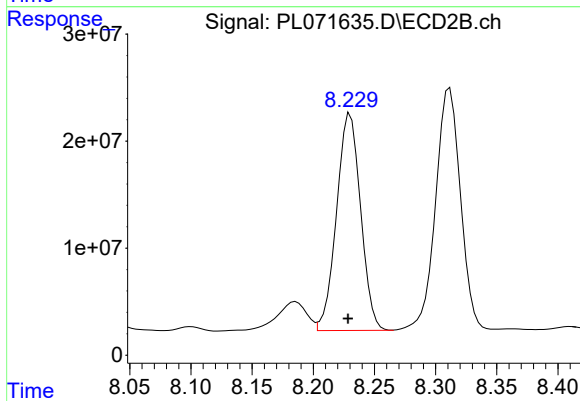

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.002 min
Response: 277763950
Conc: 997.85 ng/ml

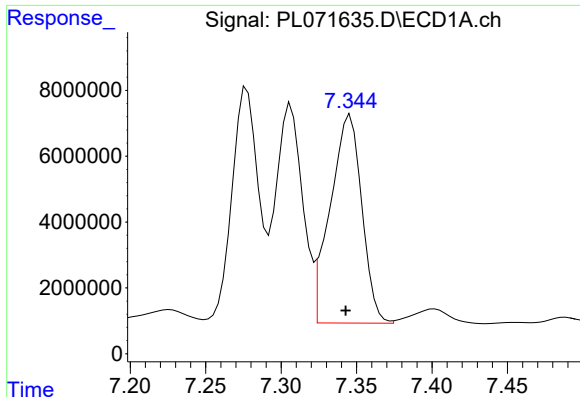

#26 Chlordane-4


R.T.: 7.346 min
Delta R.T.: 0.003 min
Response: 92020436
Conc: 994.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

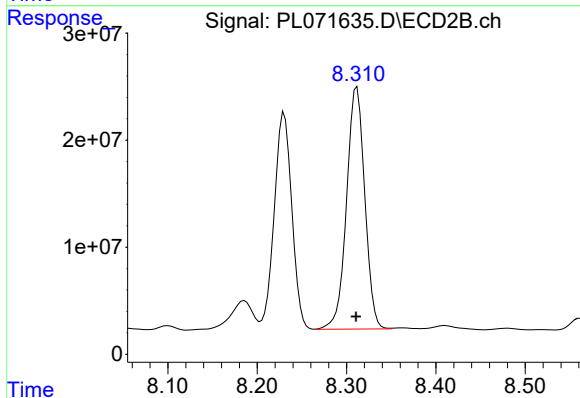


#26 Chlordane-4

R.T.: 8.312 min
Delta R.T.: 0.001 min
Response: 320519190
Conc: 985.33 ng/ml

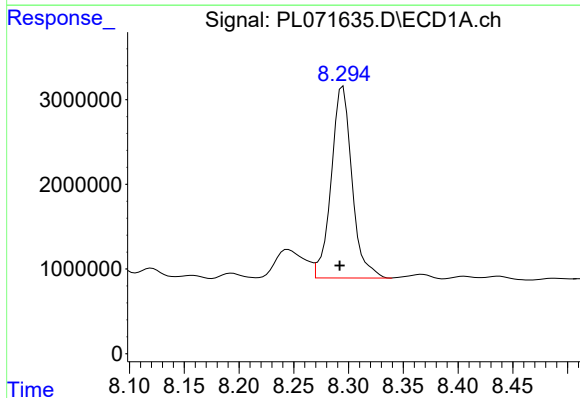


#27 Chlordane-5

R.T.: 8.295 min
Delta R.T.: 0.003 min
Response: 29883710
Conc: 969.31 ng/ml

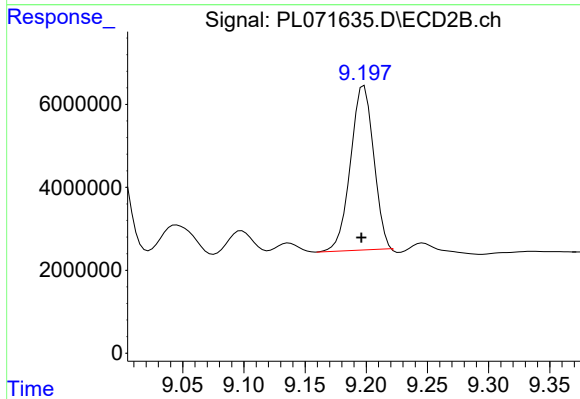

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.002 min
Response: 52067535
Conc: 963.25 ng/ml

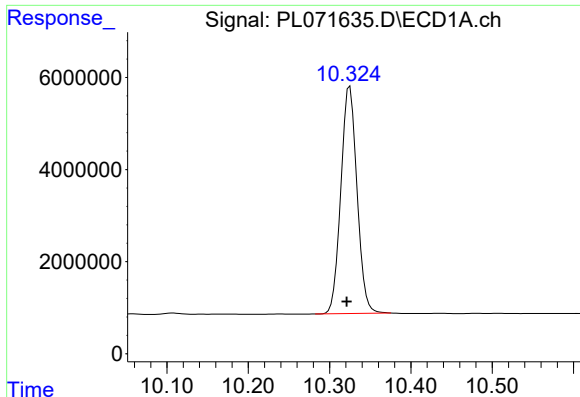

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: 0.004 min
Response: 68007276
Conc: 90.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

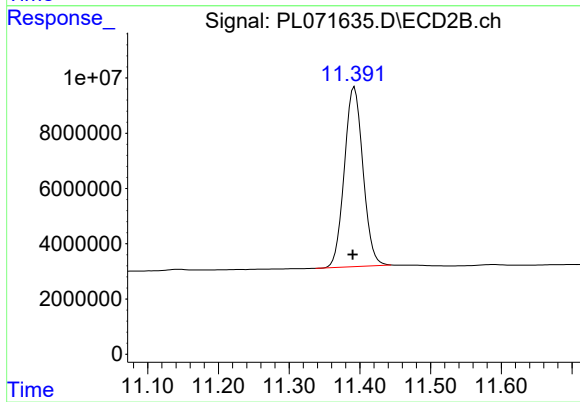

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.003 min
Response: 119118361
Conc: 94.12 ng/ml