

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 13:14
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 13:44:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 13:44:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.498	33519798	84336294	50.000	50.000
28)	SA Decachlor...	10.321	11.390	37440543	63281524	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.886	6.880	12375020	34752920	500.000	500.000
24)	Chlordane-2	6.575	7.472	15927840	36333487	500.000	500.000
25)	Chlordane-3	7.275	8.229	43493832	139.2E6	500.000	500.000
26)	Chlordane-4	7.343	8.311	46272234	162.6E6	500.000	500.000
27)	Chlordane-5	8.292	9.196	15414917	27026895	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 13:14
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 13:44:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 13:44:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

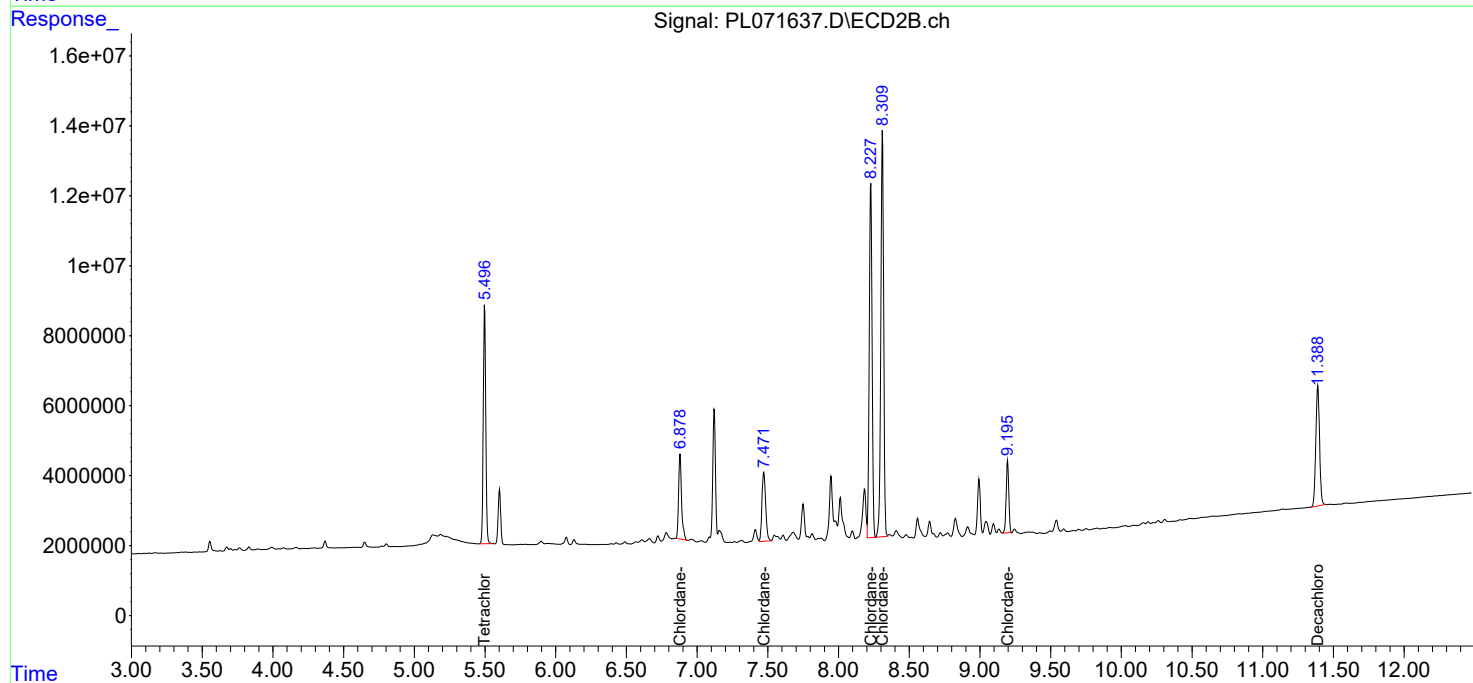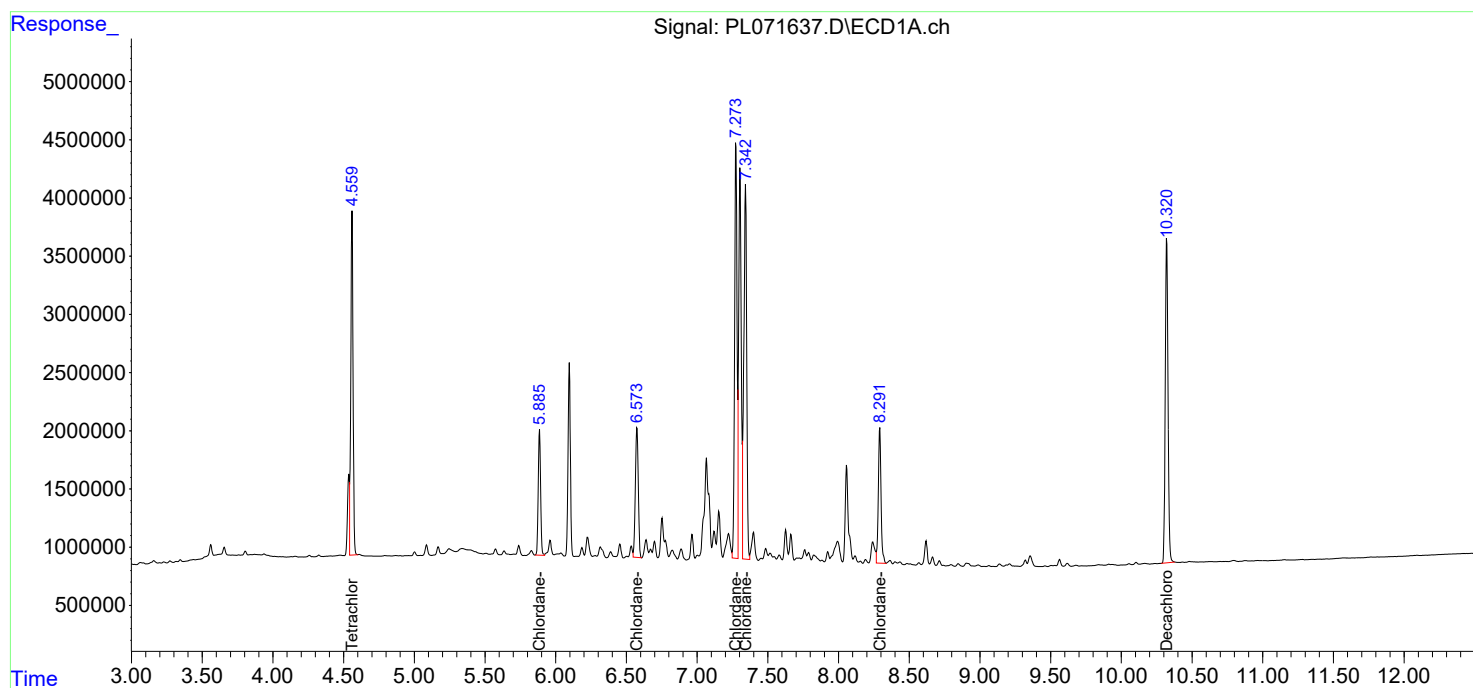


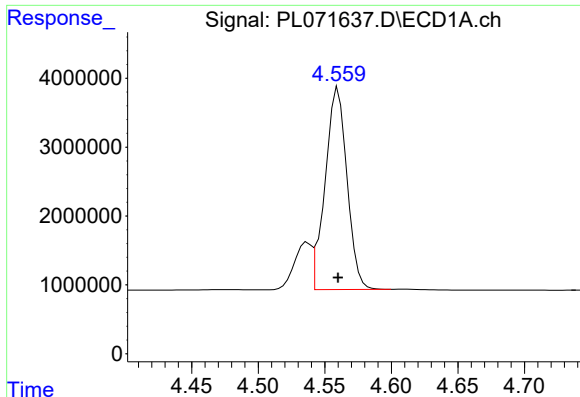

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 33519798
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

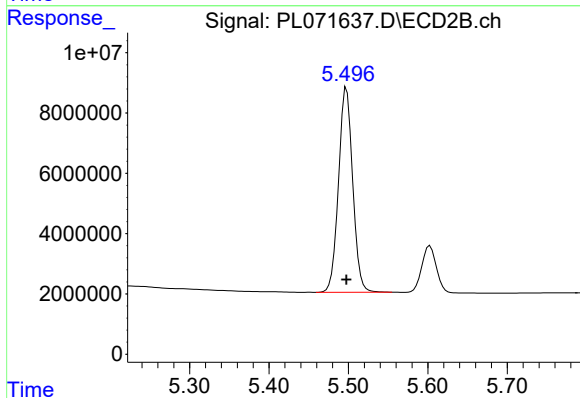


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 84336294
Conc: 50.00 ng/ml

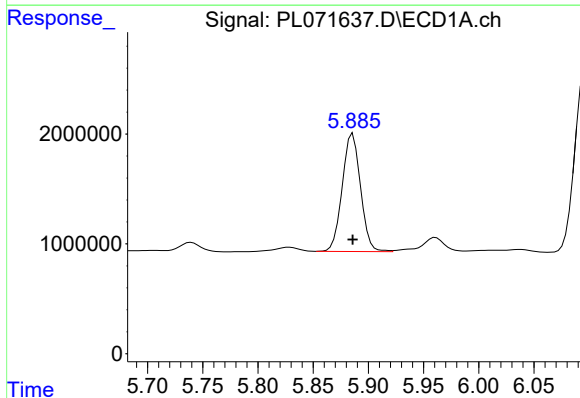


#23 Chlordane-1

R.T.: 5.886 min
Delta R.T.: 0.000 min
Response: 12375020
Conc: 500.00 ng/ml

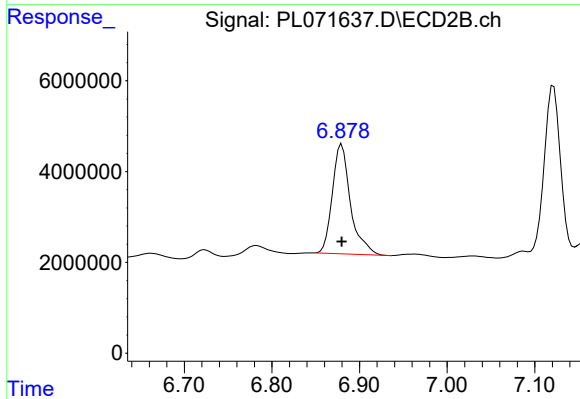

#23 Chlordane-1


R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 34752920
Conc: 500.00 ng/ml

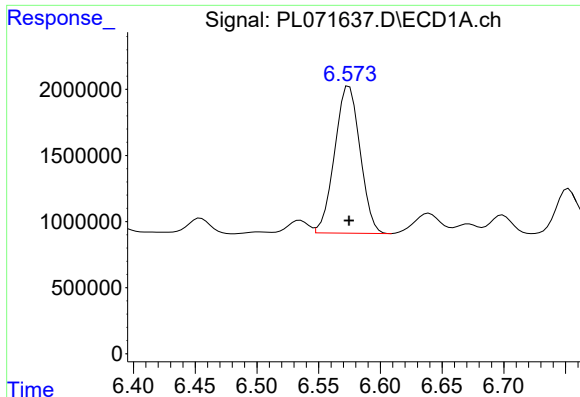

#24 Chlordane-2


R.T.: 6.575 min
Delta R.T.: 0.000 min
Response: 15927840
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

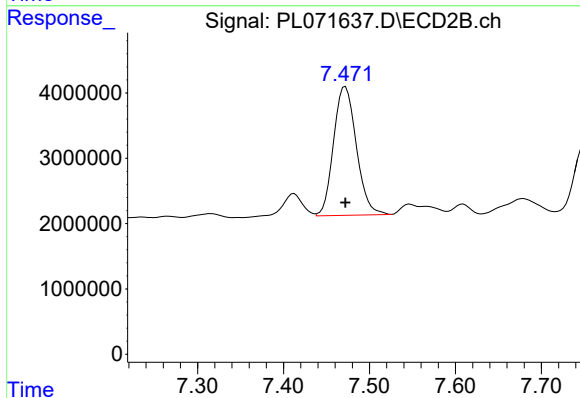


#24 Chlordane-2

R.T.: 7.472 min
Delta R.T.: 0.000 min
Response: 36333487
Conc: 500.00 ng/ml

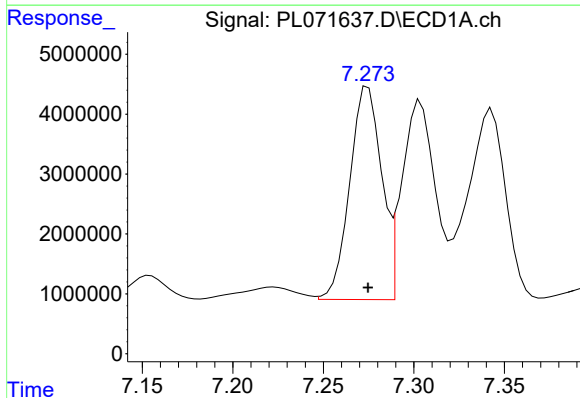


#25 Chlordane-3

R.T.: 7.275 min
Delta R.T.: 0.000 min
Response: 43493832
Conc: 500.00 ng/ml

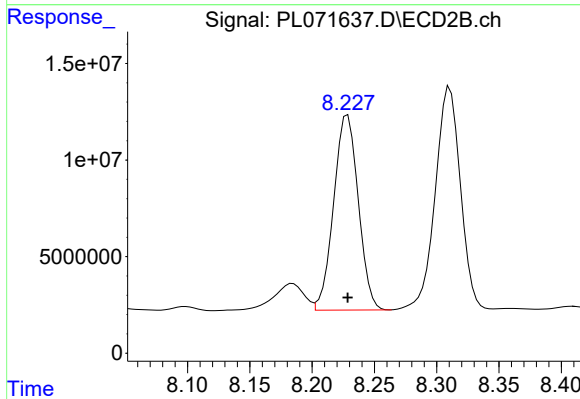

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 139181035
Conc: 500.00 ng/ml

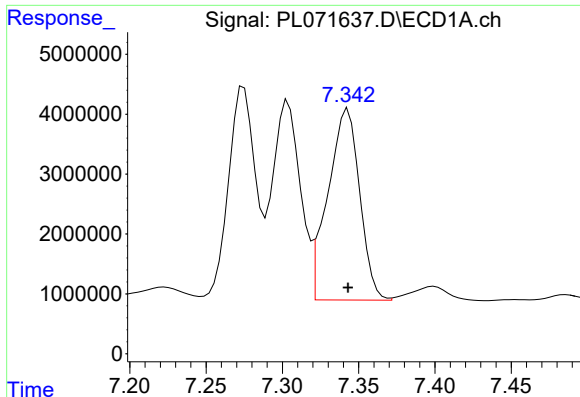

#26 Chlordane-4


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 46272234
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

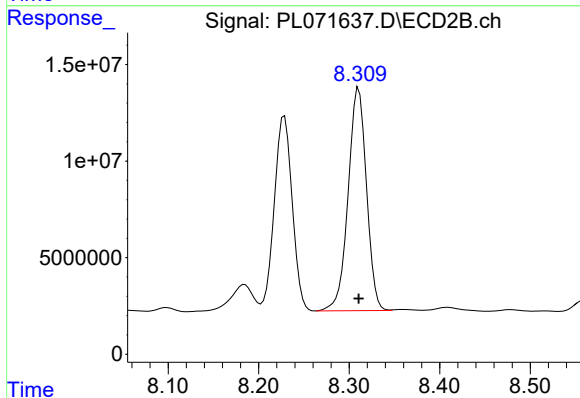


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 162644912
Conc: 500.00 ng/ml

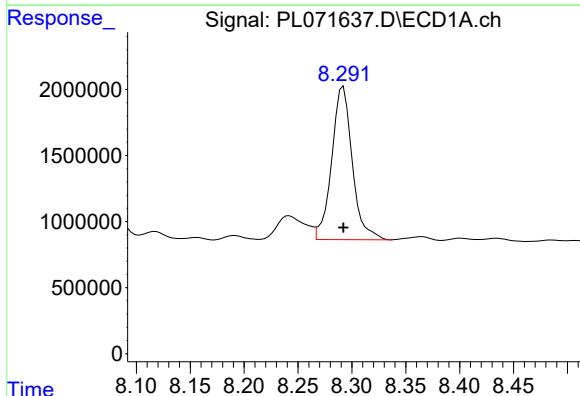


#27 Chlordane-5

R.T.: 8.292 min
Delta R.T.: 0.000 min
Response: 15414917
Conc: 500.00 ng/ml

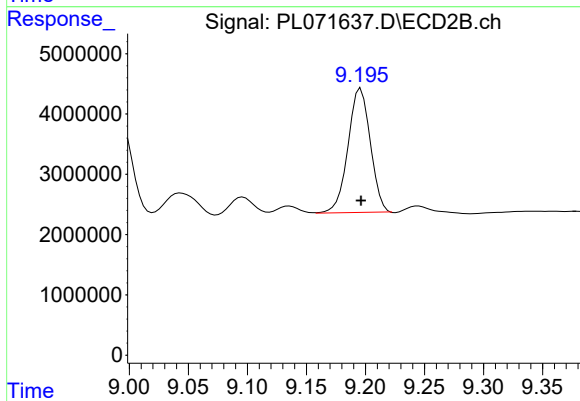

#27 Chlordane-5


R.T.: 9.196 min
Delta R.T.: 0.000 min
Response: 27026895
Conc: 500.00 ng/ml

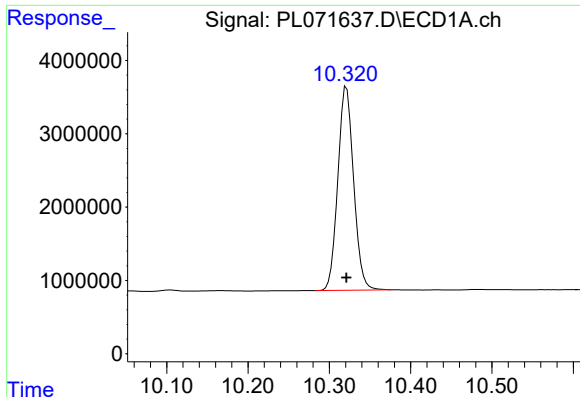

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.000 min
Response: 37440543
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

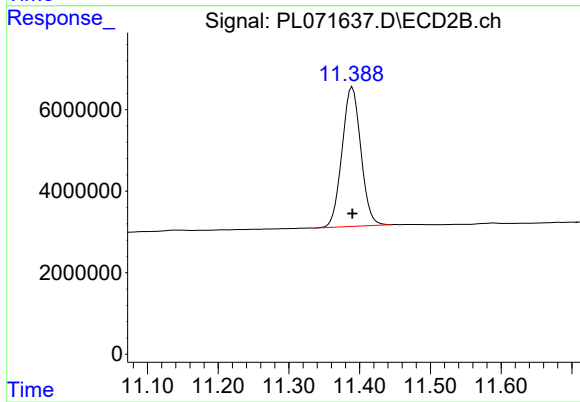

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.000 min
Response: 63281524
Conc: 50.00 ng/ml