

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 16:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:37:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.496	10868030	28480185	16.751	16.690
28)	SA Decachlor...	10.321	11.388	14012341	23163394	18.822	18.482
Target Compounds							
8)	B Heptachlo...	0.000	7.966	0	170365	N.D.	0.087 #
9)	A Endosulfan I	0.000	8.363	0	26679	N.D.	0.016 #
10)	B gamma-Chl...	0.000	8.237	0	110545	N.D.	0.057 #
11)	B alpha-Chl...	0.000	8.316	0	53157	N.D.	0.029 #
15)	B Endosulfa...	0.000	9.151f	0	214456	N.D.	0.144 #
17)	MA 4,4'-DDT	0.000	9.382f	0	45829	N.D.	0.034 #
18)	B Endrin al...	0.000	9.272	0	42319	N.D.	0.037 #
25)	Chlordane-3	0.000	8.237	0	110545	N.D.	0.400 #
26)	Chlordane-4	0.000	8.316	0	53157	N.D.	0.164 #
27)	Chlordane-5	0.000	9.204	0	12193	N.D.	0.225 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 16:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:37:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

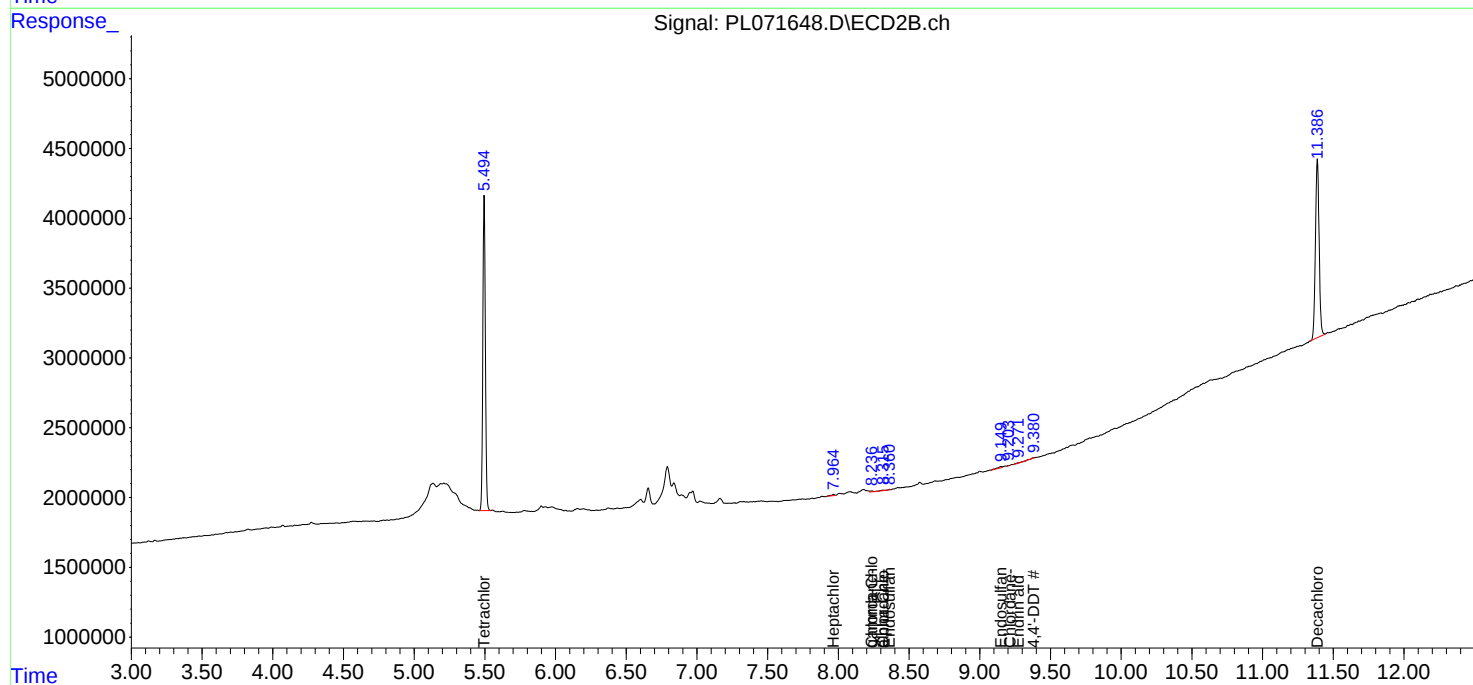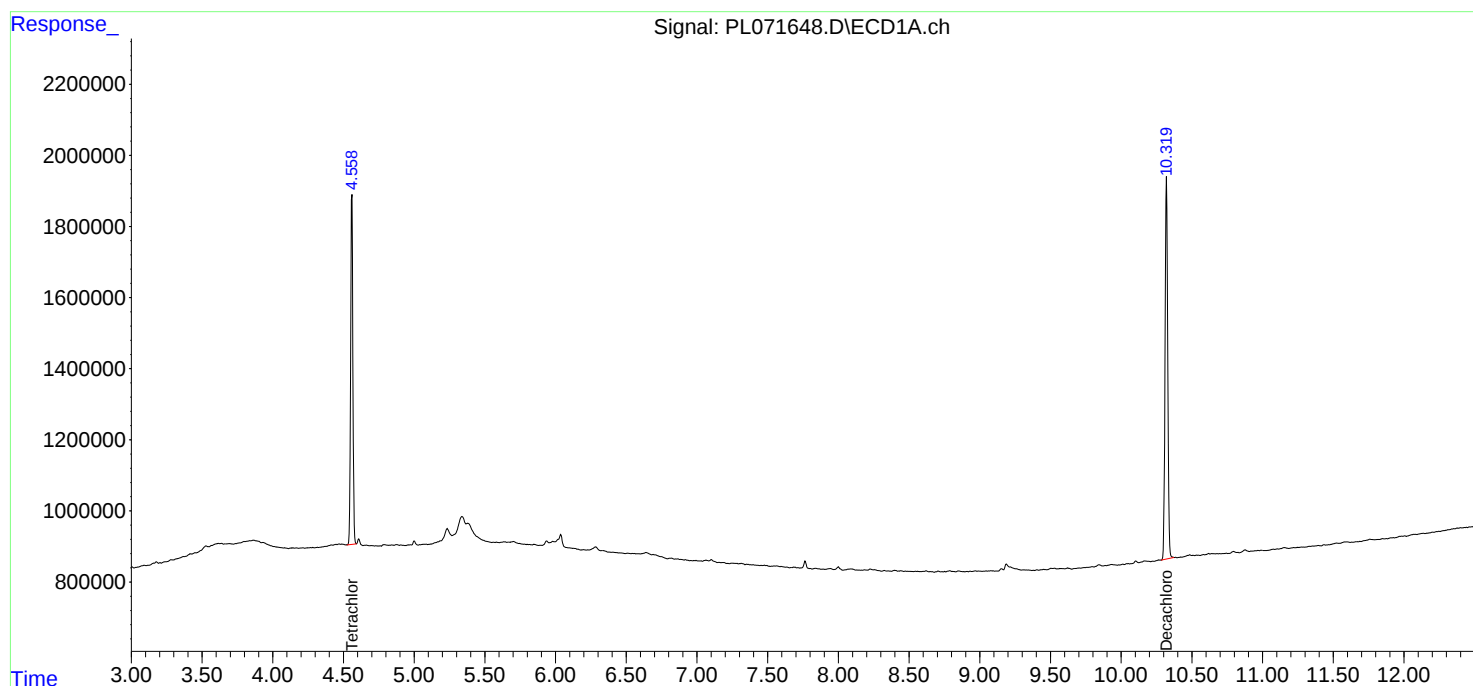


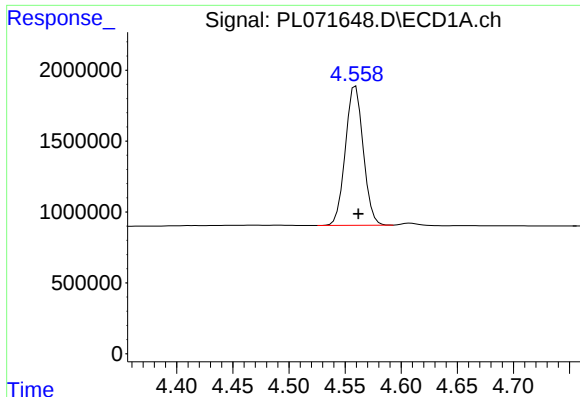

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 10868030
Conc: 16.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

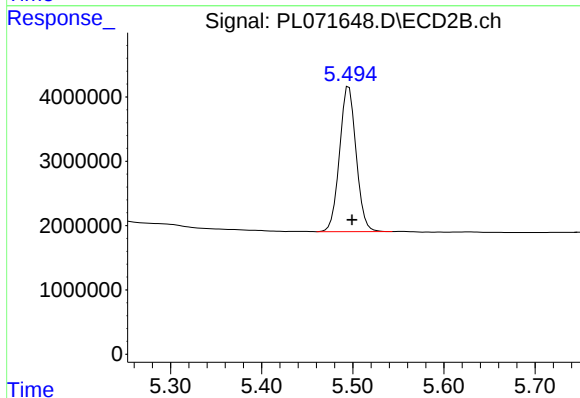


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: -0.004 min
Response: 28480185
Conc: 16.69 ng/ml

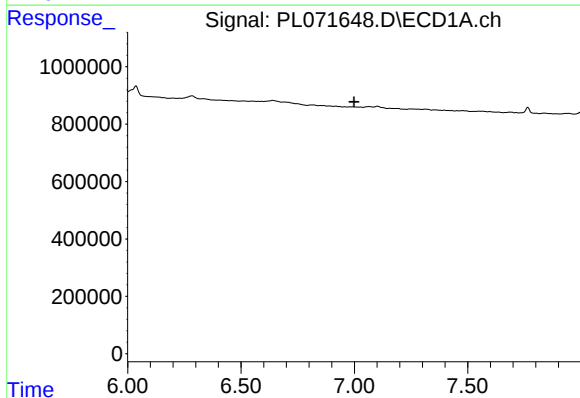


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

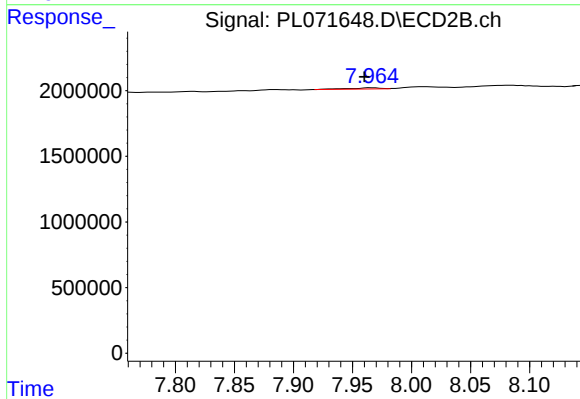

#8 Heptachlor epoxide


R.T.: 7.966 min
Delta R.T.: 0.006 min
Response: 170365
Conc: 0.09 ng/ml

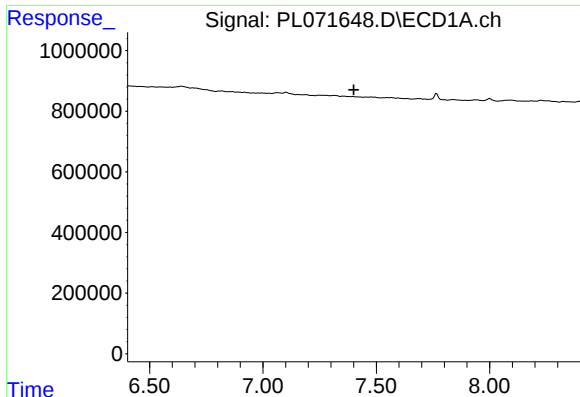

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

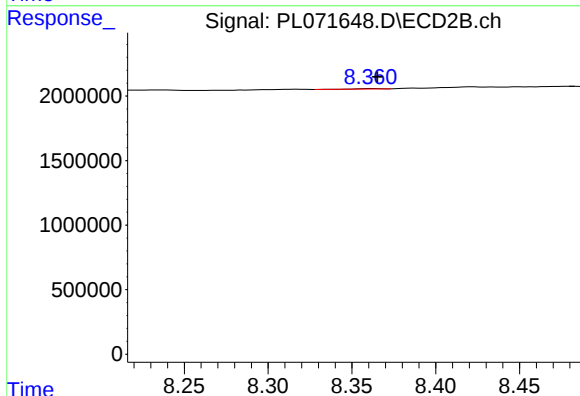


#9 Endosulfan I

R.T.: 8.363 min
Delta R.T.: -0.003 min
Response: 26679
Conc: 0.02 ng/ml

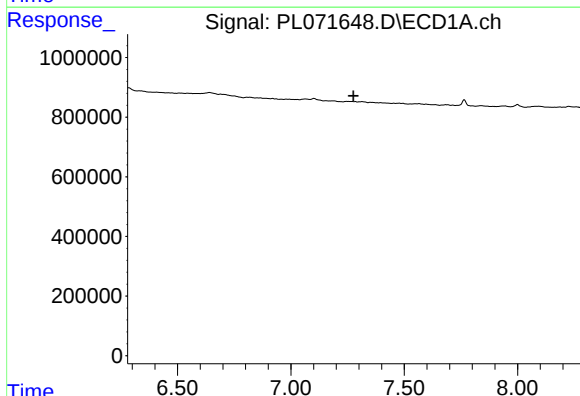


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

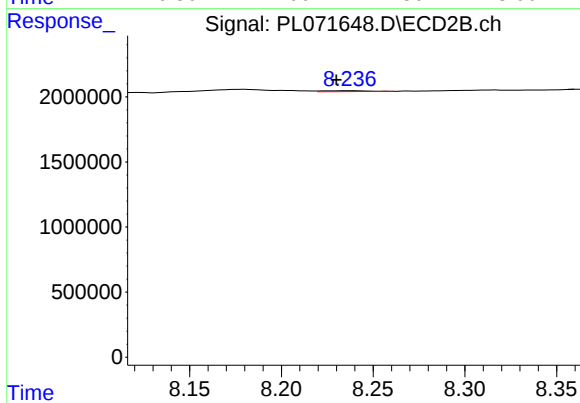

#10 gamma-Chlordane


R.T.: 8.237 min
Delta R.T.: 0.007 min
Response: 110545
Conc: 0.06 ng/ml

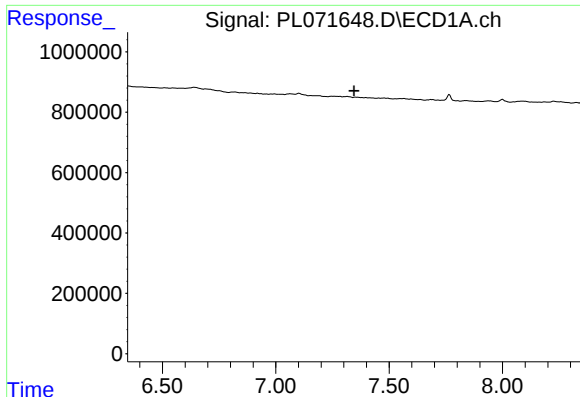

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

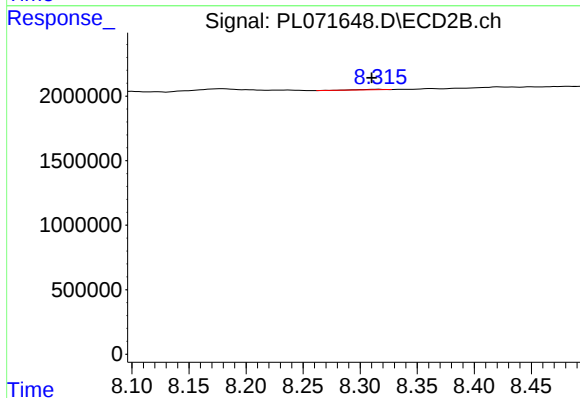


#11 alpha-Chlordane

R.T.: 8.316 min
Delta R.T.: 0.006 min
Response: 53157
Conc: 0.03 ng/ml

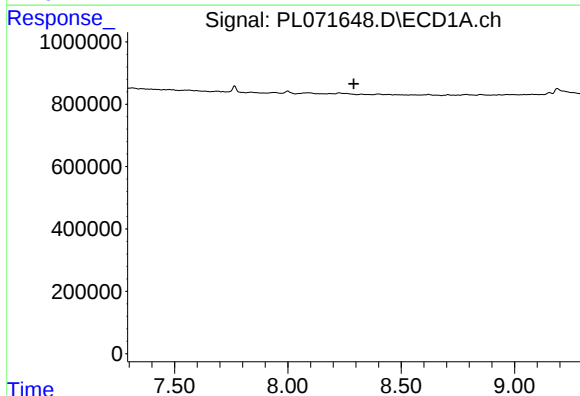


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

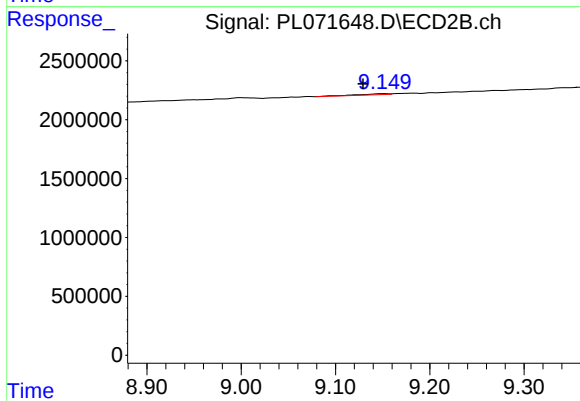

#15 Endosulfan II


R.T.: 9.151 min
Delta R.T.: 0.022 min
Response: 214456
Conc: 0.14 ng/ml

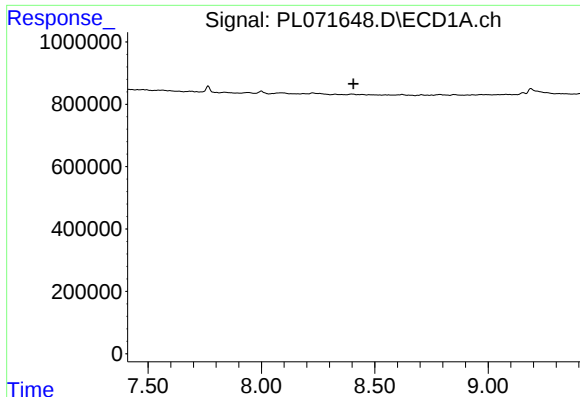

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

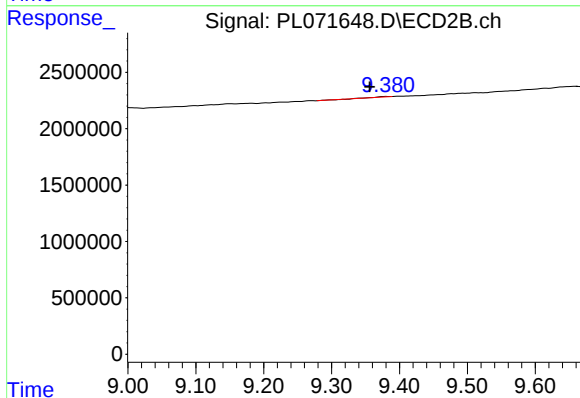


#17 4,4'-DDT

R.T.: 9.382 min
Delta R.T.: 0.026 min
Response: 45829
Conc: 0.03 ng/ml

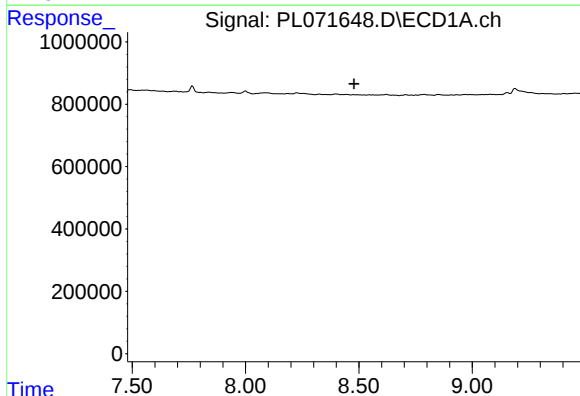


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

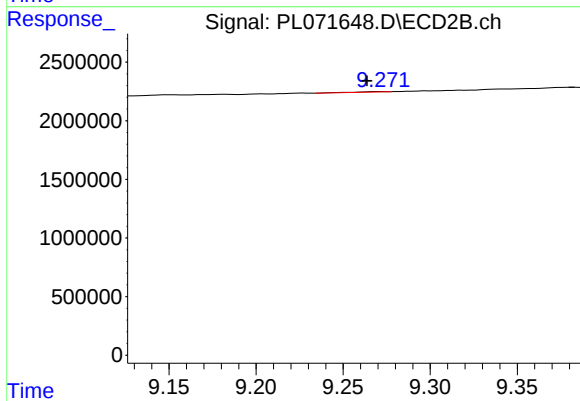

#18 Endrin aldehyde


R.T.: 9.272 min
Delta R.T.: 0.008 min
Response: 42319
Conc: 0.04 ng/ml

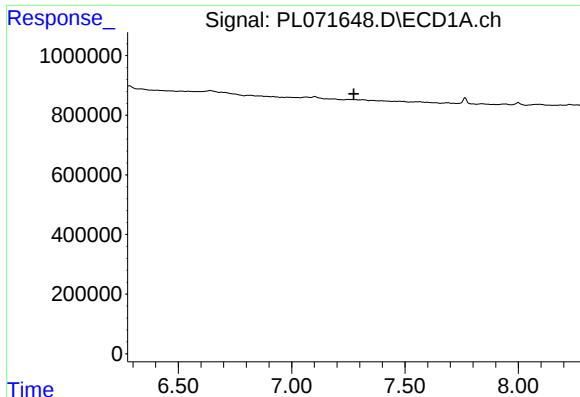

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

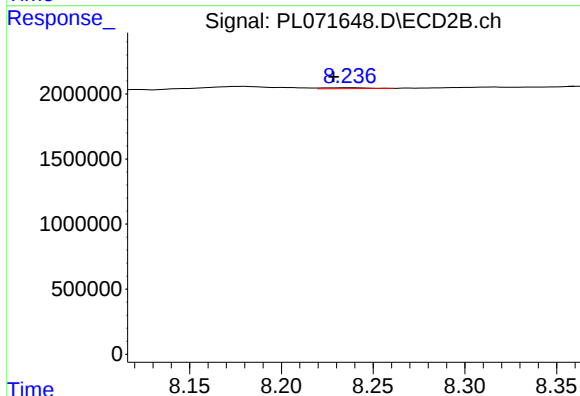


#25 Chlordane-3

R.T.: 8.237 min
Delta R.T.: 0.008 min
Response: 110545
Conc: 0.40 ng/ml

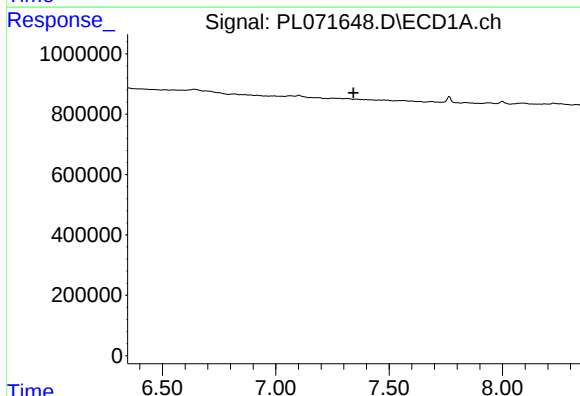


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

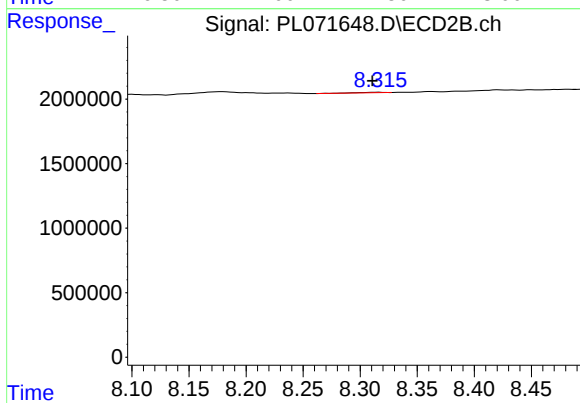

#26 Chlordane-4


R.T.: 8.316 min
Delta R.T.: 0.006 min
Response: 53157
Conc: 0.16 ng/ml

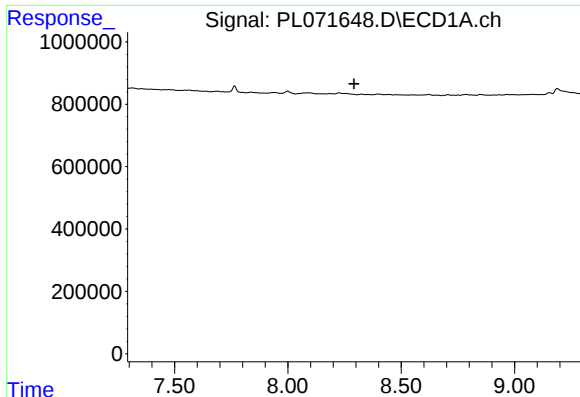

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

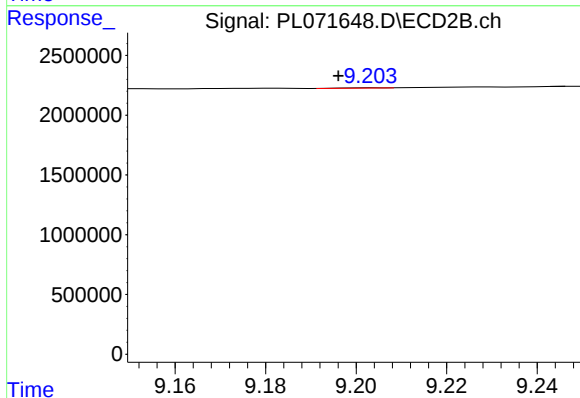


#27 Chlordane-5

R.T.: 9.204 min
Delta R.T.: 0.008 min
Response: 12193
Conc: 0.22 ng/ml

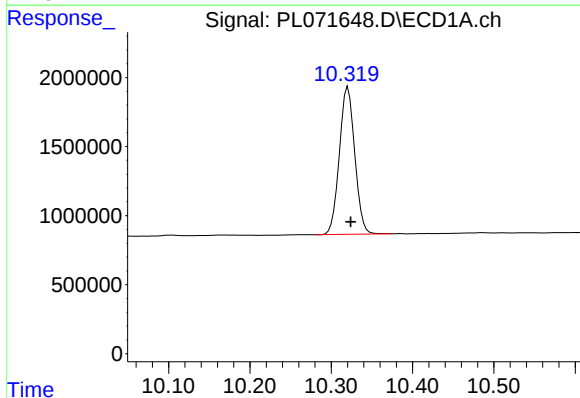

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.003 min
Response: 14012341
Conc: 18.82 ng/ml

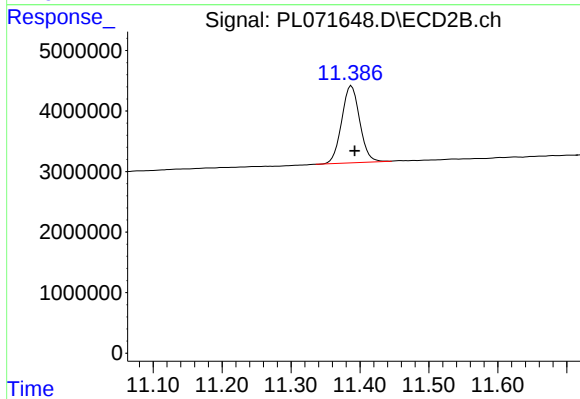

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.005 min
Response: 23163394
Conc: 18.48 ng/ml