

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:52
 Operator : AR\AJ
 Sample : PB141639TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB141639TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:39:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.496	10565146	27673619	16.284	16.217
28)	SA Decachlor...	10.321	11.387	15074344	25018873	20.249	19.963
Target Compounds							
7)	B delta-BHC	0.000	7.021f	0	140887	N.D.	0.067 #
10)	B gamma-Chl...	0.000	8.228	0	173403	N.D.	0.089 #
11)	B alpha-Chl...	0.000	8.314	0	43491	N.D.	0.023 #
15)	B Endosulfa...	0.000	9.144	0	140498	N.D.	0.094 #
16)	A 4,4'-DDD	0.000	9.028	0	24887	N.D.	0.019 #
18)	B Endrin al...	0.000	9.292f	0	77303	N.D.	0.067 #
19)	B Endosulfa...	0.000	9.499	0	33892	N.D.	0.024 #
24)	Chlordane-2	0.000	7.442f	0	30731	N.D.	0.417 #
25)	Chlordane-3	0.000	8.228	0	173403	N.D.	0.628 #
26)	Chlordane-4	0.000	8.314	0	43491	N.D.	0.134 #
27)	Chlordane-5	0.000	9.168f	0	20274	N.D.	0.374 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:52
Operator : AR\AJ
Sample : PB141639TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB141639TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:39:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

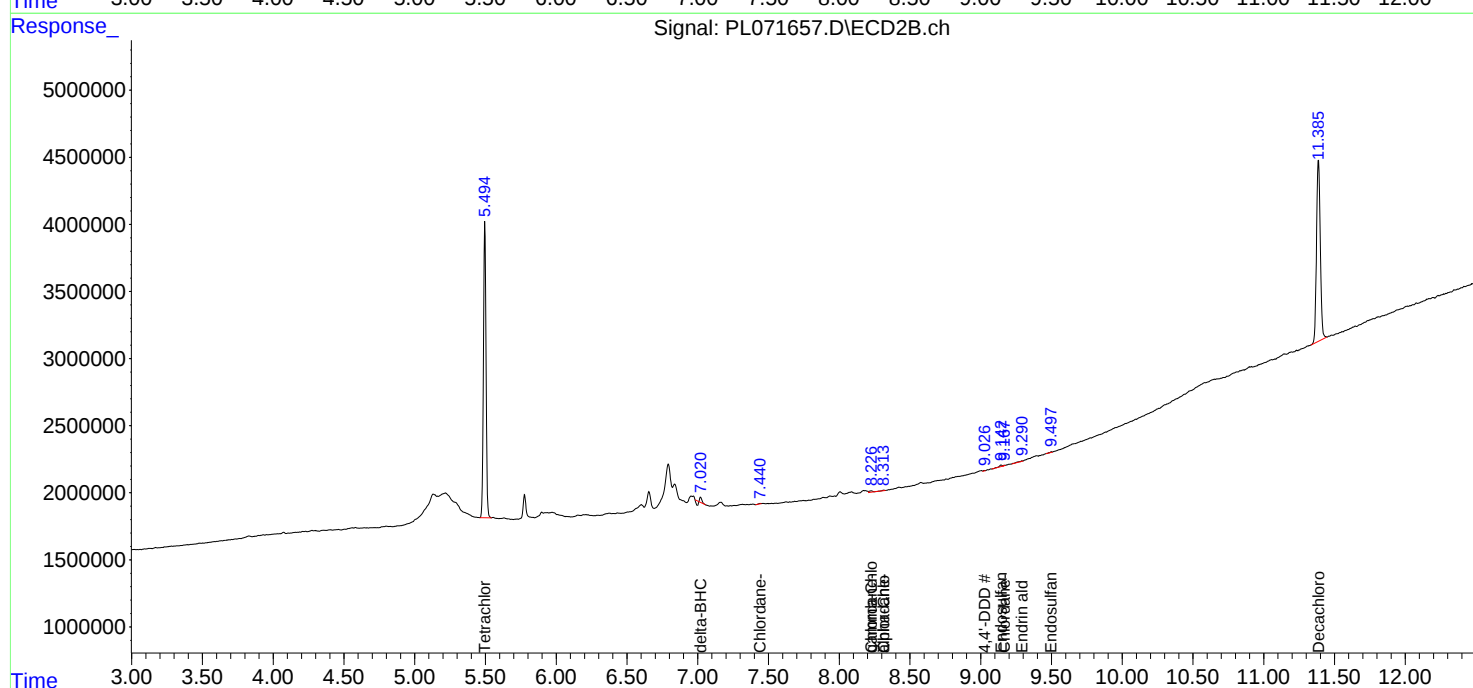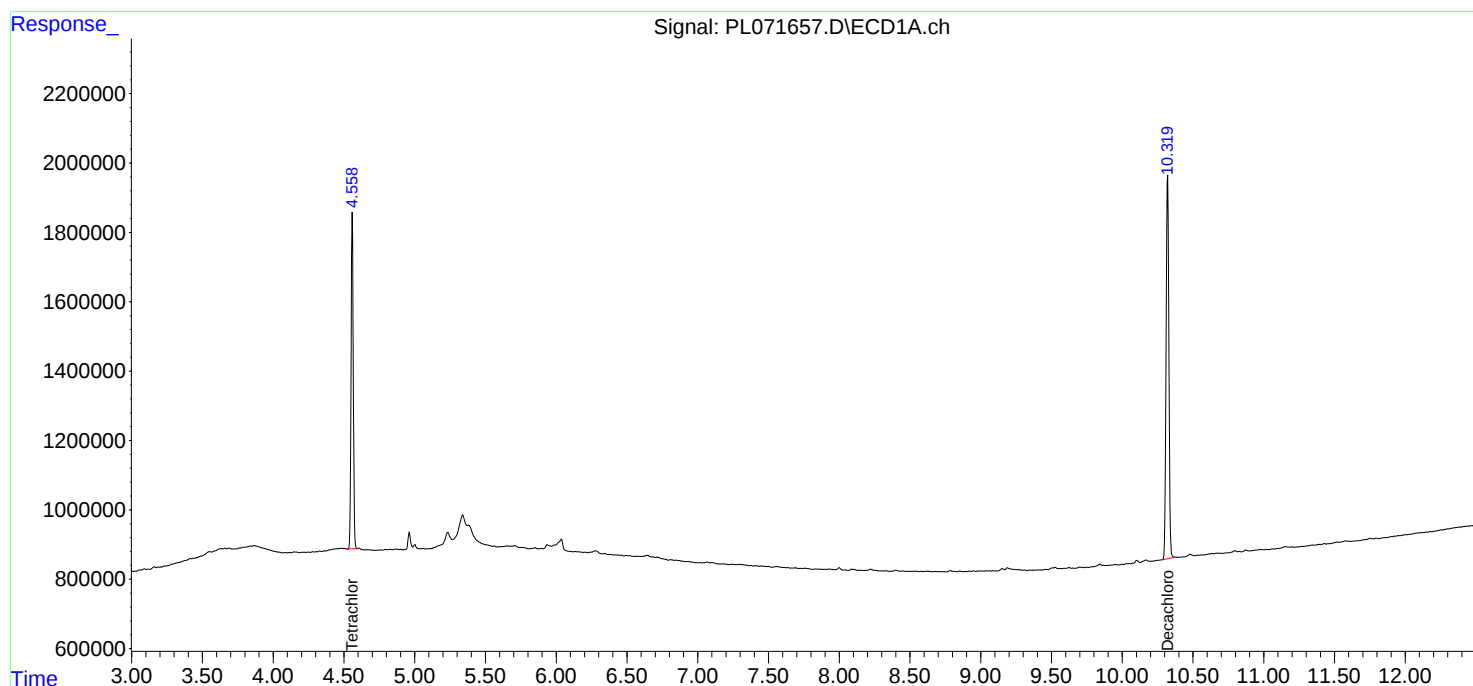


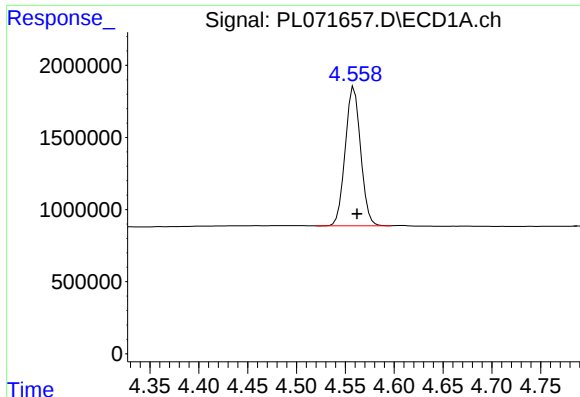

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 10565146
Conc: 16.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB141639TB

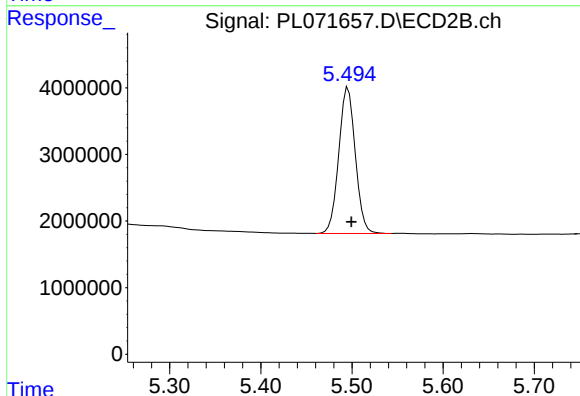


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 27673619
Conc: 16.22 ng/ml

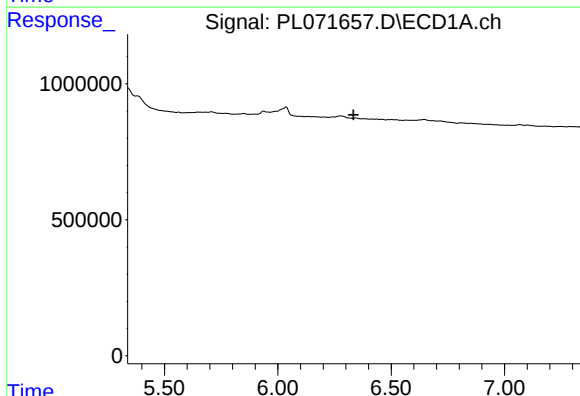


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

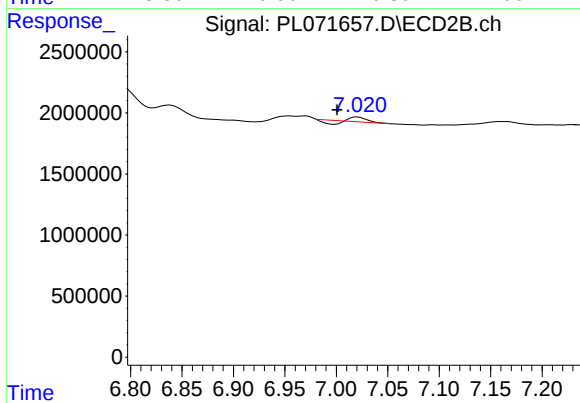

#7 delta-BHC


R.T.: 7.021 min
Delta R.T.: 0.020 min
Response: 140887
Conc: 0.07 ng/ml

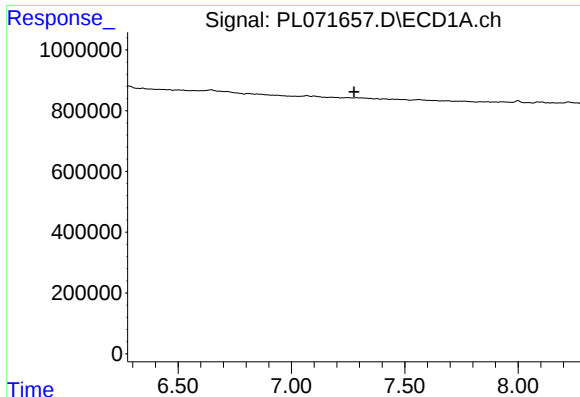

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141639TB

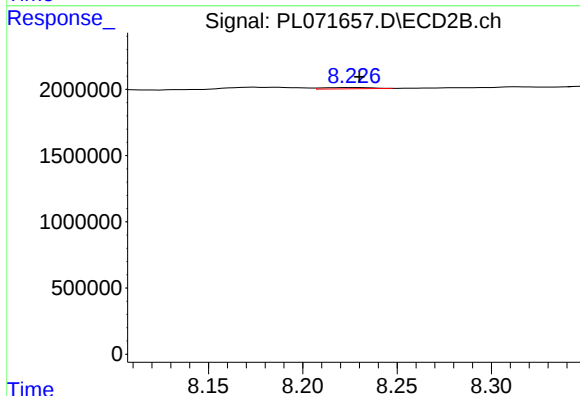


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: -0.002 min
Response: 173403
Conc: 0.09 ng/ml

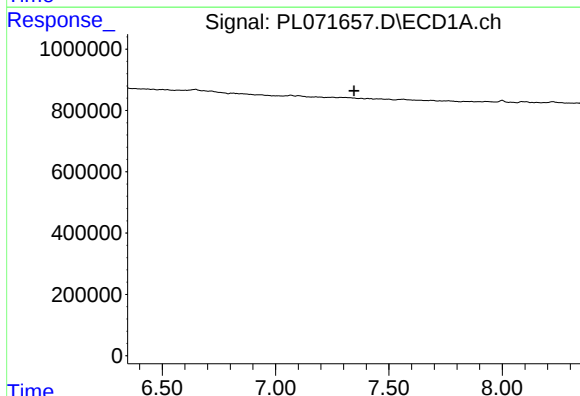


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

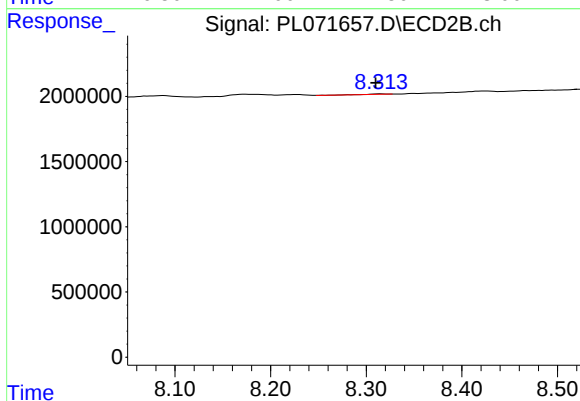

#11 alpha-Chlordane


R.T.: 8.314 min
Delta R.T.: 0.004 min
Response: 43491
Conc: 0.02 ng/ml

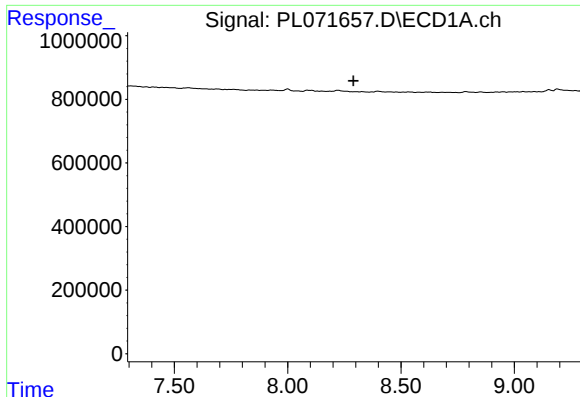

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141639TB

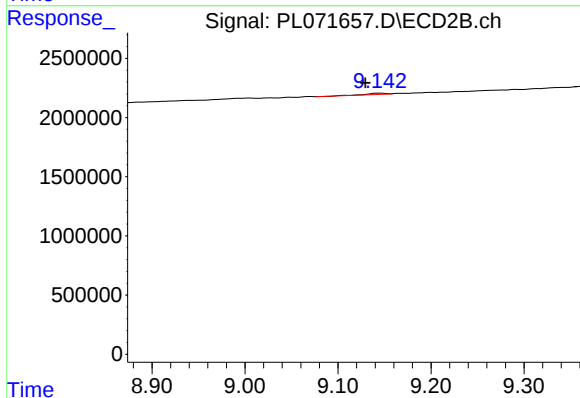


#15 Endosulfan II

R.T.: 9.144 min
Delta R.T.: 0.015 min
Response: 140498
Conc: 0.09 ng/ml

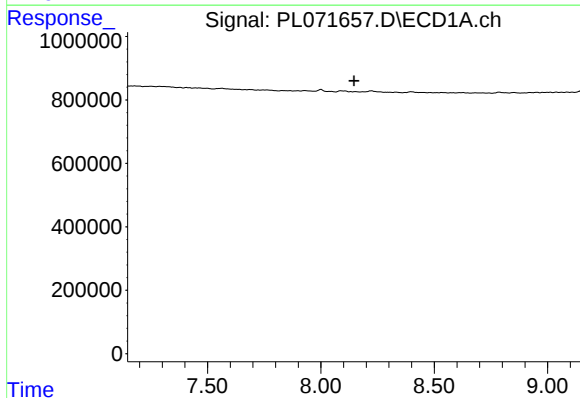


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

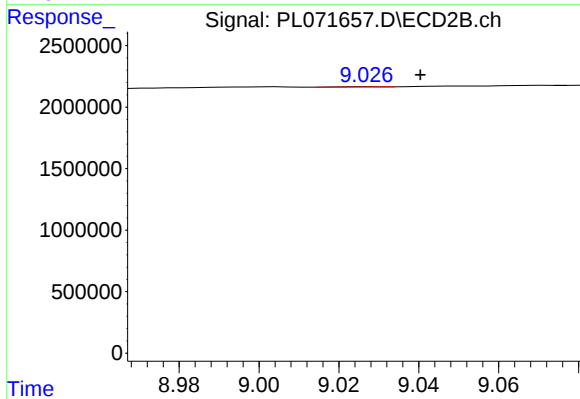

#16 4,4'-DDD


R.T.: 9.028 min
Delta R.T.: -0.013 min
Response: 24887
Conc: 0.02 ng/ml

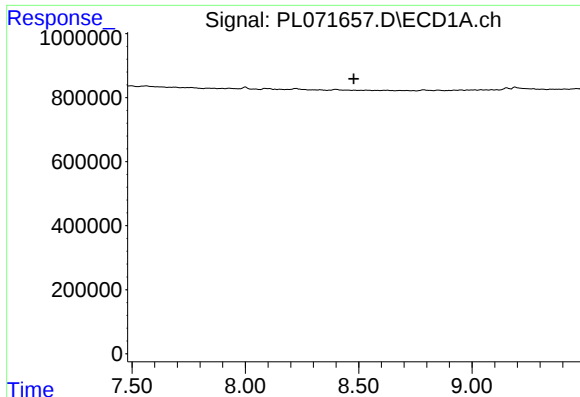

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141639TB

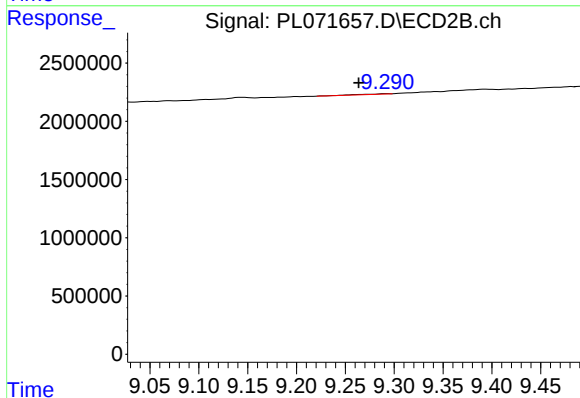


#18 Endrin aldehyde

R.T.: 9.292 min
Delta R.T.: 0.029 min
Response: 77303
Conc: 0.07 ng/ml

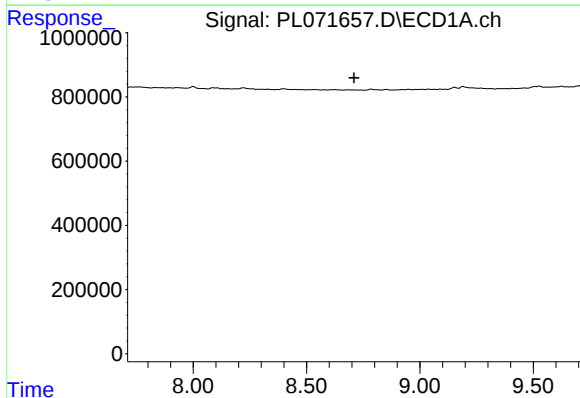


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

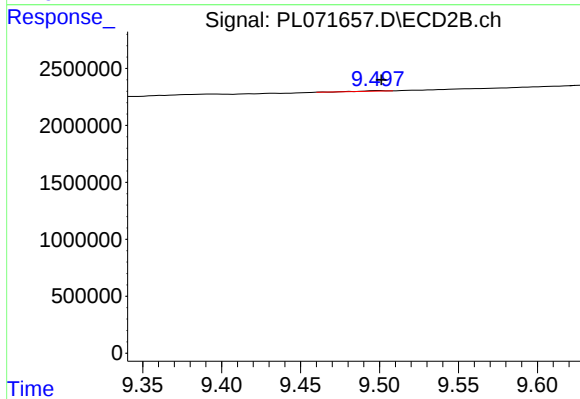

#19 Endosulfan Sulfate


R.T.: 9.499 min
Delta R.T.: -0.002 min
Response: 33892
Conc: 0.02 ng/ml

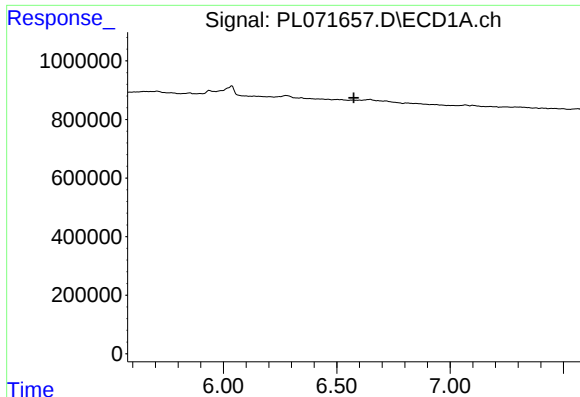

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141639TB

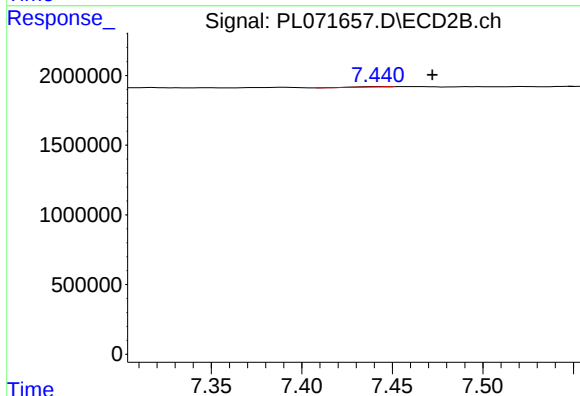


#24 Chlordane-2

R.T.: 7.442 min
Delta R.T.: -0.030 min
Response: 30731
Conc: 0.42 ng/ml

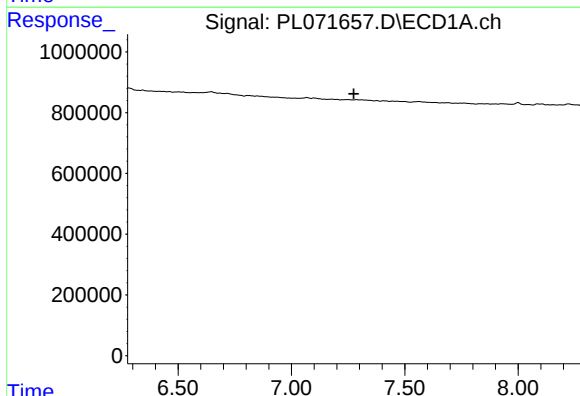


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

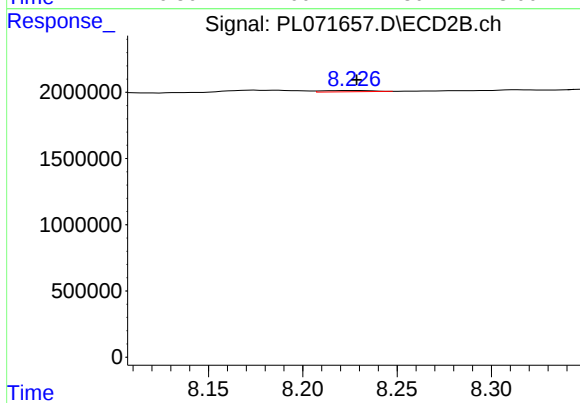

#25 Chlordane-3


R.T.: 8.228 min
Delta R.T.: 0.000 min
Response: 173403
Conc: 0.63 ng/ml

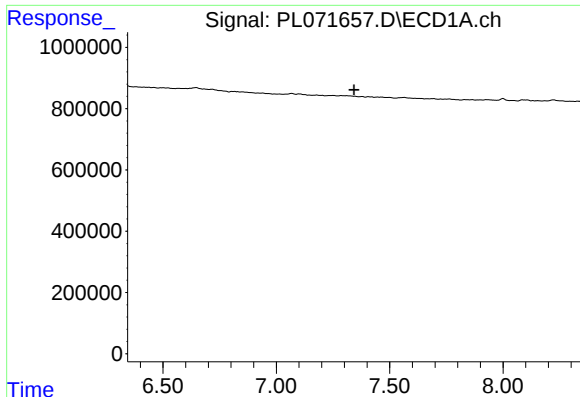

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141639TB

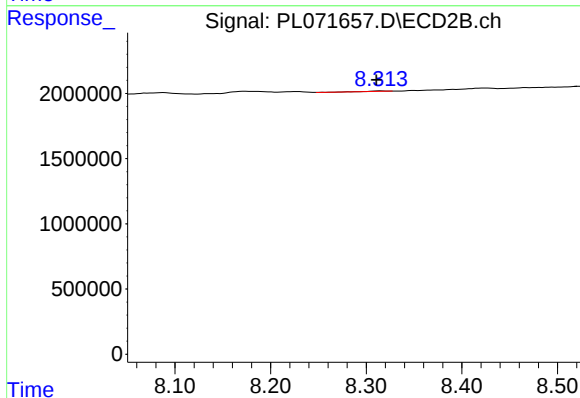


#26 Chlordane-4

R.T.: 8.314 min
Delta R.T.: 0.004 min
Response: 43491
Conc: 0.13 ng/ml

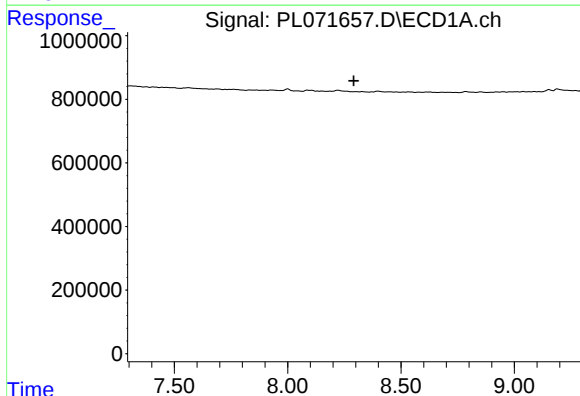


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

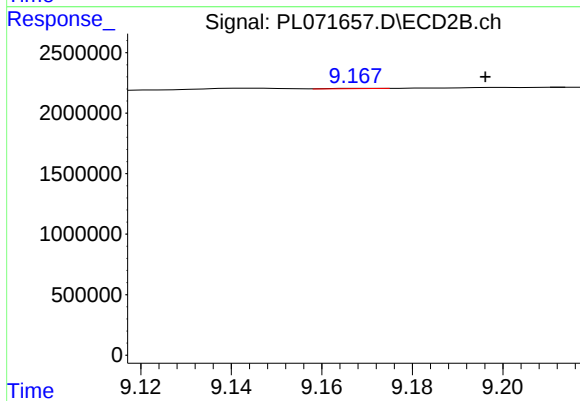

#27 Chlordane-5


R.T.: 9.168 min
Delta R.T.: -0.028 min
Response: 20274
Conc: 0.37 ng/ml

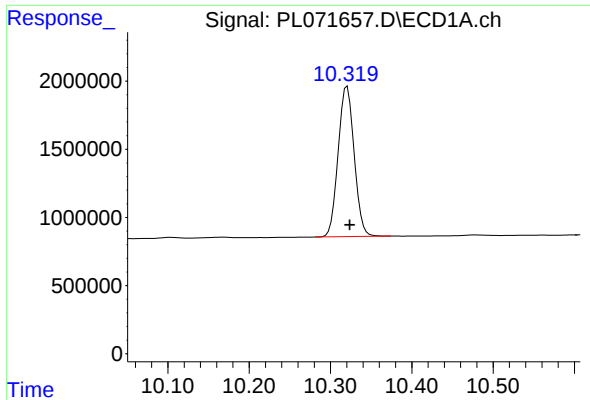

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.003 min
Response: 15074344
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB141639TB

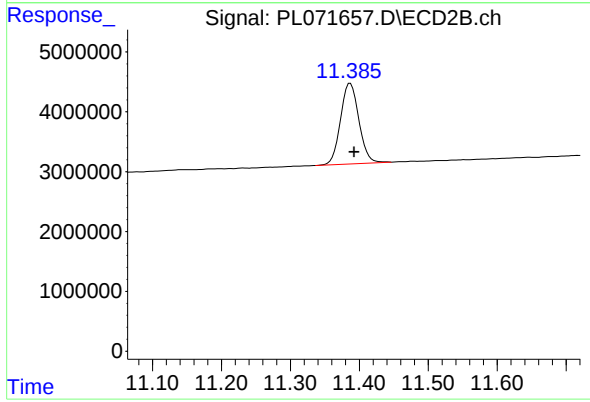

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.005 min
Response: 25018873
Conc: 19.96 ng/ml