

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 19:09
 Operator : AR\AJ
 Sample : M5065-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 UV-1WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:39:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.496	10674917	27732547	16.453	16.252
28)	SA Decachlor...	10.320	11.387	15028571	24994045	20.187	19.943
Target Compounds							
9)	A Endosulfan I	0.000	8.364	0	8850	N.D.	0.005 #
10)	B gamma-Chl...	0.000	8.227	0	103252	N.D.	0.053 #
11)	B alpha-Chl...	0.000	8.318	0	43030	N.D.	0.023 #
13)	MA Dieldrin	0.000	8.665	0	12436	N.D.	0.007 #
14)	MA Endrin	0.000	8.913f	0	126252	N.D.	0.084 #
15)	B Endosulfa...	0.000	9.147f	0	65667	N.D.	0.044 #
16)	A 4,4'-DDD	0.000	9.044	0	85056	N.D.	0.065 #
24)	Chlordane-2	0.000	7.443f	0	94896	N.D.	1.288 #
25)	Chlordane-3	0.000	8.227	0	103252	N.D.	0.374 #
26)	Chlordane-4	0.000	8.318	0	43030	N.D.	0.133 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 19:09
Operator : AR\AJ
Sample : M5065-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
UV-1WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:39:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

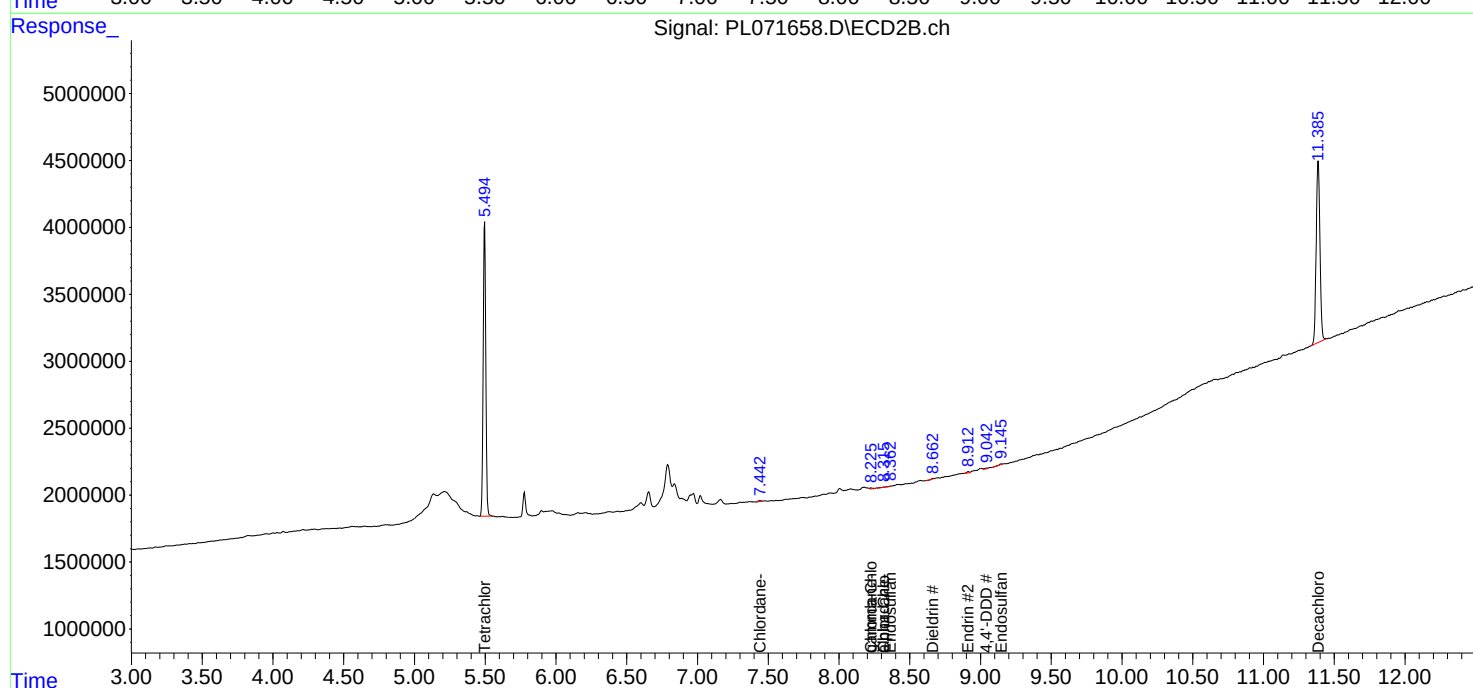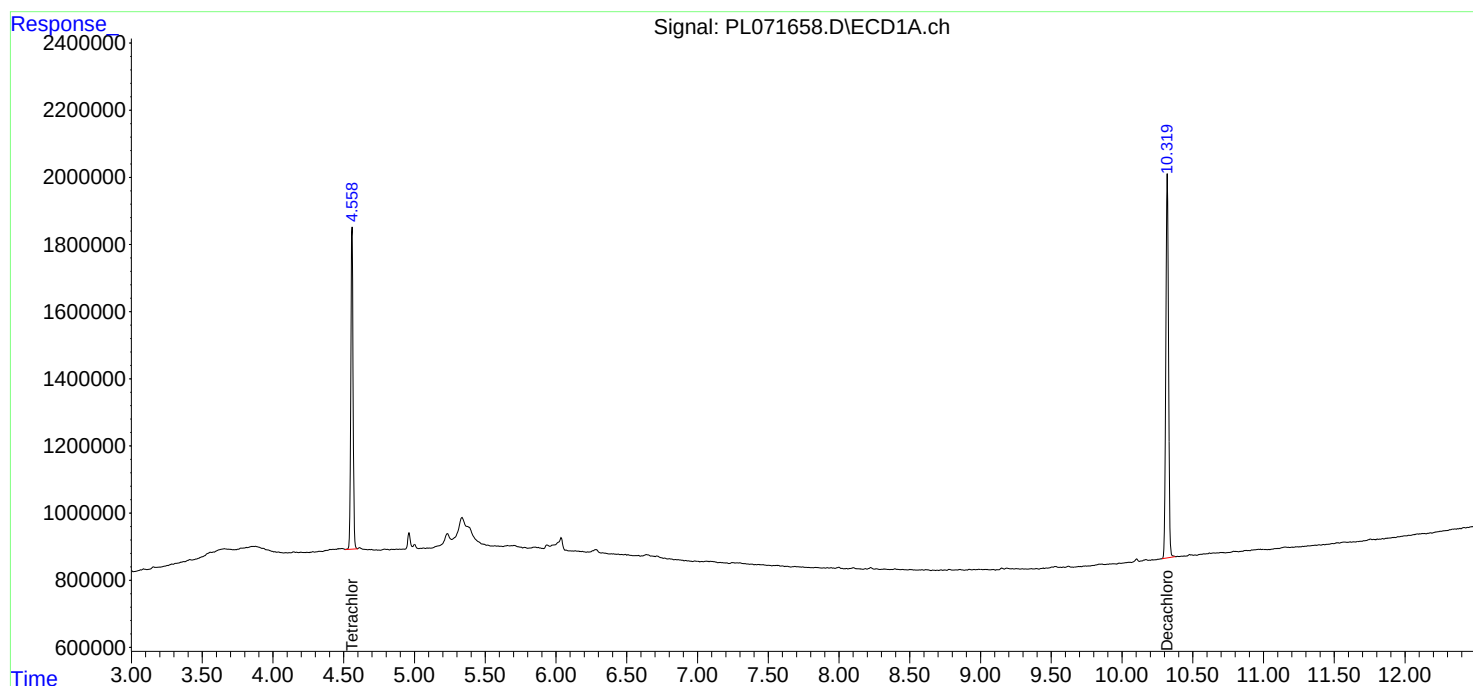


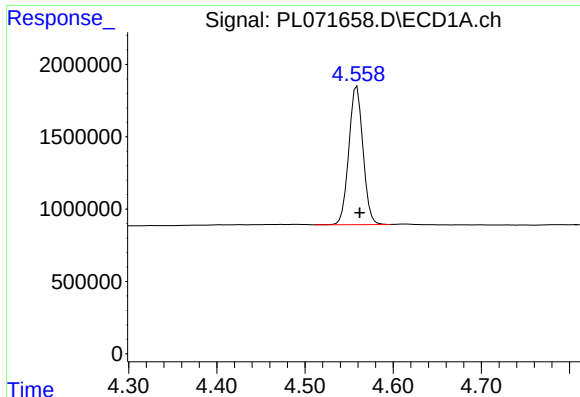

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 10674917
Conc: 16.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
UV-1WC

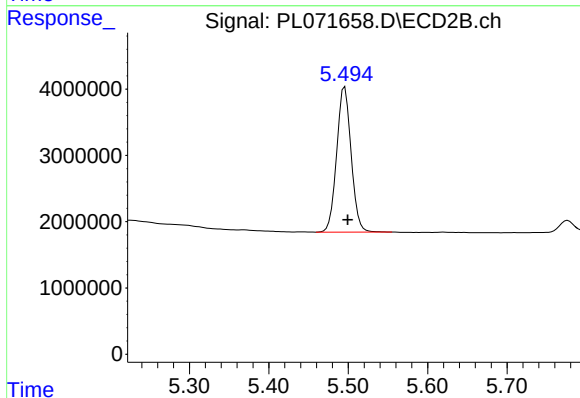


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: -0.004 min
Response: 27732547
Conc: 16.25 ng/ml

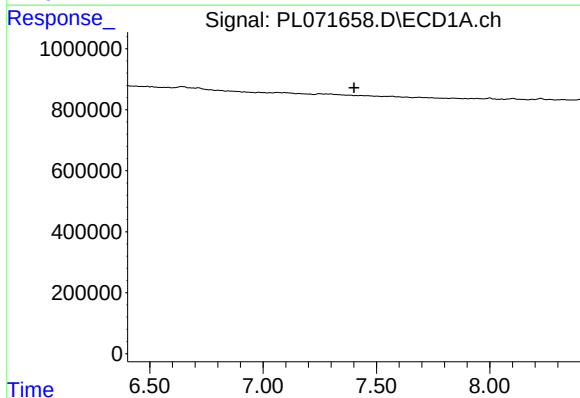


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

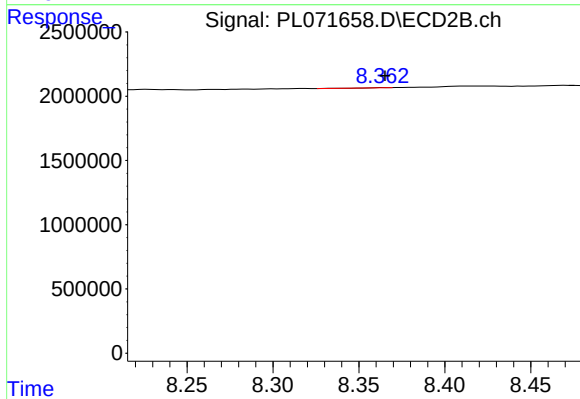

#9 Endosulfan I


R.T.: 8.364 min
Delta R.T.: 0.000 min
Response: 8850
Conc: 0.01 ng/ml

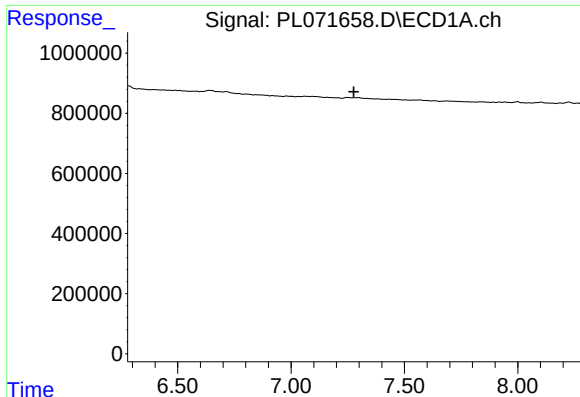

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

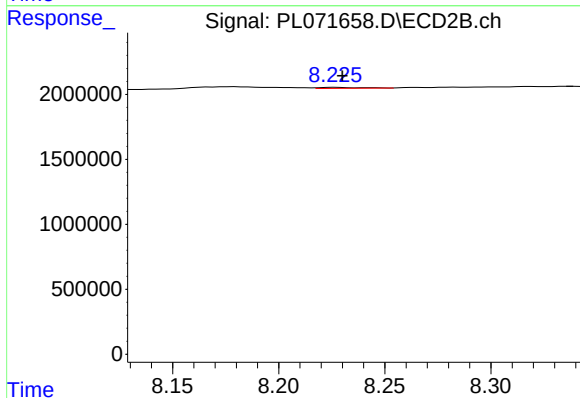


#10 gamma-Chlordane

R.T.: 8.227 min
Delta R.T.: -0.003 min
Response: 103252
Conc: 0.05 ng/ml

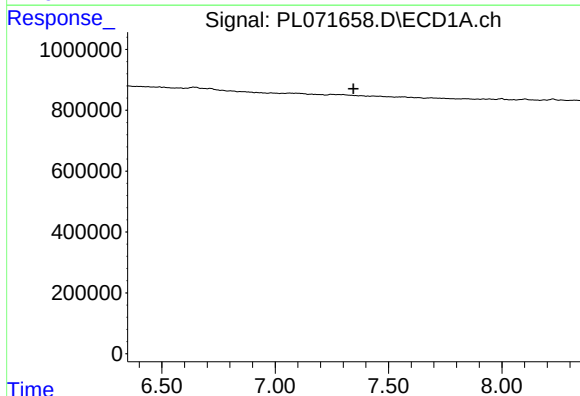


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

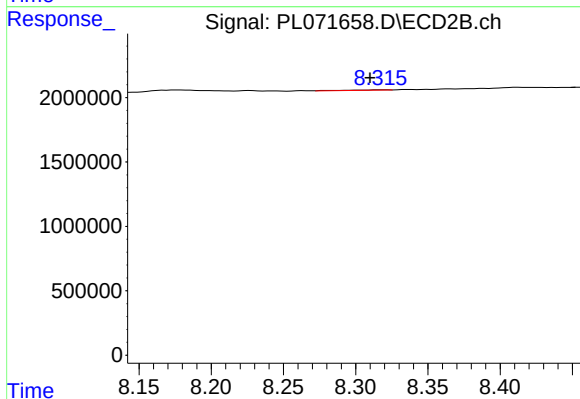

#11 alpha-Chlordane


R.T.: 8.318 min
Delta R.T.: 0.008 min
Response: 43030
Conc: 0.02 ng/ml

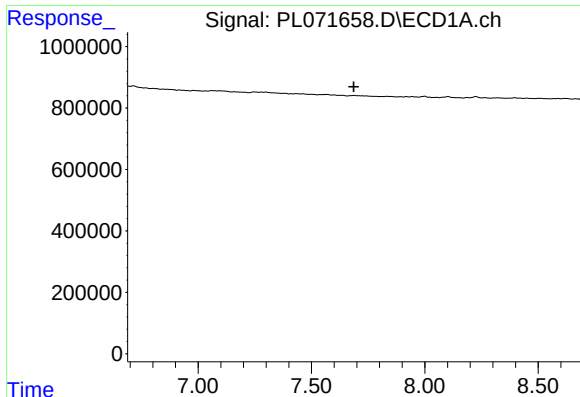

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.687 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

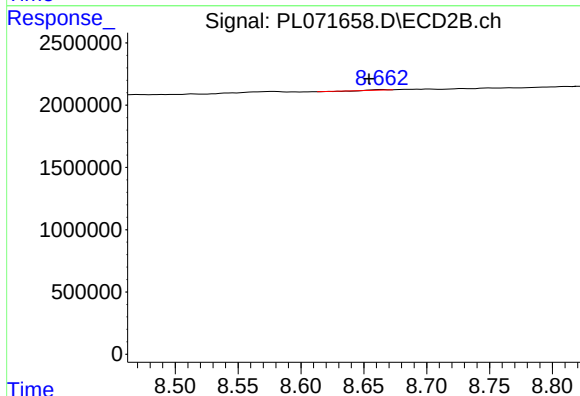


#13 Dieldrin

R.T.: 8.665 min
Delta R.T.: 0.011 min
Response: 12436
Conc: 0.01 ng/ml

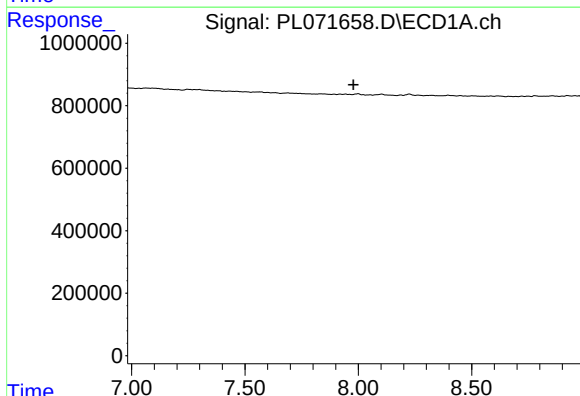


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.979 min
Response: 0
Conc: N.D.

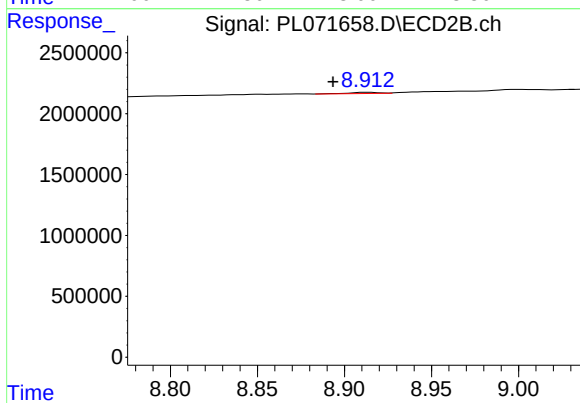

#14 Endrin


R.T.: 8.913 min
Delta R.T.: 0.020 min
Response: 126252
Conc: 0.08 ng/ml

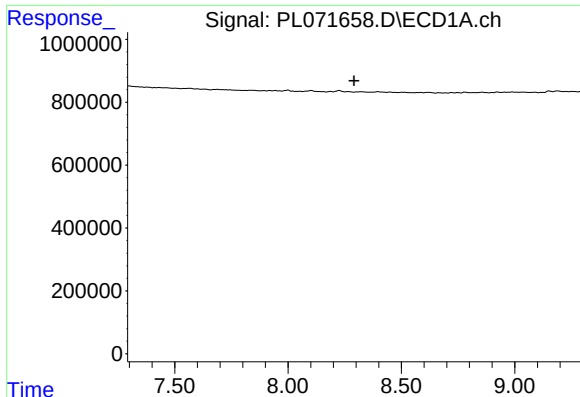

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

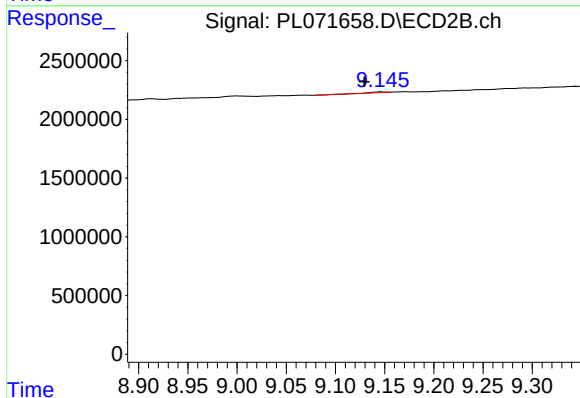


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 65667
Conc: 0.04 ng/ml

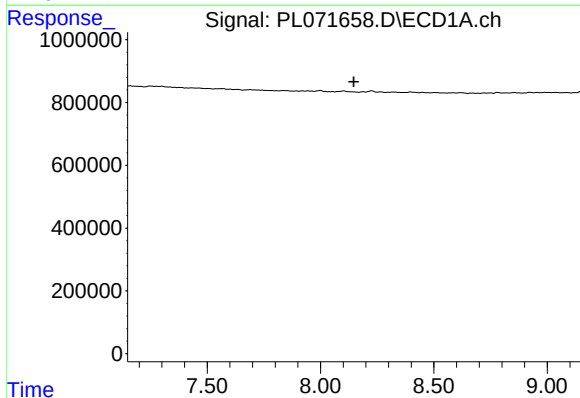


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

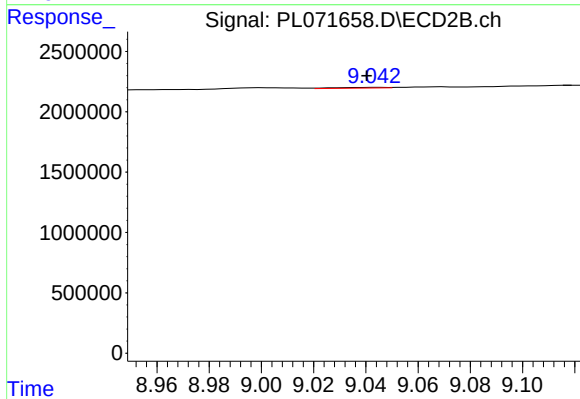

#16 4,4'-DDD


R.T.: 9.044 min
Delta R.T.: 0.004 min
Response: 85056
Conc: 0.07 ng/ml

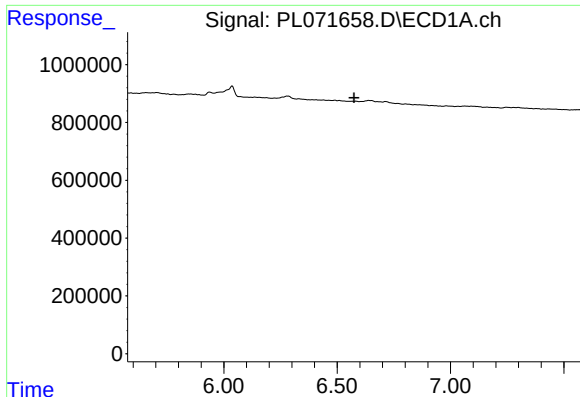

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

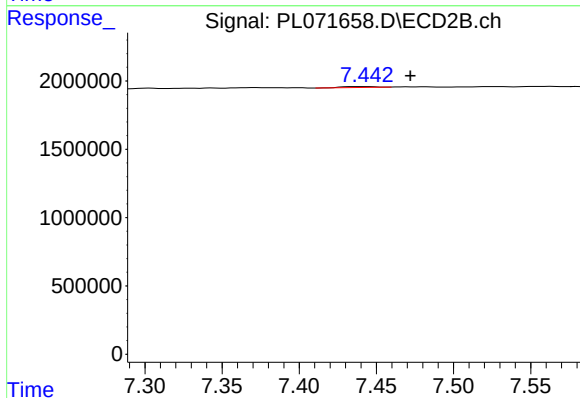


#24 Chlordane-2

R.T.: 7.443 min
Delta R.T.: -0.029 min
Response: 94896
Conc: 1.29 ng/ml

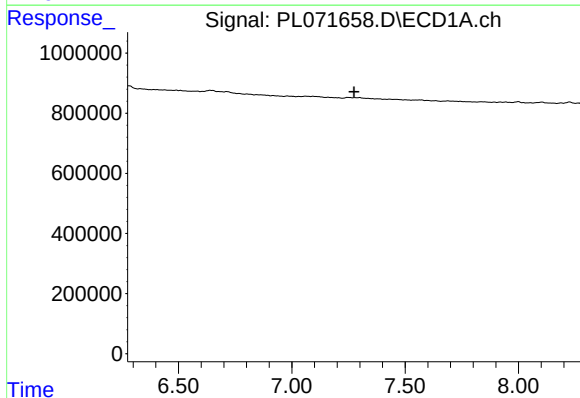


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

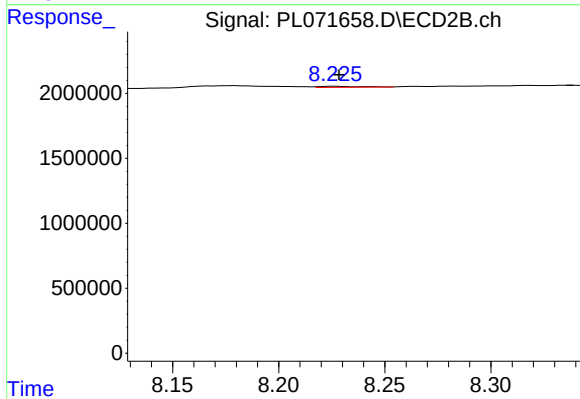

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 103252
Conc: 0.37 ng/ml

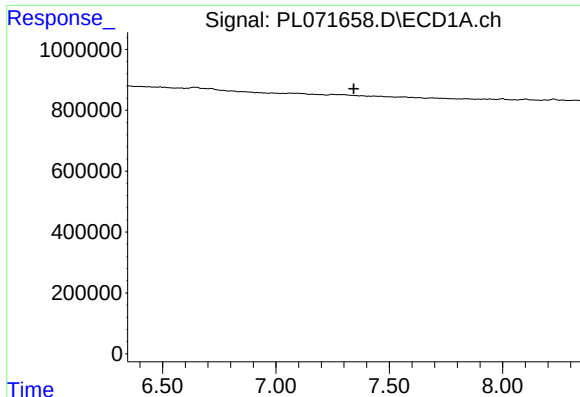

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
UV-1WC

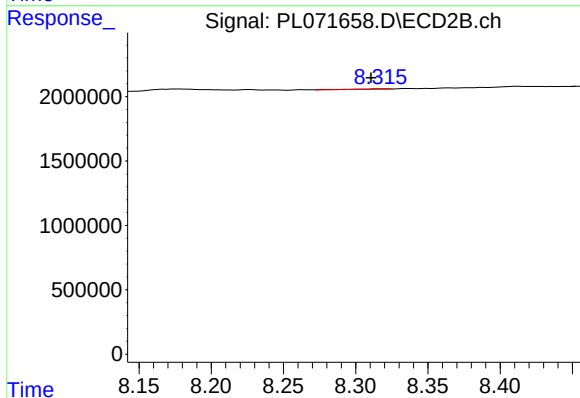


#26 Chlordane-4

R.T.: 8.318 min
Delta R.T.: 0.008 min
Response: 43030
Conc: 0.13 ng/ml

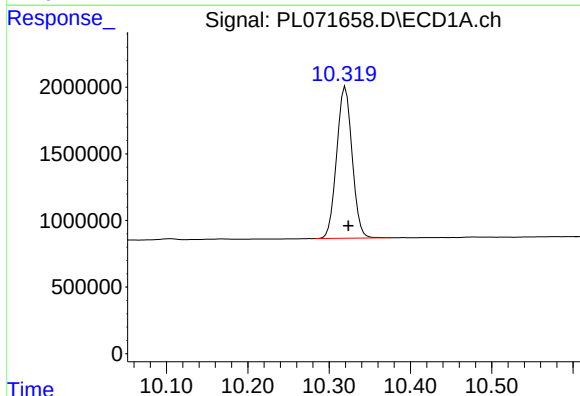

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.004 min
Response: 15028571
Conc: 20.19 ng/ml

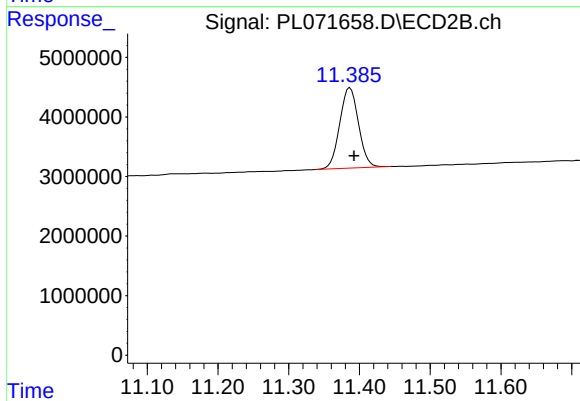

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.006 min
Response: 24994045
Conc: 19.94 ng/ml