

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 20:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:41:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.496	10252334	27008076	15.802	15.827
28)	SA Decachlor...	10.321	11.388	13921817	23722831	18.700	18.928
Target Compounds							
9)	A Endosulfan I	0.000	8.356	0	26155	N.D.	0.015 #
10)	B gamma-Chl...	0.000	8.233	0	140447	N.D.	0.072 #
11)	B alpha-Chl...	0.000	8.325	0	78382	N.D.	0.042 #
13)	MA Dieldrin	0.000	8.660	0	33341	N.D.	0.018 #
15)	B Endosulfa...	0.000	9.156f	0	439145	N.D.	0.295 #
18)	B Endrin al...	0.000	9.281f	0	94649	N.D.	0.082 #
19)	B Endosulfa...	0.000	9.501	0	59009	N.D.	0.042 #
25)	Chlordane-3	0.000	8.233	0	140447	N.D.	0.508 #
26)	Chlordane-4	0.000	8.325	0	78382	N.D.	0.242 #
27)	Chlordane-5	0.000	9.174f	0	43993	N.D.	0.811 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 20:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:41:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

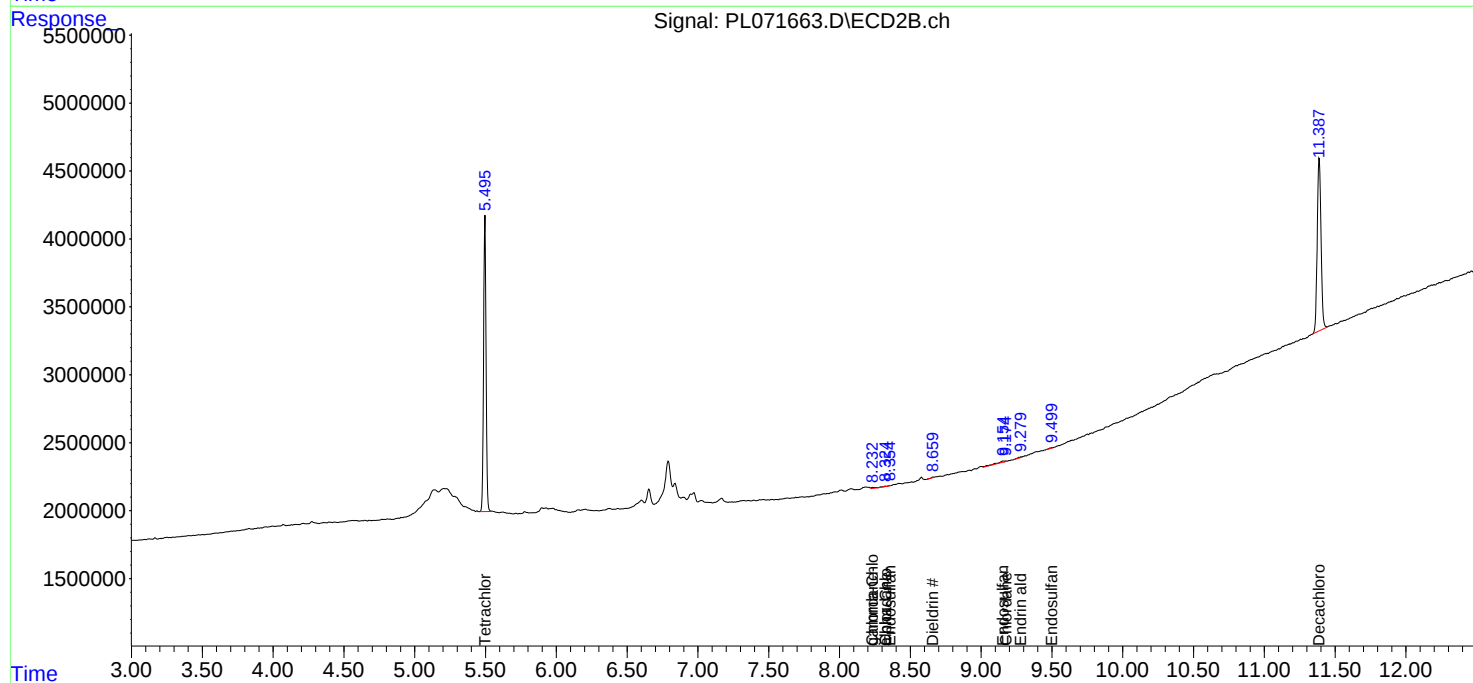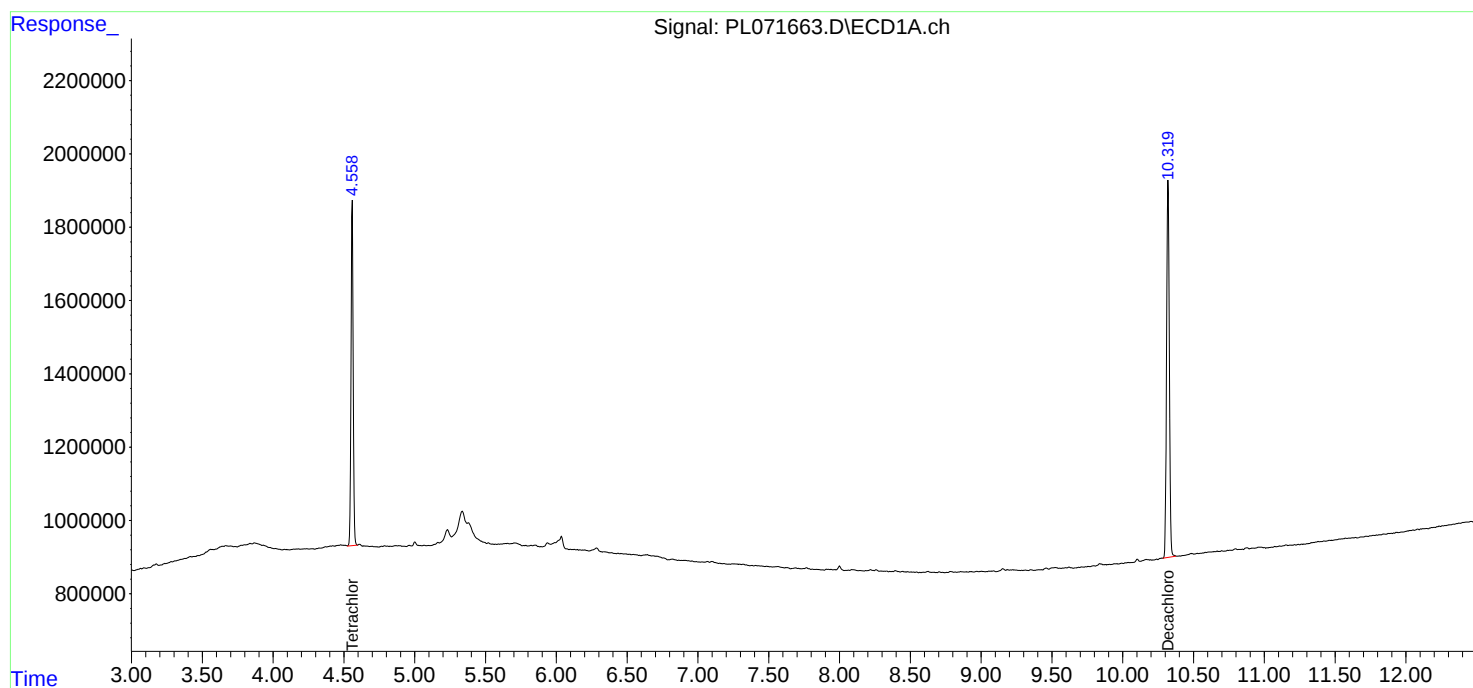


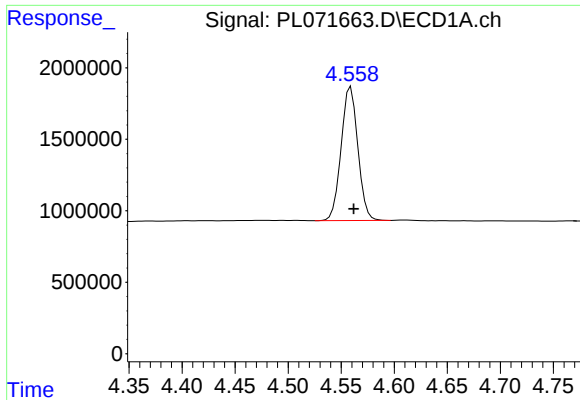

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 10252334
Conc: 15.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

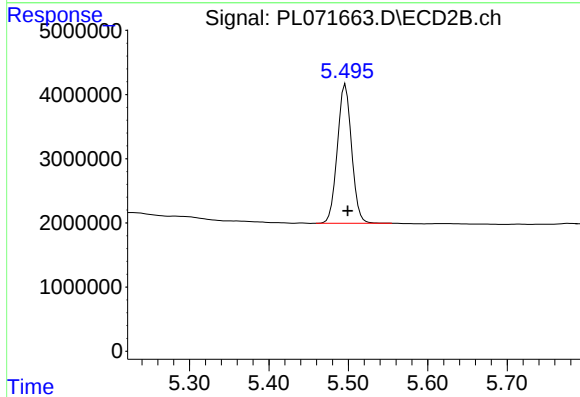


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 27008076
Conc: 15.83 ng/ml

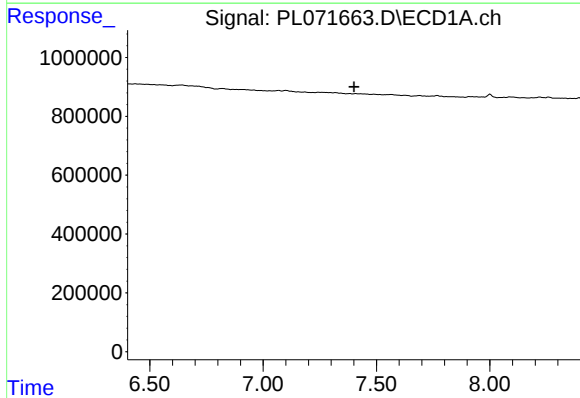


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

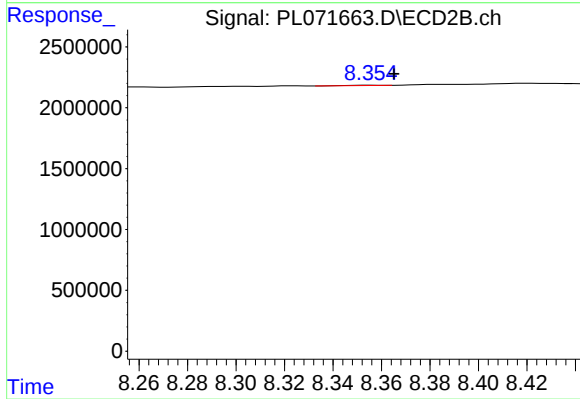

#9 Endosulfan I


R.T.: 8.356 min
Delta R.T.: -0.009 min
Response: 26155
Conc: 0.02 ng/ml

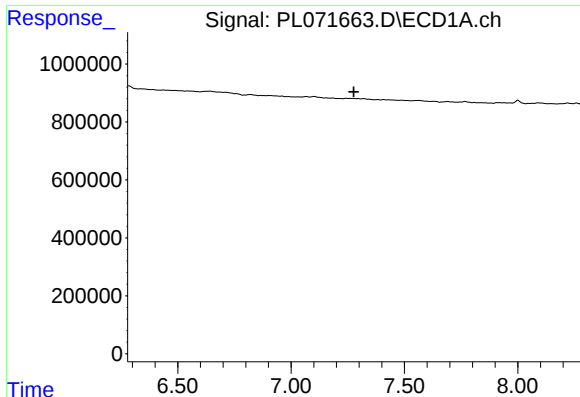

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

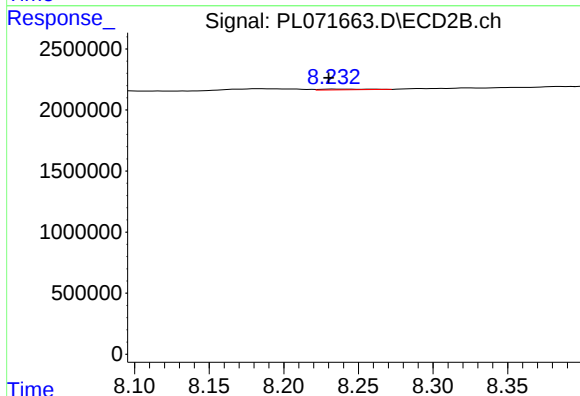


#10 gamma-Chlordane

R.T.: 8.233 min
Delta R.T.: 0.003 min
Response: 140447
Conc: 0.07 ng/ml

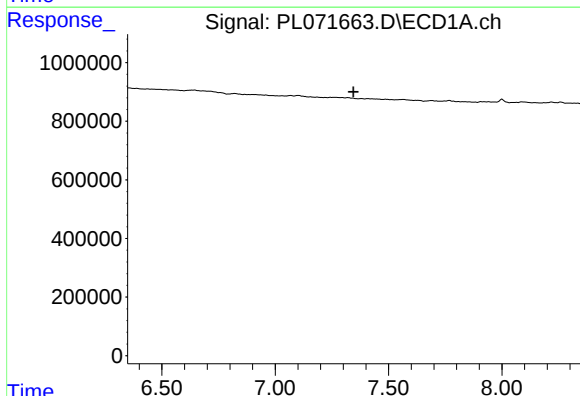


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

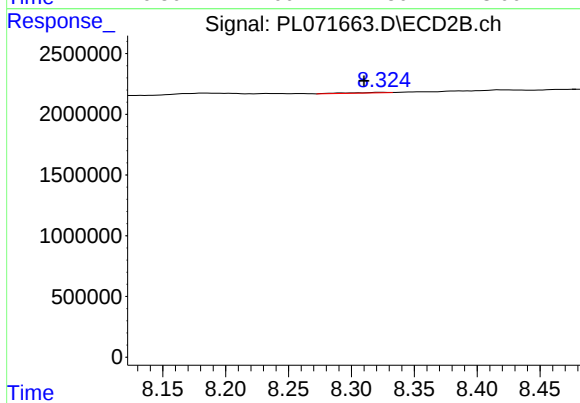

#11 alpha-Chlordane


R.T.: 8.325 min
Delta R.T.: 0.015 min
Response: 78382
Conc: 0.04 ng/ml

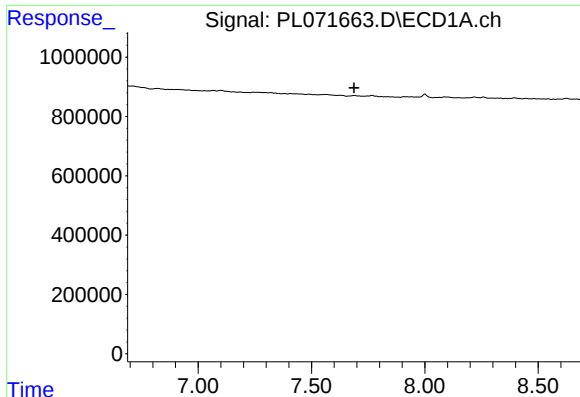

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.687 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

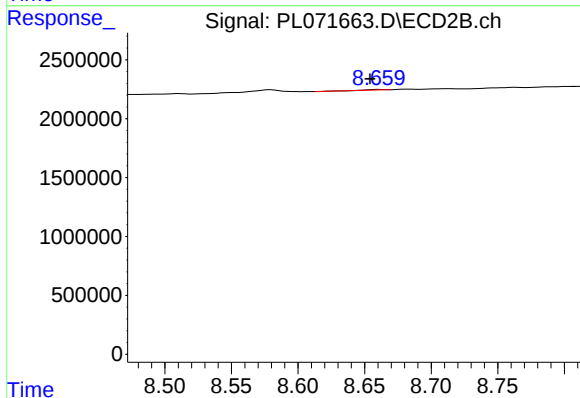


#13 Dieldrin

R.T.: 8.660 min
Delta R.T.: 0.006 min
Response: 33341
Conc: 0.02 ng/ml

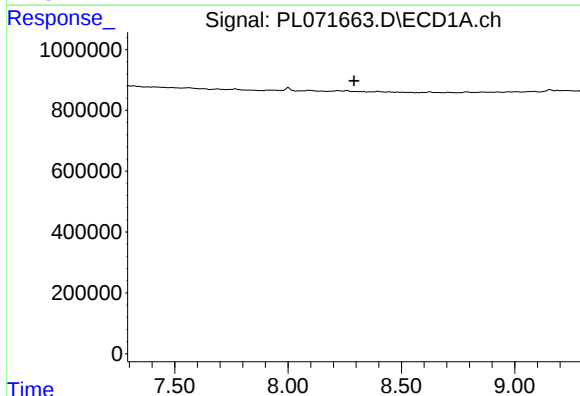


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

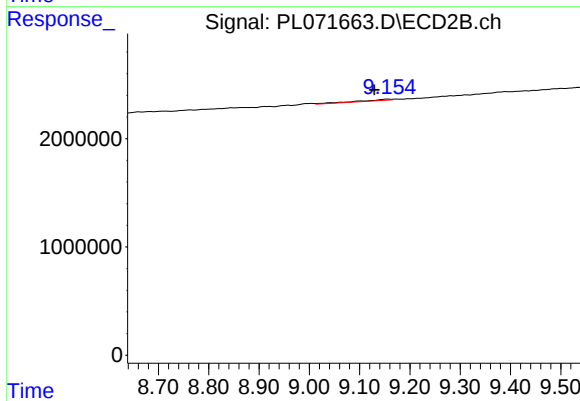

#15 Endosulfan II

R.T.: 9.156 min
Delta R.T.: 0.027 min
Response: 439145
Conc: 0.30 ng/ml

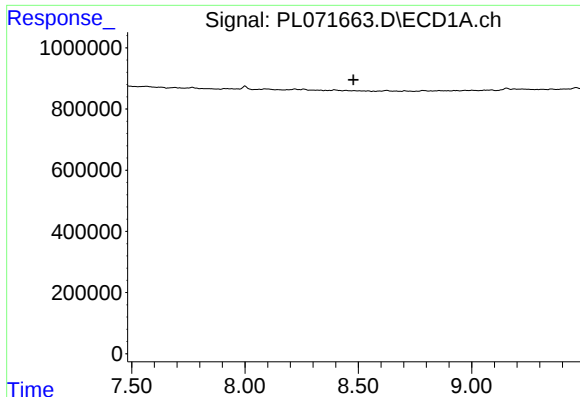

#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

#18 Endrin aldehyde


R.T.: 9.281 min
Delta R.T.: 0.018 min
Response: 94649
Conc: 0.08 ng/ml

#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

#19 Endosulfan Sulfate


R.T.: 9.501 min
Delta R.T.: 0.000 min
Response: 59009
Conc: 0.04 ng/ml

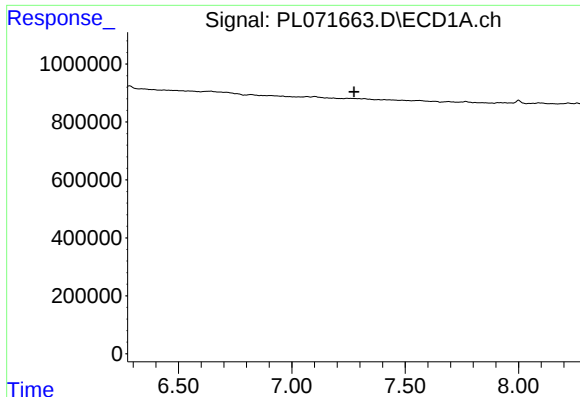

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

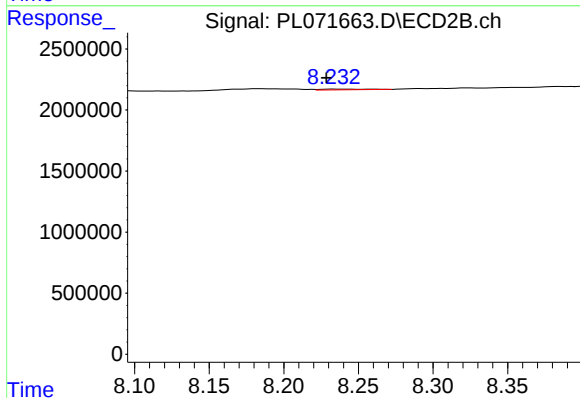


#25 Chlordane-3

R.T.: 8.233 min
Delta R.T.: 0.005 min
Response: 140447
Conc: 0.51 ng/ml

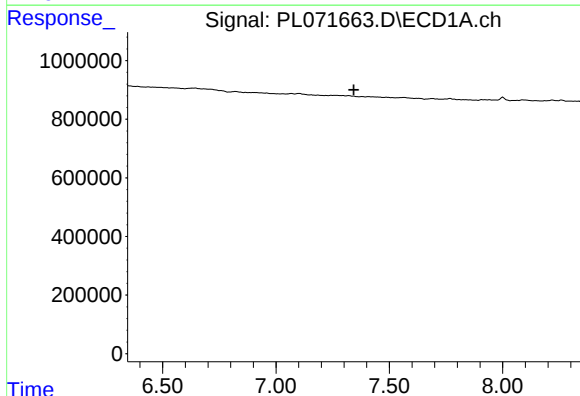


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

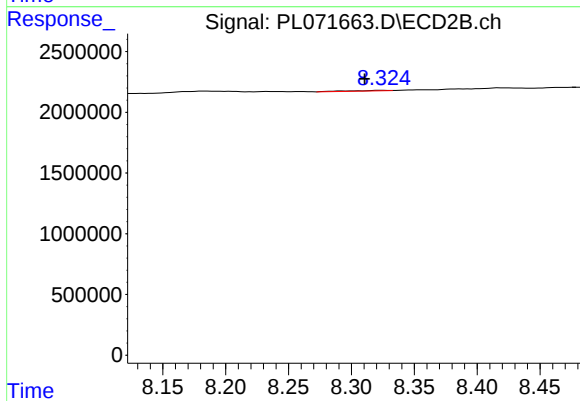

#26 Chlordane-4


R.T.: 8.325 min
Delta R.T.: 0.014 min
Response: 78382
Conc: 0.24 ng/ml

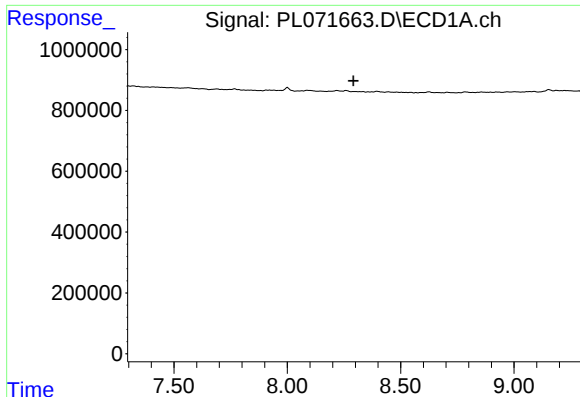

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

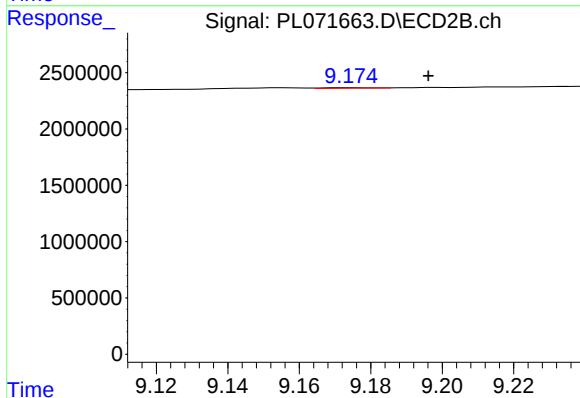


#27 Chlordane-5

R.T.: 9.174 min
Delta R.T.: -0.022 min
Response: 43993
Conc: 0.81 ng/ml

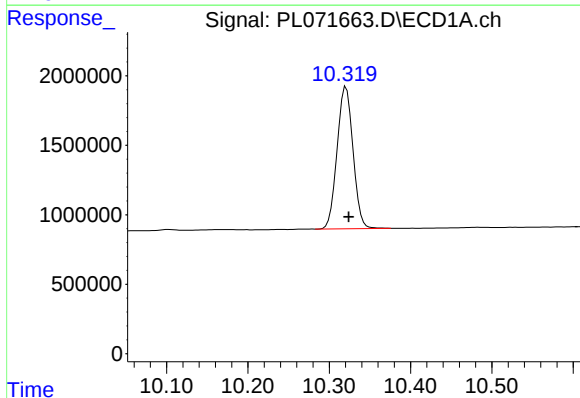

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.003 min
Response: 13921817
Conc: 18.70 ng/ml

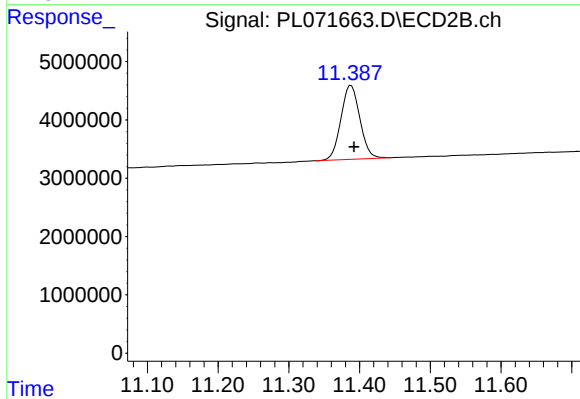

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 23722831
Conc: 18.93 ng/ml