

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 21:55
 Operator : AR\AJ
 Sample : PB141704BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB141704BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:42:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.497	10804586	27728176	16.653	16.249
28)	SA Decachlor...	10.322	11.388	15135347	23848469	20.330	19.029
Target Compounds							
5)	MB Aldrin	0.000	7.487	0	35656	N.D.	0.016 #
7)	B delta-BHC	0.000	7.021f	0	969536	N.D.	0.460 #
9)	A Endosulfan I	0.000	8.365	0	74779	N.D.	0.044 #
10)	B gamma-Chl...	0.000	8.236	0	210033	N.D.	0.108 #
11)	B alpha-Chl...	0.000	8.296	0	36494	N.D.	0.020 #
15)	B Endosulfa...	0.000	9.151f	0	317732	N.D.	0.214 #
24)	Chlordane-2	0.000	7.474	0	44347	N.D.	0.602 #
25)	Chlordane-3	0.000	8.236	0	210033	N.D.	0.760 #
26)	Chlordane-4	0.000	8.296	0	36494	N.D.	0.113 #
27)	Chlordane-5	0.000	9.178f	0	63950	N.D.	1.179 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 21:55
Operator : AR\AJ
Sample : PB141704BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB141704BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:42:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

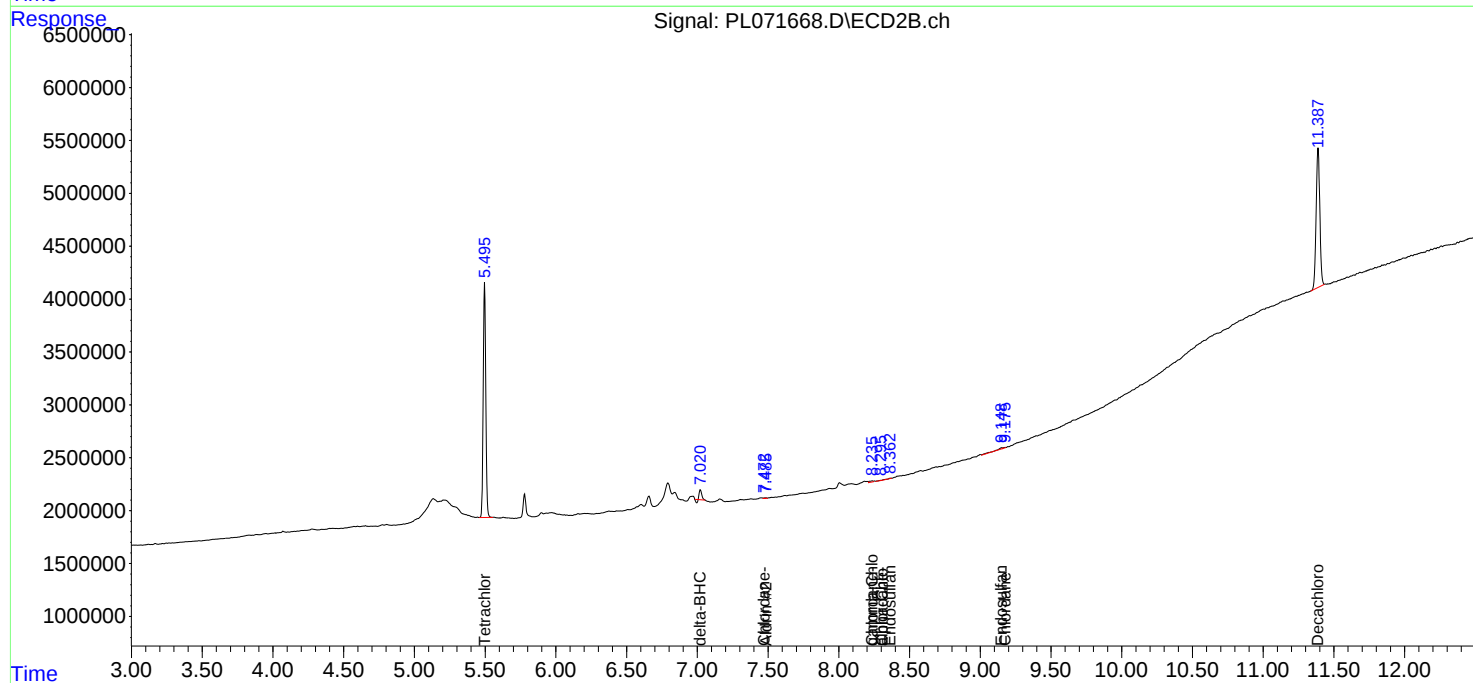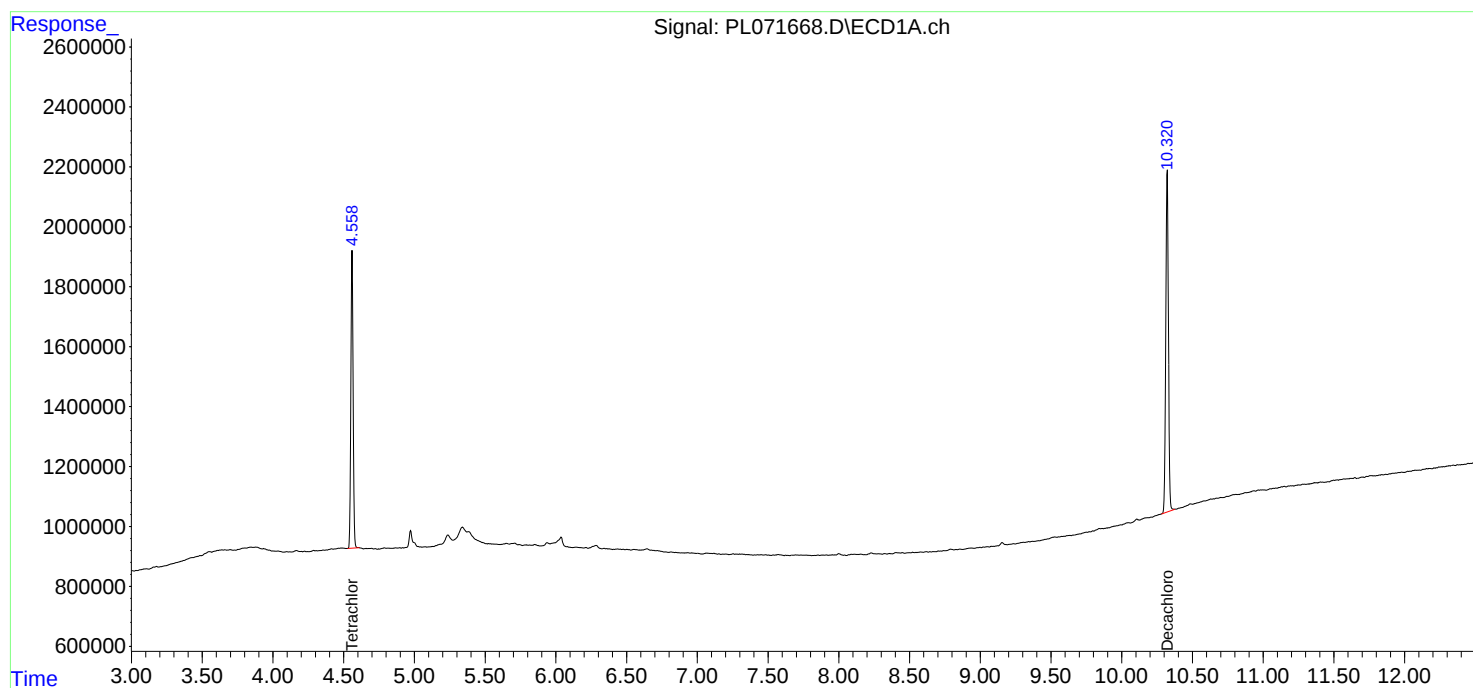


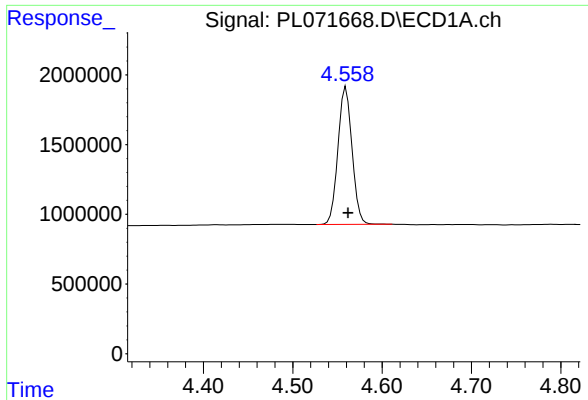

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: -0.002 min
Response: 10804586
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB141704BL

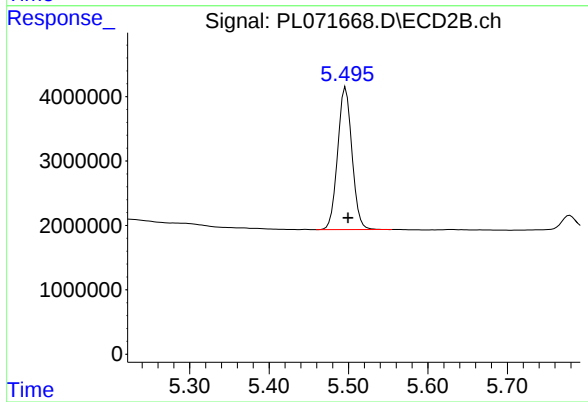


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.003 min
Response: 27728176
Conc: 16.25 ng/ml

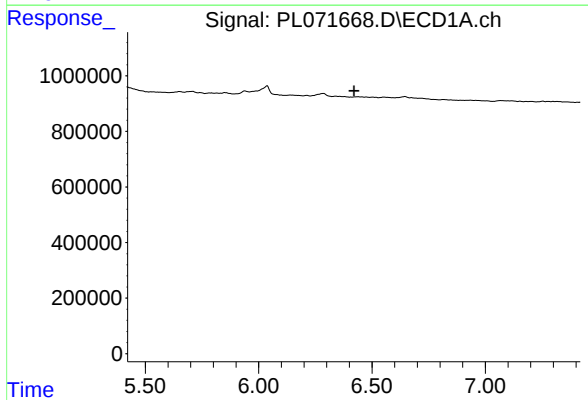


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

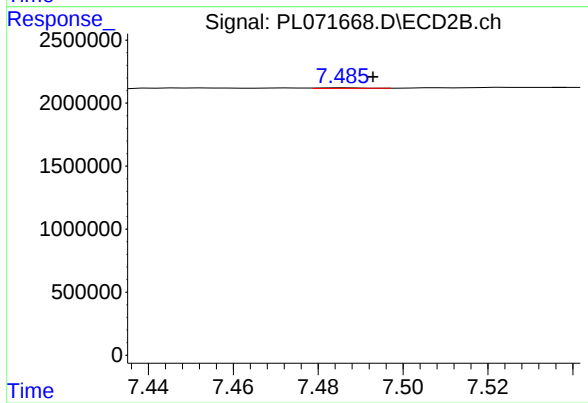

#5 Aldrin


R.T.: 7.487 min
Delta R.T.: -0.006 min
Response: 35656
Conc: 0.02 ng/ml

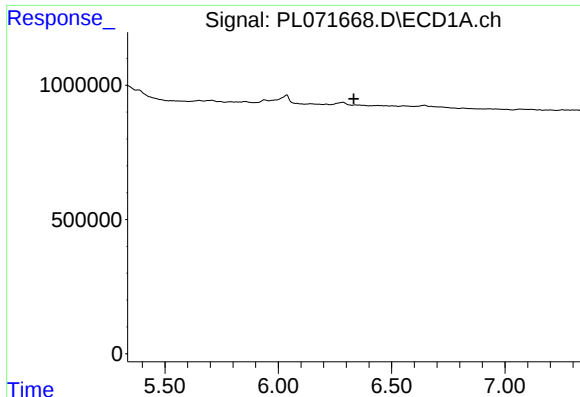

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141704BL

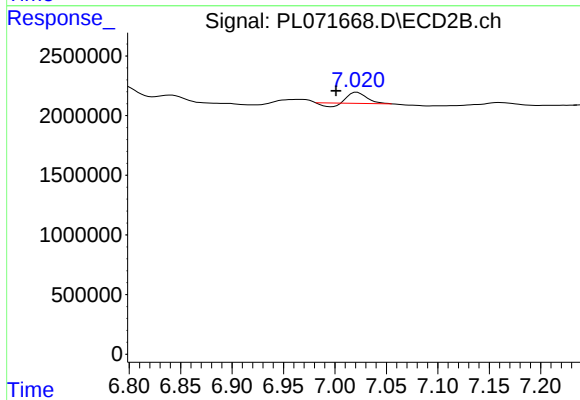


#7 delta-BHC

R.T.: 7.021 min
Delta R.T.: 0.020 min
Response: 969536
Conc: 0.46 ng/ml

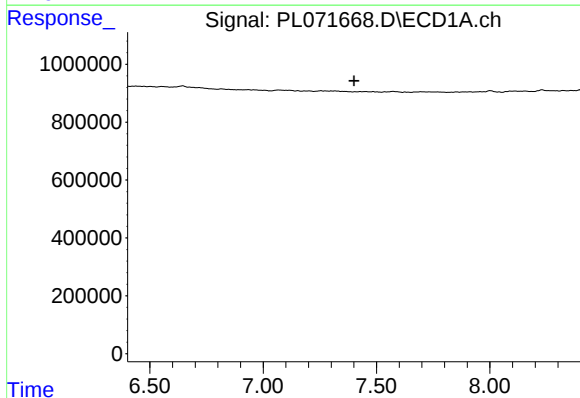


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

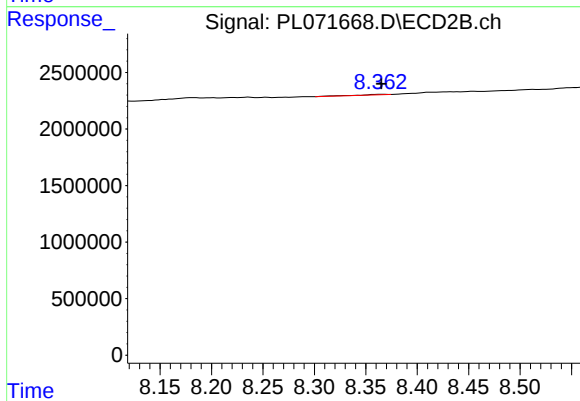

#9 Endosulfan I


R.T.: 8.365 min
Delta R.T.: 0.000 min
Response: 74779
Conc: 0.04 ng/ml

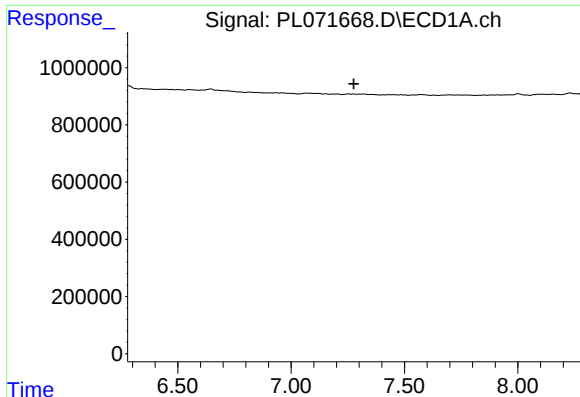

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141704BL

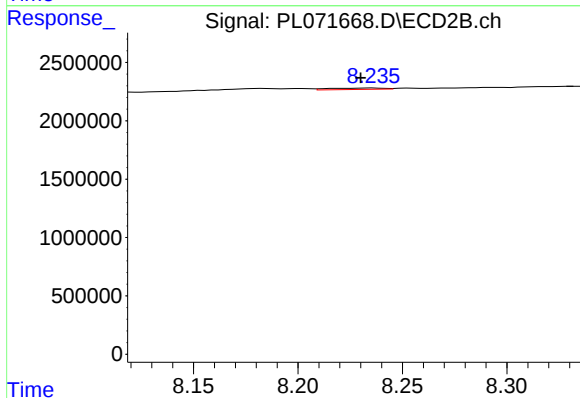


#10 gamma-Chlordane

R.T.: 8.236 min
Delta R.T.: 0.006 min
Response: 210033
Conc: 0.11 ng/ml

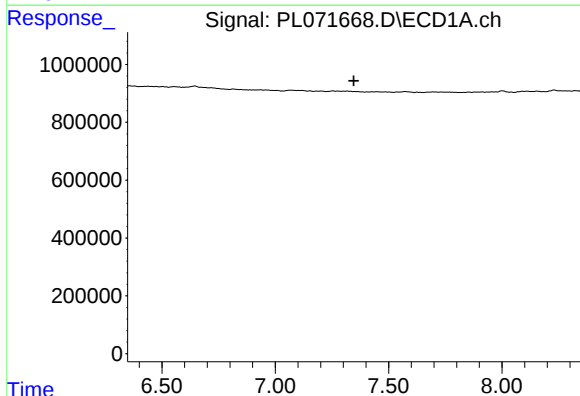


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

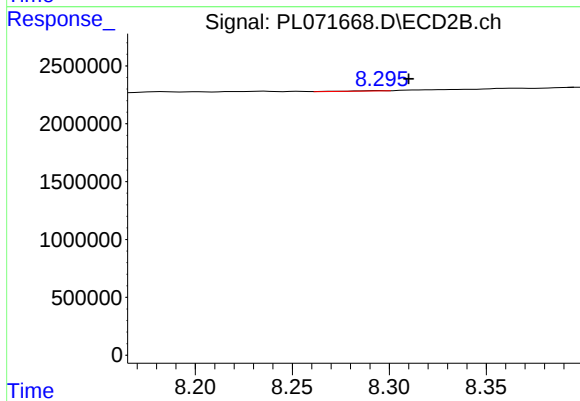

#11 alpha-Chlordane


R.T.: 8.296 min
Delta R.T.: -0.014 min
Response: 36494
Conc: 0.02 ng/ml

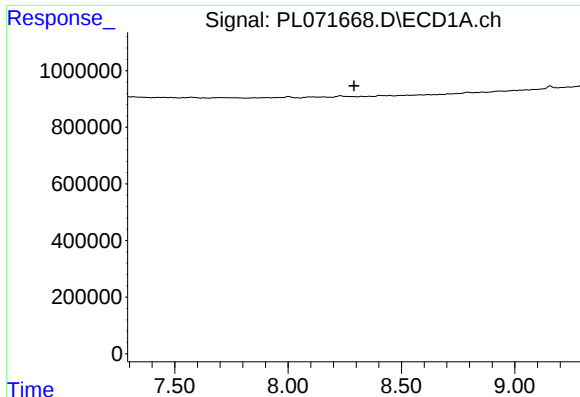

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141704BL

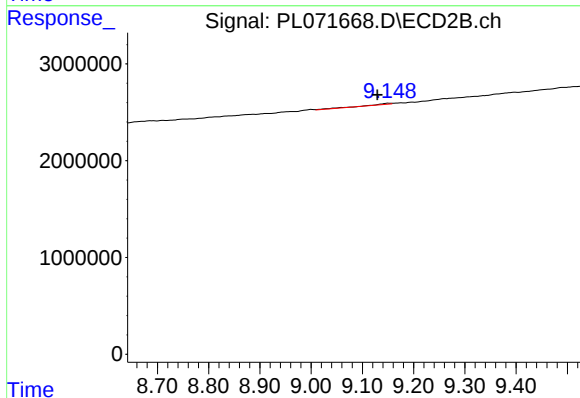


#15 Endosulfan II

R.T.: 9.151 min
Delta R.T.: 0.021 min
Response: 317732
Conc: 0.21 ng/ml

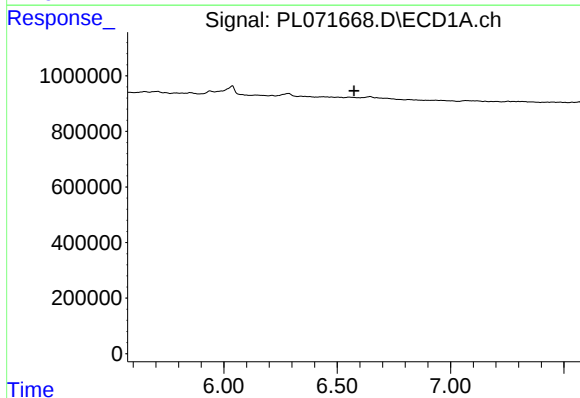


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.575 min
Response: 0
Conc: N.D.

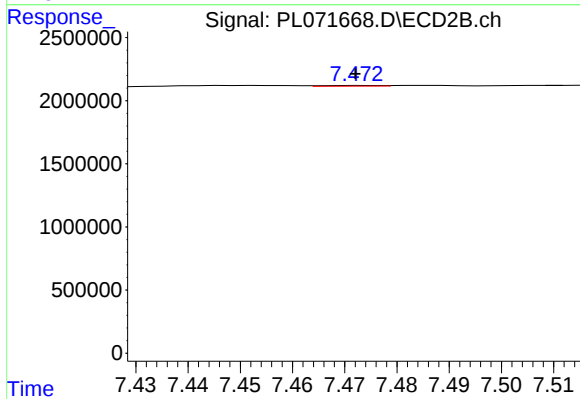

#24 Chlordane-2


R.T.: 7.474 min
Delta R.T.: 0.002 min
Response: 44347
Conc: 0.60 ng/ml

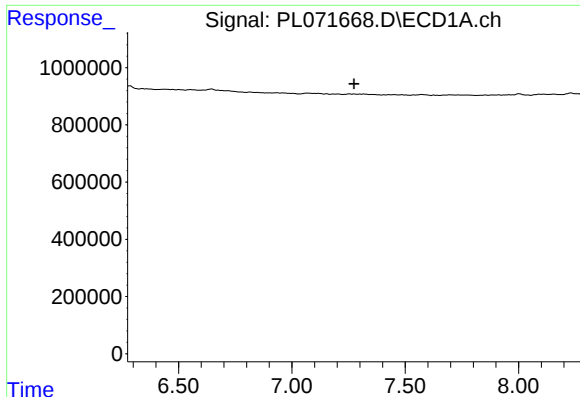

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141704BL

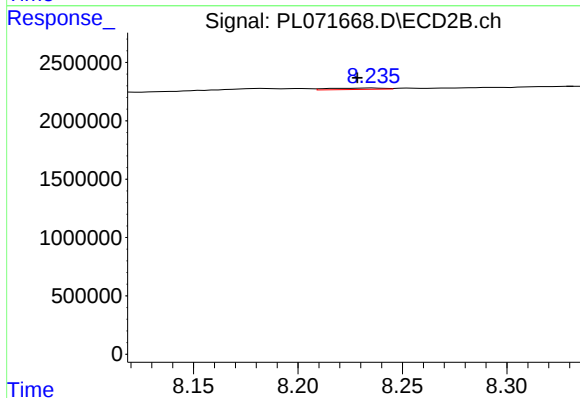


#25 Chlordane-3

R.T.: 8.236 min
Delta R.T.: 0.008 min
Response: 210033
Conc: 0.76 ng/ml

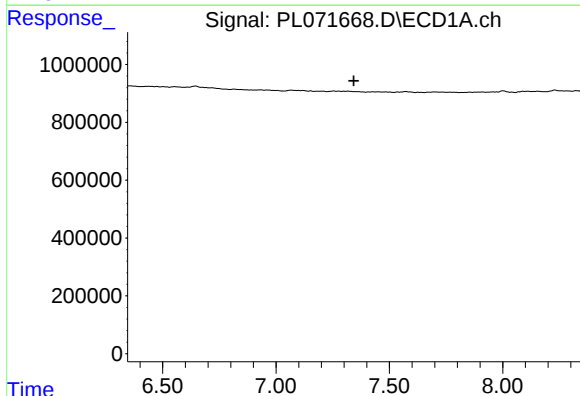


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

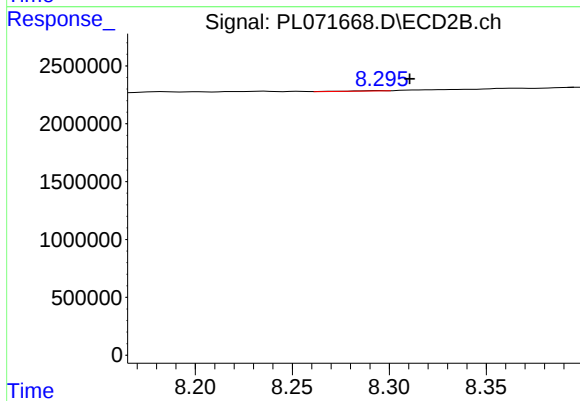

#26 Chlordane-4


R.T.: 8.296 min
Delta R.T.: -0.015 min
Response: 36494
Conc: 0.11 ng/ml

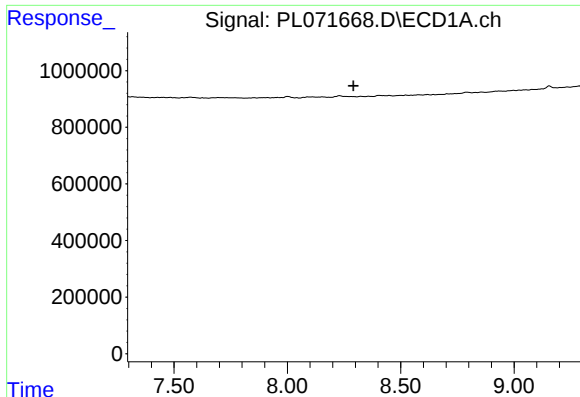

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB141704BL

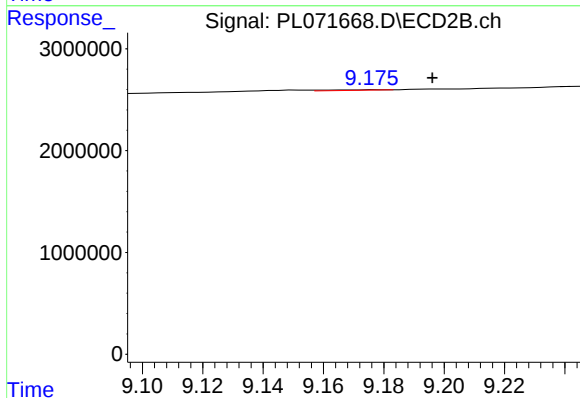


#27 Chlorine-5

R.T.: 9.178 min
Delta R.T.: -0.018 min
Response: 63950
Conc: 1.18 ng/ml

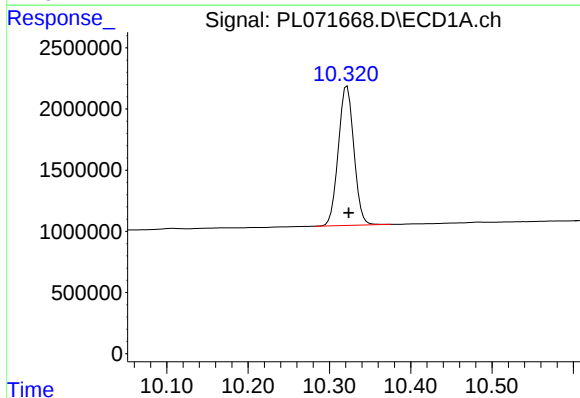

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: -0.002 min
Response: 15135347
Conc: 20.33 ng/ml

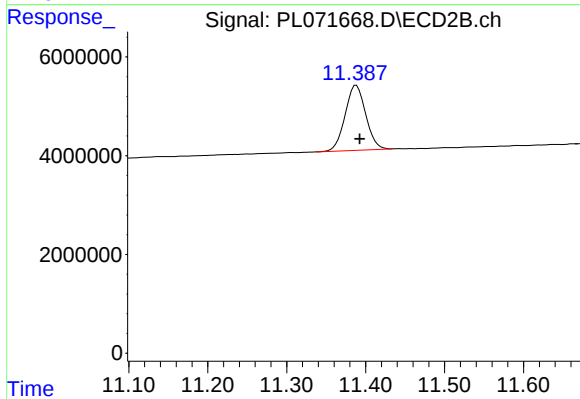

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 23848469
Conc: 19.03 ng/ml