

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 00:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:45:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.497	10762839	27517340	16.589	16.126
28)	SA Decachlor...	10.322	11.389	13228847	20827836	17.770	16.619
Target Compounds							
8)	B Heptachlo...	0.000	7.967	0	1562460	N.D.	0.794 #
9)	A Endosulfan I	0.000	8.375	0	134180	N.D.	0.079 #
10)	B gamma-Chl...	0.000	8.234	0	484118	N.D.	0.248 #
11)	B alpha-Chl...	0.000	8.306	0	165016	N.D.	0.089 #
13)	MA Dieldrin	7.699	0.000	130613	0	0.159	N.D. #
14)	MA Endrin	8.002f	0.000	396662	0	0.533	N.D. #
24)	Chlordane-2	0.000	7.461	0	138168	N.D.	1.875 #
25)	Chlordane-3	0.000	8.234	0	484118	N.D.	1.752 #
26)	Chlordane-4	0.000	8.306	0	165016	N.D.	0.509 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 00:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:45:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

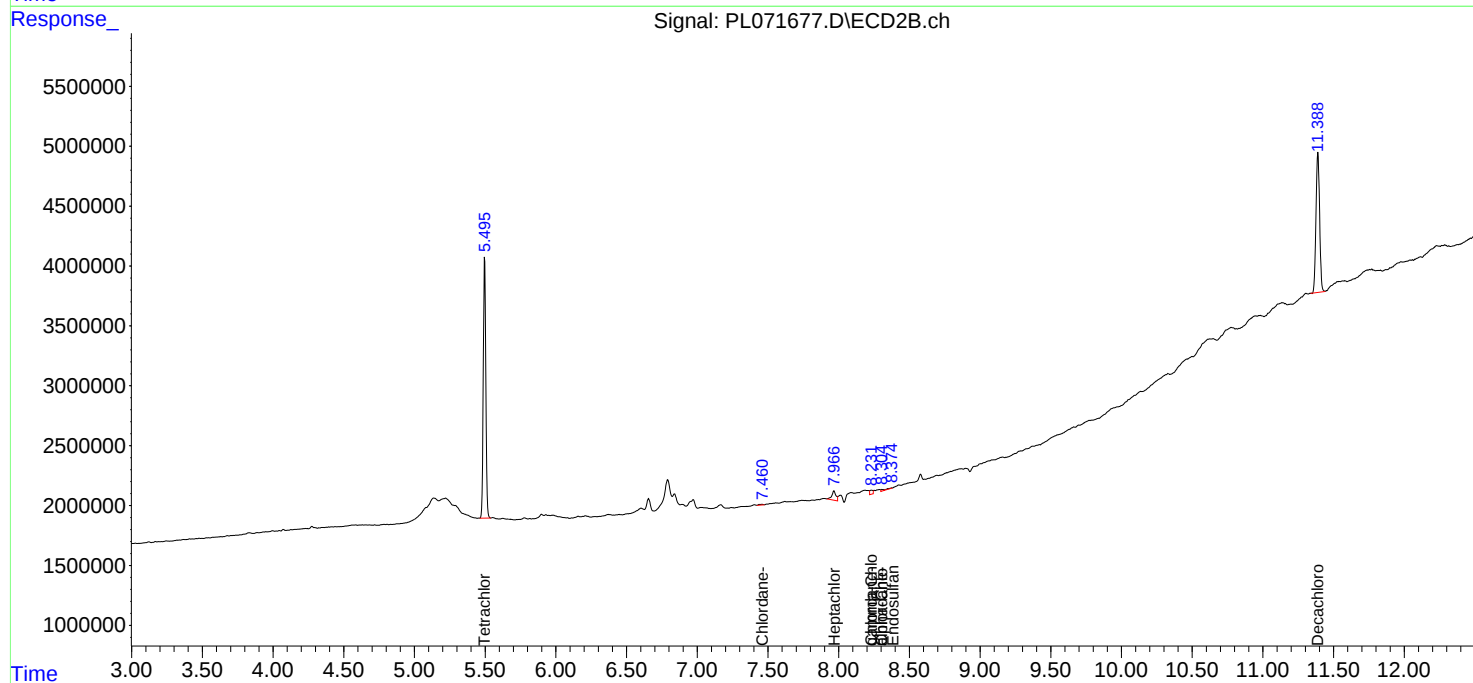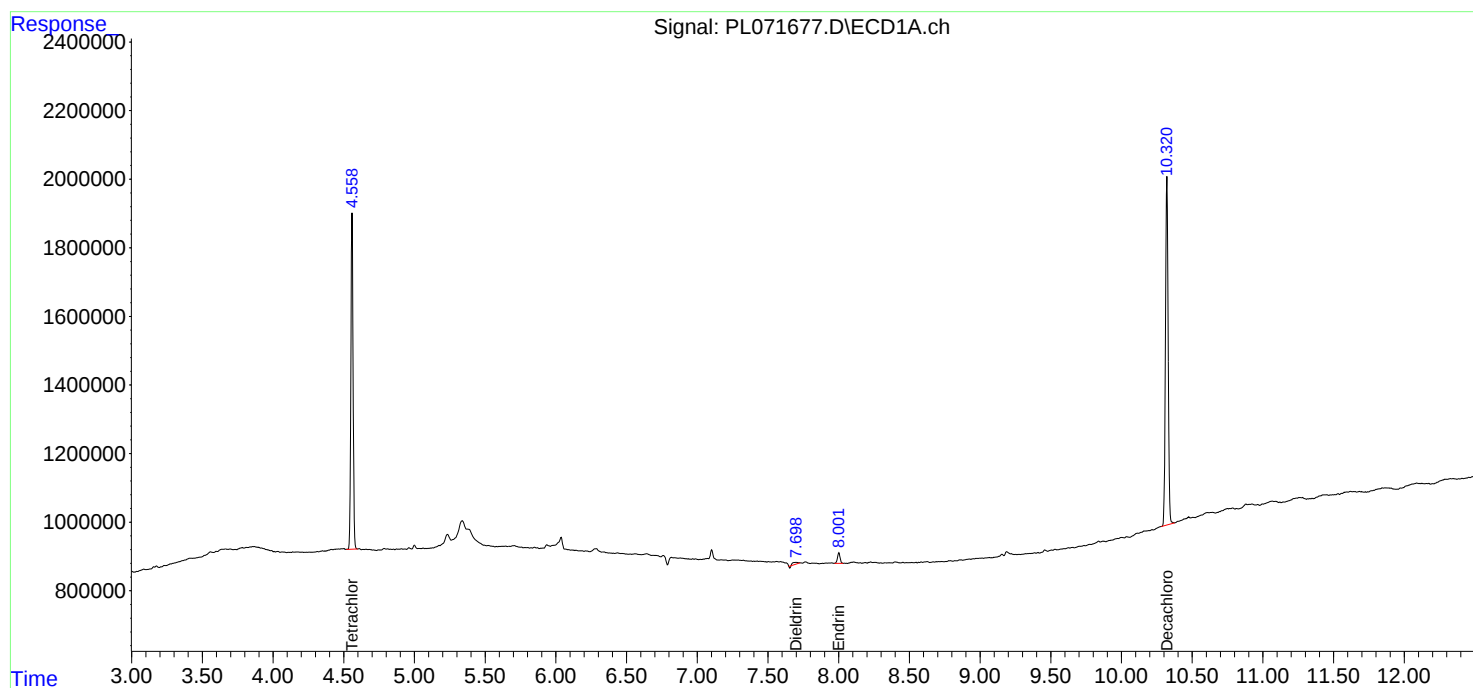


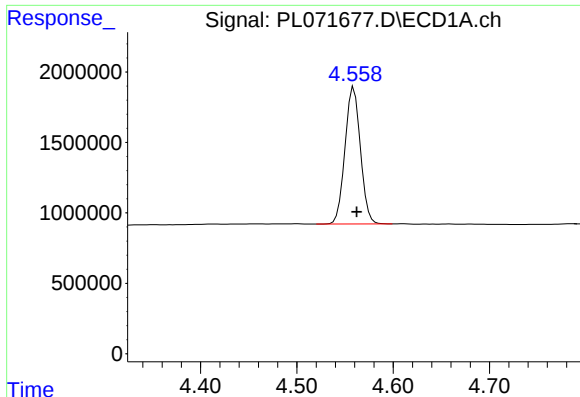

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 10762839
Conc: 16.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

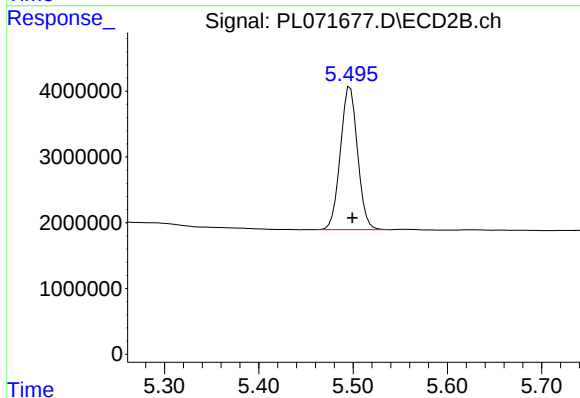


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 27517340
Conc: 16.13 ng/ml

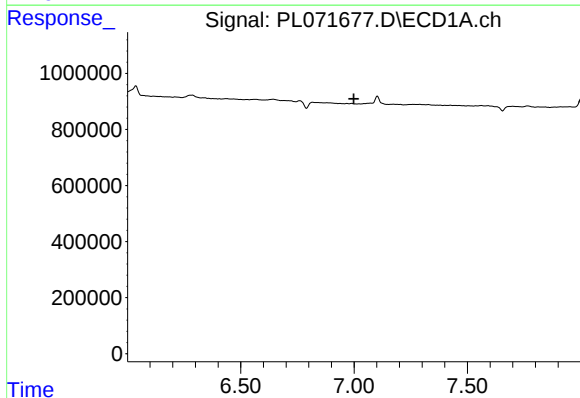


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

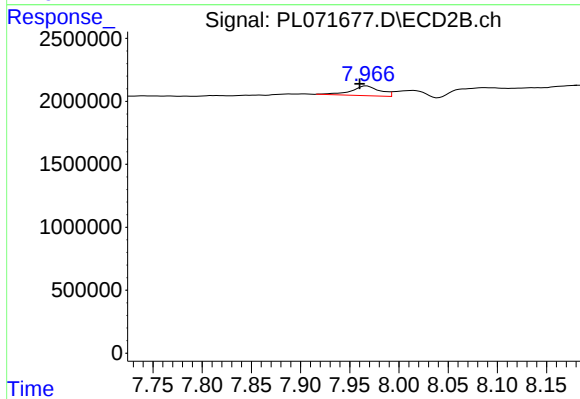

#8 Heptachlor epoxide


R.T.: 7.967 min
Delta R.T.: 0.007 min
Response: 1562460
Conc: 0.79 ng/ml

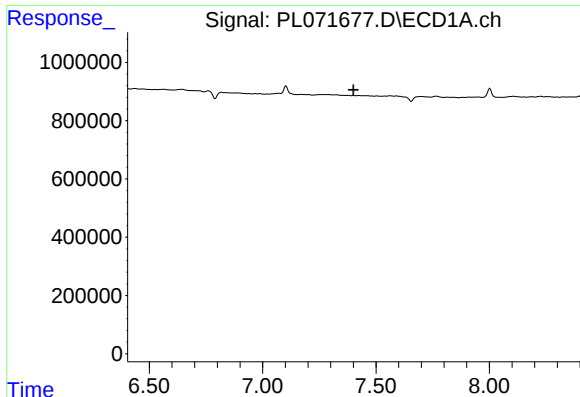

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

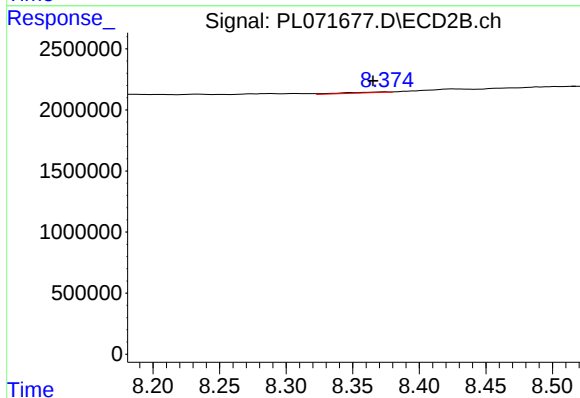


#9 Endosulfan I

R.T.: 8.375 min
Delta R.T.: 0.010 min
Response: 134180
Conc: 0.08 ng/ml

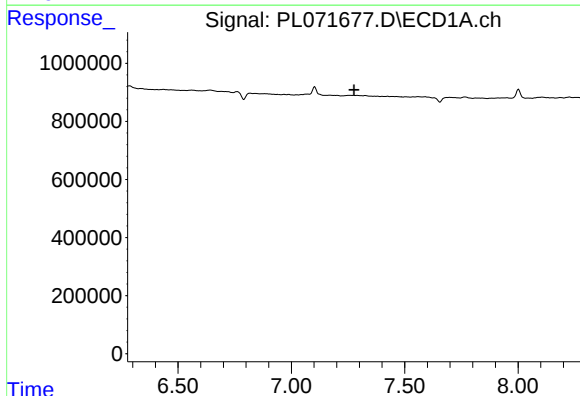


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

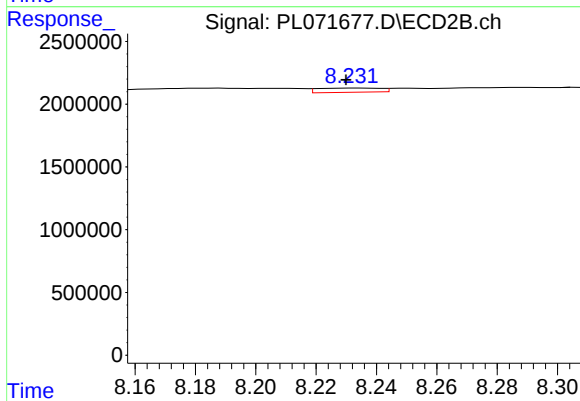

#10 gamma-Chlordane


R.T.: 8.234 min
Delta R.T.: 0.004 min
Response: 484118
Conc: 0.25 ng/ml

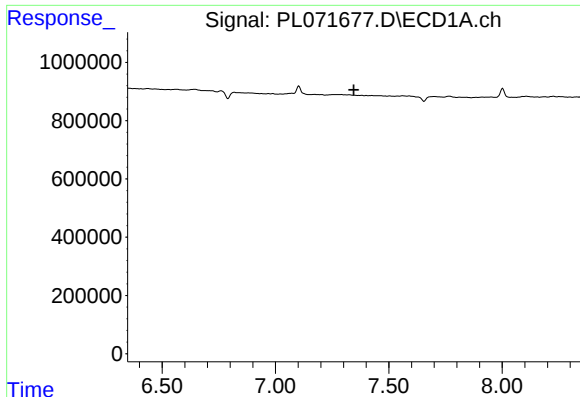

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

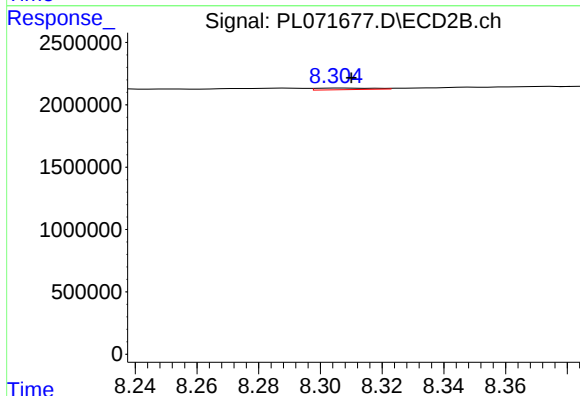


#11 alpha-Chlordane

R.T.: 8.306 min
Delta R.T.: -0.004 min
Response: 165016
Conc: 0.09 ng/ml

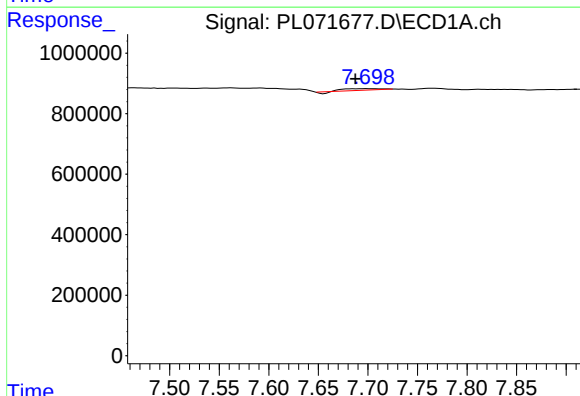


#13 Dieldrin

R.T.: 7.699 min
Delta R.T.: 0.012 min
Response: 130613
Conc: 0.16 ng/ml

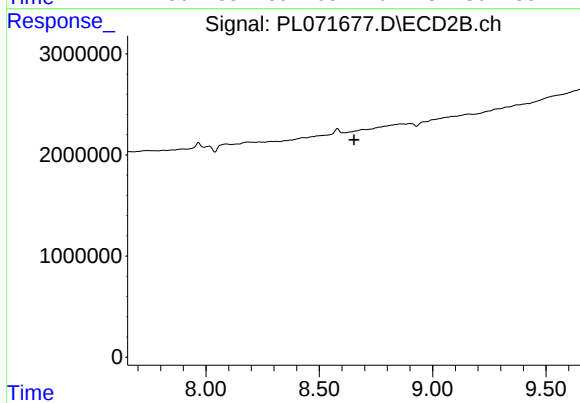

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.654 min
Response: 0
Conc: N.D.

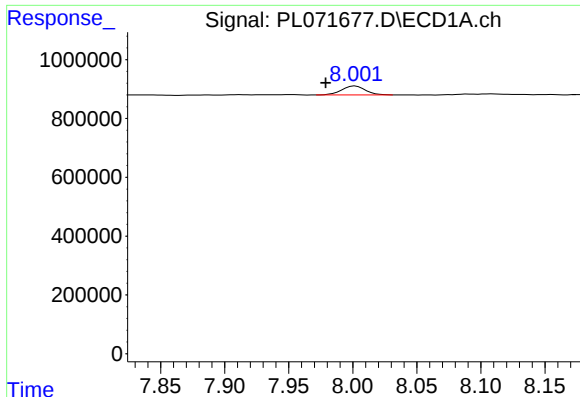

#14 Endrin


R.T.: 8.002 min
Delta R.T.: 0.023 min
Response: 396662
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

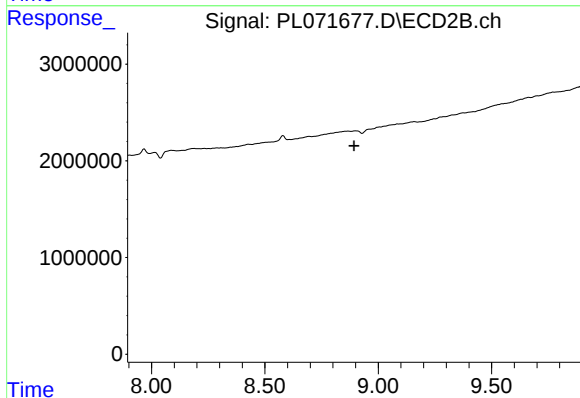


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

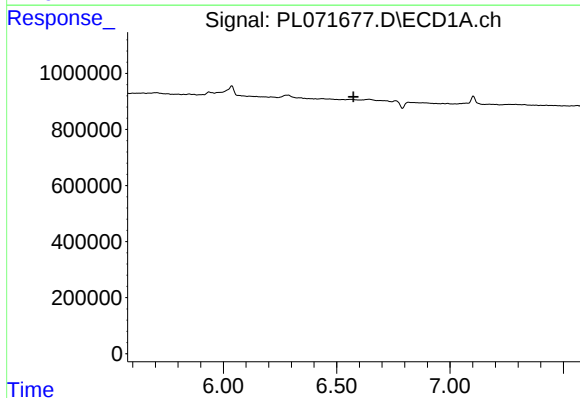


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.575 min
Response: 0
Conc: N.D.

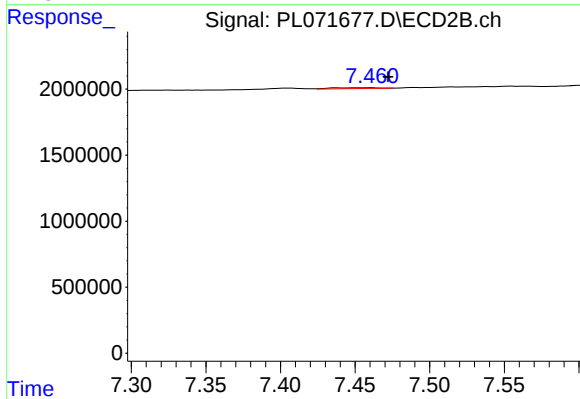

#24 Chlordane-2


R.T.: 7.461 min
Delta R.T.: -0.011 min
Response: 138168
Conc: 1.88 ng/ml

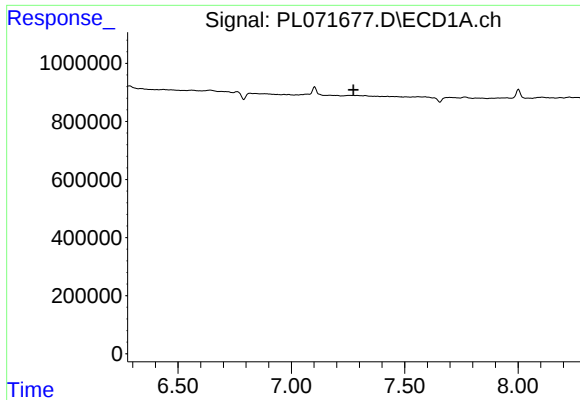

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

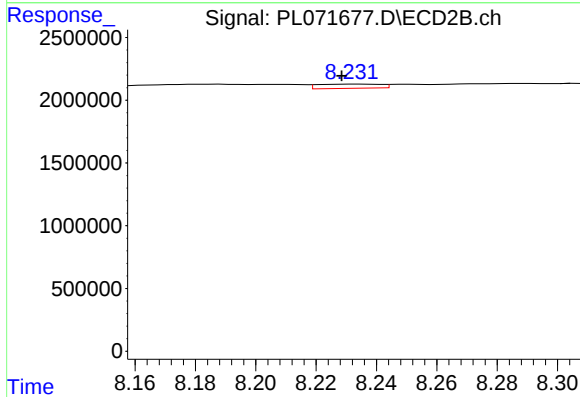


#25 Chlordane-3

R.T.: 8.234 min
Delta R.T.: 0.005 min
Response: 484118
Conc: 1.75 ng/ml

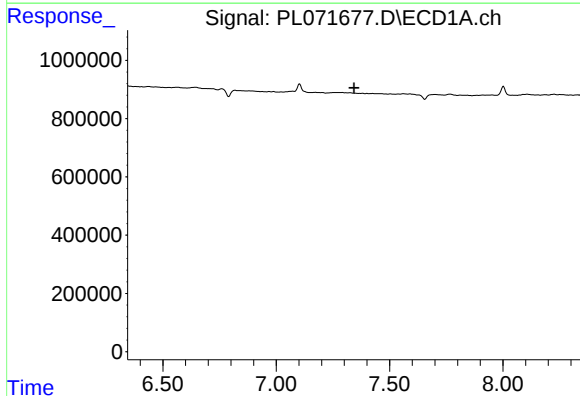


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

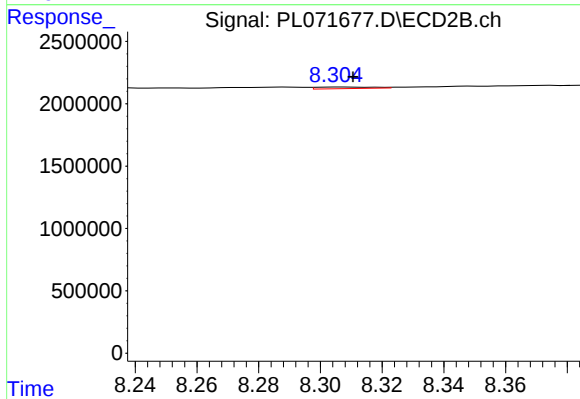

#26 Chlordane-4


R.T.: 8.306 min
Delta R.T.: -0.004 min
Response: 165016
Conc: 0.51 ng/ml

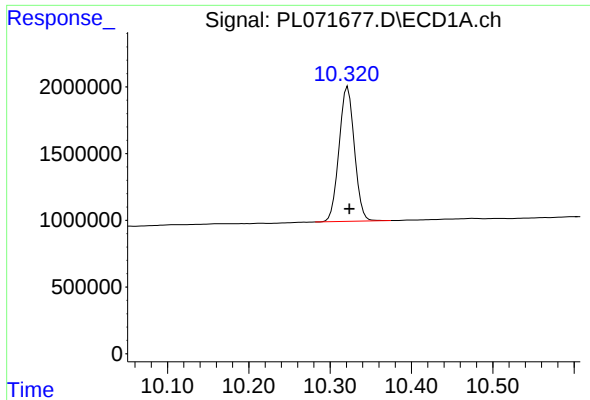

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: -0.002 min
Response: 13228847
Conc: 17.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

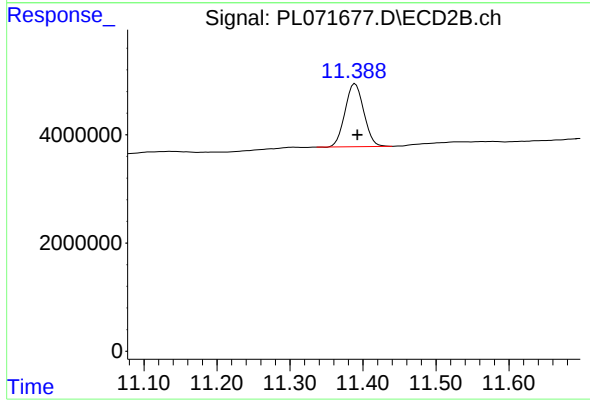

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.003 min
Response: 20827836
Conc: 16.62 ng/ml