

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 04:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 05:53:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.497	10547533	27150718	16.257	15.911
28)	SA Decachlor...	10.322	11.389	13775161	21876150	18.503	17.455
Target Compounds							
5)	MB Aldrin	0.000	7.470f	0	11767	N.D.	0.005 #
8)	B Heptachlo...	0.000	7.967	0	1152378	N.D.	0.586 #
9)	A Endosulfan I	0.000	8.366	0	42855	N.D.	0.025 #
10)	B gamma-Chl...	0.000	8.226	0	594773	N.D.	0.305 #
14)	MA Endrin	8.003f	0.000	318678	0	0.428	N.D. #
19)	B Endosulfa...	0.000	9.505	0	191627	N.D.	0.136 #
24)	Chlordane-2	0.000	7.470	0	11767	N.D.	0.160 #
25)	Chlordane-3	0.000	8.226	0	594773	N.D.	2.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 04:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 05:53:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

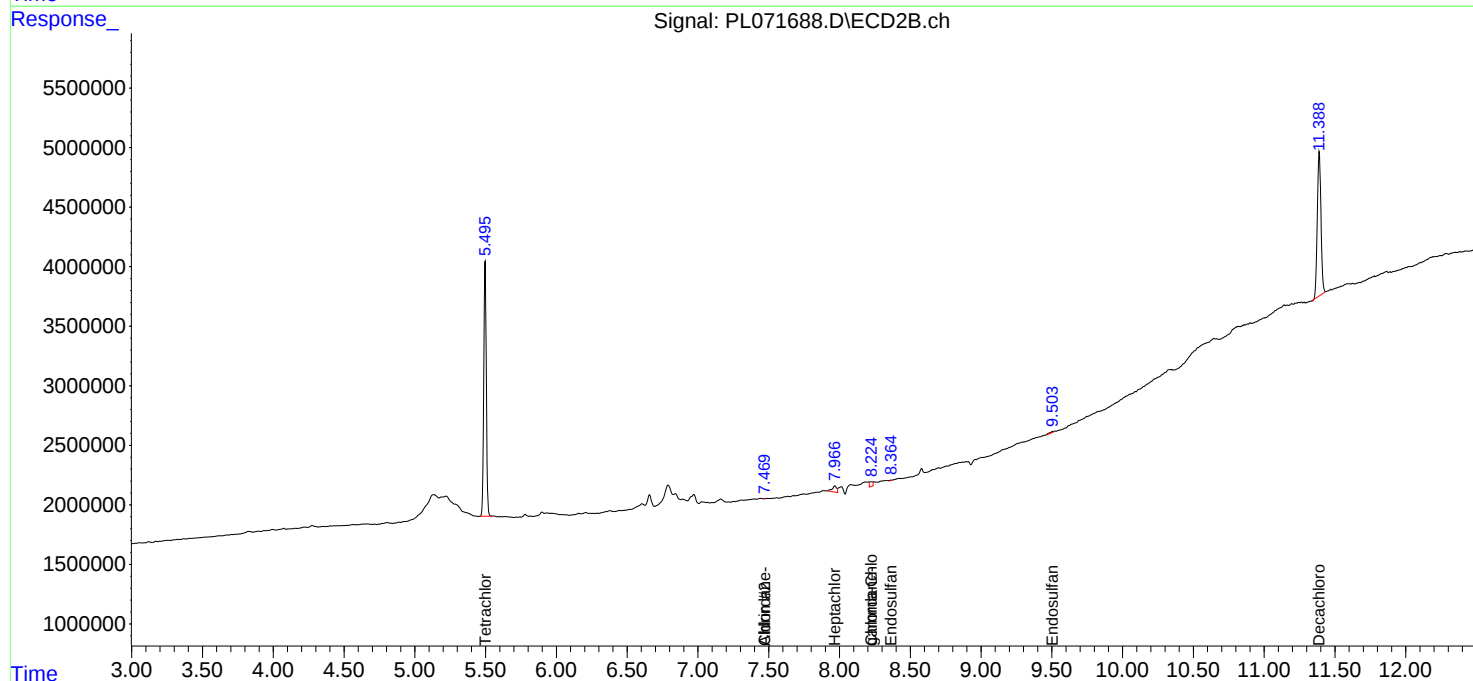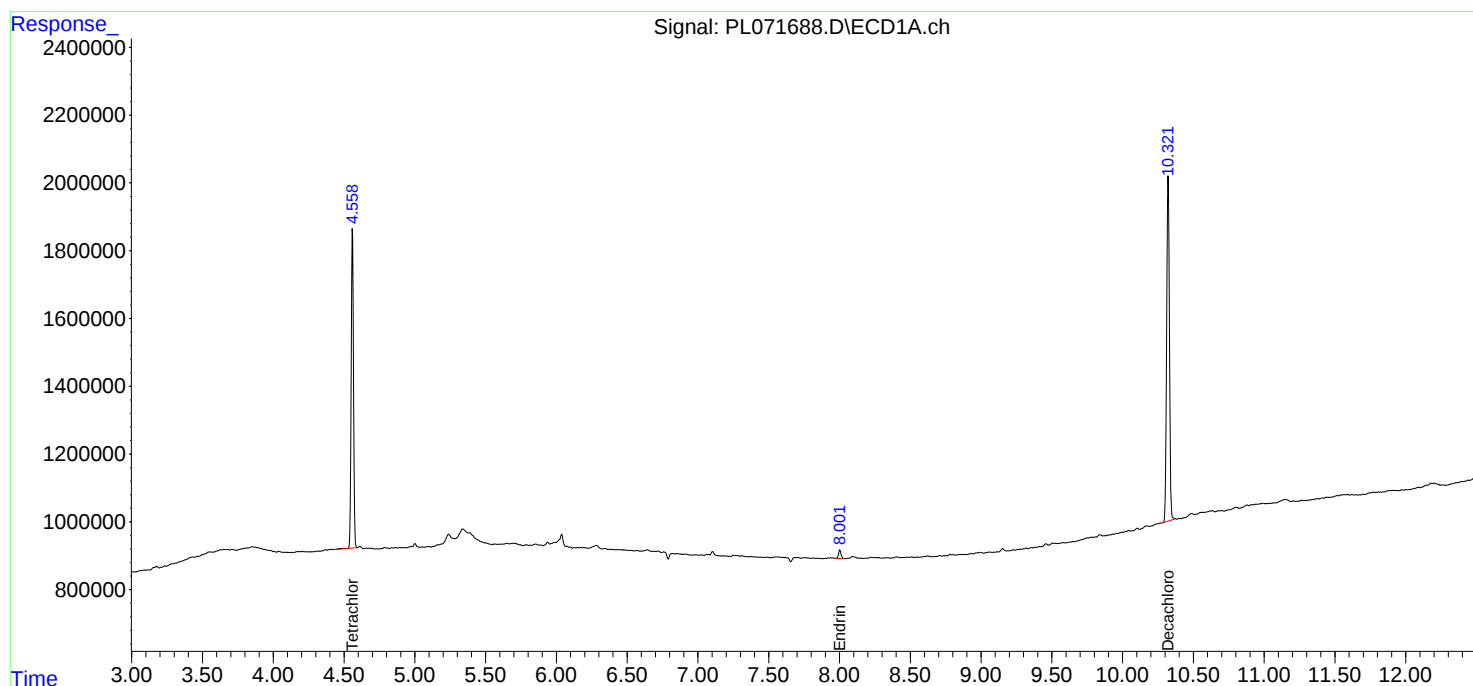


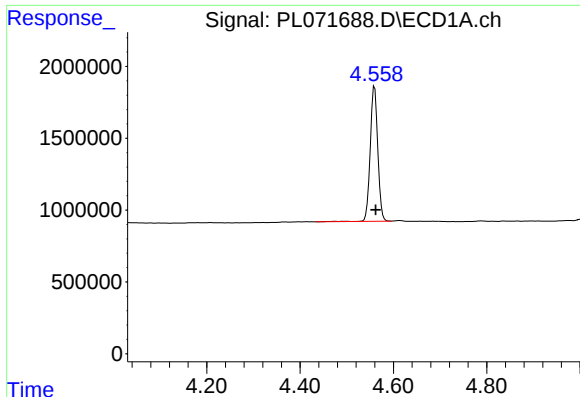

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: -0.002 min
Response: 10547533
Conc: 16.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

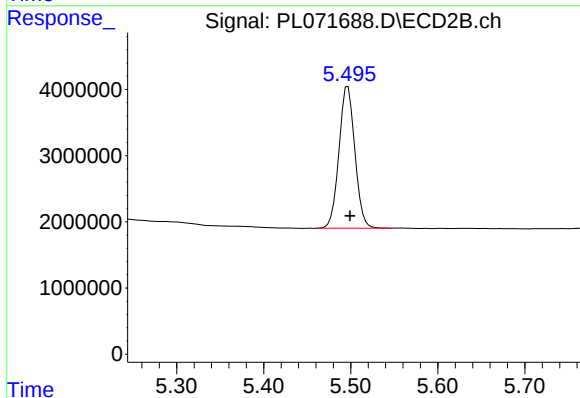


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 27150718
Conc: 15.91 ng/ml

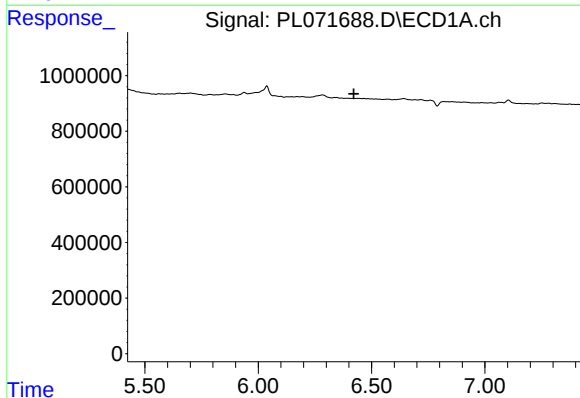


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

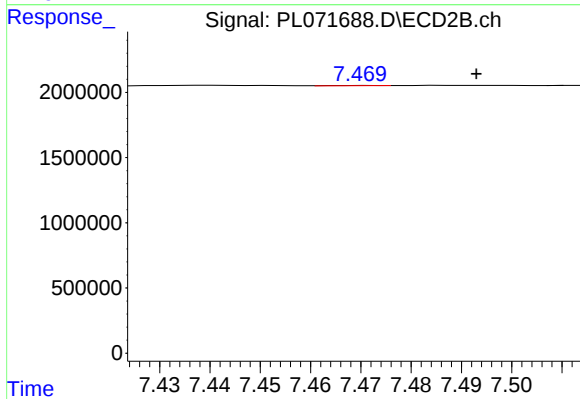

#5 Aldrin


R.T.: 7.470 min
Delta R.T.: -0.023 min
Response: 11767
Conc: 0.01 ng/ml

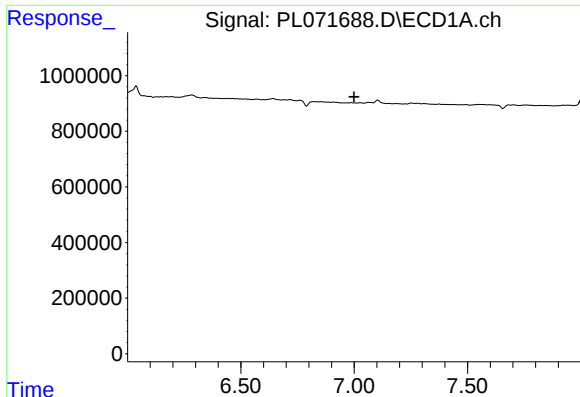

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

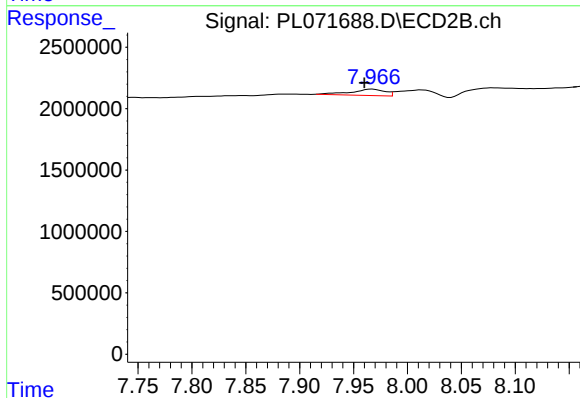


#8 Heptachlor epoxide

R.T.: 7.967 min
Delta R.T.: 0.007 min
Response: 1152378
Conc: 0.59 ng/ml

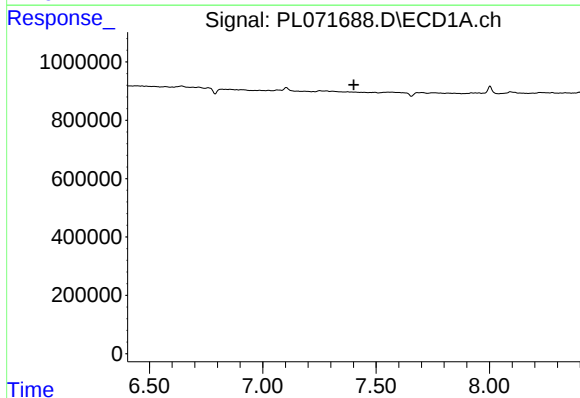


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

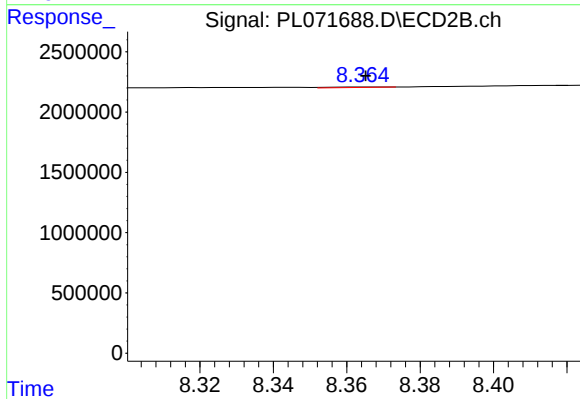

#9 Endosulfan I


R.T.: 8.366 min
Delta R.T.: 0.001 min
Response: 42855
Conc: 0.03 ng/ml

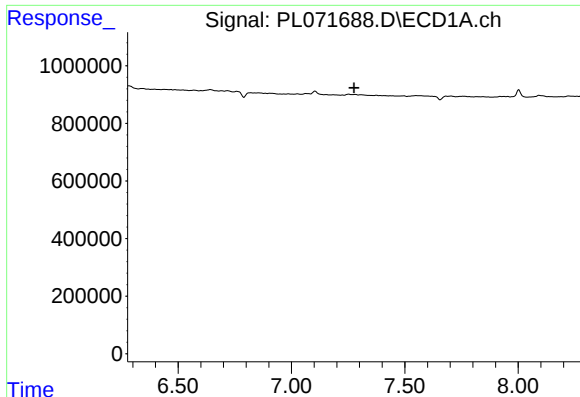

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

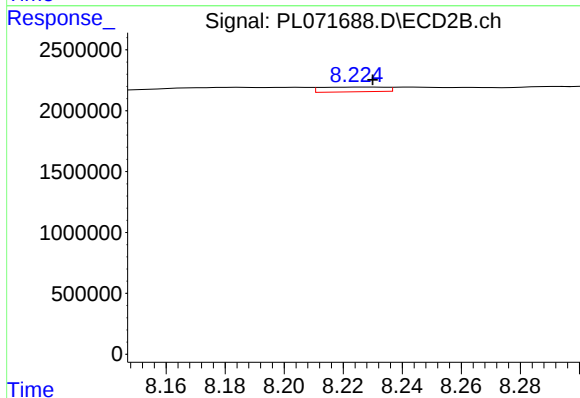


#10 gamma-Chlordane

R.T.: 8.226 min
Delta R.T.: -0.004 min
Response: 594773
Conc: 0.30 ng/ml

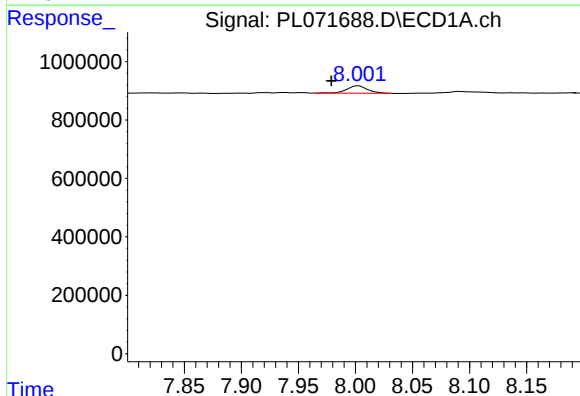


#14 Endrin

R.T.: 8.003 min
Delta R.T.: 0.024 min
Response: 318678
Conc: 0.43 ng/ml

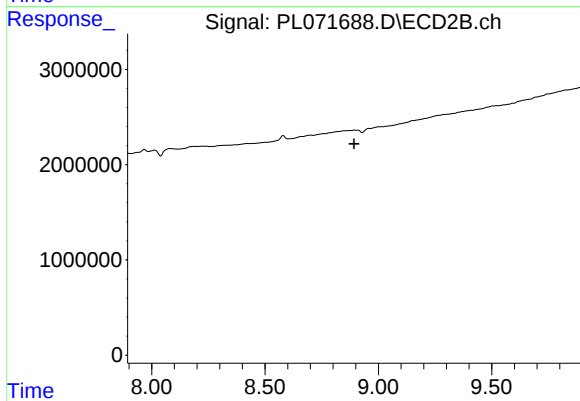

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

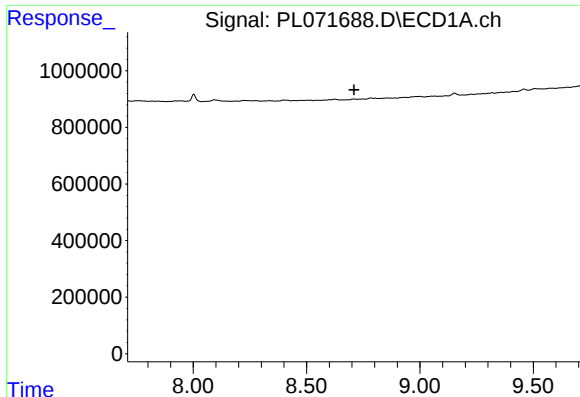

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

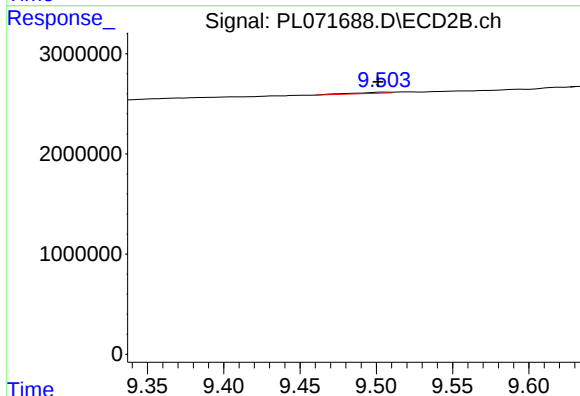


#19 Endosulfan Sulfate

R.T.: 9.505 min
Delta R.T.: 0.003 min
Response: 191627
Conc: 0.14 ng/ml

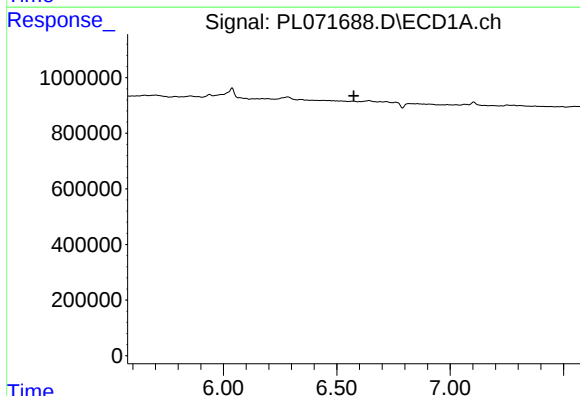


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

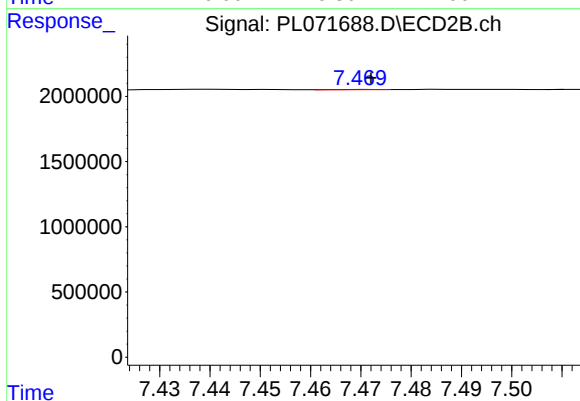

#24 Chlordane-2


R.T.: 7.470 min
Delta R.T.: -0.002 min
Response: 11767
Conc: 0.16 ng/ml

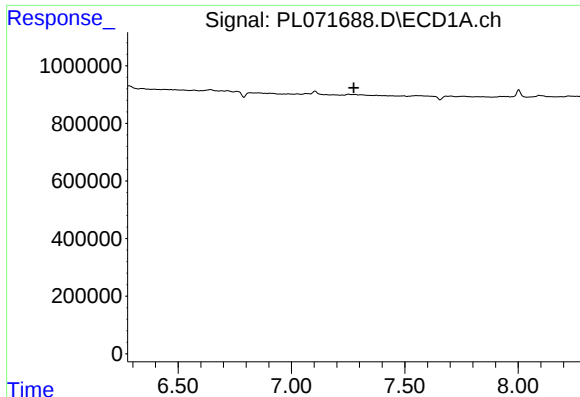

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

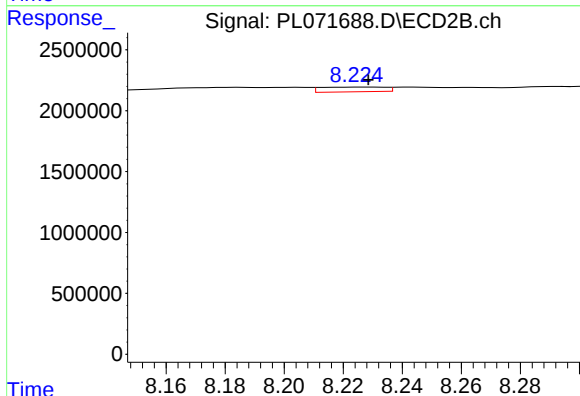


#25 Chlordane-3

R.T.: 8.226 min
Delta R.T.: -0.002 min
Response: 594773
Conc: 2.15 ng/ml

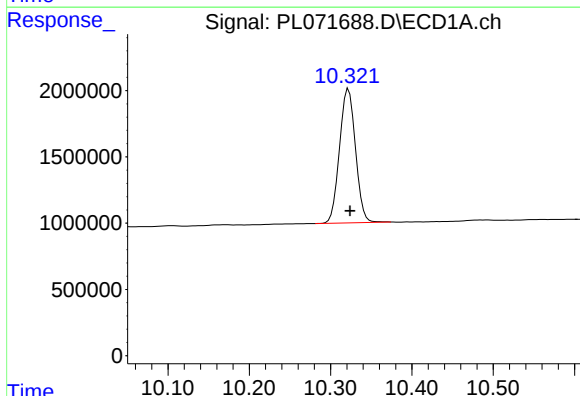

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: -0.002 min
Response: 13775161
Conc: 18.50 ng/ml

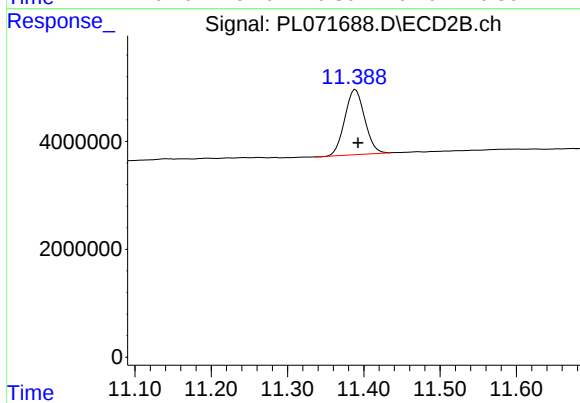

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.003 min
Response: 21876150
Conc: 17.45 ng/ml