

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 12:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 13:46:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 13:44:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	5.498	51444089	130.2E6	76.737	77.173
28)	SA Decachlor...	10.323	11.391	53573856	92148330	71.545	72.808
Target Compounds							
23)	Chlordane-1	5.886	6.880	19163950	53383929	774.300	768.050
24)	Chlordane-2	6.575	7.473	24002253	55567497	753.469	764.687
25)	Chlordane-3	7.275	8.230	68246231	220.0E6	784.551	790.382
26)	Chlordane-4	7.344	8.311	72660206	255.6E6	785.138	785.797
27)	Chlordane-5	8.292	9.198	23872122	41114428	774.319	760.621



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 12:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 13:46:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 13:44:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

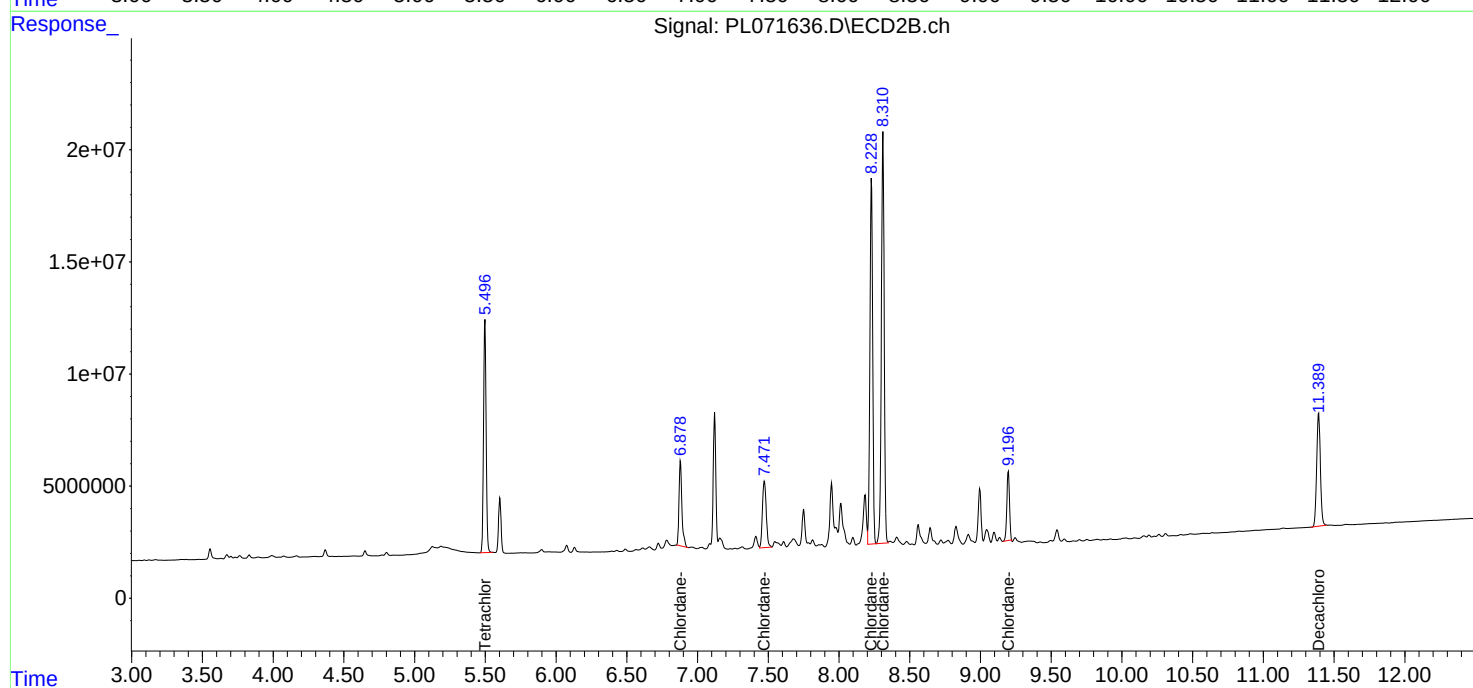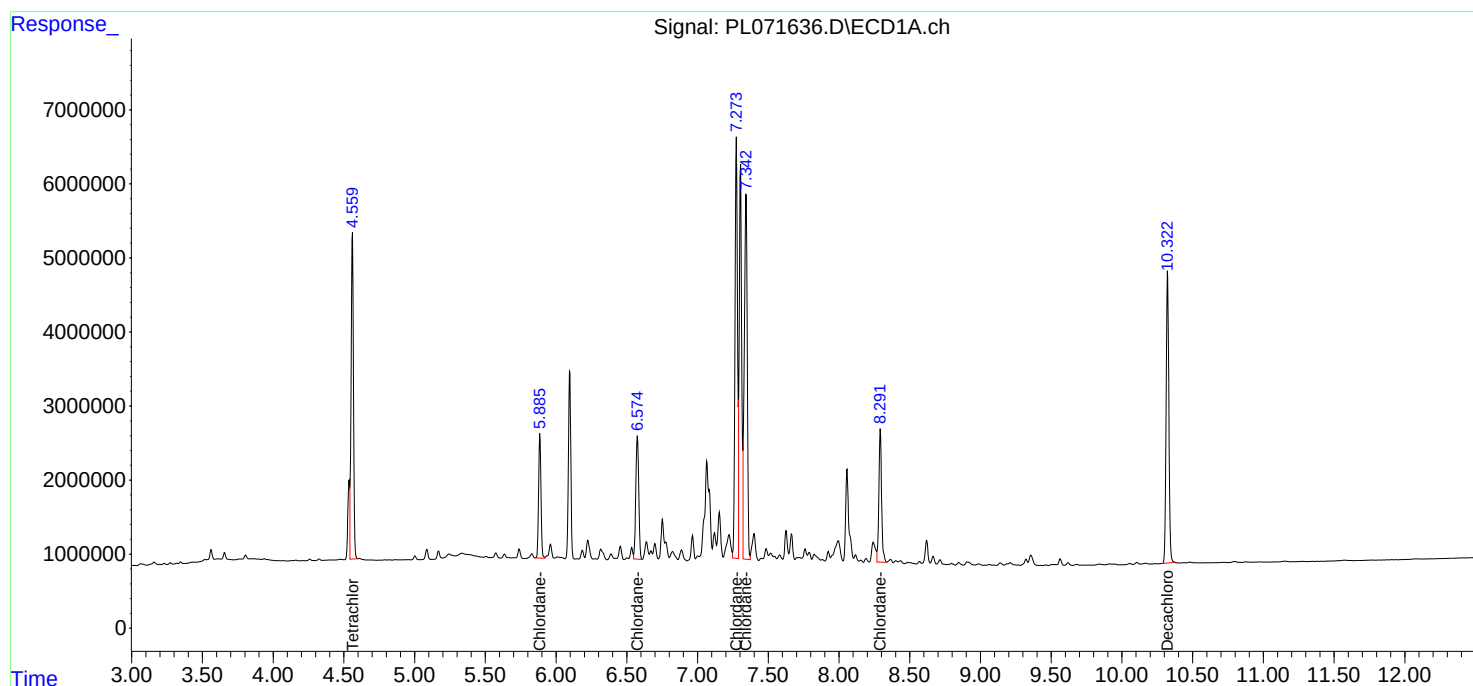


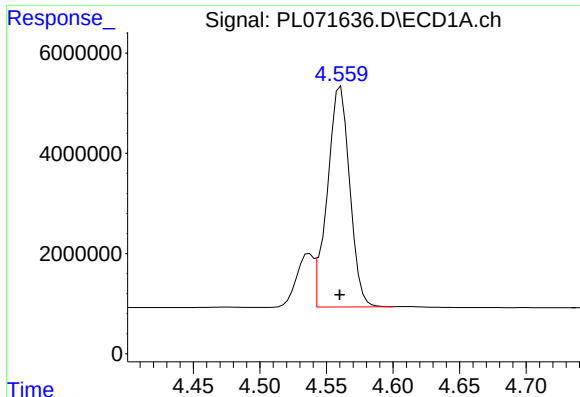

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 51444089
Conc: 76.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

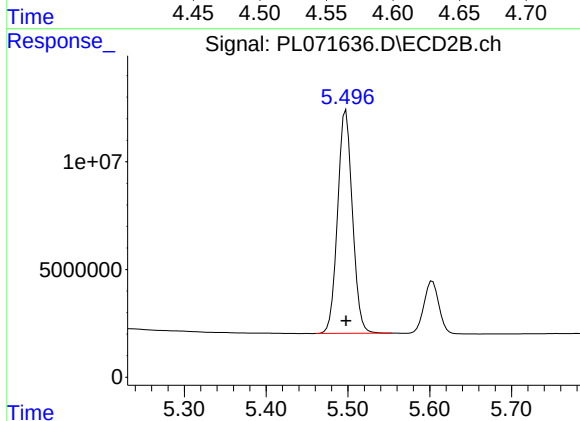


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 130169272
Conc: 77.17 ng/ml

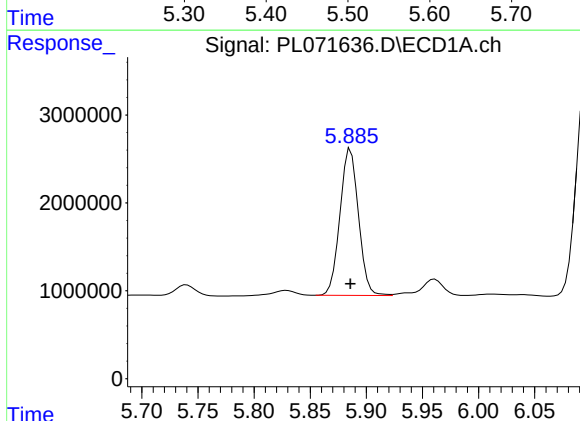


#23 Chlordane-1

R.T.: 5.886 min
Delta R.T.: 0.000 min
Response: 19163950
Conc: 774.30 ng/ml

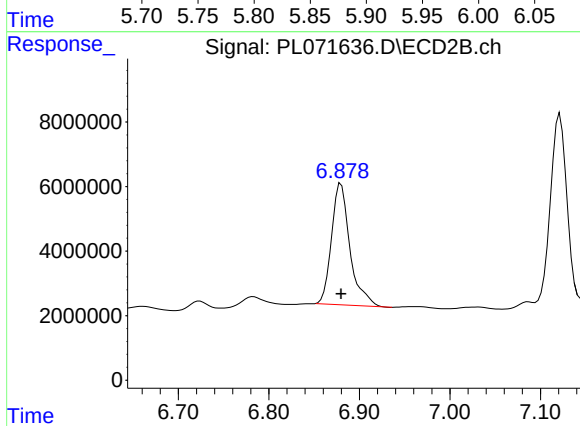

#23 Chlordane-1


R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 53383929
Conc: 768.05 ng/ml

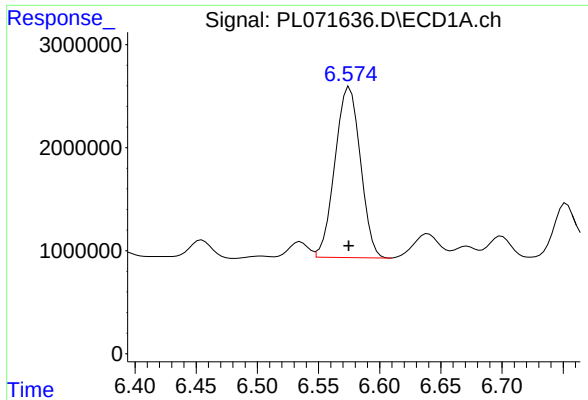

#24 Chlordane-2


R.T.: 6.575 min
Delta R.T.: 0.000 min
Response: 24002253
Conc: 753.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

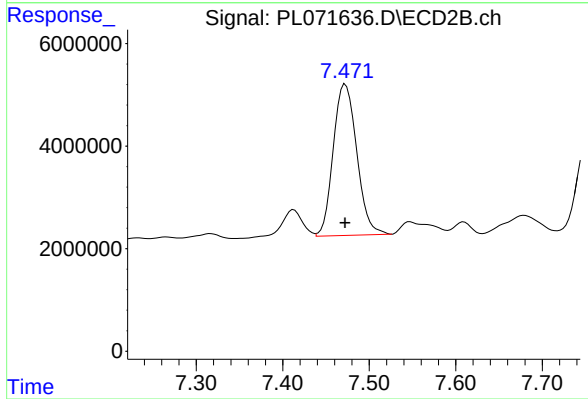


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 55567497
Conc: 764.69 ng/ml

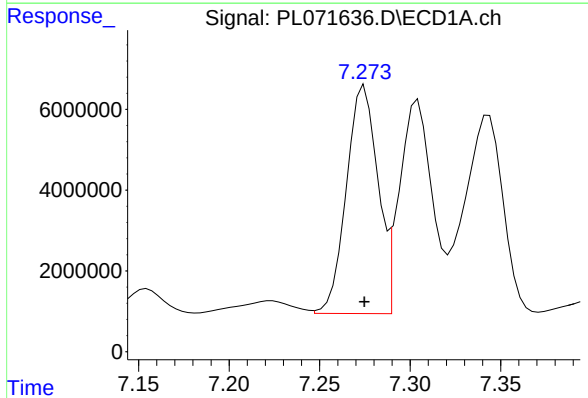


#25 Chlordane-3

R.T.: 7.275 min
Delta R.T.: 0.000 min
Response: 68246231
Conc: 784.55 ng/ml

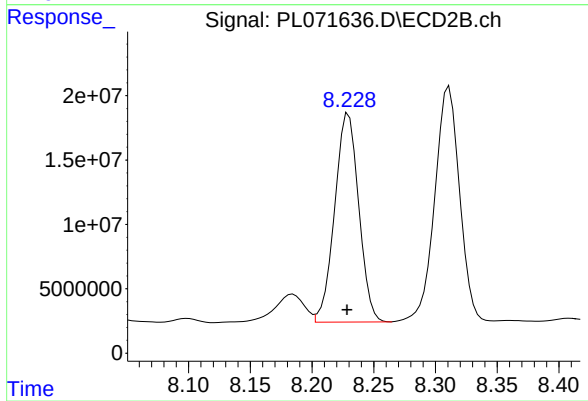

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.001 min
Response: 220012383
Conc: 790.38 ng/ml

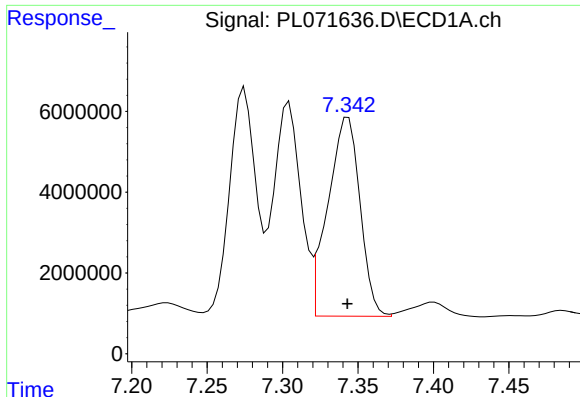

#26 Chlordane-4


R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 72660206
Conc: 785.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

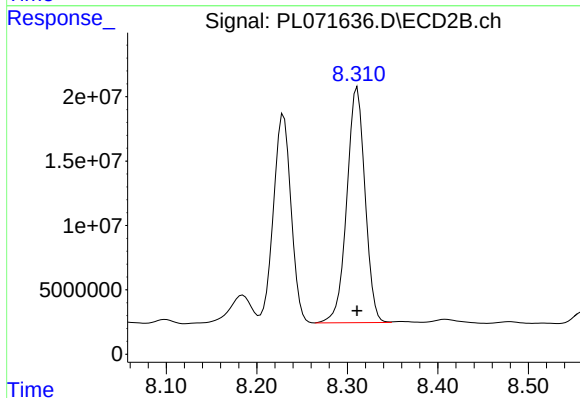


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 255611767
Conc: 785.80 ng/ml

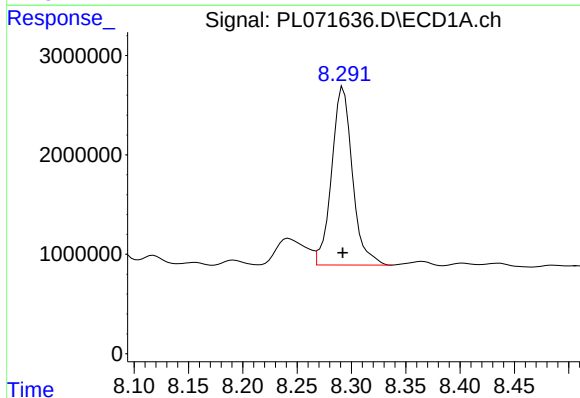


#27 Chlordane-5

R.T.: 8.292 min
Delta R.T.: 0.000 min
Response: 23872122
Conc: 774.32 ng/ml

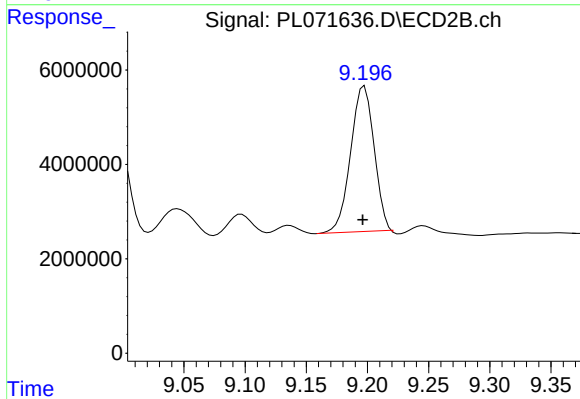

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.001 min
Response: 41114428
Conc: 760.62 ng/ml

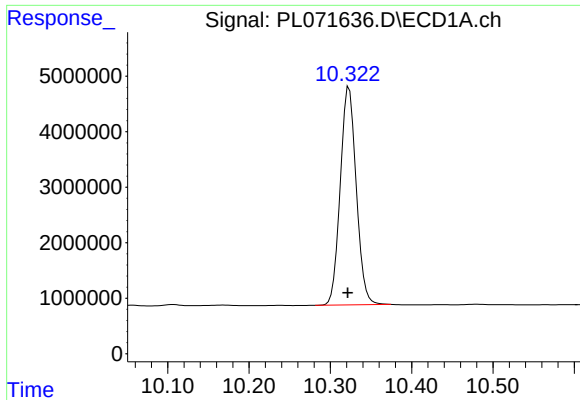

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.002 min
Response: 53573856
Conc: 71.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

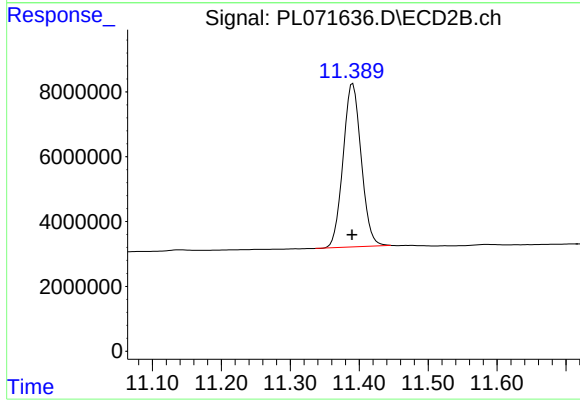

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.001 min
Response: 92148330
Conc: 72.81 ng/ml