

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 15:49
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL122721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 16:02:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.495	31035278	77828711	47.835	45.609
28)	SA Decachlor...	10.323	11.389	35687958	61852780	47.938	49.352
Target Compounds							
23)	Chlordane-1	5.888	6.877	11381972	32247179	459.901	478.986
24)	Chlordane-2	6.577	7.469	14475484	33390961	444.854	453.163
25)	Chlordane-3	7.276	8.227	39068282	126.5E6	452.969	457.748
26)	Chlordane-4	7.344	8.309	41814321	148.2E6	453.068	457.002
27)	Chlordane-5	8.293	9.195	13916794	25230546	458.915	465.080



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 15:49
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL122721

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 16:02:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

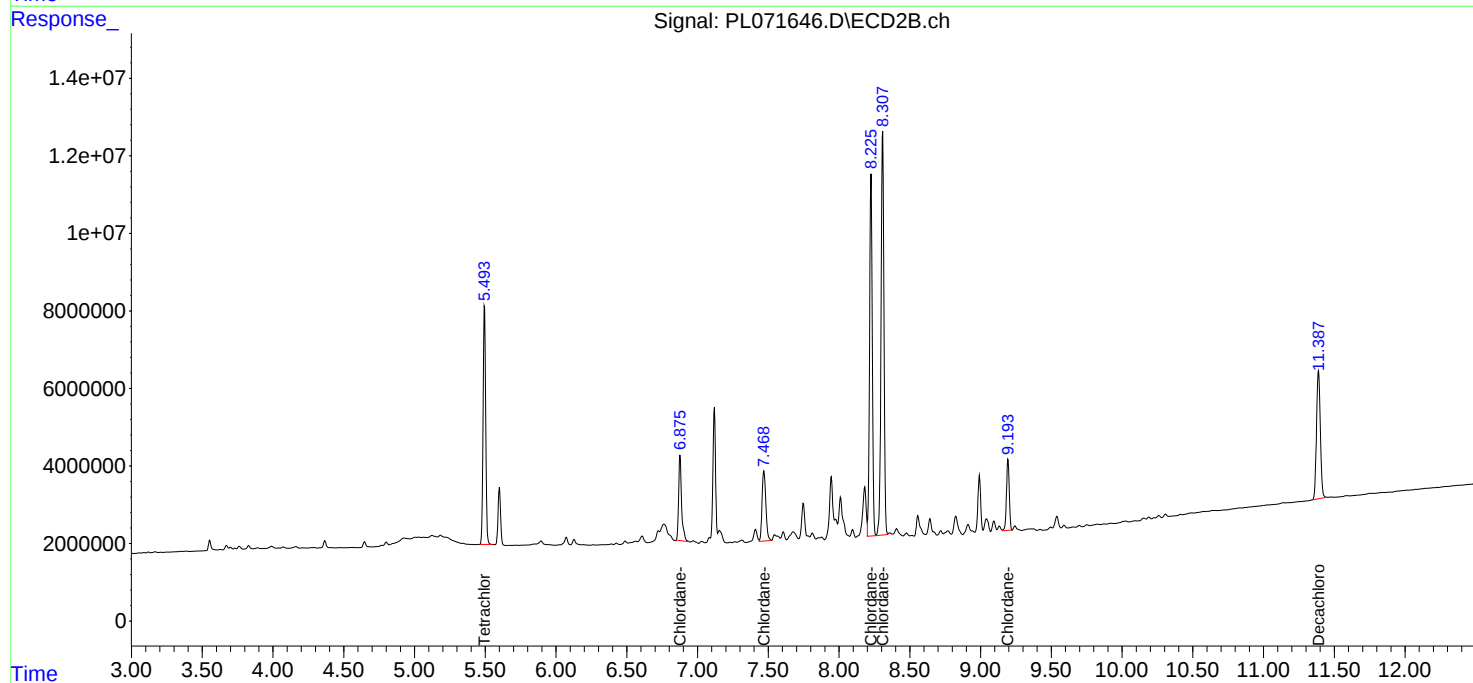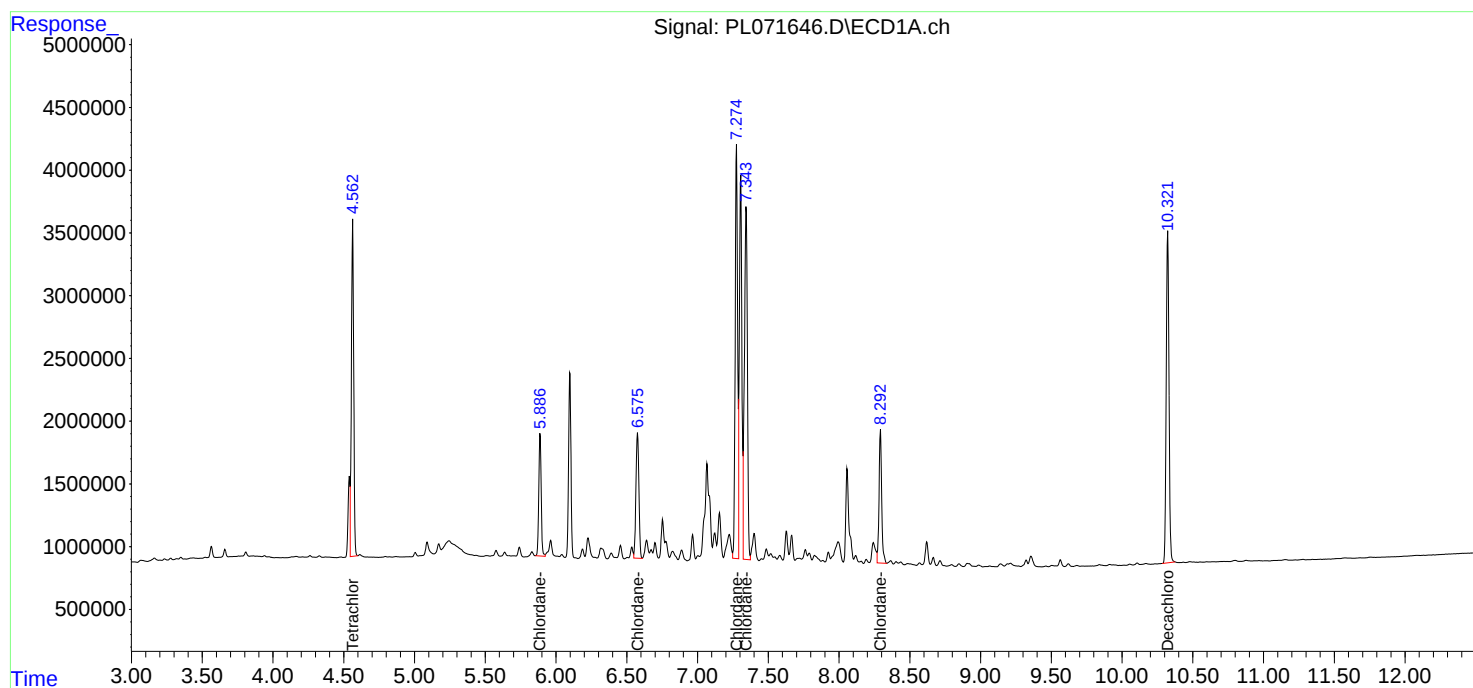


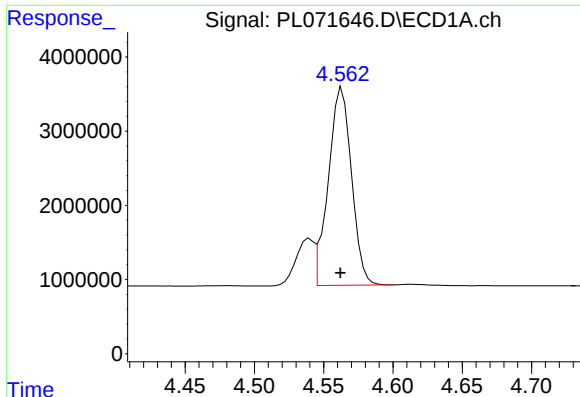

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.001 min
Response: 31035278
Conc: 47.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122721

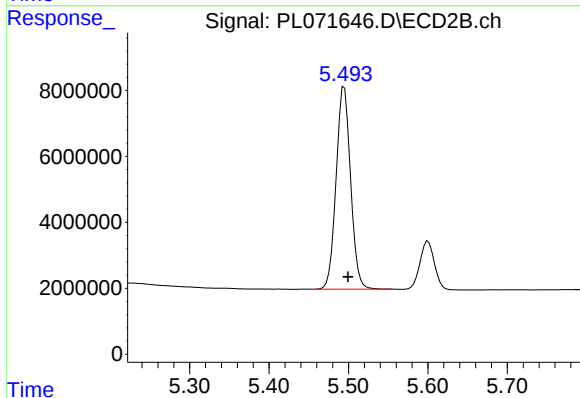


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: -0.005 min
Response: 77828711
Conc: 45.61 ng/ml

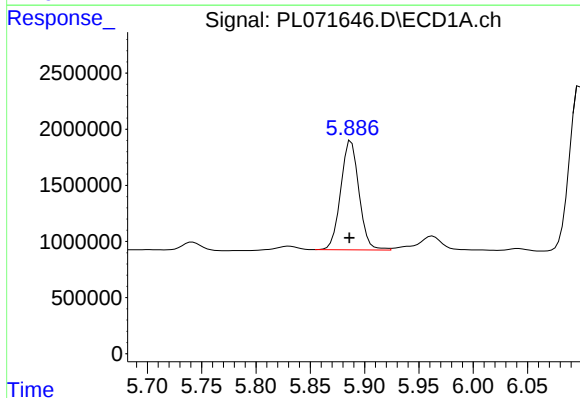


#23 Chlordane-1

R.T.: 5.888 min
Delta R.T.: 0.002 min
Response: 11381972
Conc: 459.90 ng/ml

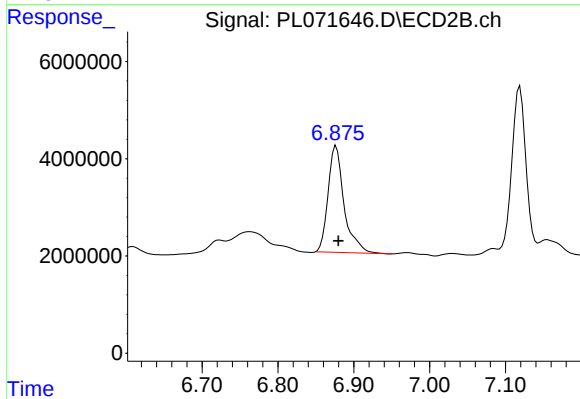

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: -0.003 min
Response: 32247179
Conc: 478.99 ng/ml

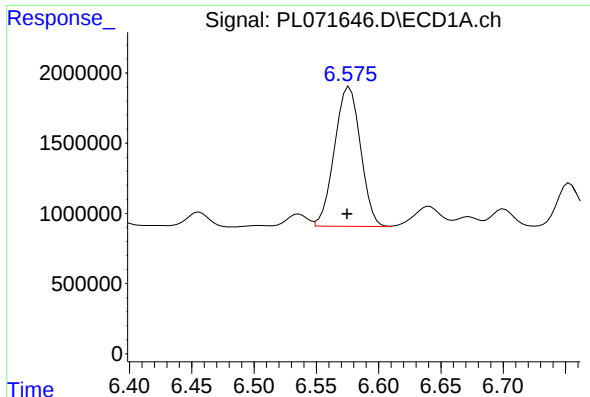

#24 Chlordane-2


R.T.: 6.577 min
Delta R.T.: 0.002 min
Response: 14475484
Conc: 444.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122721

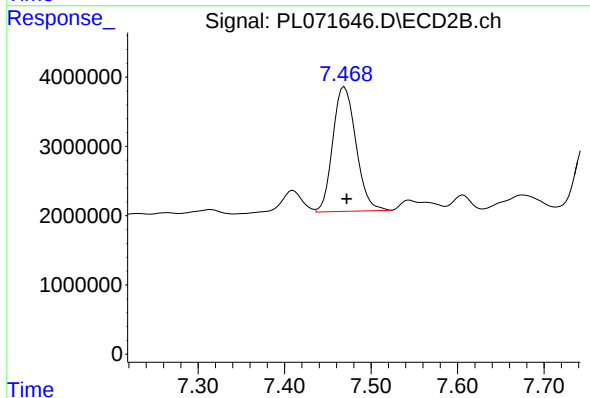


#24 Chlordane-2

R.T.: 7.469 min
Delta R.T.: -0.003 min
Response: 33390961
Conc: 453.16 ng/ml

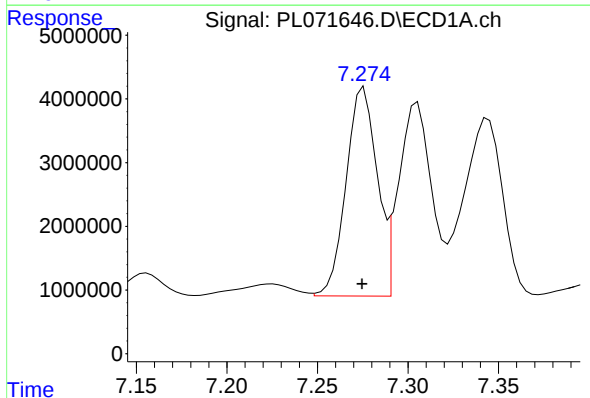


#25 Chlordane-3

R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 39068282
Conc: 452.97 ng/ml

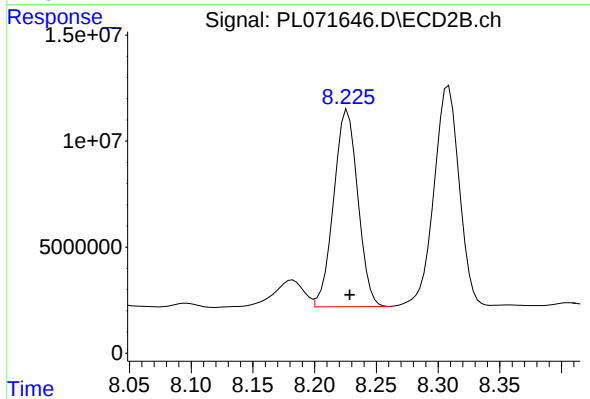

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 126488776
Conc: 457.75 ng/ml

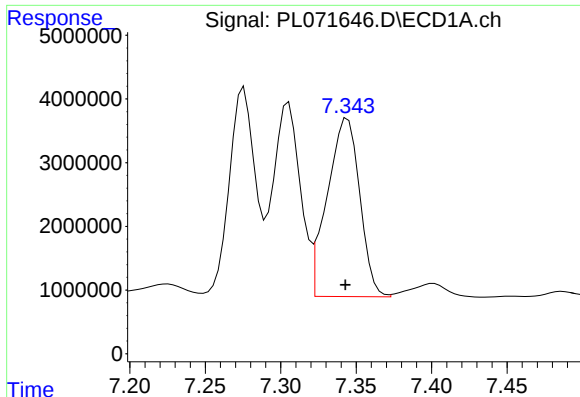

#26 Chlordane-4


R.T.: 7.344 min
Delta R.T.: 0.001 min
Response: 41814321
Conc: 453.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122721

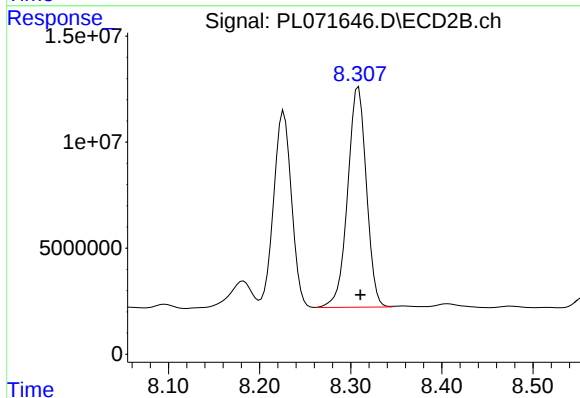


#26 Chlordane-4

R.T.: 8.309 min
Delta R.T.: -0.002 min
Response: 148244247
Conc: 457.00 ng/ml

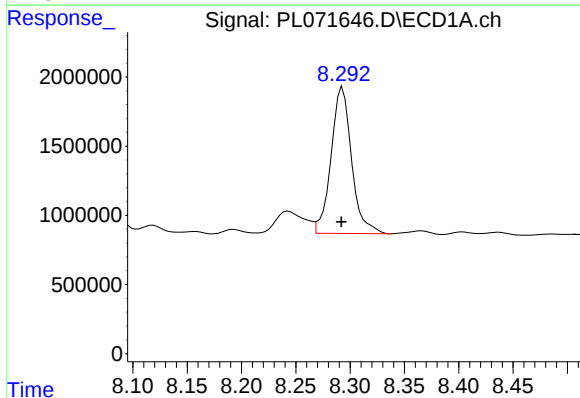


#27 Chlordane-5

R.T.: 8.293 min
Delta R.T.: 0.001 min
Response: 13916794
Conc: 458.91 ng/ml

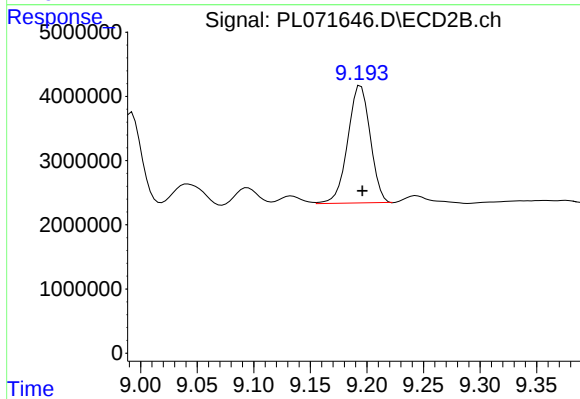

#27 Chlordane-5


R.T.: 9.195 min
Delta R.T.: -0.002 min
Response: 25230546
Conc: 465.08 ng/ml

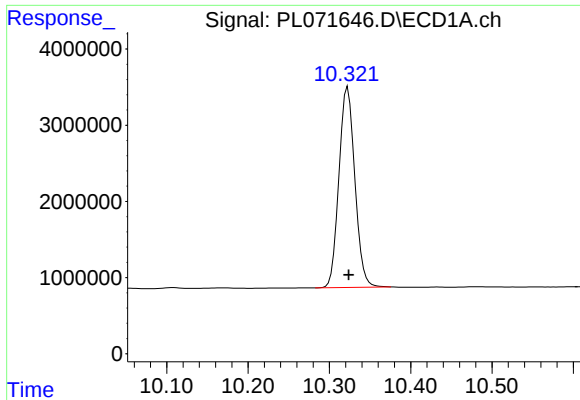

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.001 min
Response: 35687958
Conc: 47.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122721

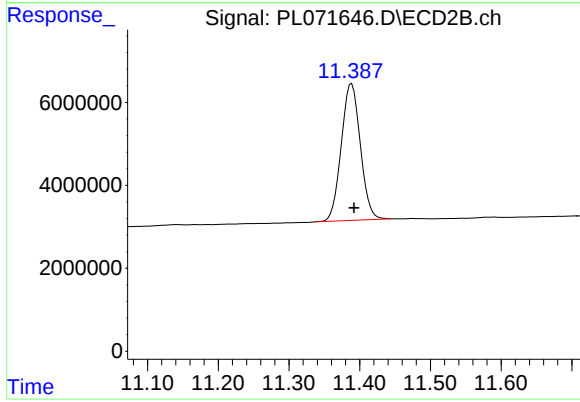

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.004 min
Response: 61852780
Conc: 49.35 ng/ml