

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 17:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 04:14:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.497	30147703	77202601	46.467	45.242
28)	SA Decachlor...	10.320	11.387	41952507	72676210	56.353	57.988
Target Compounds							
23)	Chlordane-1	5.884	6.878	11073781	29496241	447.448	438.125
24)	Chlordane-2	6.573	7.470	13982611	32893378	429.707	446.410
25)	Chlordane-3	7.273	8.227	37901919	123.8E6	439.446	447.936
26)	Chlordane-4	7.341	8.308	40533481	145.7E6	439.189	449.242
27)	Chlordane-5	8.290	9.194	13341805	24404798	439.954	449.858



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 17:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 04:14:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

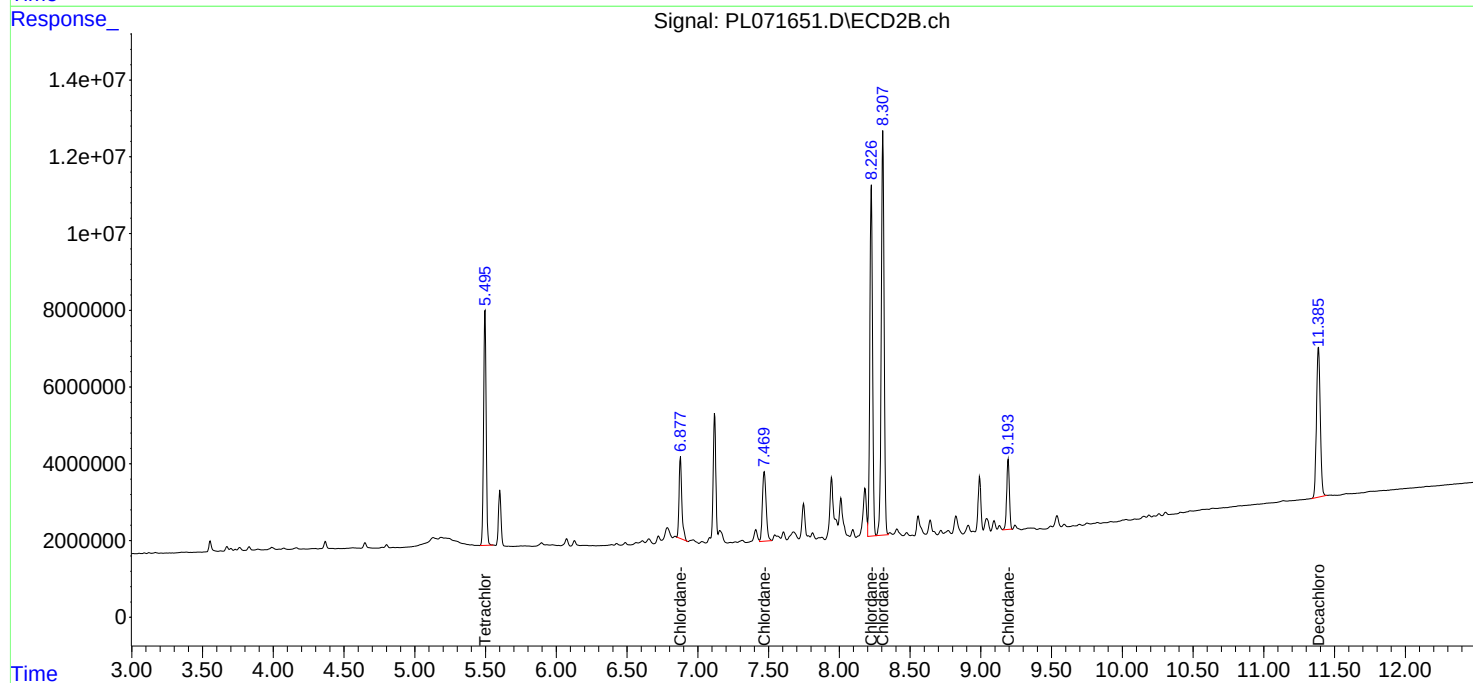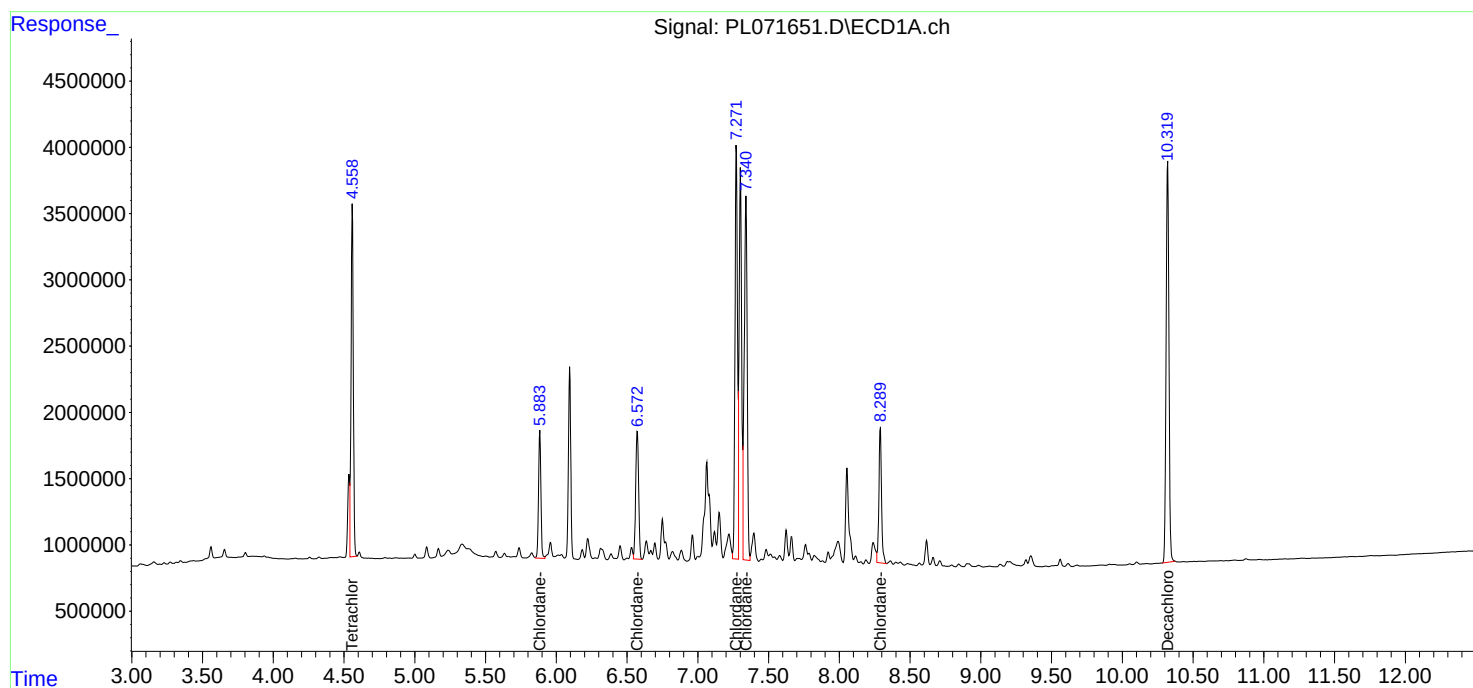


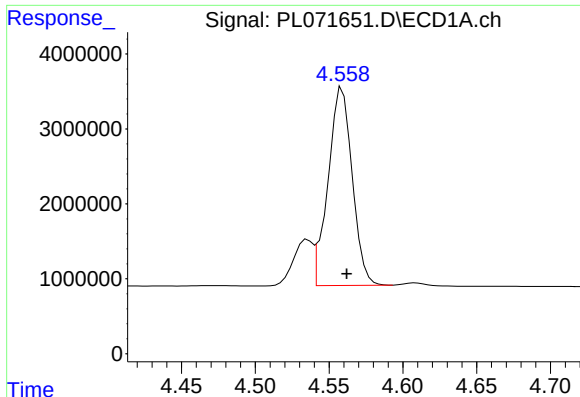

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 30147703
Conc: 46.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

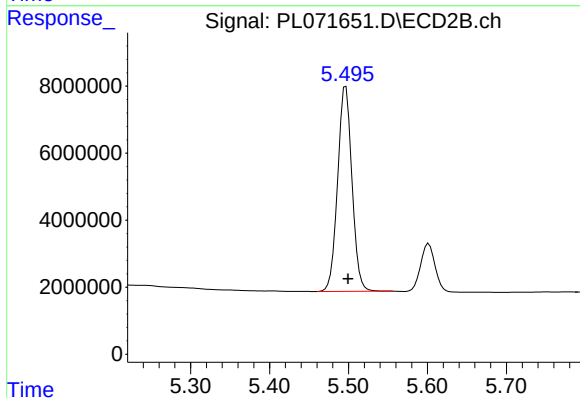


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.003 min
Response: 77202601
Conc: 45.24 ng/ml

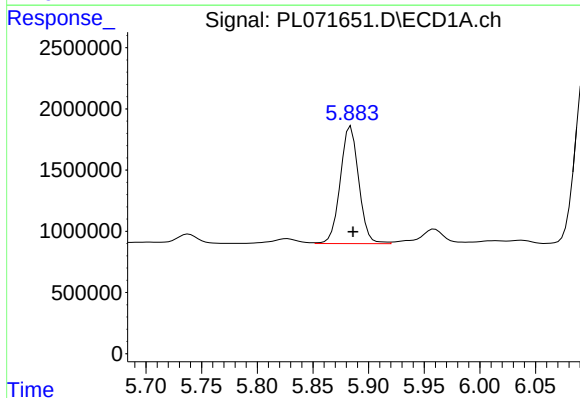


#23 Chlordane-1

R.T.: 5.884 min
Delta R.T.: -0.002 min
Response: 11073781
Conc: 447.45 ng/ml

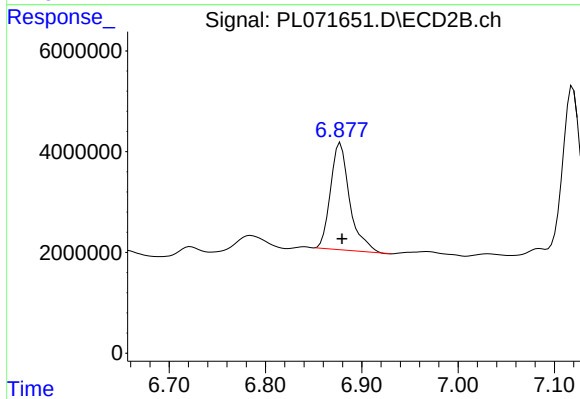

#23 Chlordane-1


R.T.: 6.878 min
Delta R.T.: -0.002 min
Response: 29496241
Conc: 438.12 ng/ml

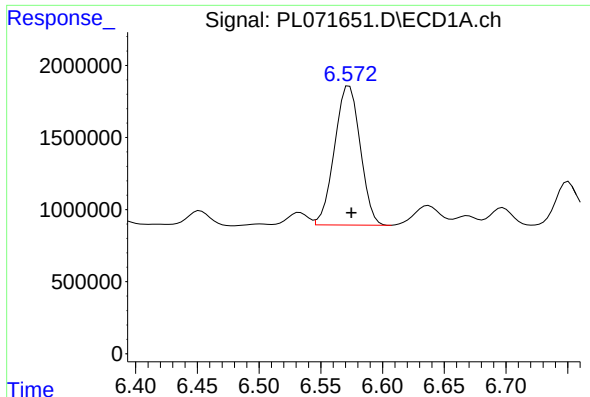

#24 Chlordane-2


R.T.: 6.573 min
Delta R.T.: -0.002 min
Response: 13982611
Conc: 429.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

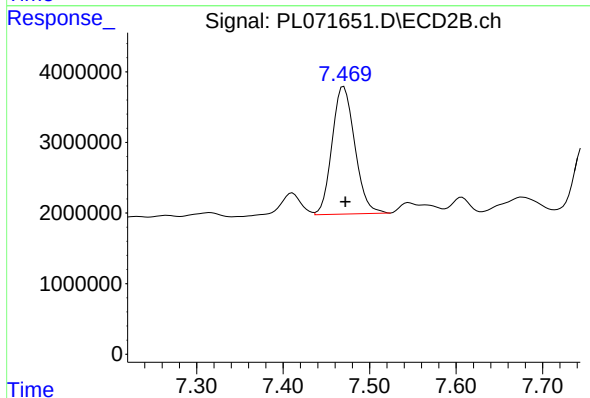


#24 Chlordane-2

R.T.: 7.470 min
Delta R.T.: -0.002 min
Response: 32893378
Conc: 446.41 ng/ml

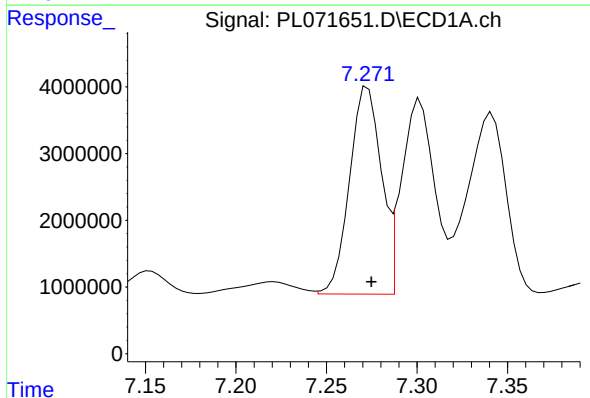


#25 Chlordane-3

R.T.: 7.273 min
Delta R.T.: -0.002 min
Response: 37901919
Conc: 439.45 ng/ml

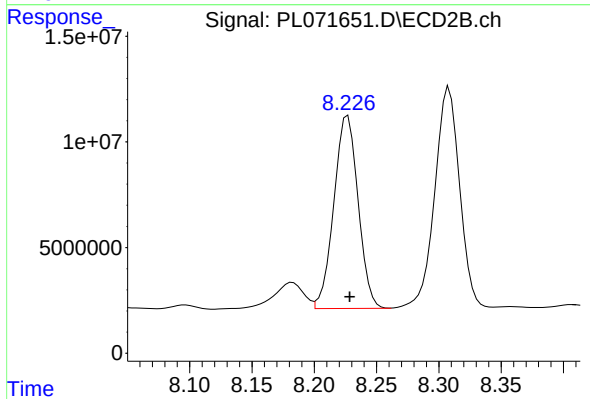

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 123777496
Conc: 447.94 ng/ml

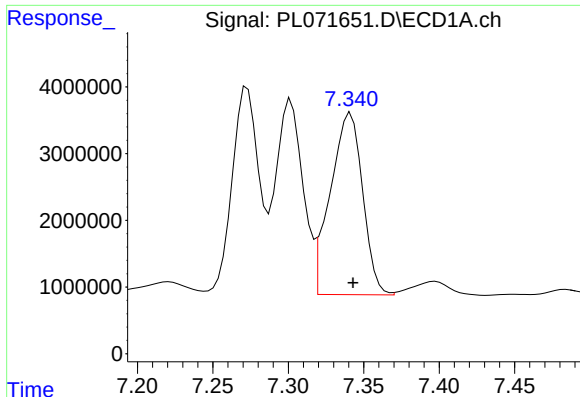

#26 Chlordane-4


R.T.: 7.341 min
Delta R.T.: -0.002 min
Response: 40533481
Conc: 439.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

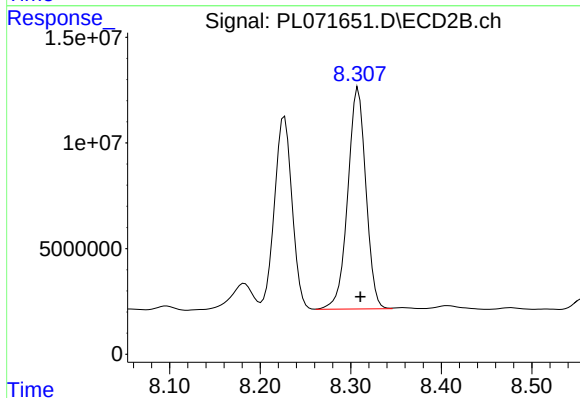


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.002 min
Response: 145727038
Conc: 449.24 ng/ml

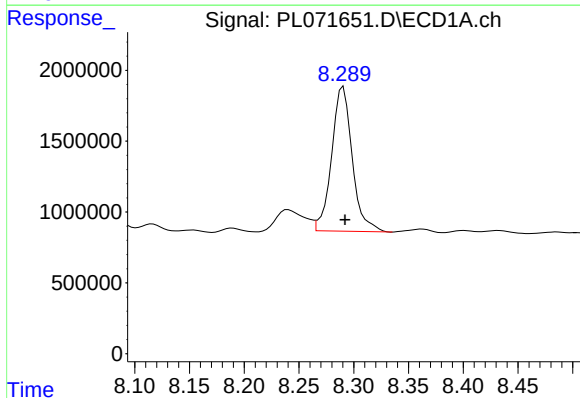


#27 Chlordane-5

R.T.: 8.290 min
Delta R.T.: -0.002 min
Response: 13341805
Conc: 439.95 ng/ml

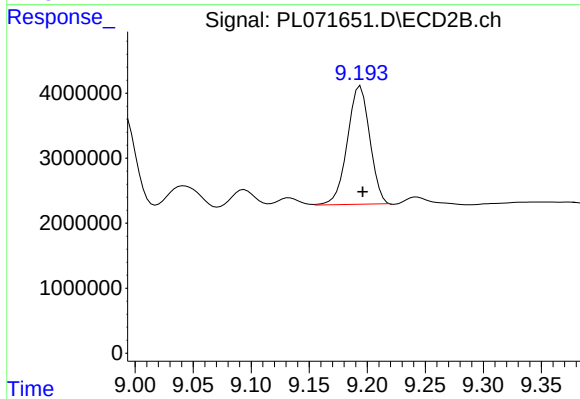

#27 Chlordane-5


R.T.: 9.194 min
Delta R.T.: -0.002 min
Response: 24404798
Conc: 449.86 ng/ml

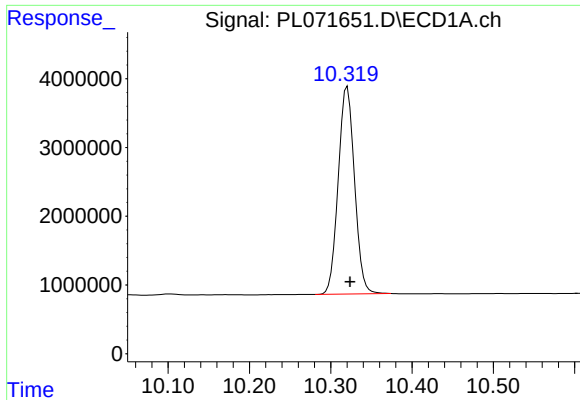

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.003 min
Response: 41952507
Conc: 56.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

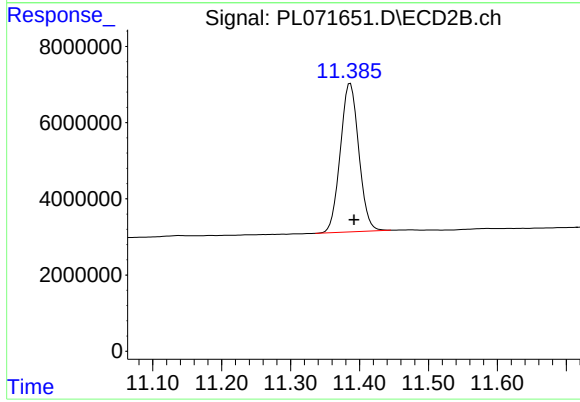

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.006 min
Response: 72676210
Conc: 57.99 ng/ml