

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
 Data File : PL071665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 21:05
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 04:14:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.496	29008403	74111796	44.711	43.431
28)	SA Decachlor...	10.320	11.387	42221192	73730851	56.713	58.830
Target Compounds							
23)	Chlordane-1	5.884	6.877	10630625	28481834	429.542	423.057
24)	Chlordane-2	6.573	7.469	13518898	31395481	415.456	426.081
25)	Chlordane-3	7.273	8.226	36813211	119.9E6	426.823	433.810
26)	Chlordane-4	7.341	8.308	39092014	140.8E6	423.571	434.199
27)	Chlordane-5	8.290	9.194	13247898	23710849	436.857	437.067



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122721\
Data File : PL071665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 21:05
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 04:14:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

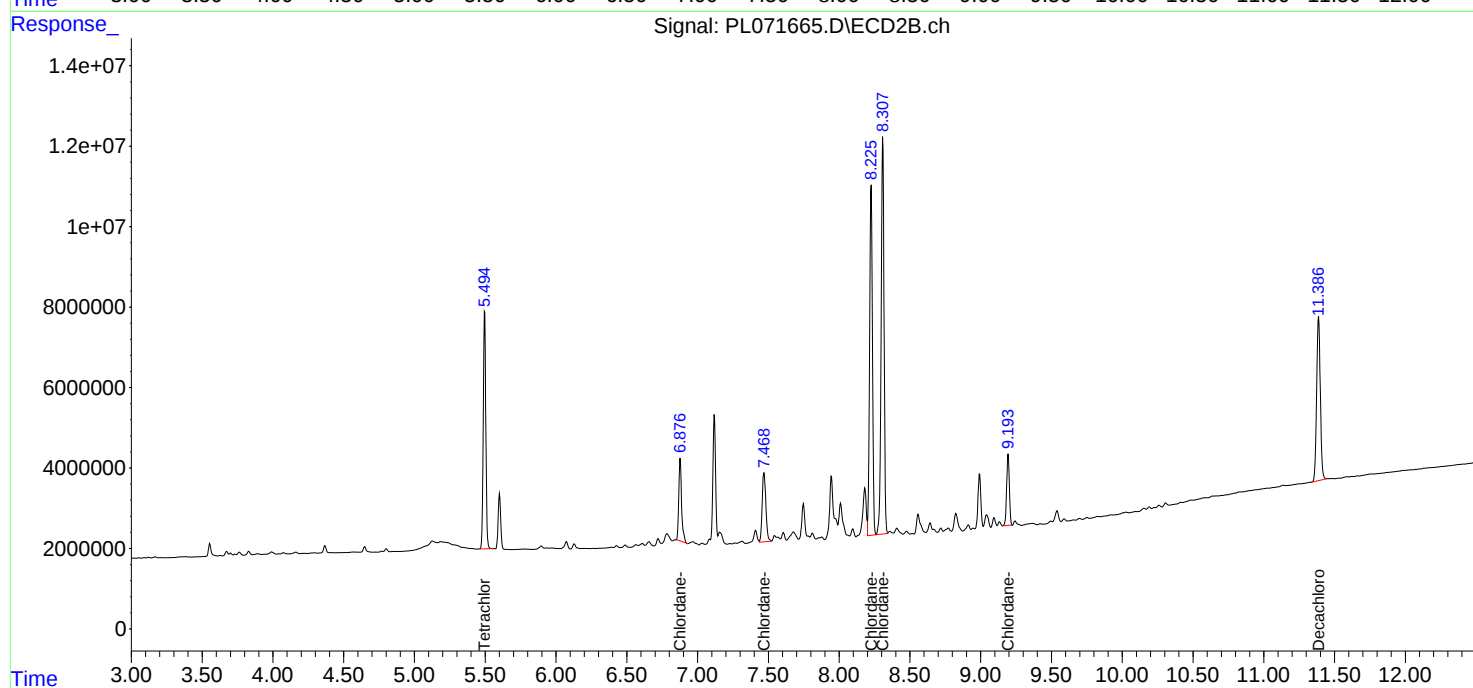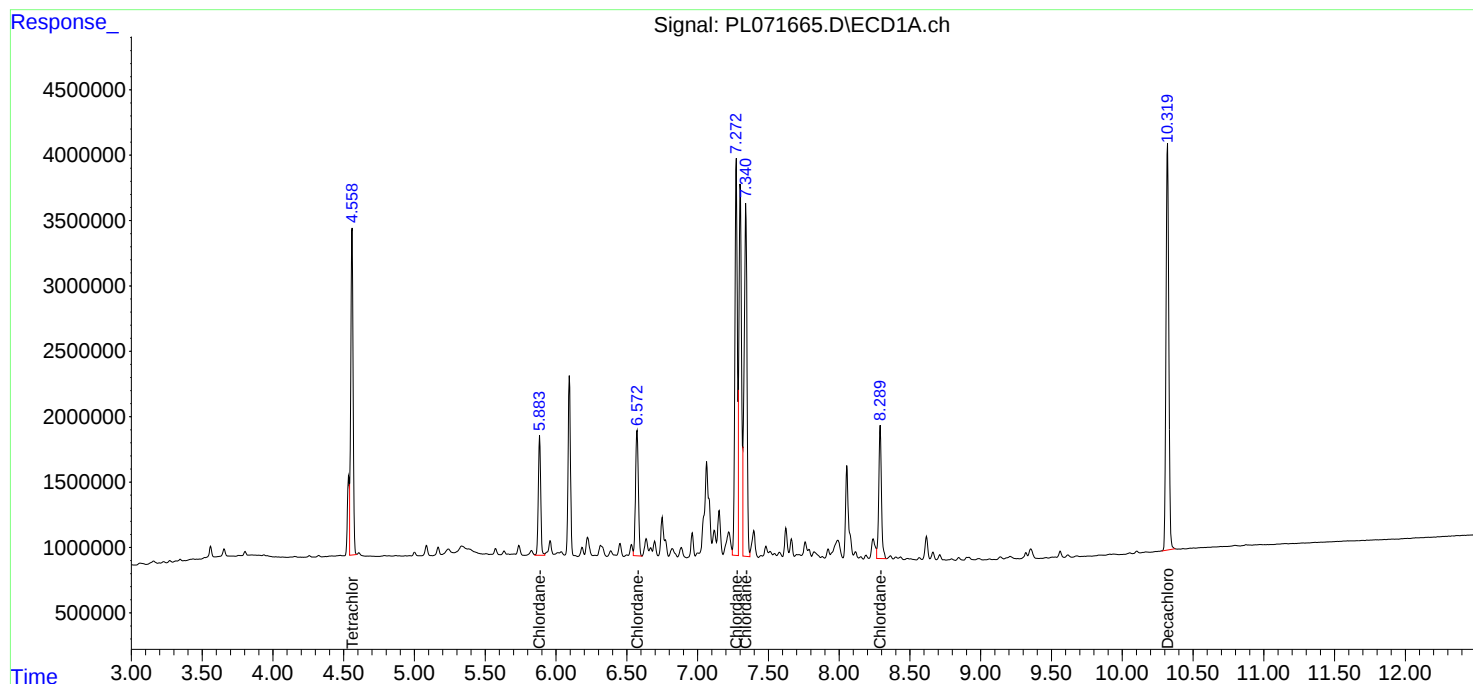


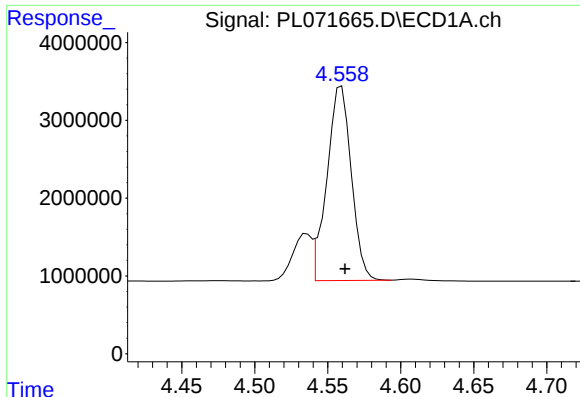

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: -0.003 min
Response: 29008403
Conc: 44.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

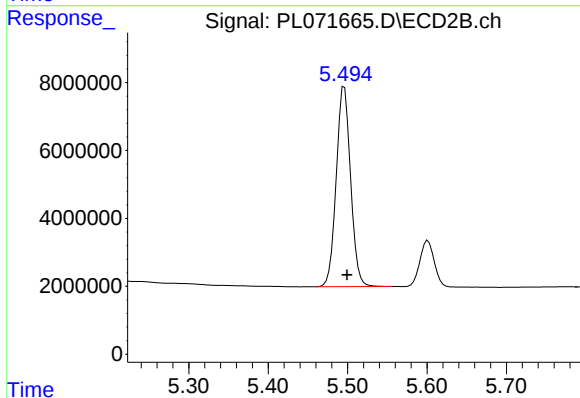


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 74111796
Conc: 43.43 ng/ml

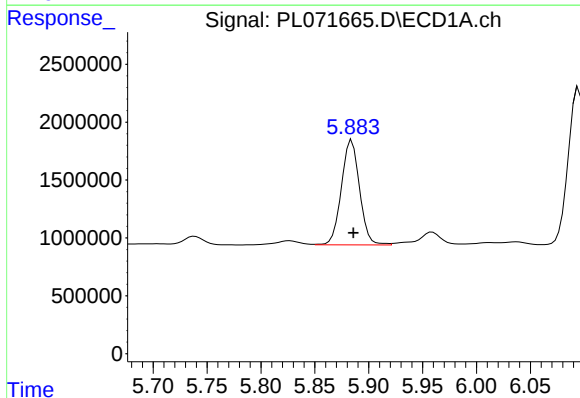


#23 Chlordane-1

R.T.: 5.884 min
Delta R.T.: -0.002 min
Response: 10630625
Conc: 429.54 ng/ml

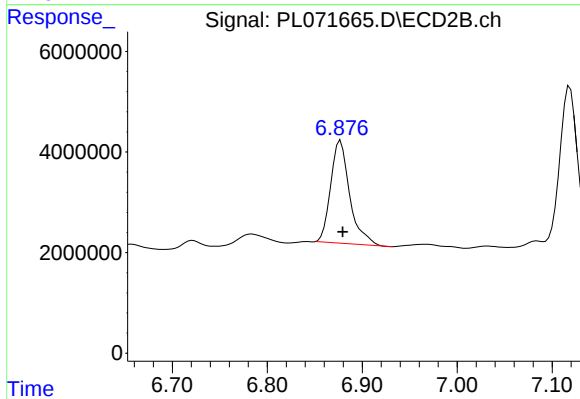

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: -0.003 min
Response: 28481834
Conc: 423.06 ng/ml

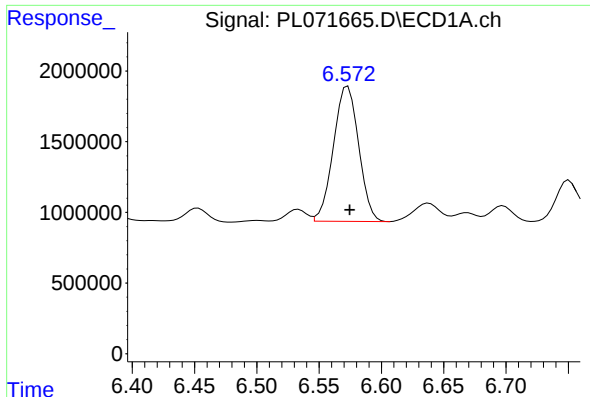

#24 Chlordane-2


R.T.: 6.573 min
Delta R.T.: -0.002 min
Response: 13518898
Conc: 415.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

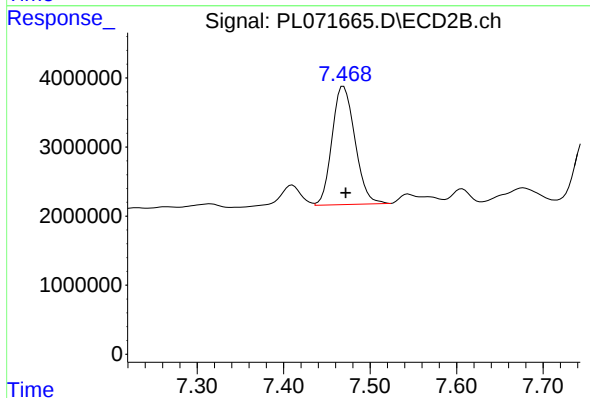


#24 Chlordane-2

R.T.: 7.469 min
Delta R.T.: -0.003 min
Response: 31395481
Conc: 426.08 ng/ml

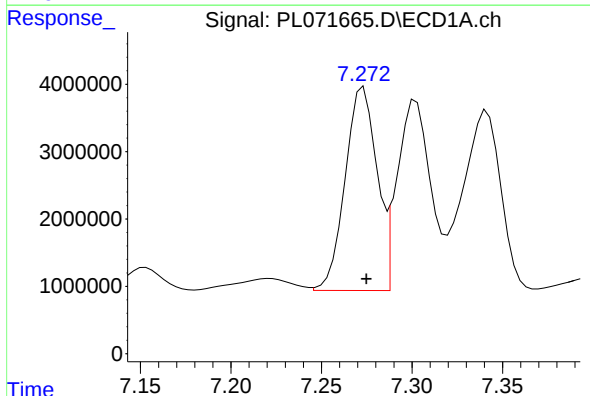


#25 Chlordane-3

R.T.: 7.273 min
Delta R.T.: -0.001 min
Response: 36813211
Conc: 426.82 ng/ml

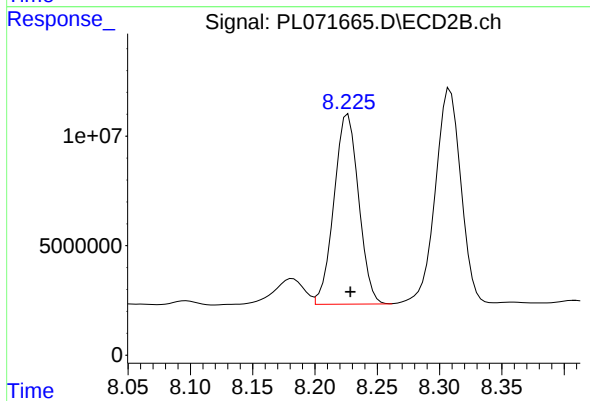

#25 Chlordane-3


R.T.: 8.226 min
Delta R.T.: -0.002 min
Response: 119873922
Conc: 433.81 ng/ml

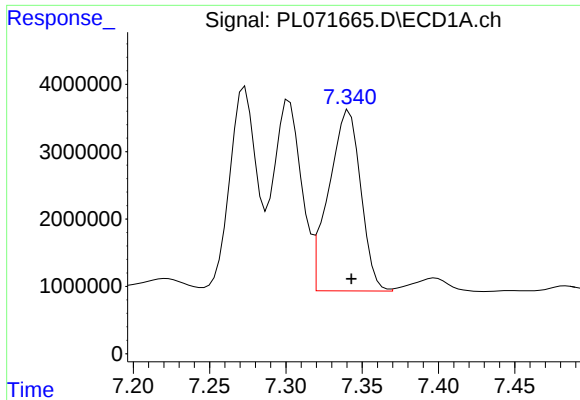

#26 Chlordane-4


R.T.: 7.341 min
Delta R.T.: -0.002 min
Response: 39092014
Conc: 423.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

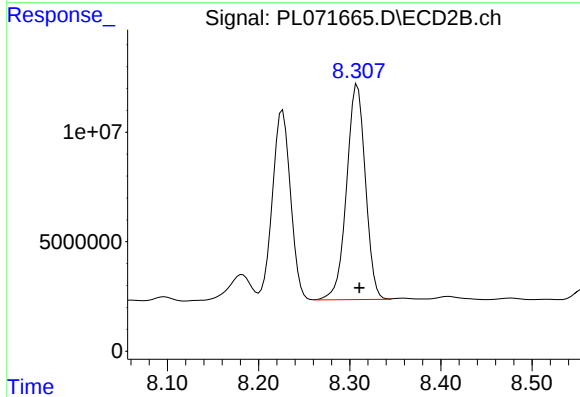


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.002 min
Response: 140847319
Conc: 434.20 ng/ml

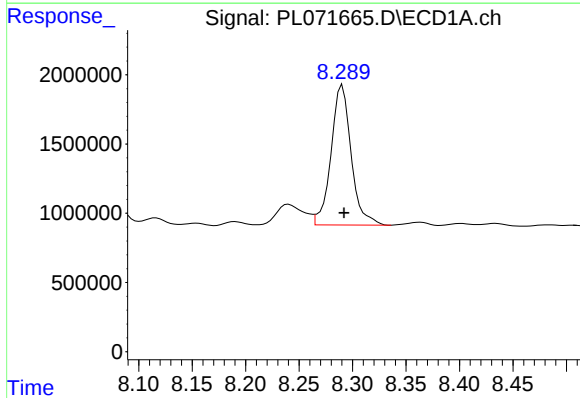


#27 Chlordane-5

R.T.: 8.290 min
Delta R.T.: -0.002 min
Response: 13247898
Conc: 436.86 ng/ml

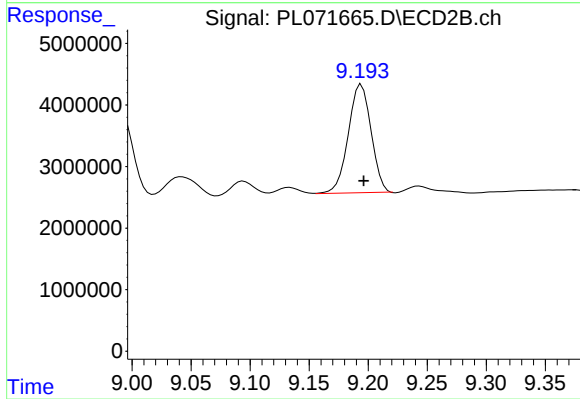

#27 Chlordane-5


R.T.: 9.194 min
Delta R.T.: -0.002 min
Response: 23710849
Conc: 437.07 ng/ml

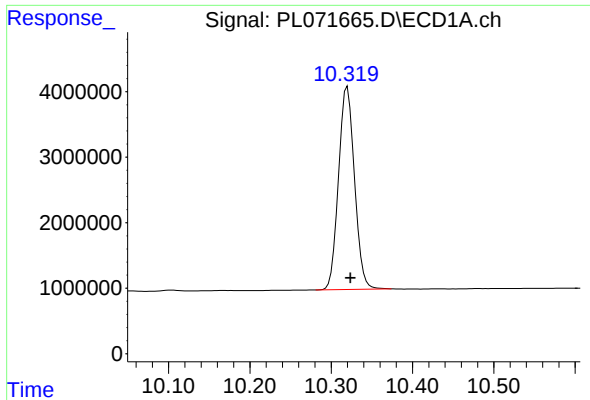

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.004 min
Response: 42221192
Conc: 56.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

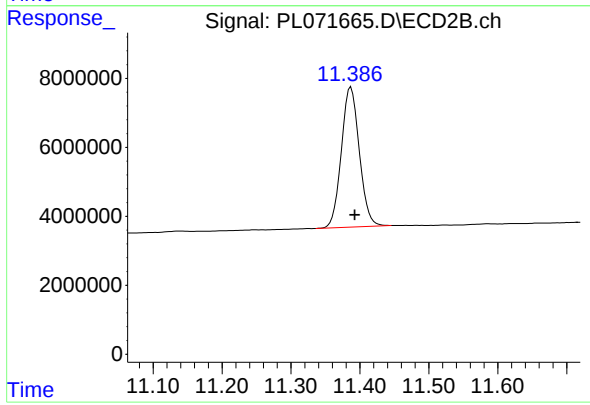

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.005 min
Response: 73730851
Conc: 58.83 ng/ml