

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
 Data File : PL093533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2024 12:18
 Operator : AR\AJ
 Sample : P5386-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MOO-24-00398

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/30/2024
 Supervised By : Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:54:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.780	16656205	33020228	6.728m	11.342m#
28) SA Decachlor...	9.059	7.913	18885291	25867126	10.214	8.663m
Target Compounds						
12) B 4,4'-DDE	6.195	5.247	11628629	26598981	5.182m	7.233m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
Data File : PL093533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2024 12:18
Operator : AR\AJ
Sample : P5386-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MOO-24-00398


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/30/2024
Supervised By : Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:54:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

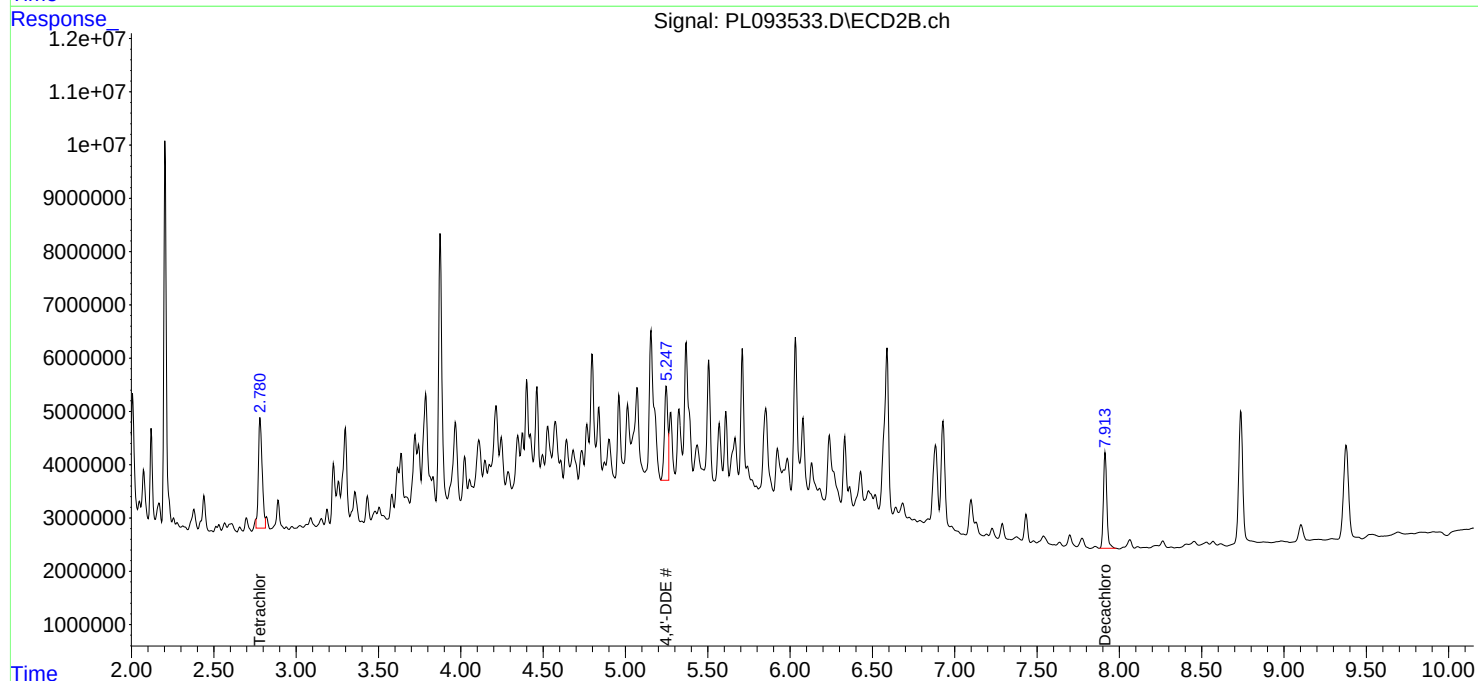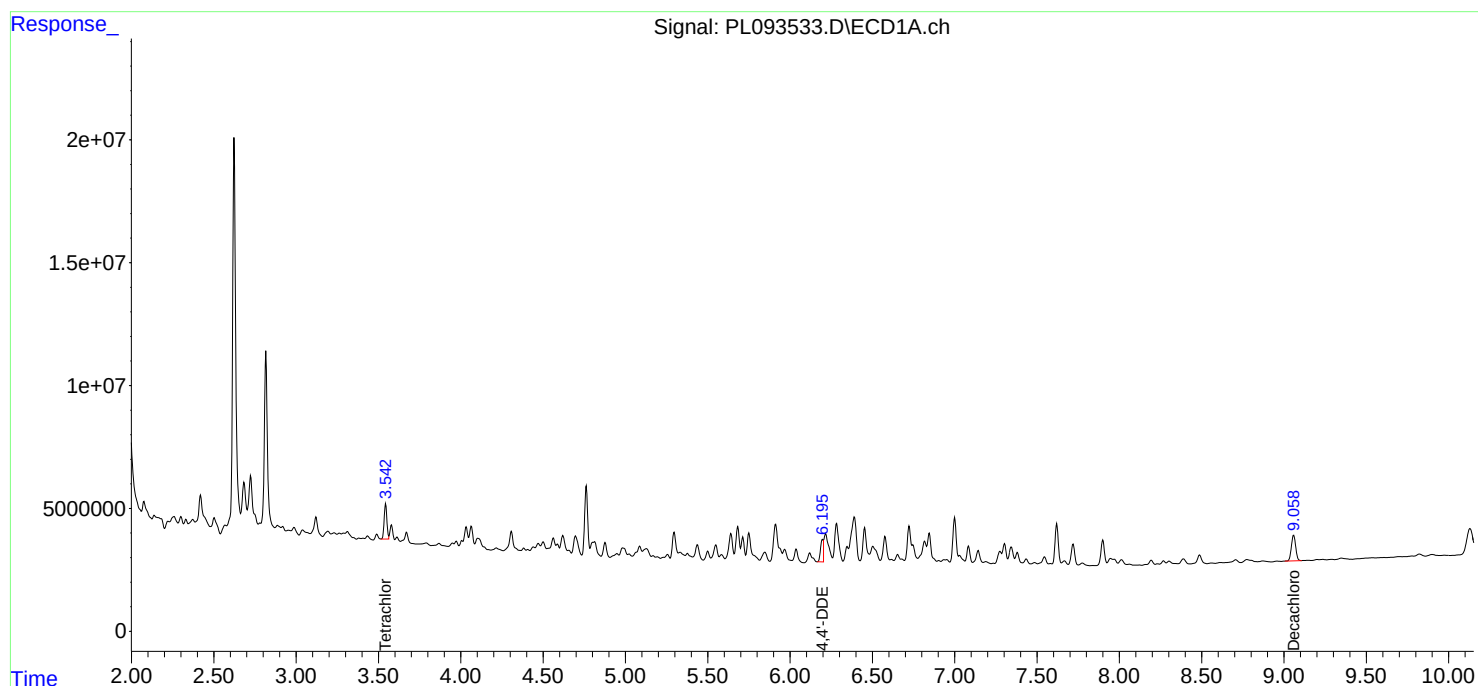

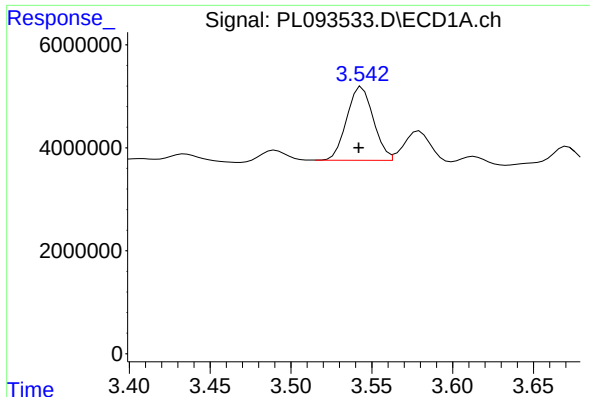


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 16656205
Conc: 6.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-24-00398


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/30/2024
Supervised By :Ankita Jodhani 12/30/2024

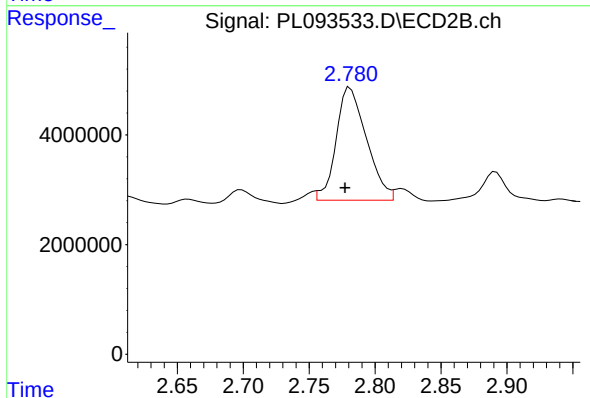


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: 0.002 min
Response: 33020228
Conc: 11.34 ng/ml m

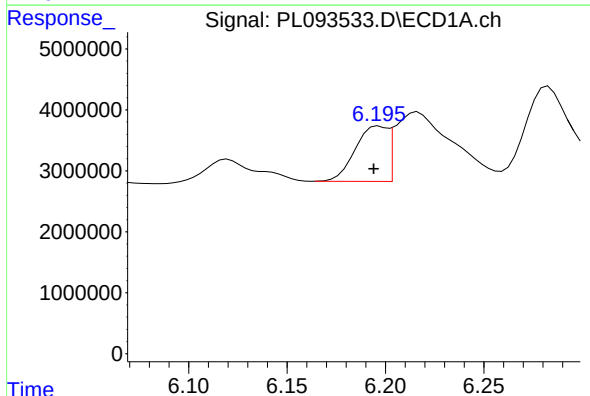


#12 4,4'-DDE

R.T.: 6.195 min
Delta R.T.: 0.001 min
Response: 11628629
Conc: 5.18 ng/ml m

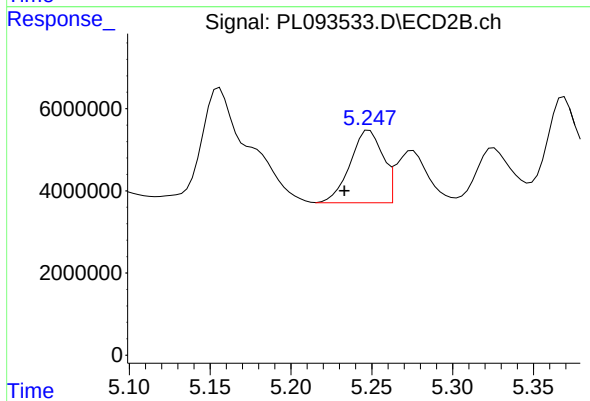

#12 4,4'-DDE

R.T.: 5.247 min
Delta R.T.: 0.014 min
Response: 26598981
Conc: 7.23 ng/ml m

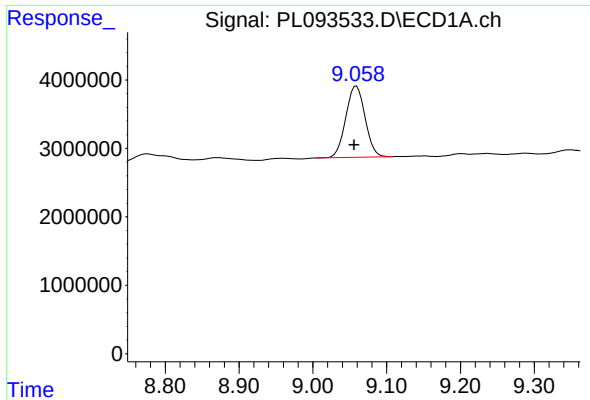


#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.003 min
Response: 18885291
Conc: 10.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-24-00398

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/30/2024
Supervised By :Ankita Jodhani 12/30/2024

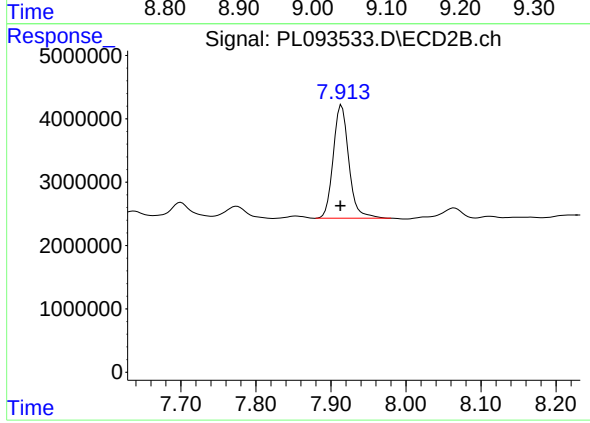

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 25867126
Conc: 8.66 ng/ml m