

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
 Data File : PL093545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2024 16:20
 Operator : AR\AJ
 Sample : P5386-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MOO-24-00397

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/30/2024
 Supervised By :Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:58:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.776	28301649	40372408	11.432	13.868
2) SA Decachlor...	9.052	7.909	17641662	23446311	9.541m	7.852m
Target Compounds						
17) MA 4,4'-DDT	7.031	6.034	5035755	9379540	2.724m	3.105m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
Data File : PL093545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2024 16:20
Operator : AR\AJ
Sample : P5386-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MOO-24-00397


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/30/2024
Supervised By : Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:58:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

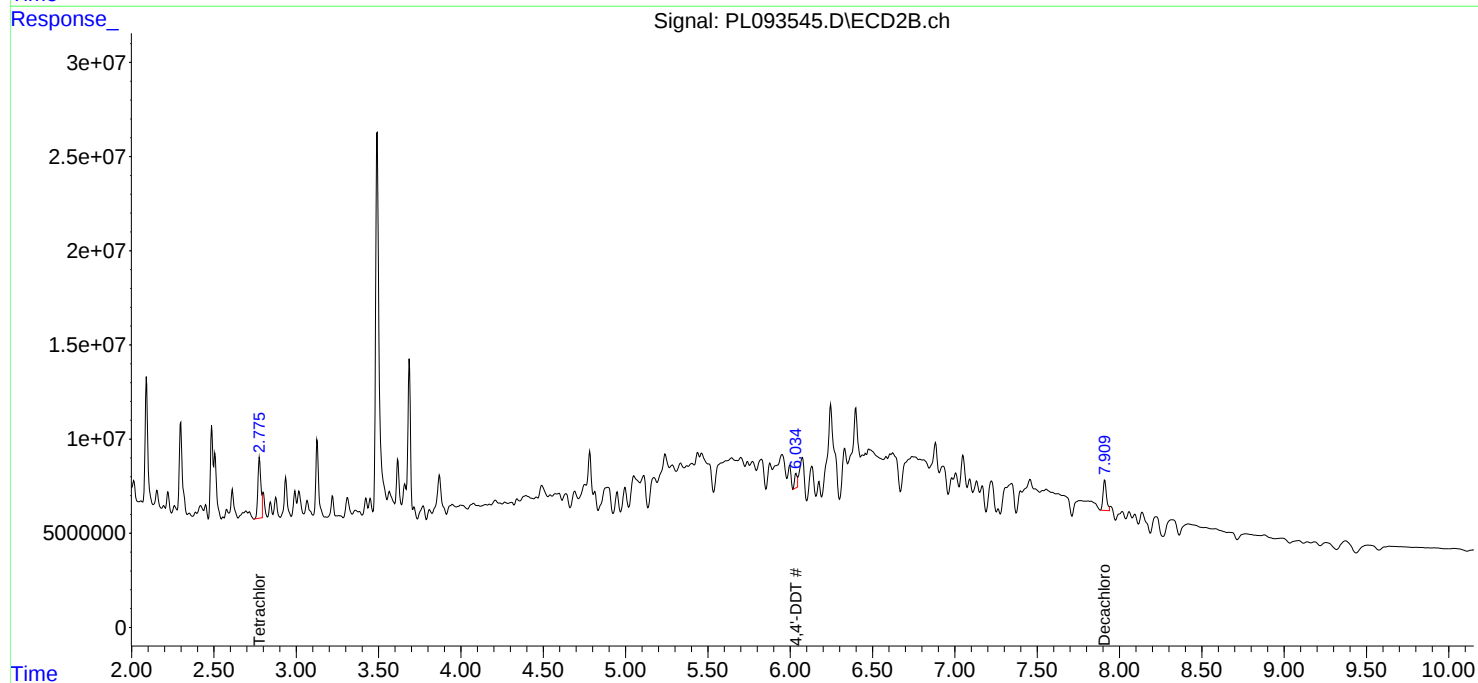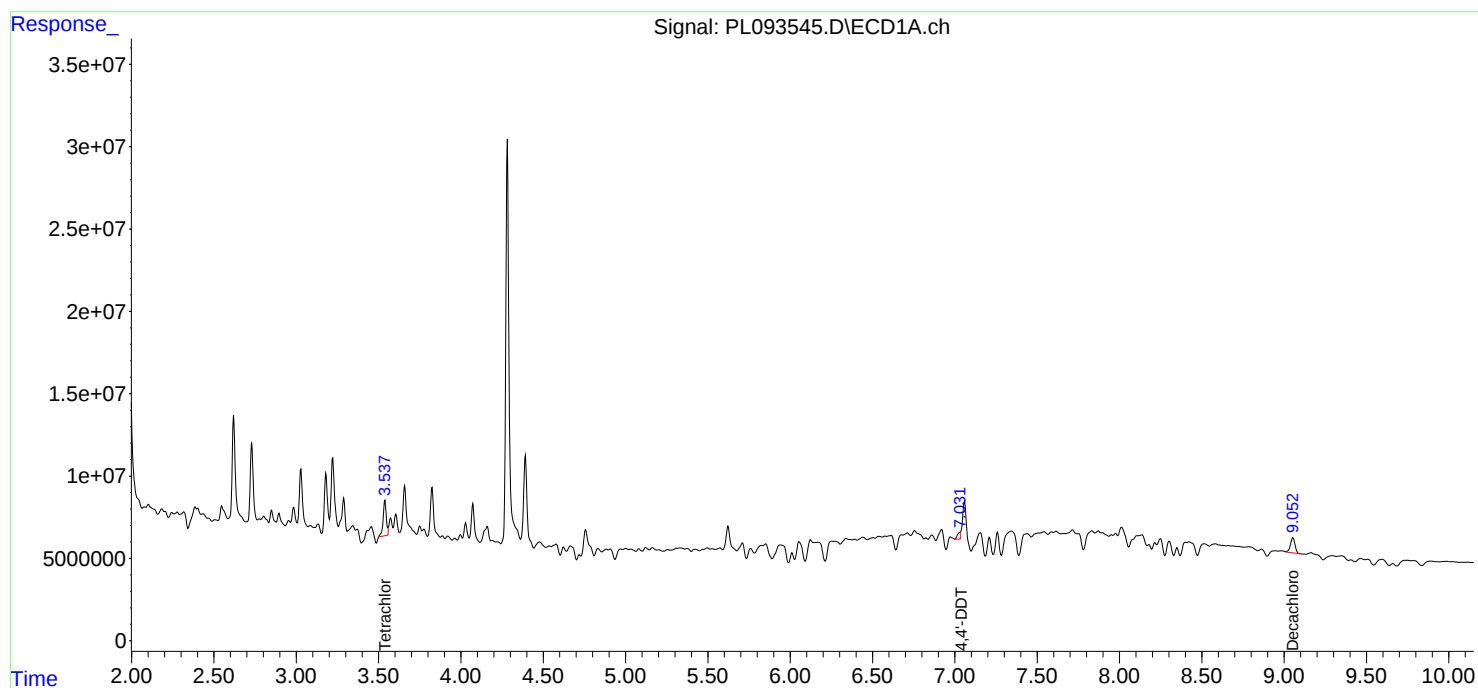

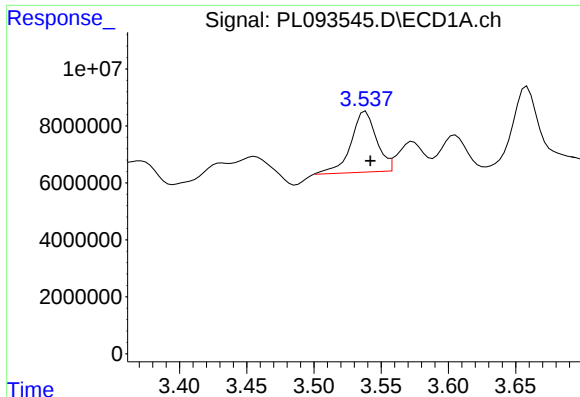


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 28301649
Conc: 11.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-24-00397


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/30/2024
Supervised By :Ankita Jodhani 12/30/2024

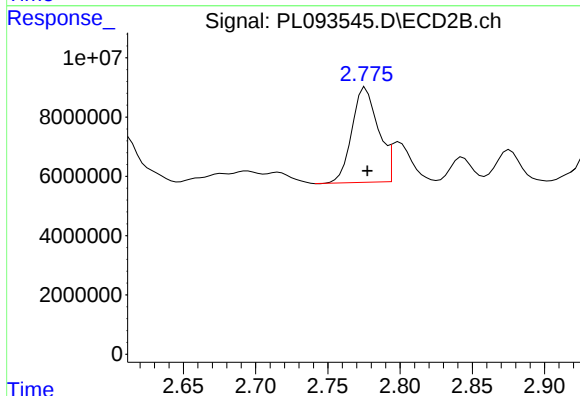


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.001 min
Response: 40372408
Conc: 13.87 ng/ml

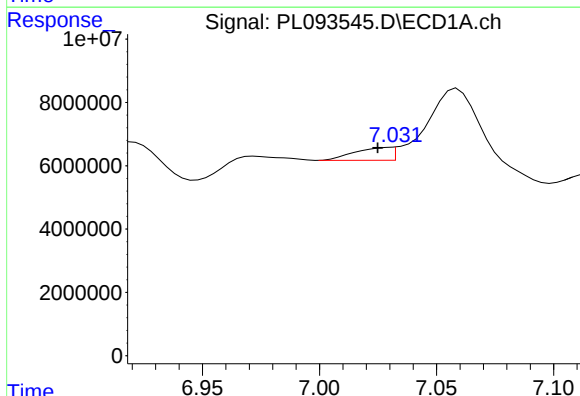


#17 4,4'-DDT

R.T.: 7.031 min
Delta R.T.: 0.006 min
Response: 5035755
Conc: 2.72 ng/ml m

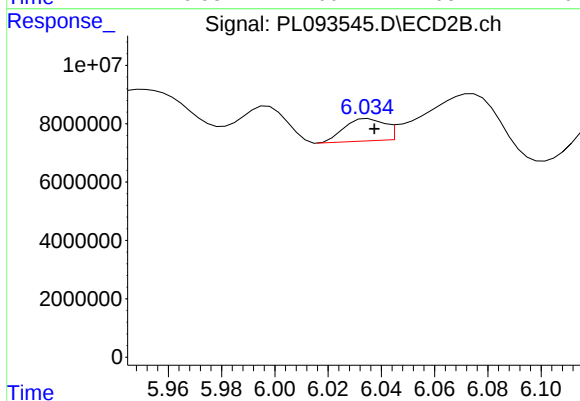

#17 4,4'-DDT

R.T.: 6.034 min
Delta R.T.: -0.004 min
Response: 9379540
Conc: 3.11 ng/ml m

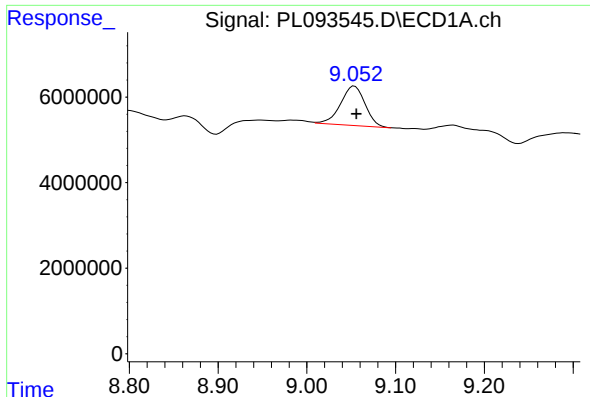


#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.004 min
Response: 17641662
Conc: 9.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-24-00397

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/30/2024
Supervised By :Ankita Jodhani 12/30/2024

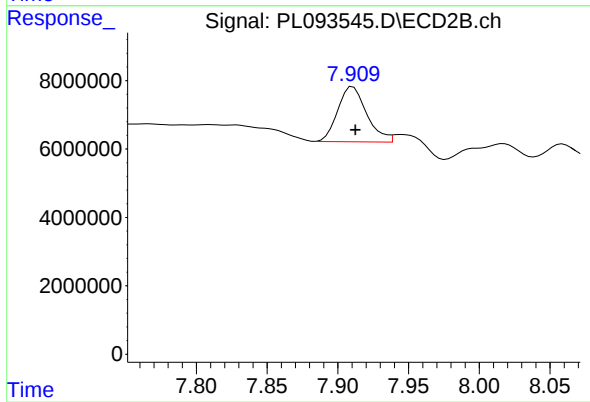

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.003 min
Response: 23446311
Conc: 7.85 ng/ml m