

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
 Data File : PL043490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 12:02
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 22:27:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.099	142.3E6	72639054	23.209	24.508
28)	SA Decachlor...	8.206	9.232	136.2E6	57383634	20.851	21.999
Target Compounds							
6)	B beta-BHC	0.000	4.965	0	4580696	N.D.	2.706 #
8)	B Heptachlo...	0.000	5.990	0	11479168	N.D.	3.027 #
10)	B gamma-Chl...	0.000	6.168f	0	4538367	N.D.	1.235 #
15)	B Endosulfa...	6.227f	0.000	2212115	0	0.333	N.D. #
25)	Chlordane-3	0.000	6.168	0	4538367	N.D.	9.242 #
27)	Chlordane-5	6.227	0.000	2212115	0	9.223	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
Data File : PL043490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 12:02
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 22:27:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

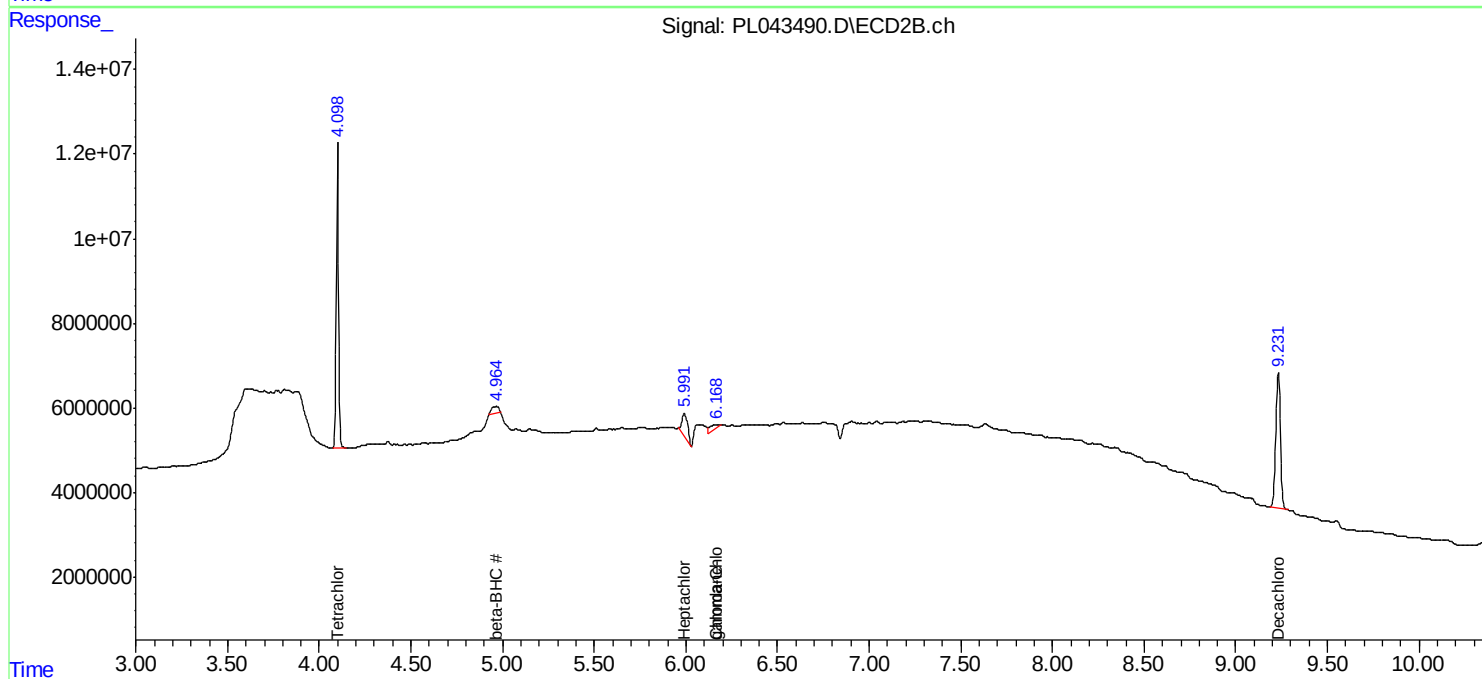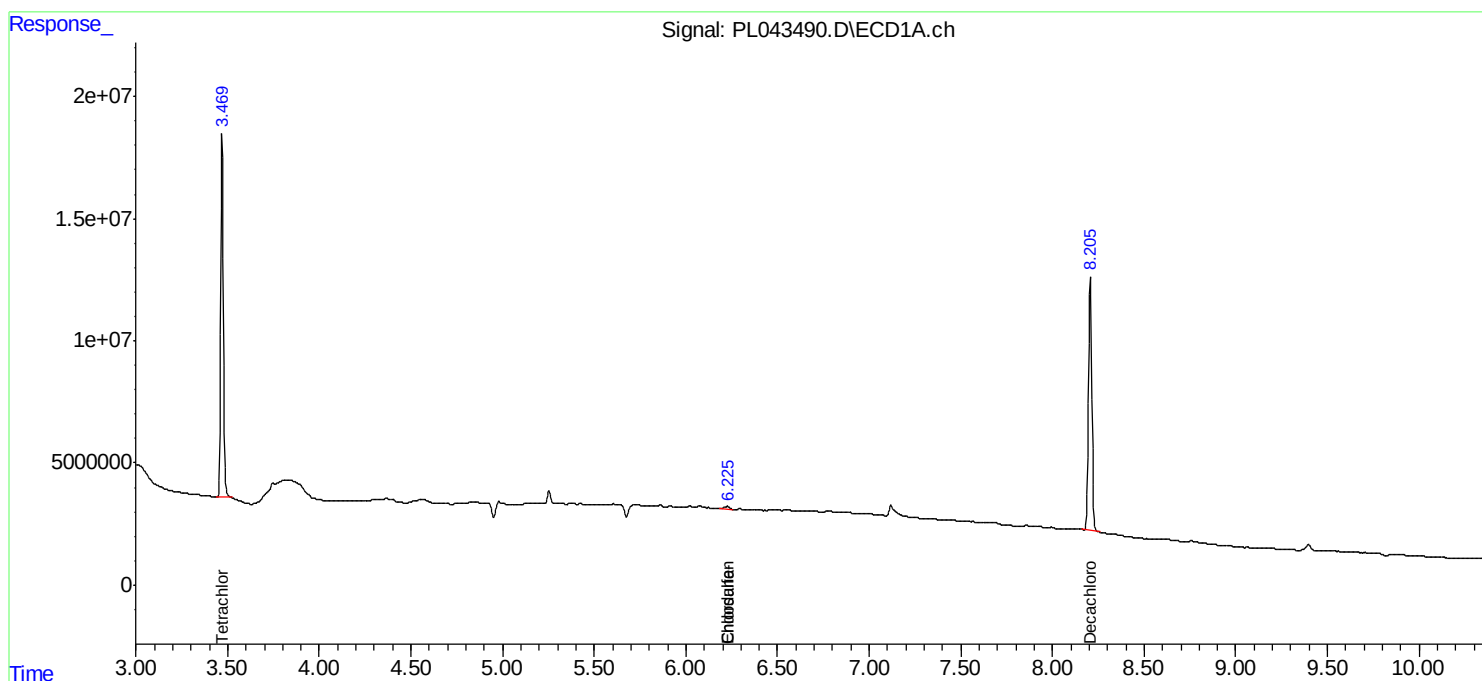


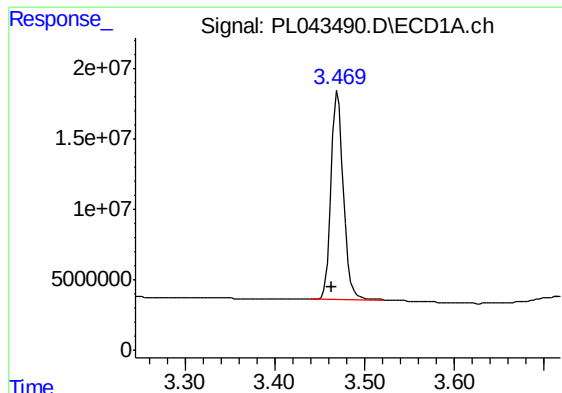

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.006 min
Response: 142340205
Conc: 23.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

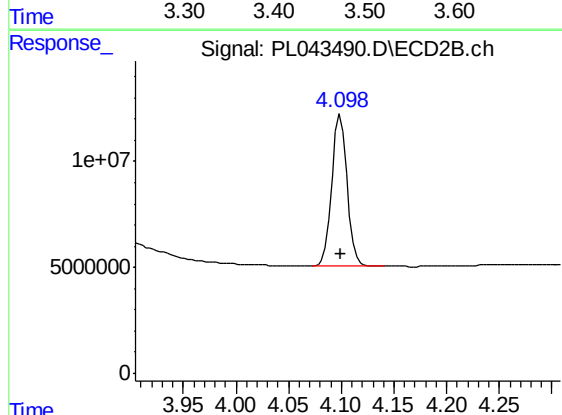


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 72639054
Conc: 24.51 ng/ml

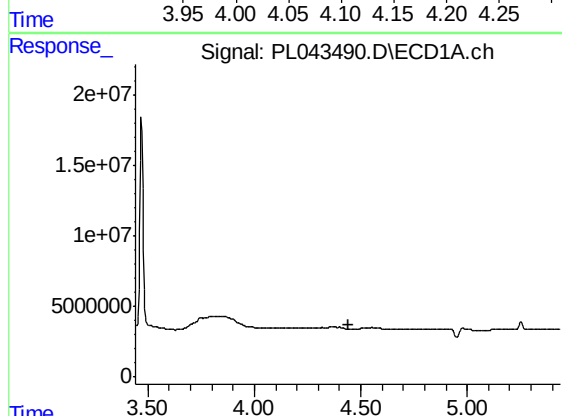


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.441 min
Response: 0
Conc: N.D.

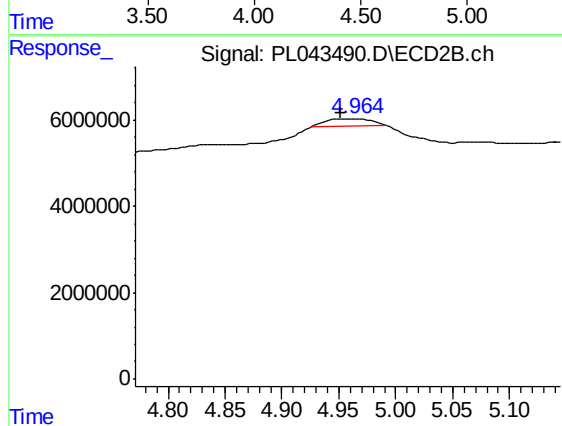

#6 beta-BHC


R.T.: 4.965 min
Delta R.T.: 0.013 min
Response: 4580696
Conc: 2.71 ng/ml

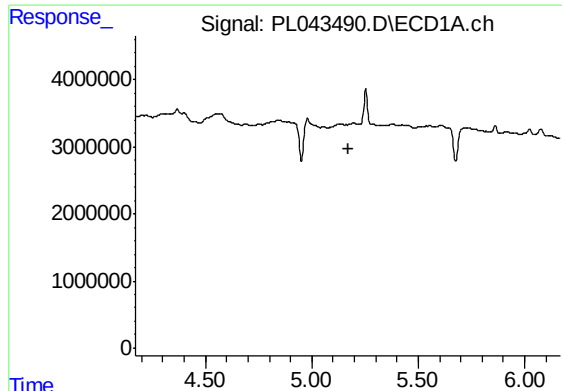

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

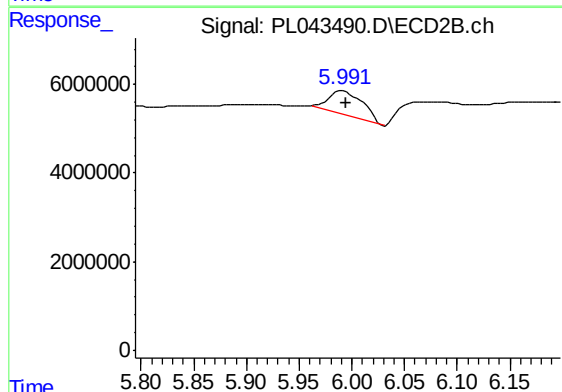


#8 Heptachlor epoxide

R.T.: 5.990 min
Delta R.T.: -0.004 min
Response: 11479168
Conc: 3.03 ng/ml

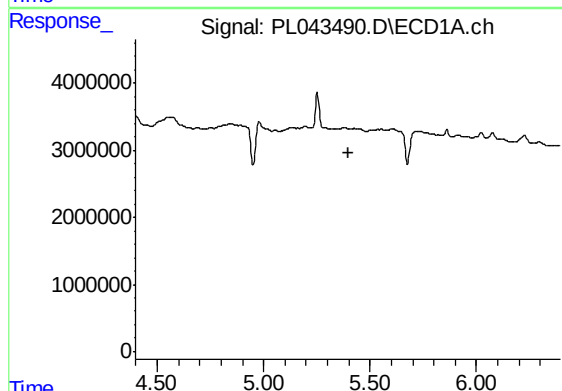


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

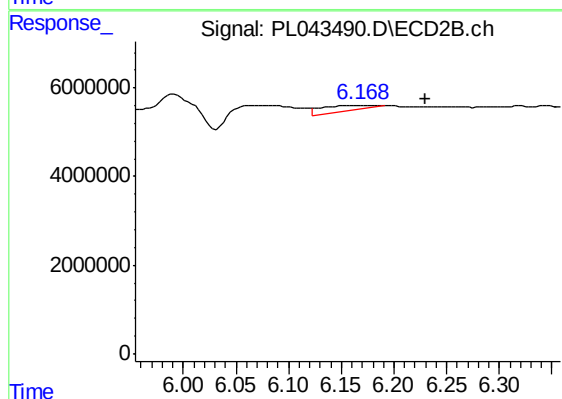

#10 gamma-Chlordane


R.T.: 6.168 min
Delta R.T.: -0.061 min
Response: 4538367
Conc: 1.24 ng/ml

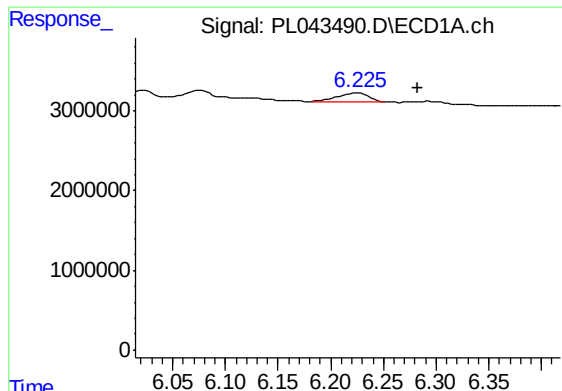

#15 Endosulfan II


R.T.: 6.227 min
Delta R.T.: -0.056 min
Response: 2212115
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

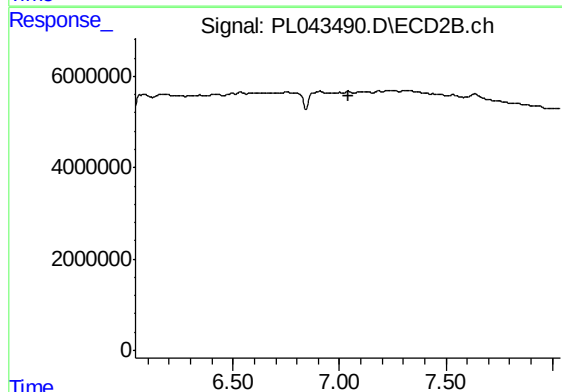


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

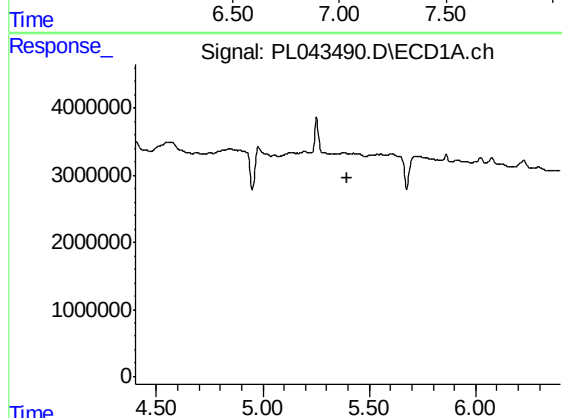


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

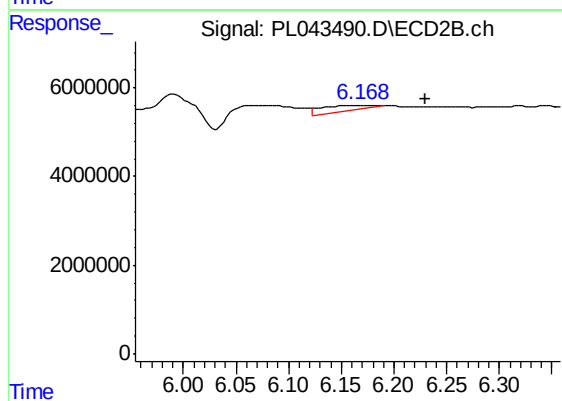

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: -0.062 min
Response: 4538367
Conc: 9.24 ng/ml

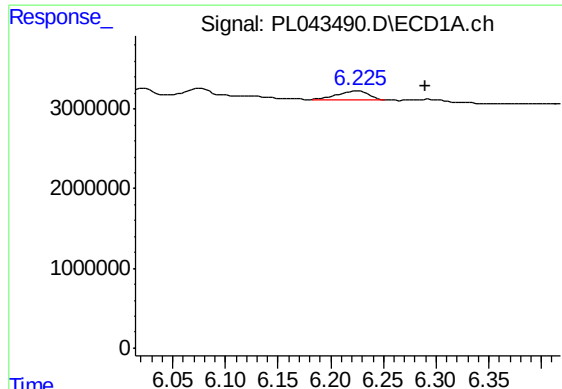

#27 Chlordane-5


R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 2212115
Conc: 9.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

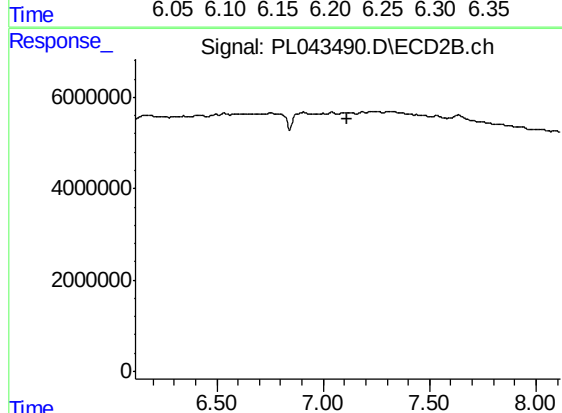


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

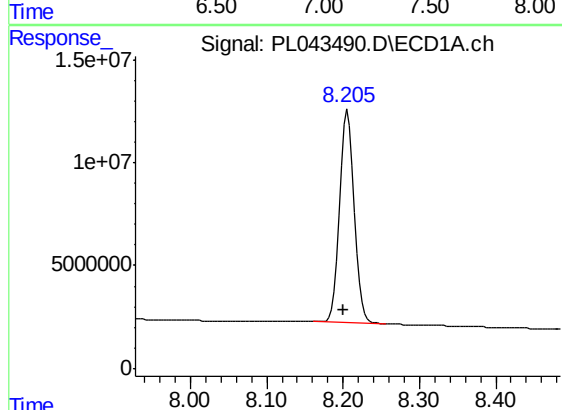

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.005 min
Response: 136153877
Conc: 20.85 ng/ml

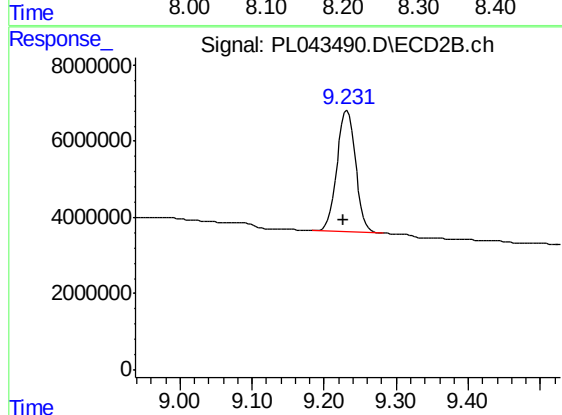

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.005 min
Response: 57383634
Conc: 22.00 ng/ml