

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
 Data File : PL043500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 15:15
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 22:31:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	148.5E6	75368101	24.208	25.429
28)	SA Decachlor...	8.200	9.230	113.3E6	47409349	17.348	18.175
Target Compounds							
6)	B beta-BHC	4.395f	0.000	2011368	0	0.545	N.D. #
8)	B Heptachlo...	0.000	5.989	0	9239159	N.D.	2.436 #
10)	B gamma-Chl...	0.000	6.162f	0	3347769	N.D.	0.911 #
20)	A Methoxychlor	0.000	7.638f	0	2650583	N.D.	1.757 #
23)	Chlordane-1	4.360	0.000	1075165	0	4.001	N.D. #
25)	Chlordane-3	0.000	6.162	0	3347769	N.D.	6.817 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
Data File : PL043500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 15:15
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 22:31:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

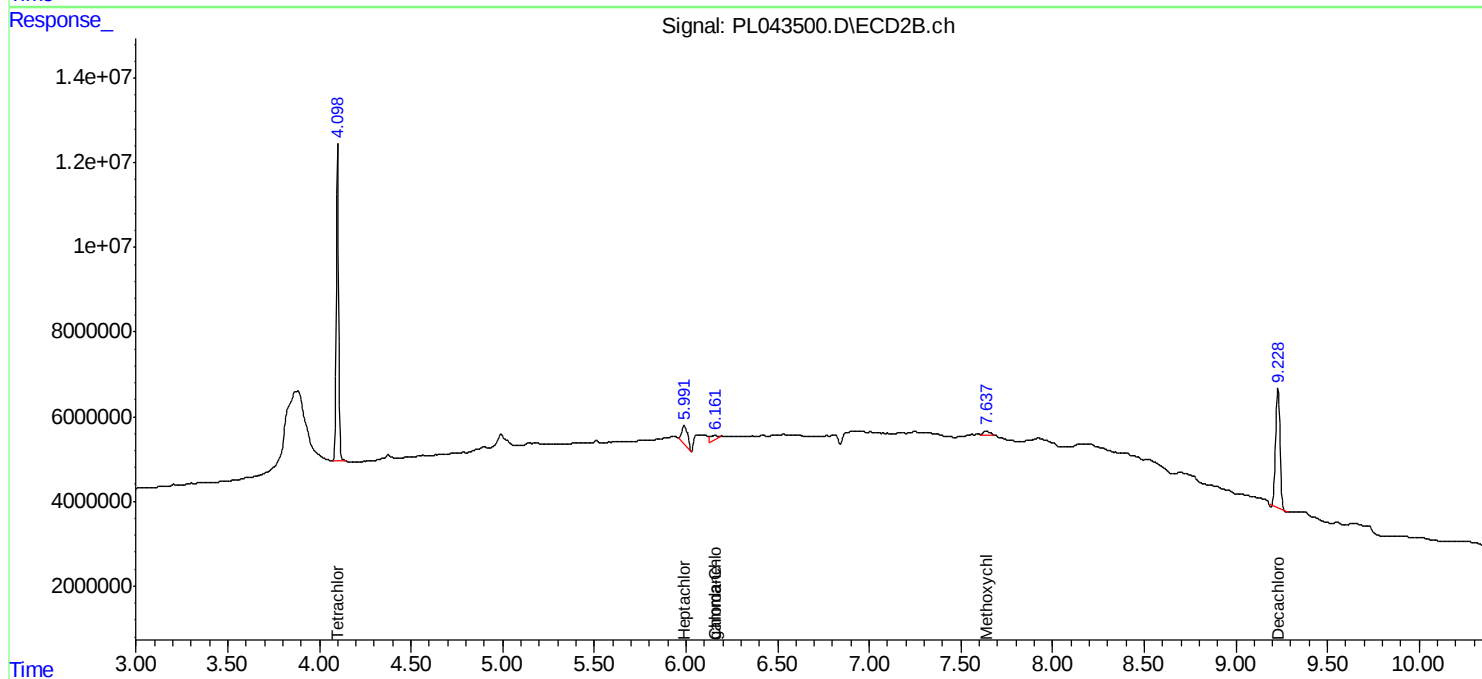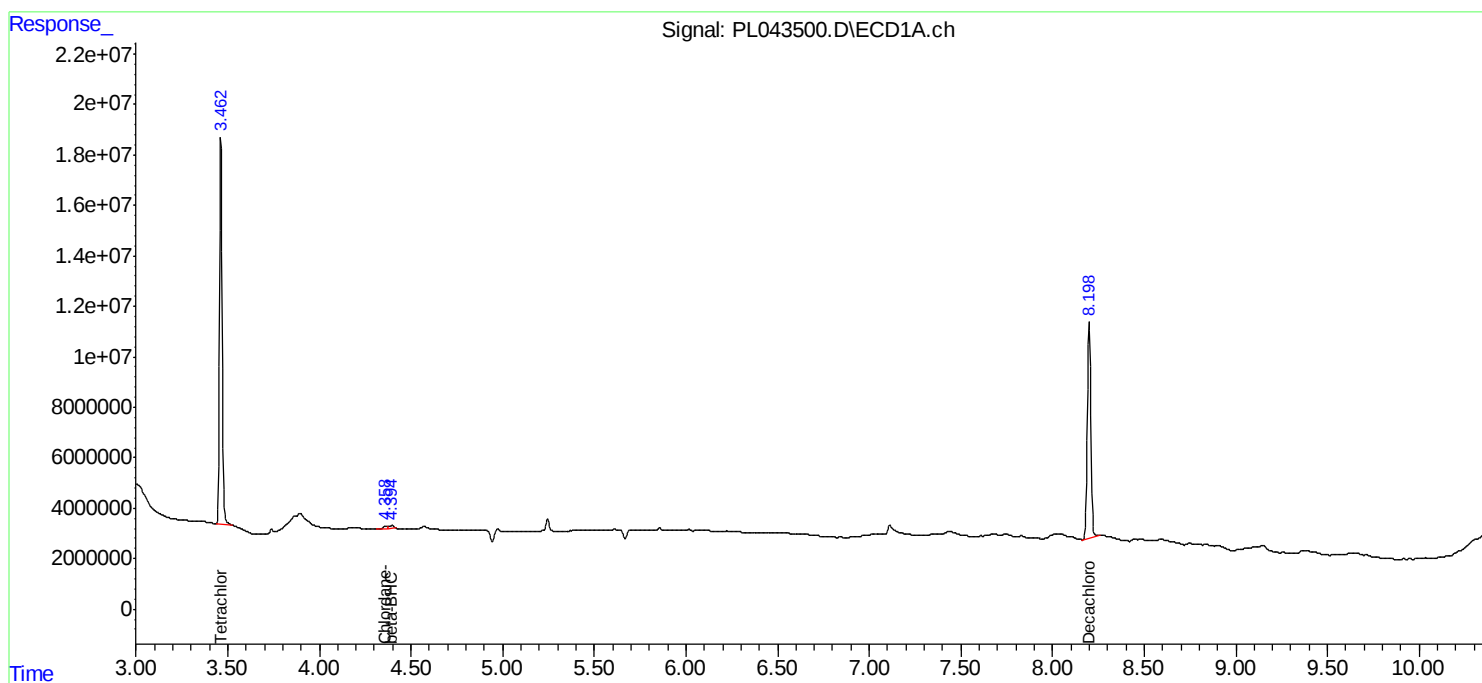


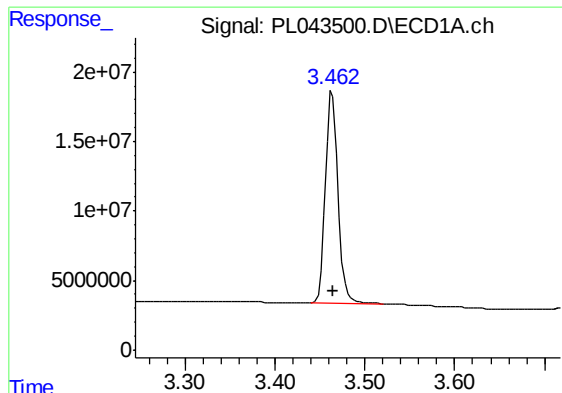

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 148466565
Conc: 24.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

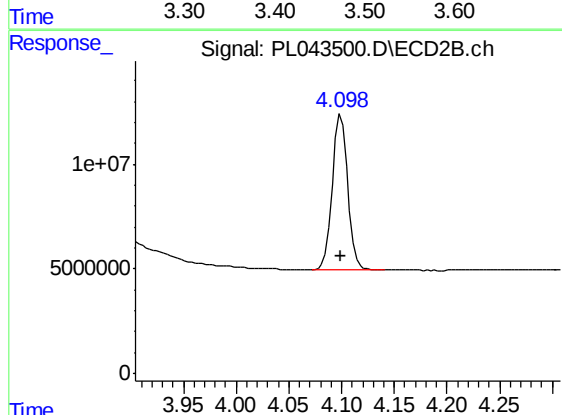


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 75368101
Conc: 25.43 ng/ml

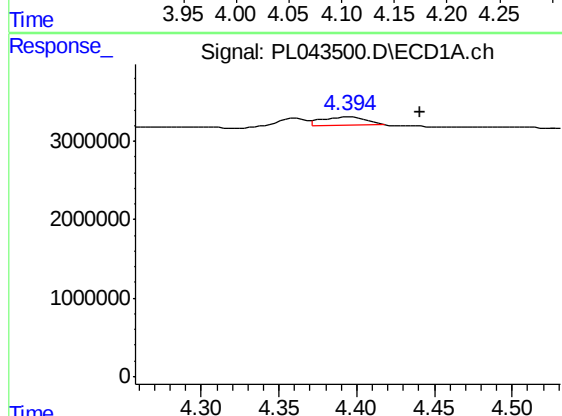


#6 beta-BHC

R.T.: 4.395 min
Delta R.T.: -0.046 min
Response: 2011368
Conc: 0.55 ng/ml

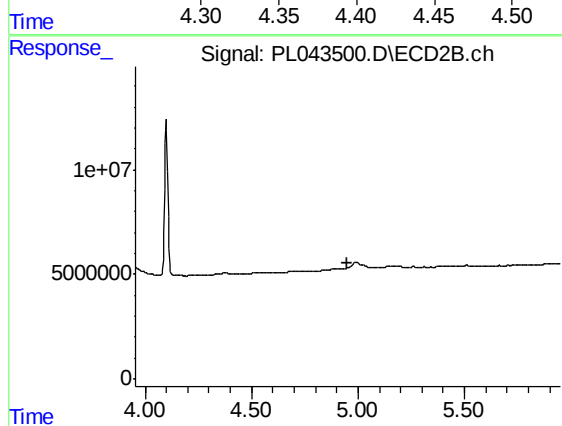

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

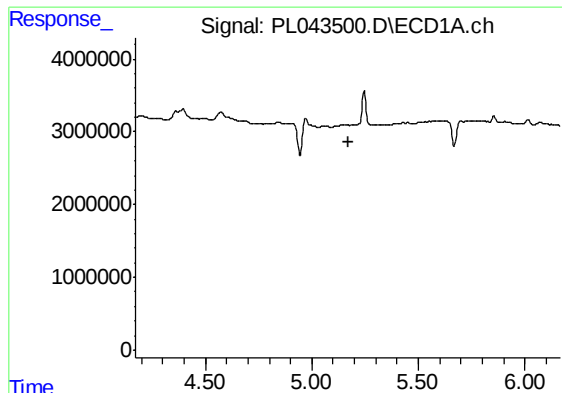

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

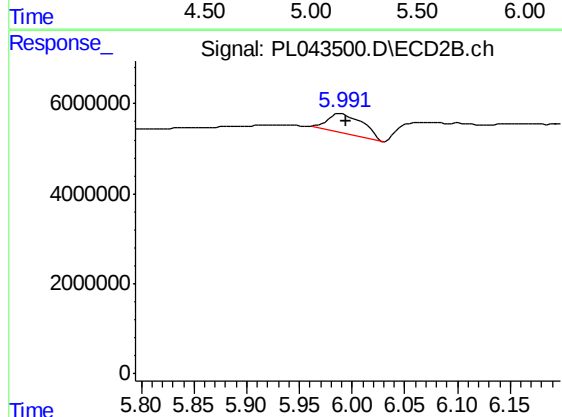


#8 Heptachlor epoxide

R.T.: 5.989 min
Delta R.T.: -0.006 min
Response: 9239159
Conc: 2.44 ng/ml

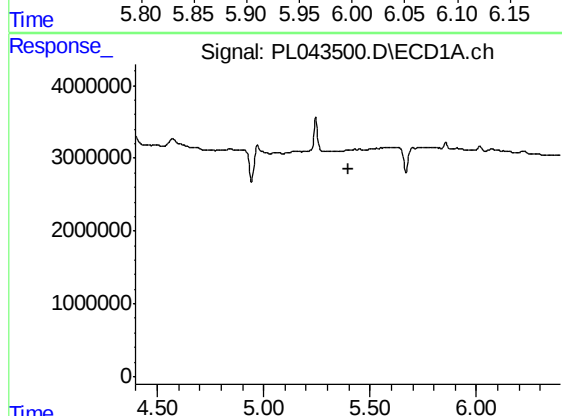


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

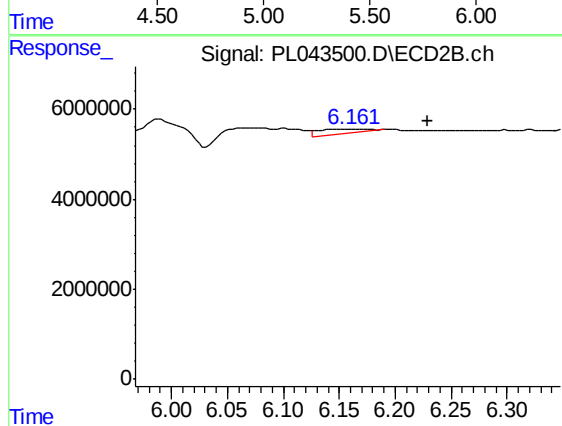

#10 gamma-Chlordane


R.T.: 6.162 min
Delta R.T.: -0.068 min
Response: 3347769
Conc: 0.91 ng/ml

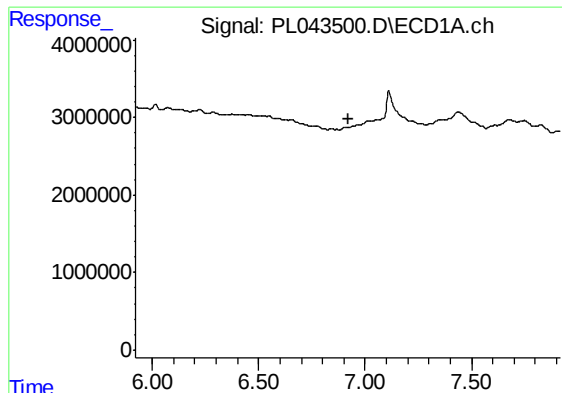

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

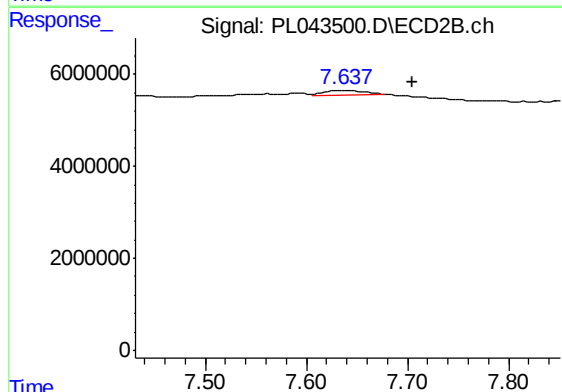


#20 Methoxychlor

R.T.: 7.638 min
Delta R.T.: -0.067 min
Response: 2650583
Conc: 1.76 ng/ml

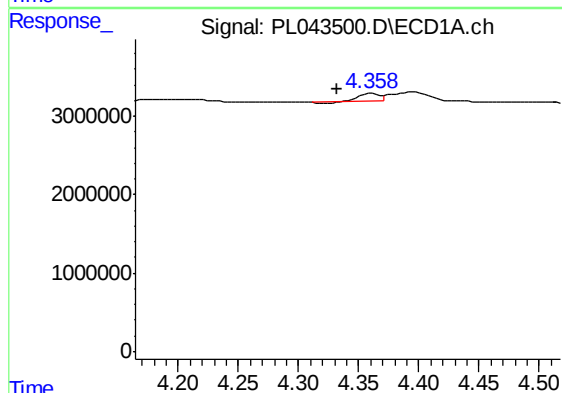


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.028 min
Response: 1075165
Conc: 4.00 ng/ml

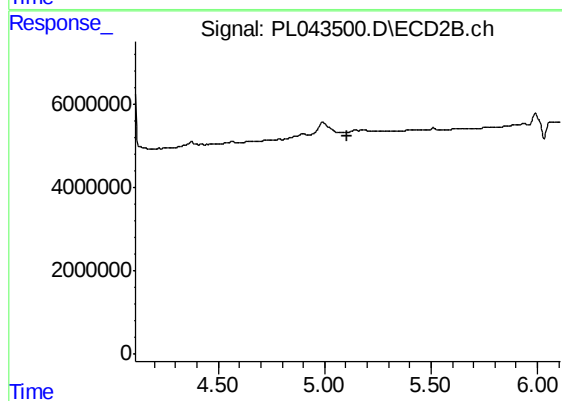

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

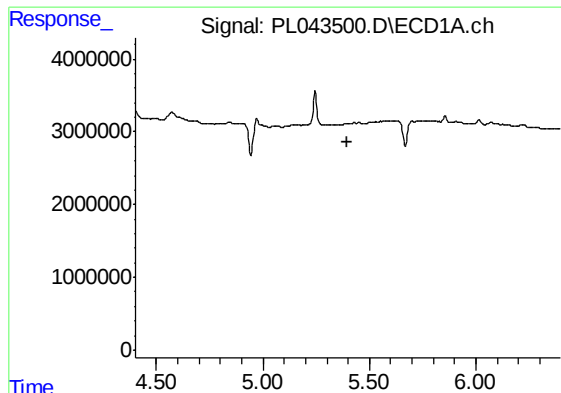

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

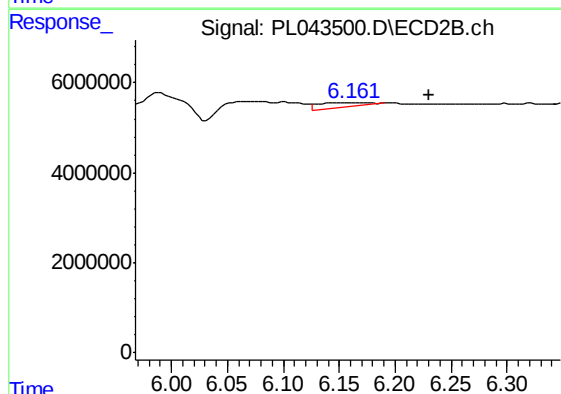


#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: -0.068 min
Response: 3347769
Conc: 6.82 ng/ml

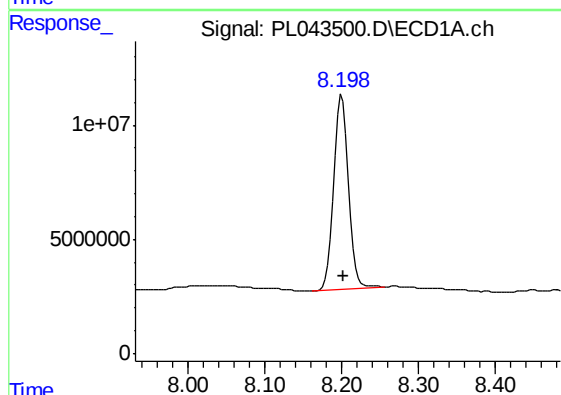

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.001 min
Response: 113283919
Conc: 17.35 ng/ml

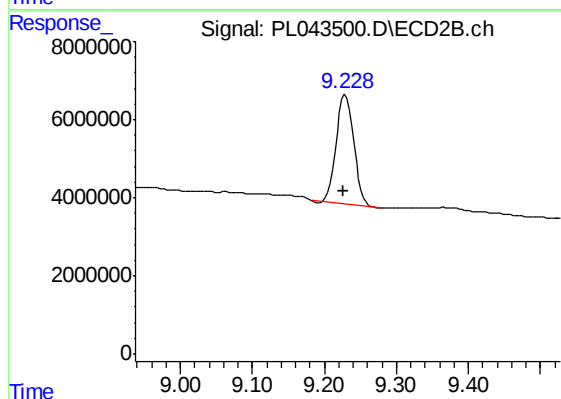

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.003 min
Response: 47409349
Conc: 18.17 ng/ml